

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
 Data File : VW021539.D
 Acq On : 21 Dec 2021 21:53
 Operator : SY/VA
 Sample : M5194-05
 Misc : 6.63g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB7

Quant Time: Dec 22 03:51:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 22 02:57:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	151827	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	147021	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81558	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	40503	14.648	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.600%
7) Chloroethane-d5	2.885	69	28184	15.418	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.680%
11) 1,1-Dichloroethene-d2	4.019	63	55922	15.169	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.680%
21) 2-Butanone-d5	7.080	46	17181	44.079	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.160%
24) Chloroform-d	7.647	84	84502	19.972	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.880%
26) 1,2-Dichloroethane-d4	8.305	65	45933	20.409	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.640%
32) Benzene-d6	8.275	84	162437	20.157	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.640%
36) 1,2-Dichloropropane-d6	9.274	67	45463	21.035	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.160%
41) Toluene-d8	10.323	98	163922	19.908	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.640%
43) trans-1,3-Dichloroprop...	10.579	79	18662	18.753	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.000%
47) 2-Hexanone-d5	10.920	63	14016	43.856	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.720%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	33910	18.252	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.000%
66) 1,2-Dichlorobenzene-d4	13.847	152	58458	18.495	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	73.960%#
Target Compounds					Qvalue	
13) Acetone	4.123	43	1570	4.493	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122121\
Data File : VW021539.D
Acq On : 21 Dec 2021 21:53
Operator : SY/VA
Sample : M5194-05
Misc : 6.63g/10.0mL/MSVOA_W/SOIL
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLB7


Quant Time: Dec 22 03:51:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 22 02:57:00 2021
Response via : Initial Calibration

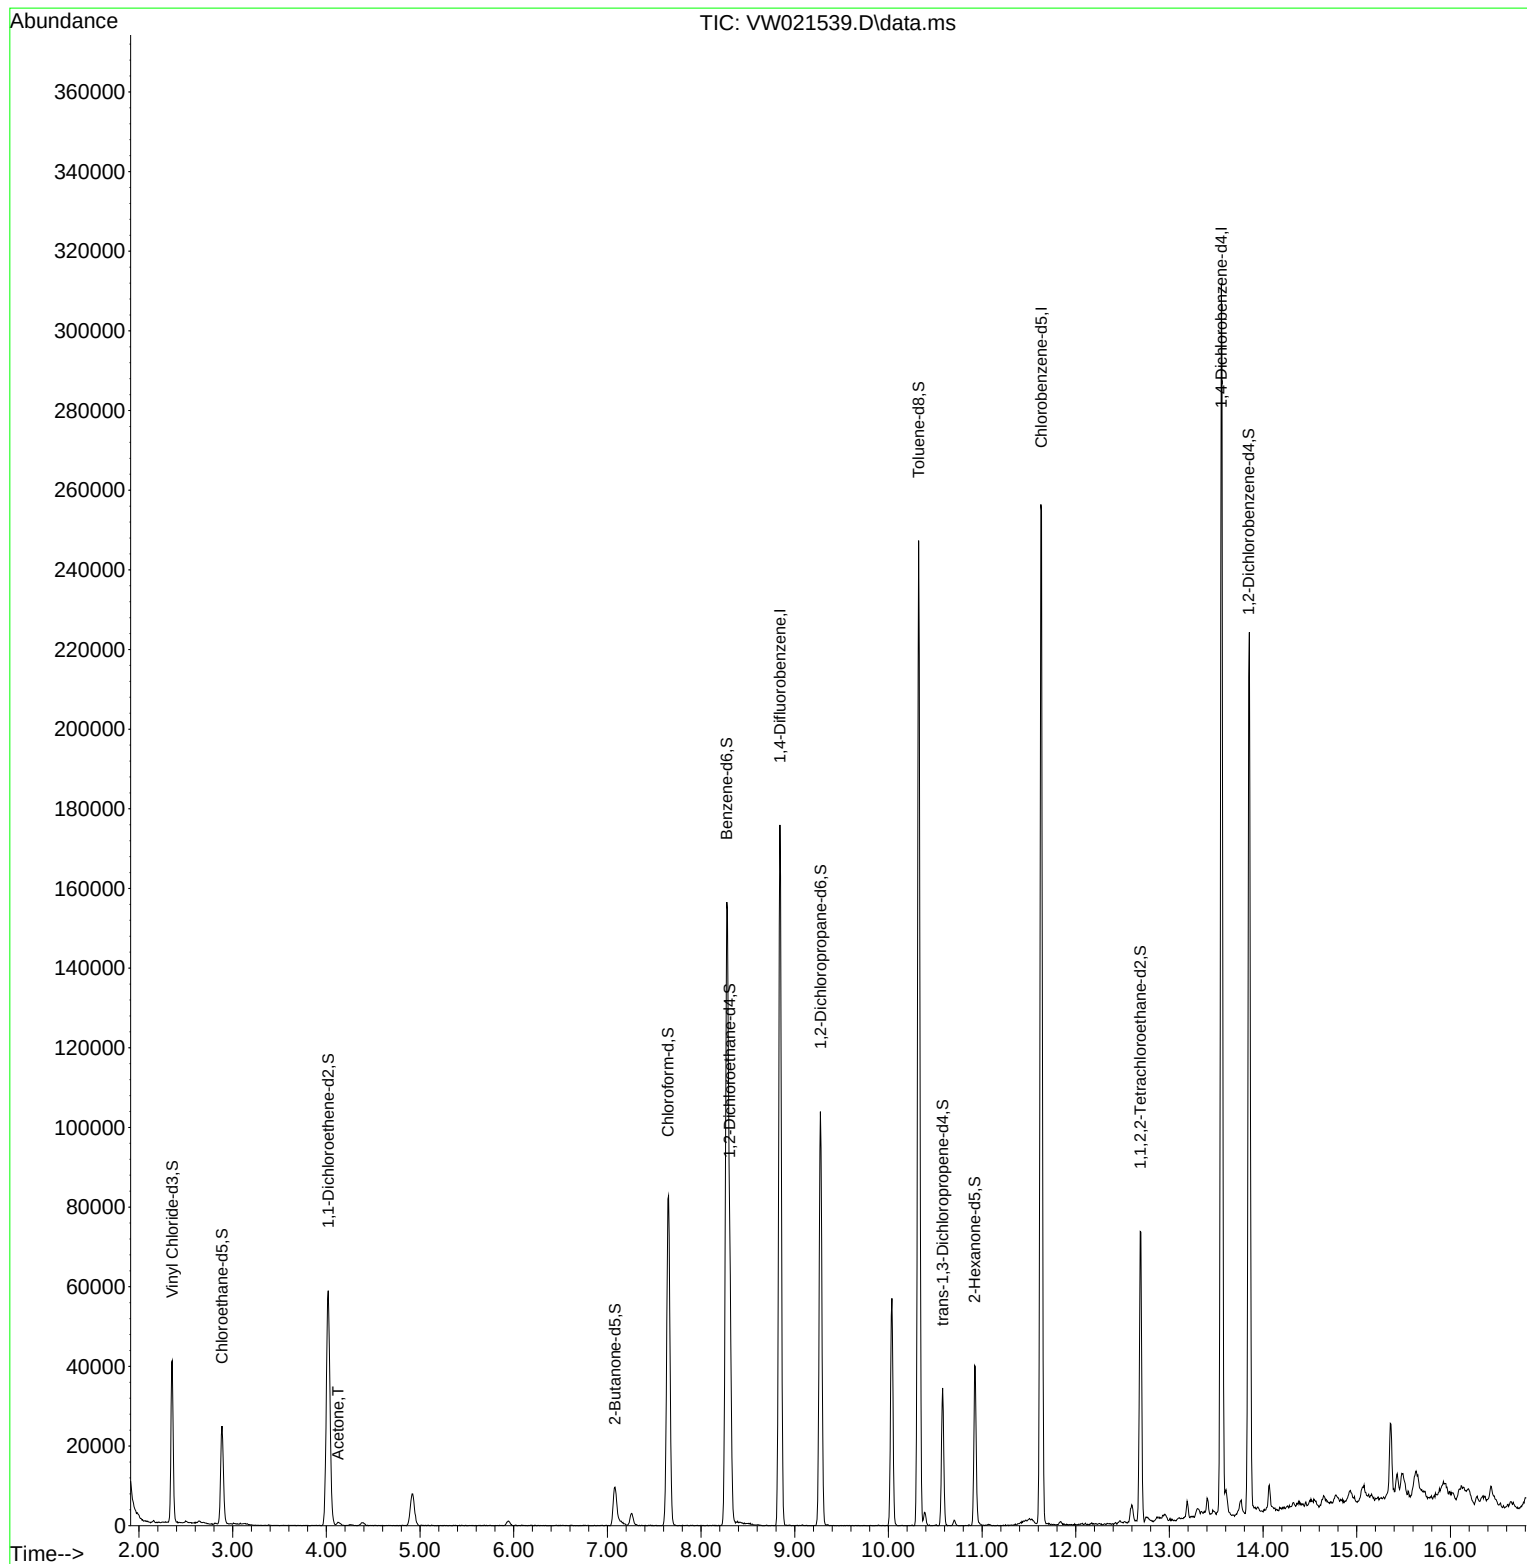

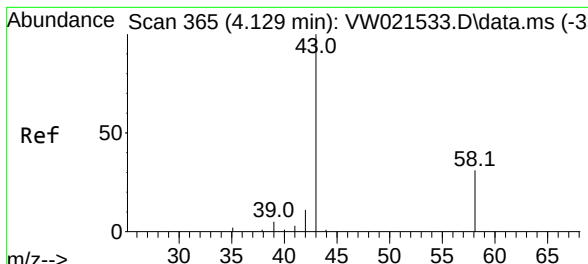

#13
 Acetone
 Concen: 4.493 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW021539.D
 Acq: 21 Dec 2021 21:53

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB7

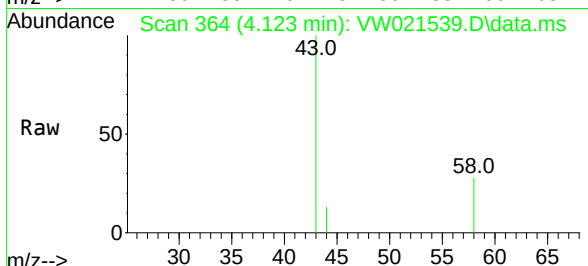

Tgt Ion: 43 Resp: 1570

Ion	Ratio	Lower	Upper
43	100		
58	28.8	0.0	52.8

