

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122124\
 Data File : VW031490.D
 Acq On : 22 Dec 2024 04:52
 Operator : SY/MD
 Sample : P5322-11
 Misc : 5.26g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 23 02:15:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 23 01:56:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	868404	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	667907	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	237008	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	216008	16.532	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.120%
7) Chloroethane-d5	2.899	69	174898	18.095	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.400%
11) 1,1-Dichloroethene-d2	4.021	65	89398	14.424	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.680%
21) 2-Butanone-d5	7.106	46	76014	30.891	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.780%
24) Chloroform-d	7.648	84	372112	15.639	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	62.560%
26) 1,2-Dichloroethane-d4	8.508	65	125	0.010	ug/L	0.20
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	741738	17.327	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.320%
36) 1,2-Dichloropropane-d6	9.270	67	224592	18.001	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	72.000%
41) Toluene-d8	10.318	98	599849	15.062	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	60.240%
43) trans-1,3-Dichloroprop...	10.581	79	72689	12.635	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	50.560%
47) 2-Hexanone-d5	10.928	63	58464	34.844	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	145119	18.525	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.120%
66) 1,2-Dichlorobenzene-d4	13.848	152	145001	16.480	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	65.920%#
Target Compounds						Qvalue
12) 1,1-Dichloroethene	4.039	96	7528	0.707	ug/L #	1
30) 1,1,1-Trichloroethane	7.874	97	8146	0.472	ug/L	91
34) Trichloroethene	9.087	95	137340	11.786	ug/L	90
46) Tetrachloroethene	10.861	164	135572	15.883	ug/L	94
48) 2-Hexanone	10.922	43	7538	1.622	ug/L #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122124\
Data File : VW031490.D
Acq On : 22 Dec 2024 04:52
Operator : SY/MD
Sample : P5322-11
Misc : 5.26g/10mL/MSVOA_W/SOIL/A
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 23 02:15:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 23 01:56:19 2024
Response via : Initial Calibration

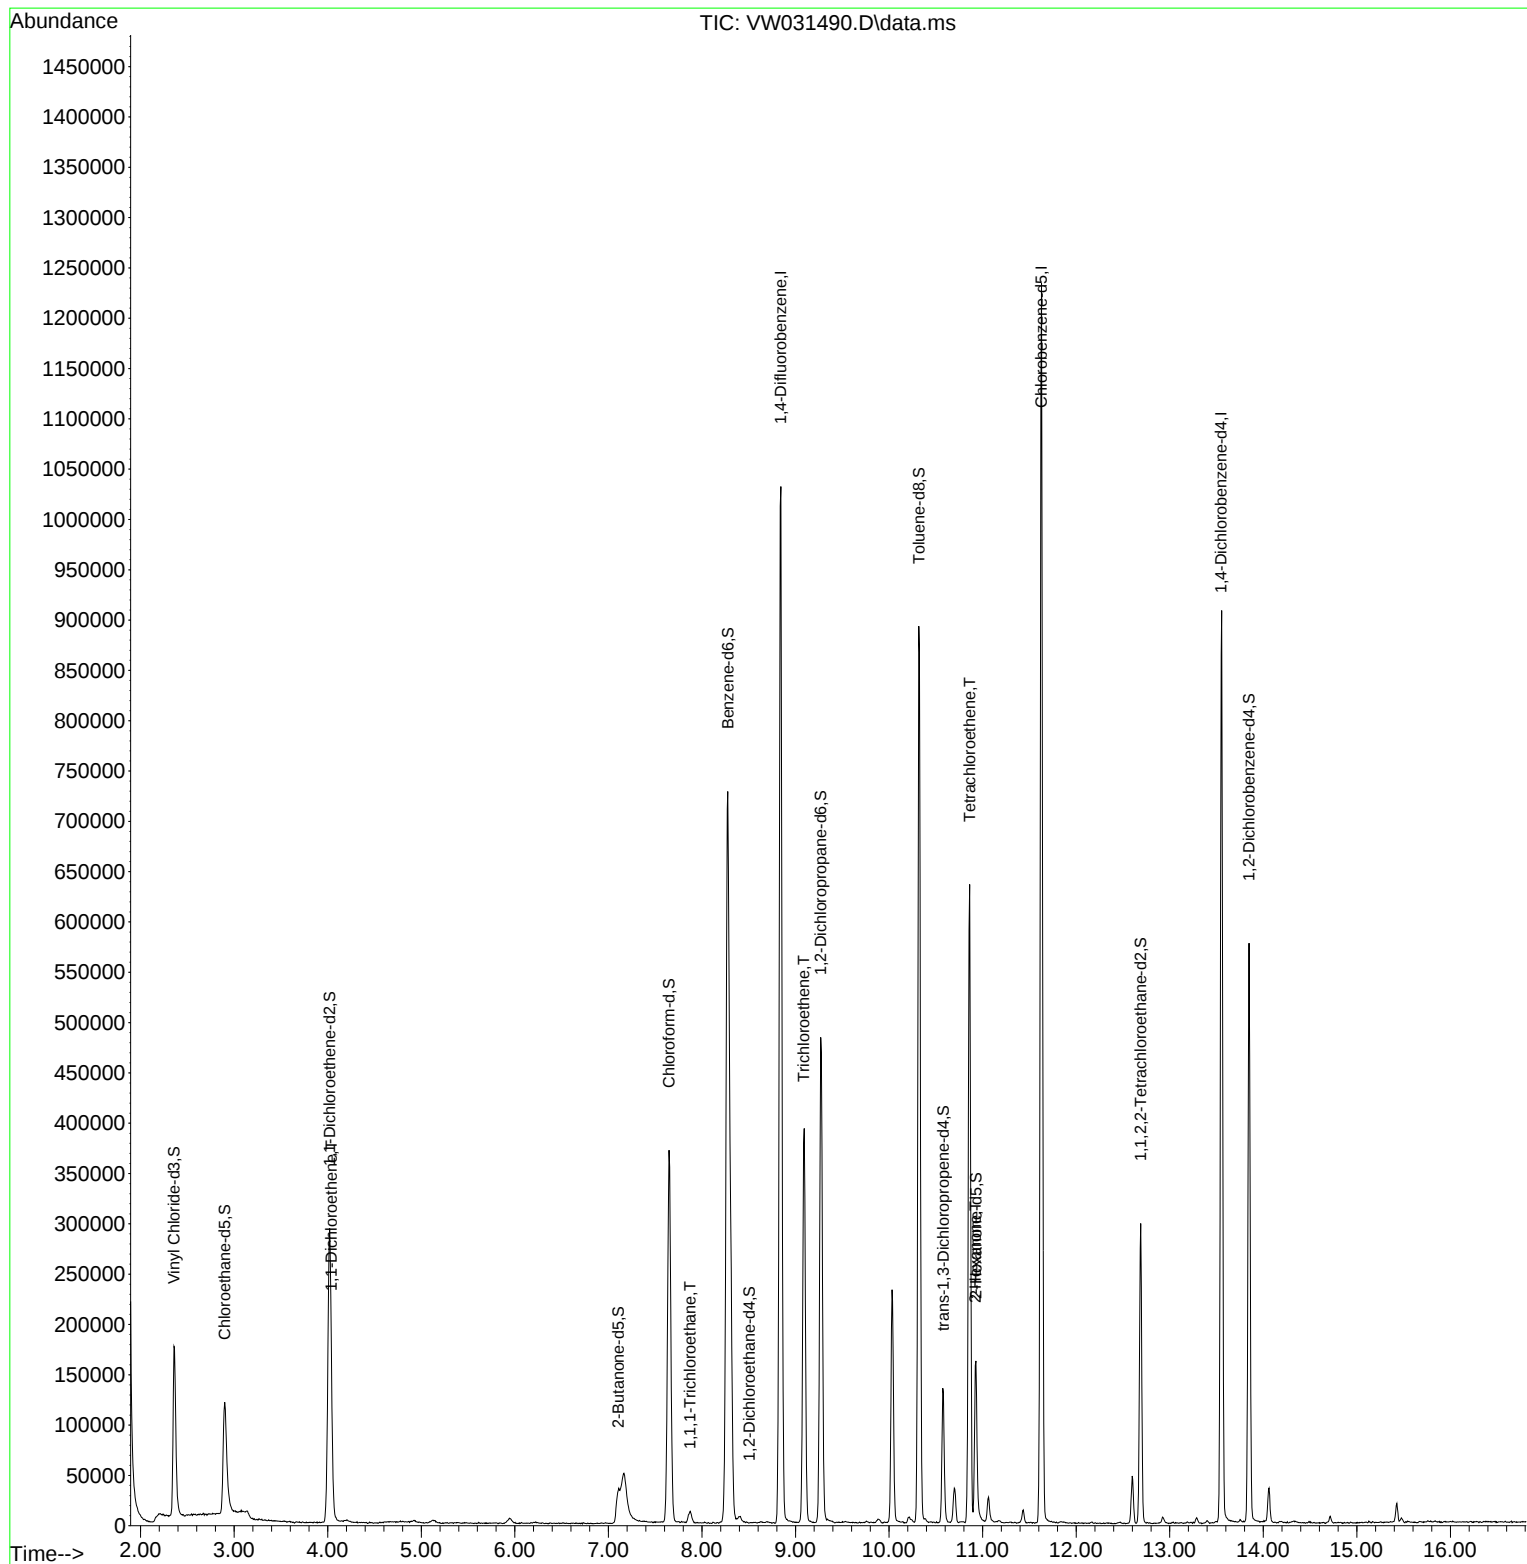



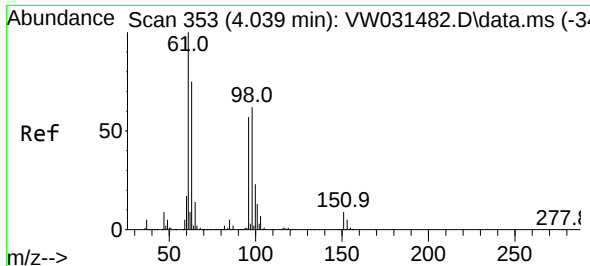


#12
1,1-Dichloroethene
Concen: 0.707 ug/L
RT: 4.039 min Scan# 353
Delta R.T. -0.000 min
Lab File: VW031490.D
Acq: 22 Dec 2024 04:52

Instrument :
MSVOA_W
ClientSampleId :



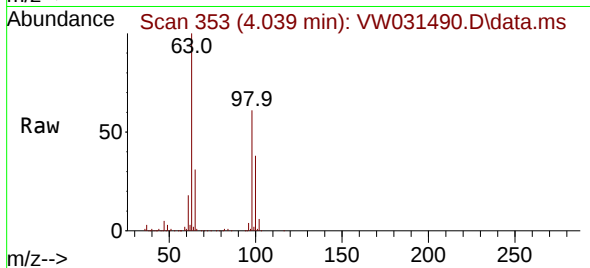



Tgt Ion: 96 Resp: 7528
Ion Ratio Lower Upper
96 100
61 437.0 125.3 232.7#
63 2463.3 104.6 194.2#

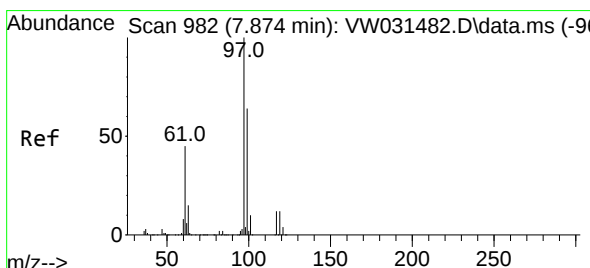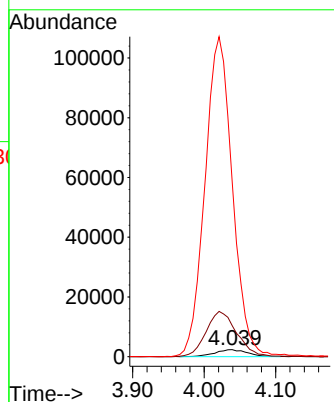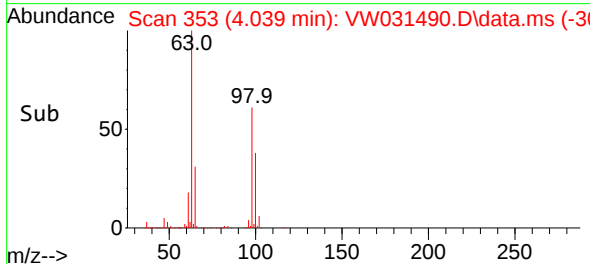

#30
1,1,1-Trichloroethane
Concen: 0.472 ug/L
RT: 7.874 min Scan# 982
Delta R.T. -0.000 min
Lab File: VW031490.D
Acq: 22 Dec 2024 04:52

Tgt Ion: 97 Resp: 8146
Ion Ratio Lower Upper
97 100
99 70.1 51.1 76.7
61 51.6 36.3 54.5

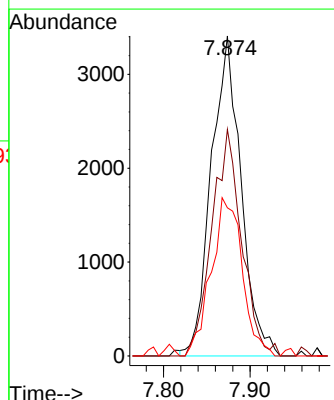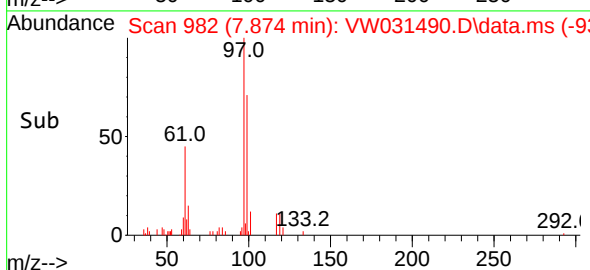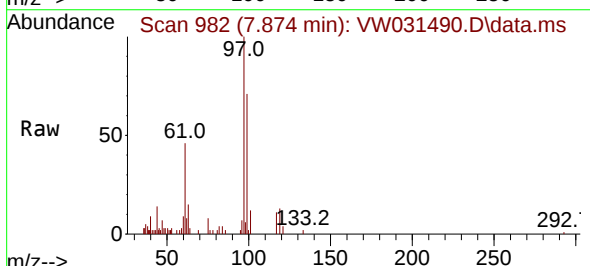

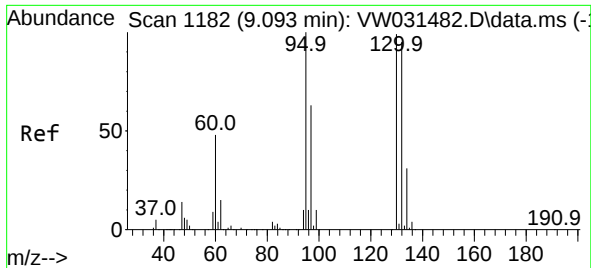

#34

Trichloroethene

Concen: 11.786 ug/L

RT: 9.087 min Scan# 1181

Delta R.T. -0.006 min

Lab File: VW031490.D

Acq: 22 Dec 2024 04:52

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion: 95 Resp: 137340





Ion Ratio Lower Upper

95 100

97 65.2 46.5 86.3

132 85.4 70.3 130.5

130 94.8 73.6 136.8

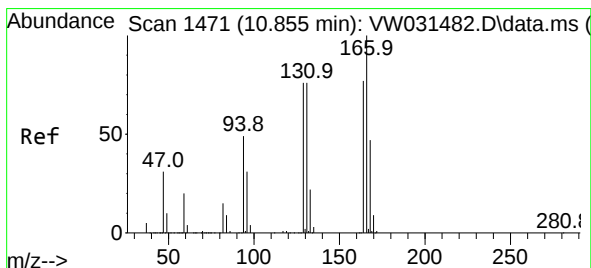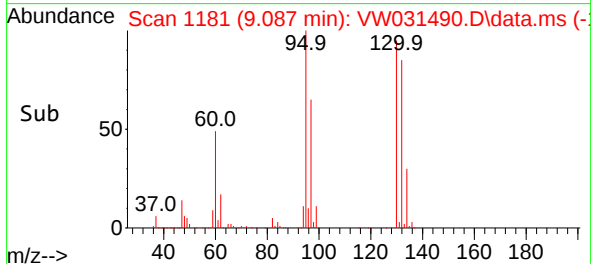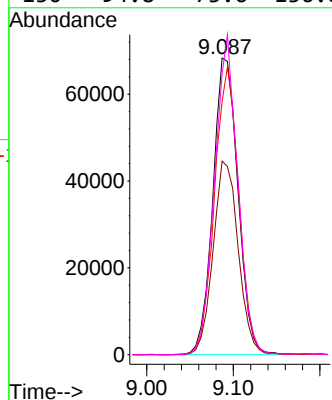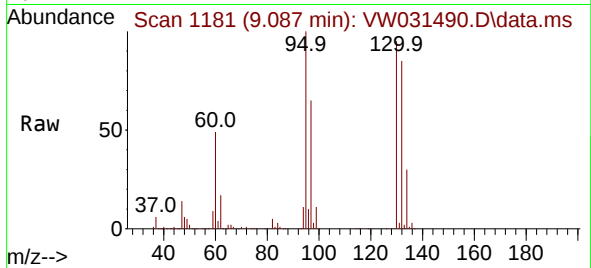

#46

Tetrachloroethene

Concen: 15.883 ug/L

RT: 10.861 min Scan# 1472

Delta R.T. 0.006 min

Lab File: VW031490.D

Acq: 22 Dec 2024 04:52

Tgt Ion:164 Resp: 135572




Ion Ratio Lower Upper


164 100

129 94.5 73.5 136.5

131 94.7 66.6 123.8


166 123.9 92.7 172.3

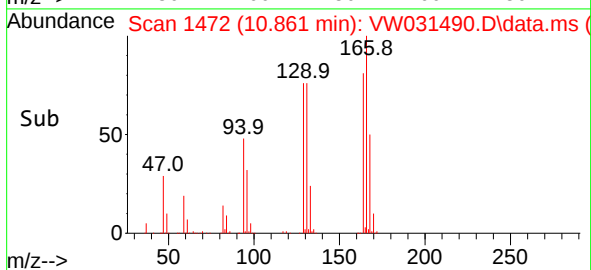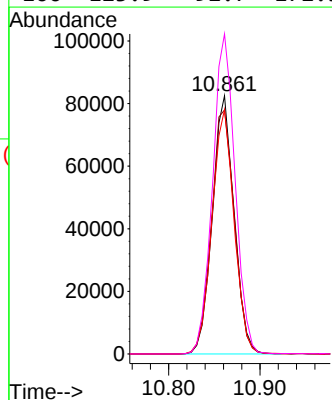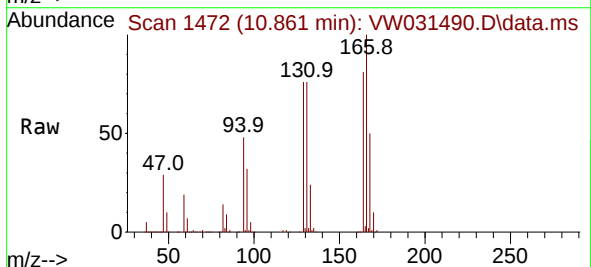

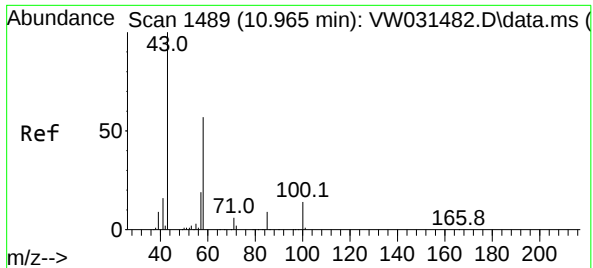

#48
 2-Hexanone
 Concen: 1.622 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW031490.D
 Acq: 22 Dec 2024 04:52

Instrument :
 MSVOA_W
 ClientSampleId :

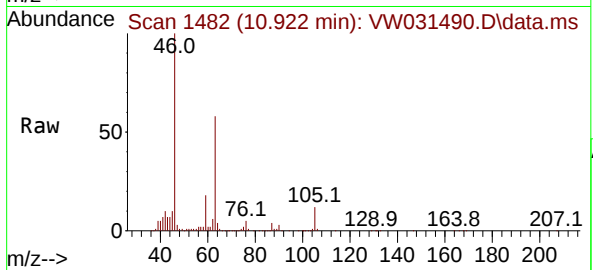

Tgt Ion: 43	Resp: 7538
Ion Ratio	Lower Upper
43 100	
58 32.7	43.0 64.6#
57 29.4	15.7 23.5#
100 1.4	10.3 15.5#

