




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122124\
Data File : VW031490.D
Acq On : 22 Dec 2024 04:52
Operator : SY/MD
Sample : P5322-11
Misc : 5.26g/10mL/MSVOA_W/SOIL/A
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YE5Z9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/24/2024

Quant Time: Dec 23 02:15:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 23 01:56:19 2024
Response via : Initial Calibration

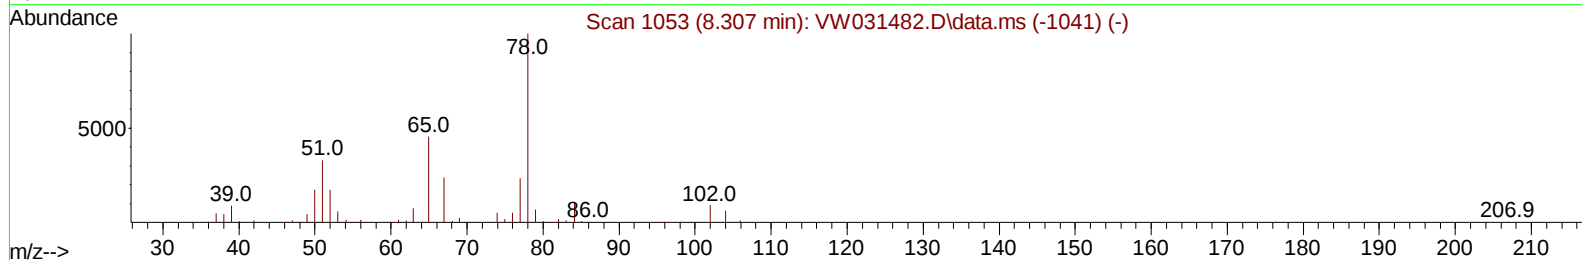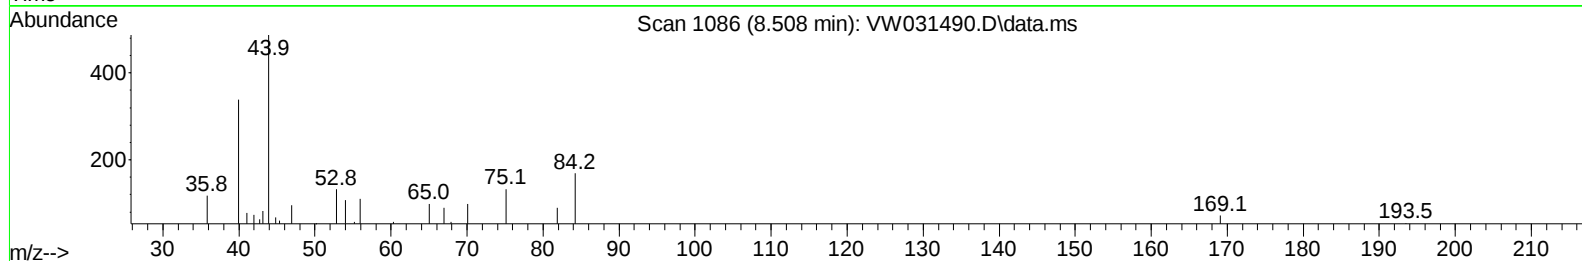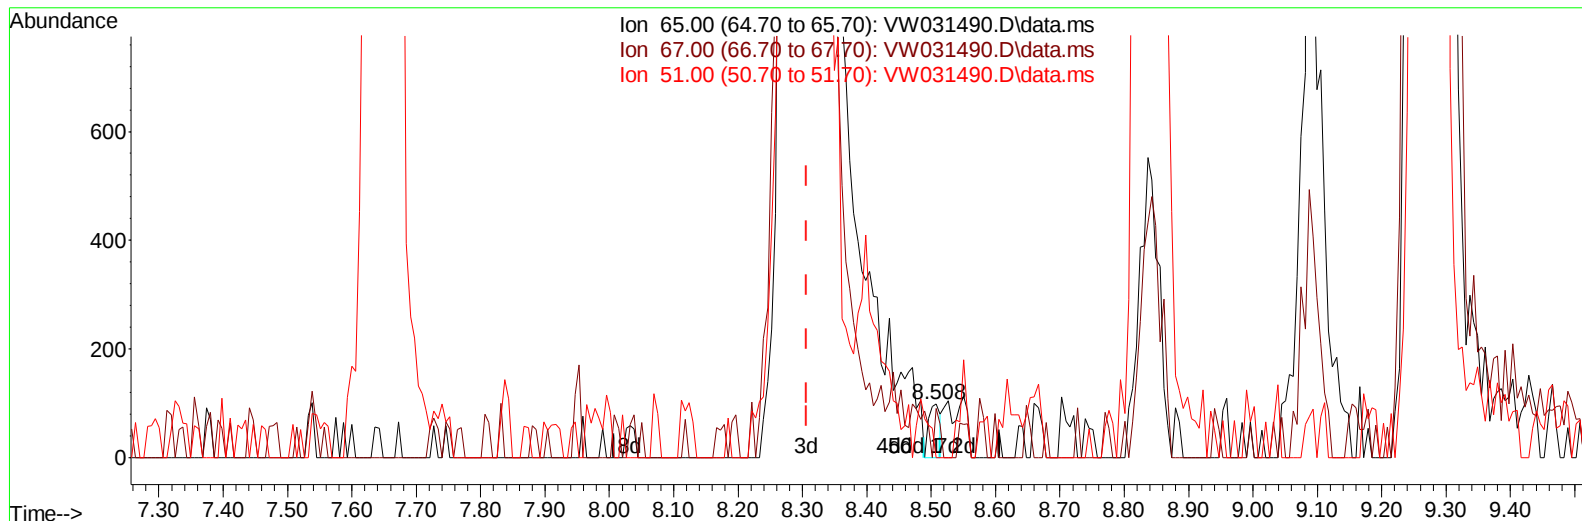

TIC: VW031490.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.508min (+ 0.201) 0.01 ug/L

response 125

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	44.80
51.00	108.10	103.20
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122124\
Data File : VW031490.D
Acq On : 22 Dec 2024 04:52
Operator : SY/MD
Sample : P5322-11
Misc : 5.26g/10mL/MSVOA_W/SOIL/A
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YE5Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 23 02:15:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 23 01:56:19 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/24/2024

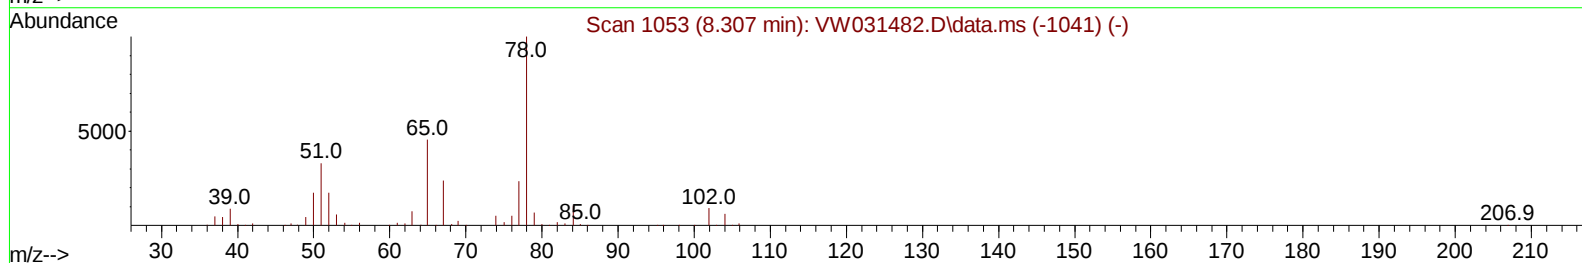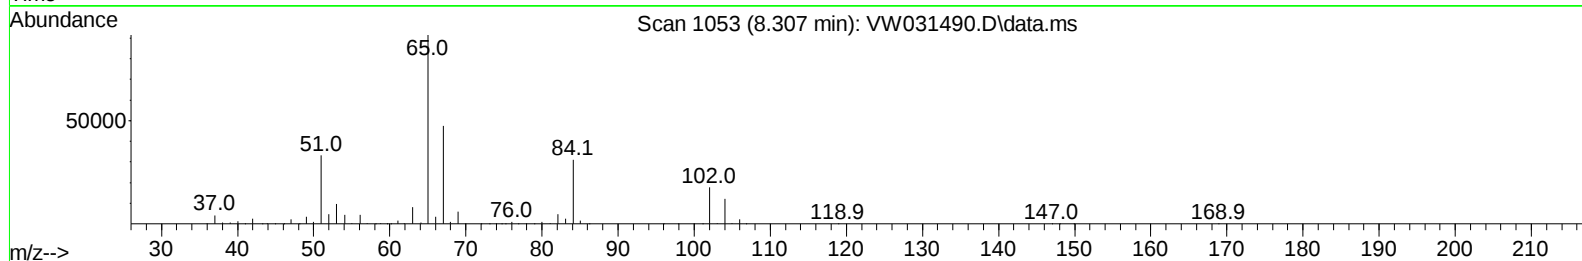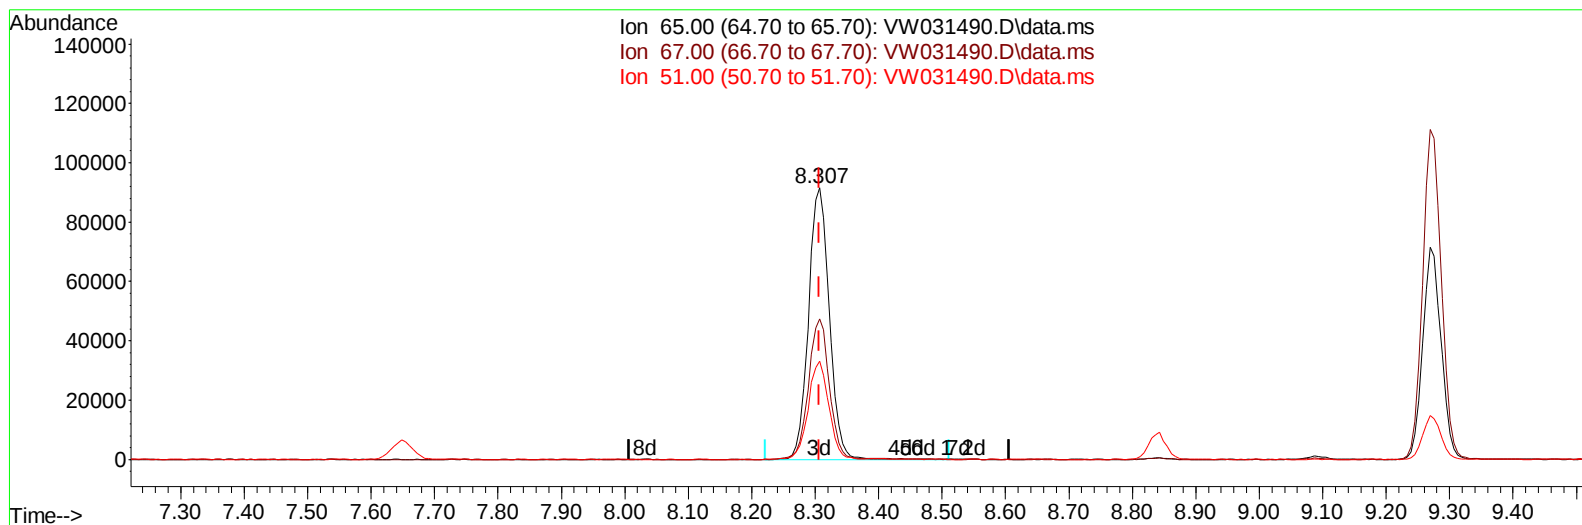

TIC: VW031490.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 17.31 ug/L m

response 206801

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.03#
51.00	108.10	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122124\
 Data File : VW031490.D
 Acq On : 22 Dec 2024 04:52
 Operator : SY/MD
 Sample : P5322-11
 Misc : 5.26g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YE5Z9

Manual IntegrationsAPPROVED

Quant Time: Dec 23 02:15:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 23 01:56:19 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/23/2024
 Supervised By :Mahesh Dadoda 12/24/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	868404	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	667907	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	237008	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	216008	16.532	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.120%	
7) Chloroethane-d5	2.899	69	174898	18.095	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.400%	
11) 1,1-Dichloroethene-d2	4.021	65	89398	14.424	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.680%	
21) 2-Butanone-d5	7.106	46	76014	30.891	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	61.780%	
24) Chloroform-d	7.648	84	372112	15.639	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	62.560%	
26) 1,2-Dichloroethane-d4	8.307	65	206801m	17.306	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	69.240%#	
32) Benzene-d6	8.276	84	741738	17.327	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	69.320%	
36) 1,2-Dichloropropane-d6	9.270	67	224592	18.001	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	72.000%	
41) Toluene-d8	10.318	98	599849	15.062	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	60.240%	
43) trans-1,3-Dichloroprop...	10.581	79	72689	12.635	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	50.560%	
47) 2-Hexanone-d5	10.928	63	58464	34.844	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	69.680%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	145119	18.525	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	74.120%	
66) 1,2-Dichlorobenzene-d4	13.848	152	145001	16.480	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	65.920%#	
Target Compounds						
12) 1,1-Dichloroethene	4.039	96	7528	0.707	ug/L #	1
30) 1,1,1-Trichloroethane	7.874	97	8146	0.472	ug/L	91
34) Trichloroethene	9.087	95	137340	11.786	ug/L	90
46) Tetrachloroethene	10.861	164	135572	15.883	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122124\
Data File : VW031490.D
Acq On : 22 Dec 2024 04:52
Operator : SY/MD
Sample : P5322-11
Misc : 5.26g/10mL/MSVOA_W/SoIL/A
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YE5Z9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/23/2024
Supervised By :Mahesh Dadoda 12/24/2024

Quant Time: Dec 23 02:15:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 23 01:56:19 2024
Response via : Initial Calibration

