

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122218\
 Data File : VW007766.D
 Acq On : 20 Dec 2018 23:36
 Operator : SY/AP
 Sample : J6392-04RE
 Misc : 7.52G/5ML/MSVOA W/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 KY001SB102-121118-(15-17)RE

Quant Time: Dec 21 03:58:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W122118S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 20 06:30:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.95
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.84
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.63
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.56

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		0.00	65	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
35) Dibromofluoromethane		0.00	113	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
50) Toluene-d8		0.00	98	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene		12.60	95	19	0.00	ug/l	-0.02
Spiked Amount	50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122218\
Data File : VW007766.D
Acq On : 20 Dec 2018 23:36
Operator : SY/AP
Sample : J6392-04RE
Misc : 7.52G/5ML/MSVOA W/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
KY001SB102-121118-(15-17)RE

Quant Time: Dec 21 03:58:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W122118S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 20 06:30:23 2018
Response via : Initial Calibration

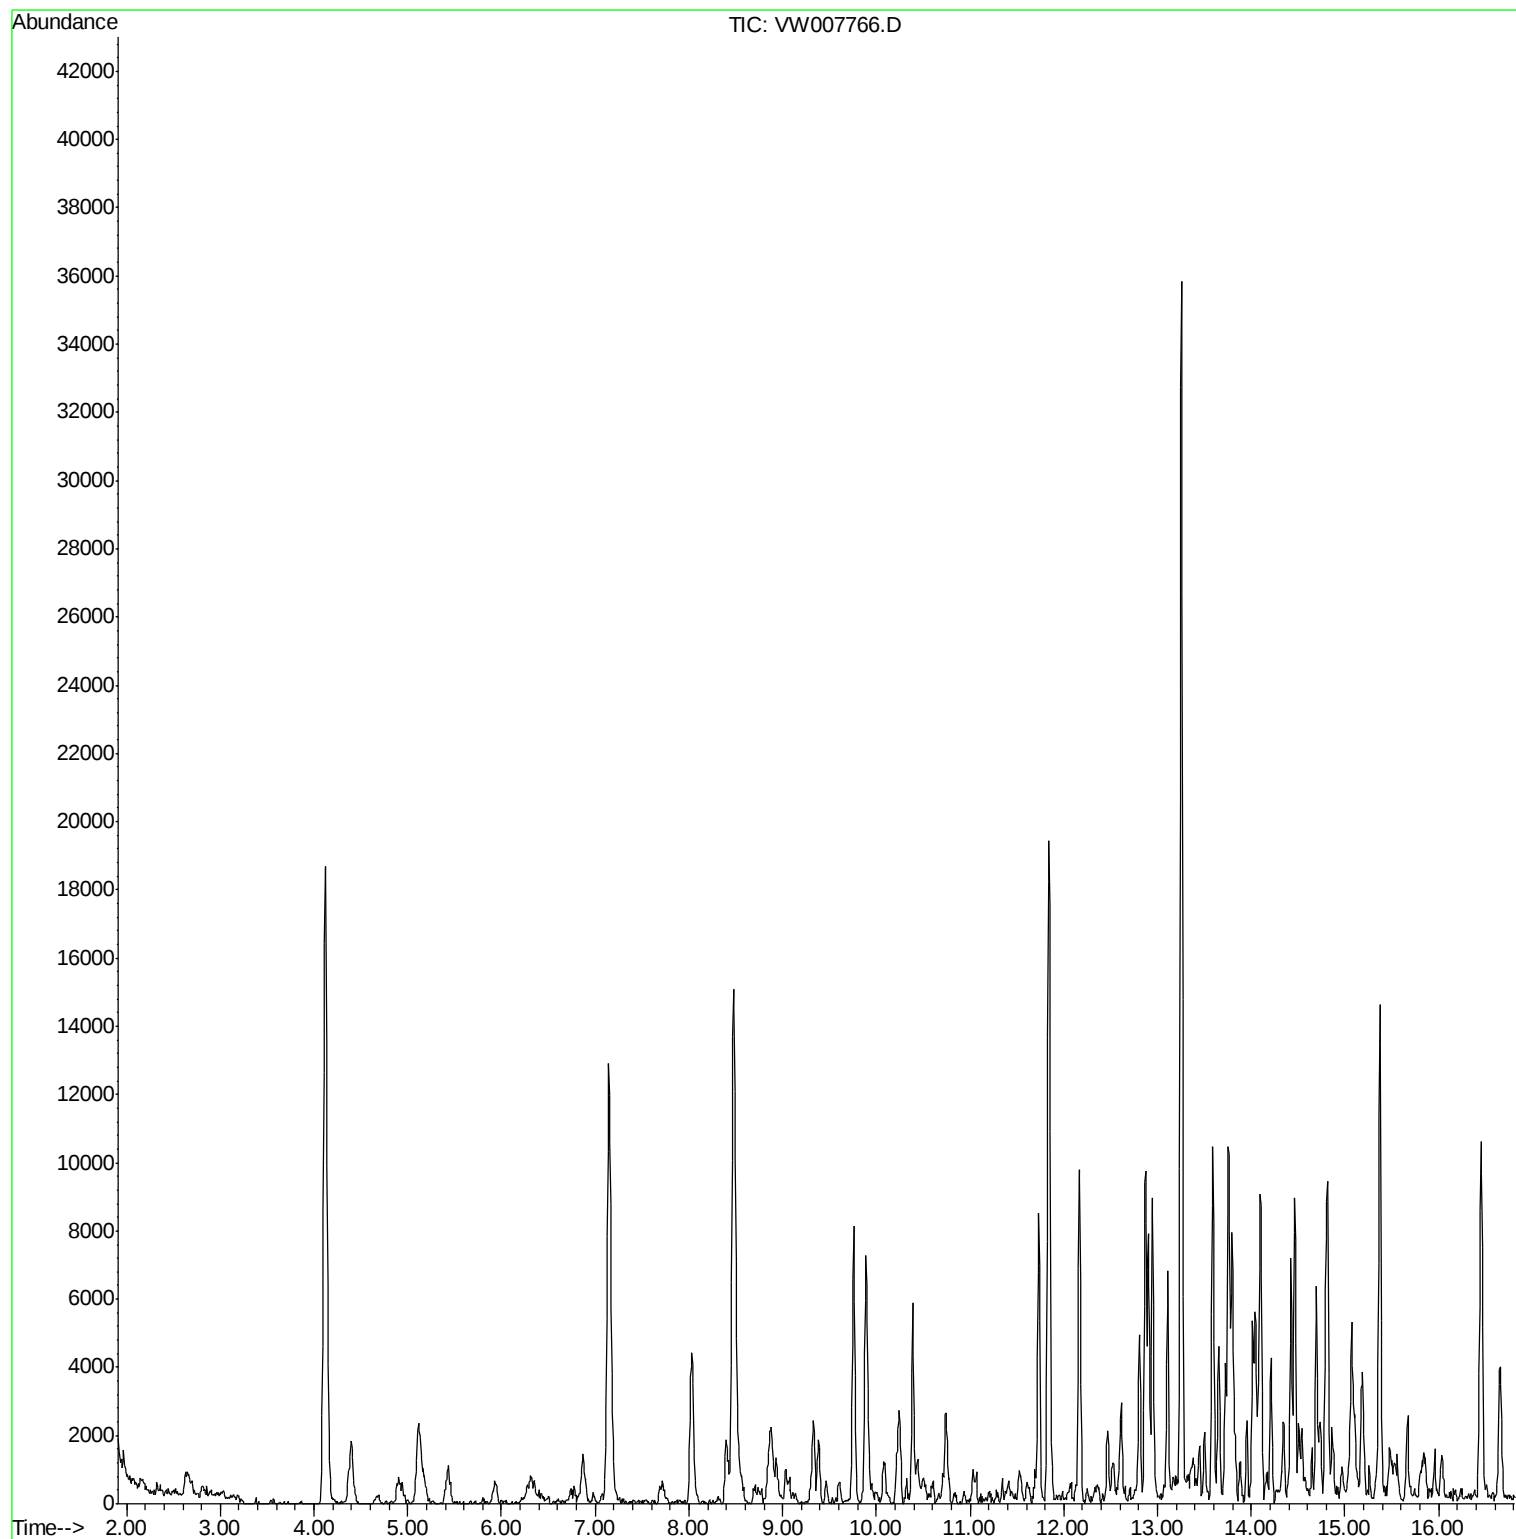

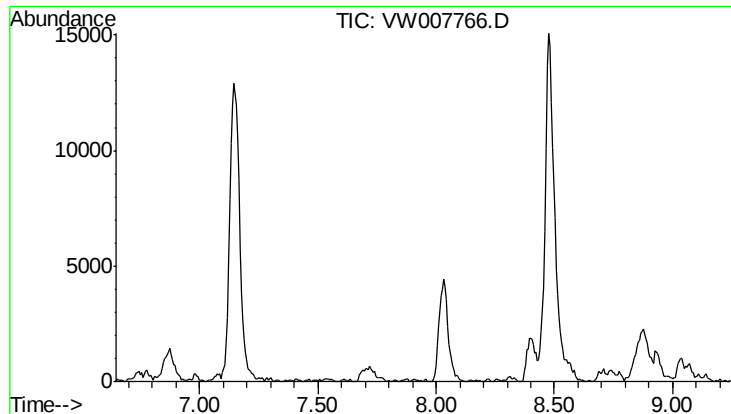

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.95 min

Lab File: VW007766.D

Acq: 20 Dec 2018 23:36

Instrument :

MSVOA_W

ClientSampleId :



KY001SB102-121118-(15-17)RE

Tot Ion: 168

Sig Exp Ratio

168 100

99 67.5

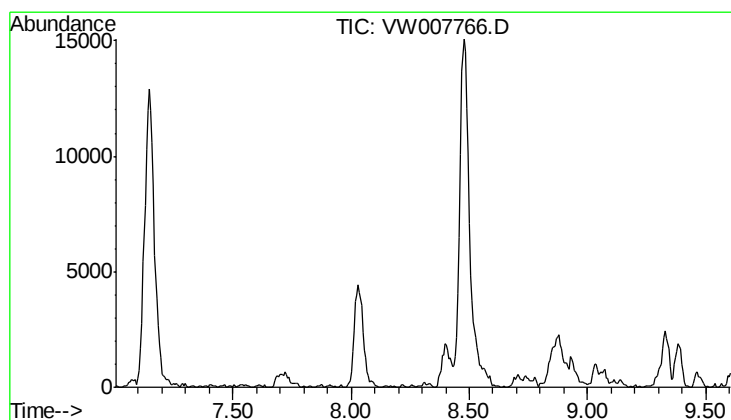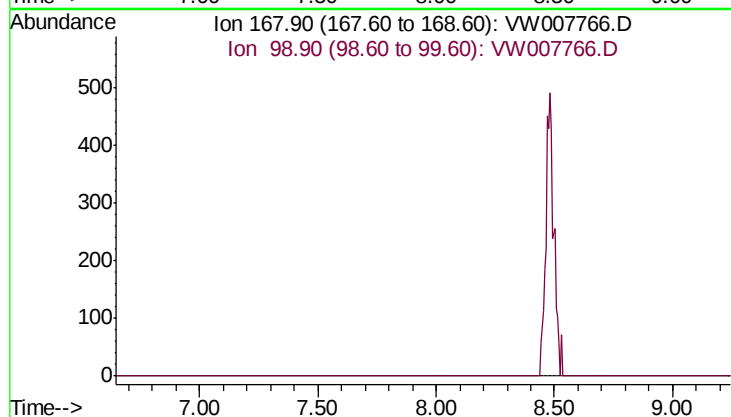

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.31 min

Lab File: VW007766.D


Acq: 20 Dec 2018 23:36


Tgt Ion: 65

Sig Exp Ratio

65 100

67 50.3

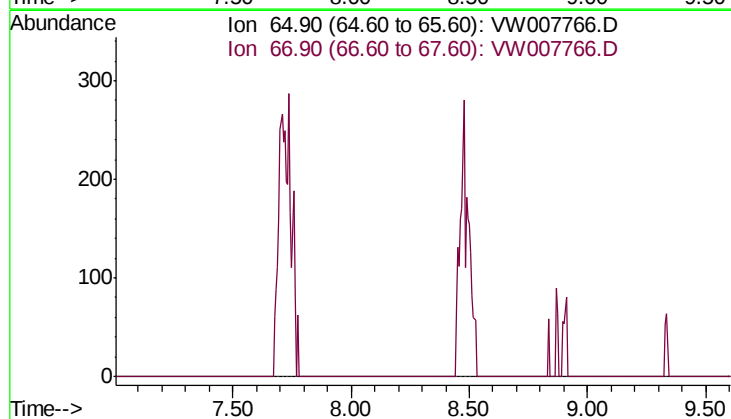

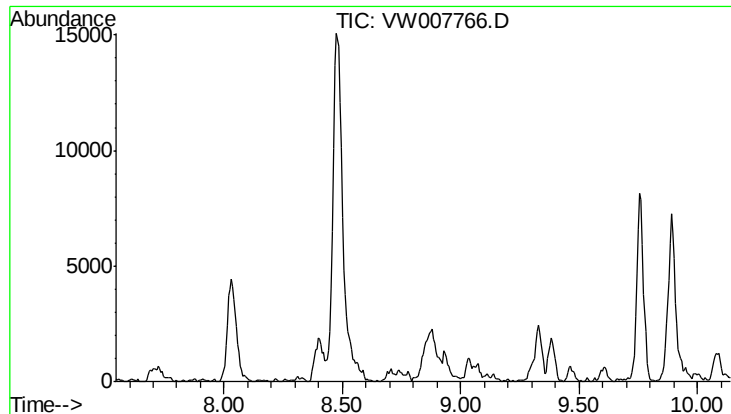

#34

1,4-Difluorobenzene

Concen: 0.000 ug/l

Expected RT: 8.84 min

Lab File: VW007766.D

Acq: 20 Dec 2018 23:36

Instrument :

MSVOA_W

ClientSampleId :

KY001SB102-121118-(15-17)RE



Tot Ion: 114

Sig Exp Ratio

114 100

63 20.0

88 16.3

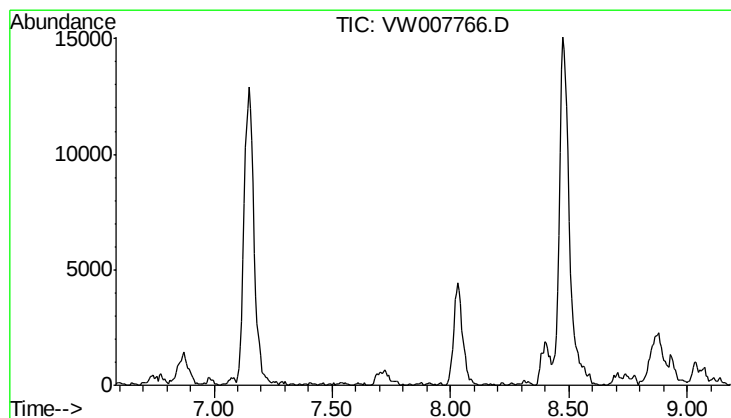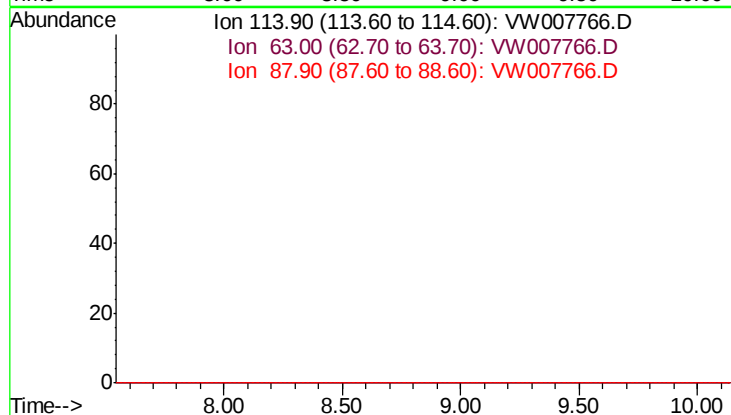

#35

Dibromofluoromethane

Concen: 0.000 ug/l

Expected RT: 7.88 min

Lab File: VW007766.D

Acq: 20 Dec 2018 23:36


Tgt Ion: 113


Sig Exp Ratio

113 100

111 103.3

192 19.4

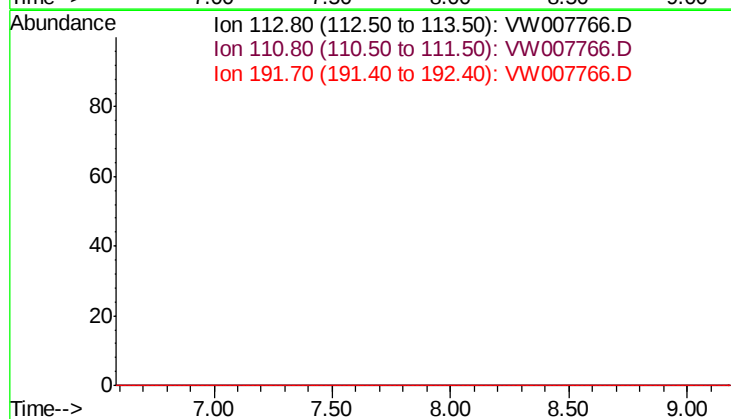


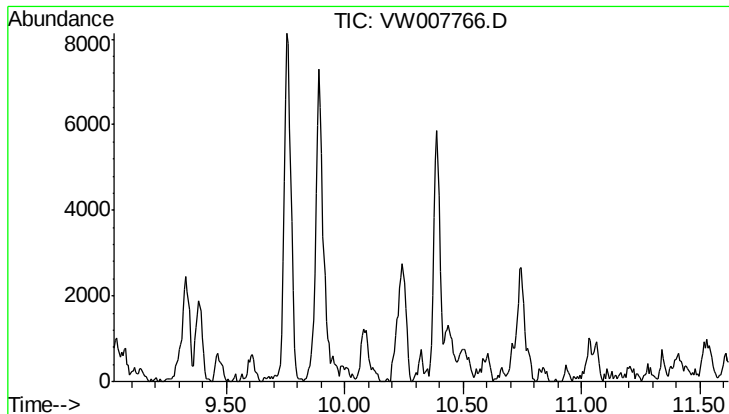


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.32 min

Lab File: VW007766.D
Acq: 20 Dec 2018 23:36




Instrument :
MSVOA_W
ClientSampleId :
KY001SB102-121118-(15-17)RE


Tot Ion: 98
Sig Exp Ratio
98 100
100 65.2

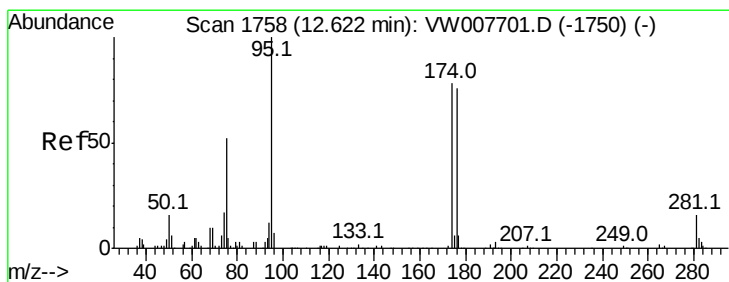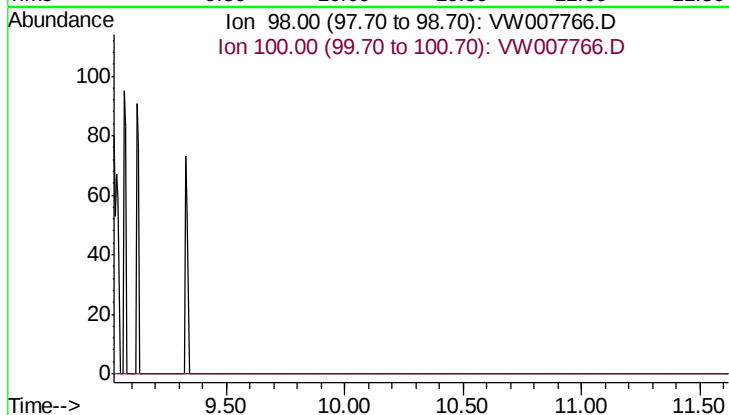

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 12.60 min Scan# 1754
Delta R.T. -0.02 min
Lab File: VW007766.D
Acq: 20 Dec 2018 23:36

Tgt Ion: 95 Resp: 19
Ion Ratio Lower Upper
95 100
174 0.0 0.0 152.2
176 0.0 0.0 146.8

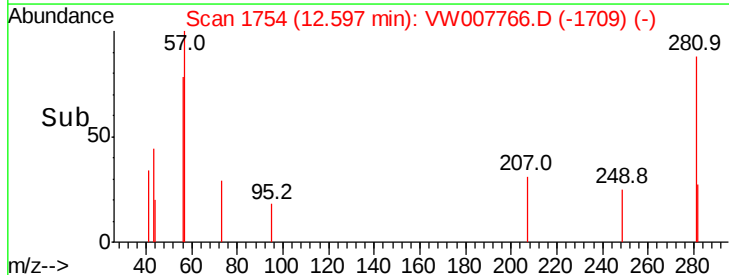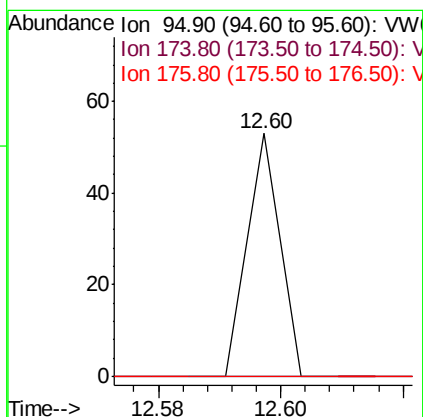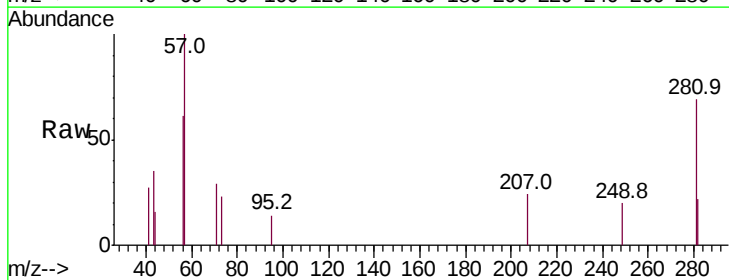


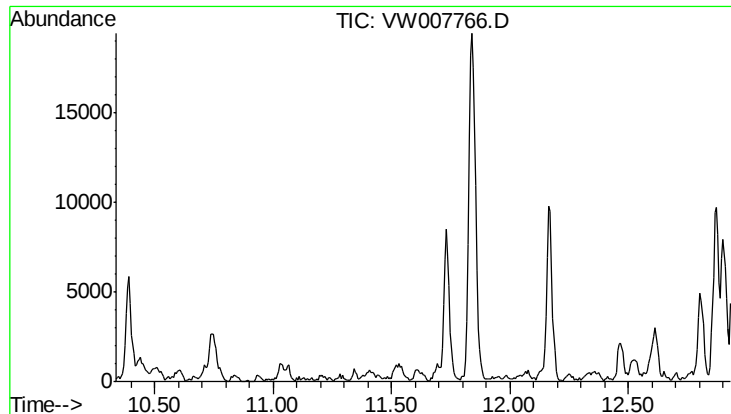


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.63 min

Lab File: VW007766.D
 Acq: 20 Dec 2018 23:36

Instrument :
 MSVOA_W
 ClientSampleId :
 KY001SB102-121118-(15-17)RE

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 55.4
 119 32.1

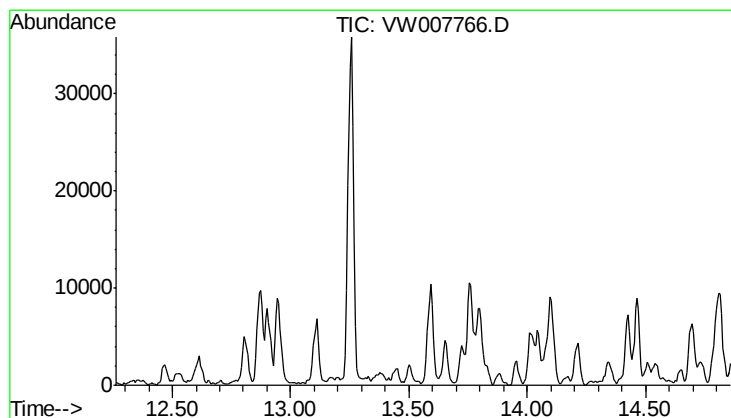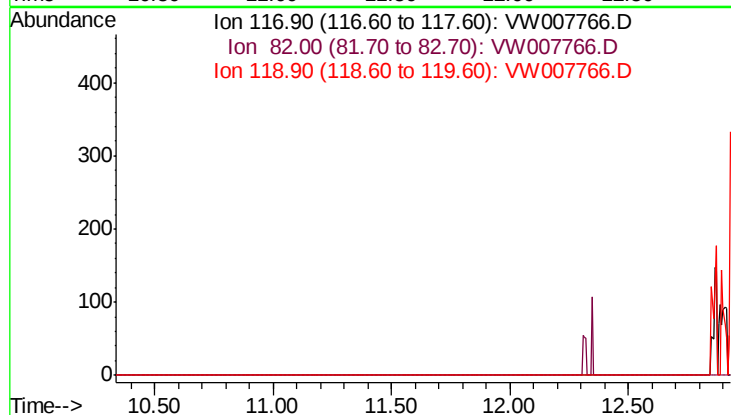

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.56 min

Lab File: VW007766.D
 Acq: 20 Dec 2018 23:36

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 63.6
 150 175.4

