

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW122218\
 Data File : VW007783.D
 Acq On : 21 Dec 2018 09:31
 Operator : SY/AP
 Sample : J6389-08
 Misc : 5.55G/5ML/MSVOA_W/SOIL
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS013-1824-01

Manual Integrations
 APPROVED

MMDadoda
 12/26/2018 4:33:44 PM

Quant Time: Dec 24 23:39:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W122118S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 20 06:30:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	28934	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	47740	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	18117	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	5761	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	24513	77.30	ug/l	0.00
Spiked Amount			Recovery	=	154.60%	
35) Dibromofluoromethane	7.88	113	17908	61.49	ug/l	0.00
Spiked Amount			Recovery	=	122.98%	
50) Toluene-d8	10.34	98	32604	29.70	ug/l	0.01
Spiked Amount			Recovery	=	59.40%	
62) 4-Bromofluorobenzene	12.62	95	4475	10.55	ug/l	0.00
Spiked Amount			Recovery	=	21.10%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	4.12	43	562763	9476.429	ug/l	94
18) Methyl Acetate	4.67	43	8395	59.441	ug/l	96
24) 1,1-Dichloroethane	6.21	63	1178	2.284	ug/l #	81
25) 2-Butanone	7.17	43	94505	1358.653	ug/l	93
27) cis-1,2-Dichloroethene	7.17	96	111162	332.330	ug/l	94
31) Cyclohexane	7.96	56	80452	170.418	ug/l	96
32) 1,1,1-Trichloroethane	7.87	97	2525	4.751	ug/l	98
39) Methylcyclohexane	9.34	83	114053	199.197	ug/l	97
40) Benzene	8.32	78	39953	32.493	ug/l	96
44) Trichloroethene	9.09	130	19438	52.275	ug/l	94
52) Toluene	10.40	92	33108637m	40133.532	ug/l	
64) Tetrachloroethene	10.87	164	40167	313.092	ug/l	97
65) Chlorobenzene	11.66	112	53656	136.833	ug/l	97
67) Ethyl Benzene	11.74	91	9241778	13734.417	ug/l	99
68) m/p-Xylenes	11.86	106	18558751	71099.623	ug/l #	1
69) o-Xylene	12.18	106	8626546	35256.861	ug/l	87
73) Isopropylbenzene	12.47	105	192514	442.086	ug/l	98
78) n-propylbenzene	12.81	91	221940	437.827	ug/l	99
80) 1,3,5-Trimethylbenzene	12.94	105	350692	933.630	ug/l	97
84) 1,2,4-Trimethylbenzene	13.26	105	977713	2579.558	ug/l	99
85) sec-Butylbenzene	13.39	105	22305m	49.106	ug/l	
86) p-Isopropyltoluene	13.50	119	131937	319.438	ug/l	99
87) 1,3-Dichlorobenzene	13.50	146	1610	8.125	ug/l #	73
88) 1,4-Dichlorobenzene	13.58	146	15867	80.053	ug/l #	77
89) n-Butylbenzene	13.83	91	19544	51.609	ug/l #	69
91) 1,2-Dichlorobenzene	13.87	146	14149	79.753	ug/l #	54
93) 1,2,4-Trichlorobenzene	15.14	180	129539	1051.892	ug/l #	90
95) Naphthalene	15.37	128	600105	2635.727	ug/l	98
96) 1,2,3-Trichlorobenzene	15.57	180	39097	370.885	ug/l #	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW122218\
Data File : VW007783.D
Acq On : 21 Dec 2018 09:31
Operator : SY/AP
Sample : J6389-08
Misc : 5.55G/5ML/MSVOA_W/SOIL
ALS Vial : 45 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
P001-SS013-1824-01

Manual Integrations
APPROVED

MMDadoda
12/26/2018 4:33:44 PM

Quant Time: Dec 24 23:39:27 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W122118S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 20 06:30:23 2018
Response via : Initial Calibration

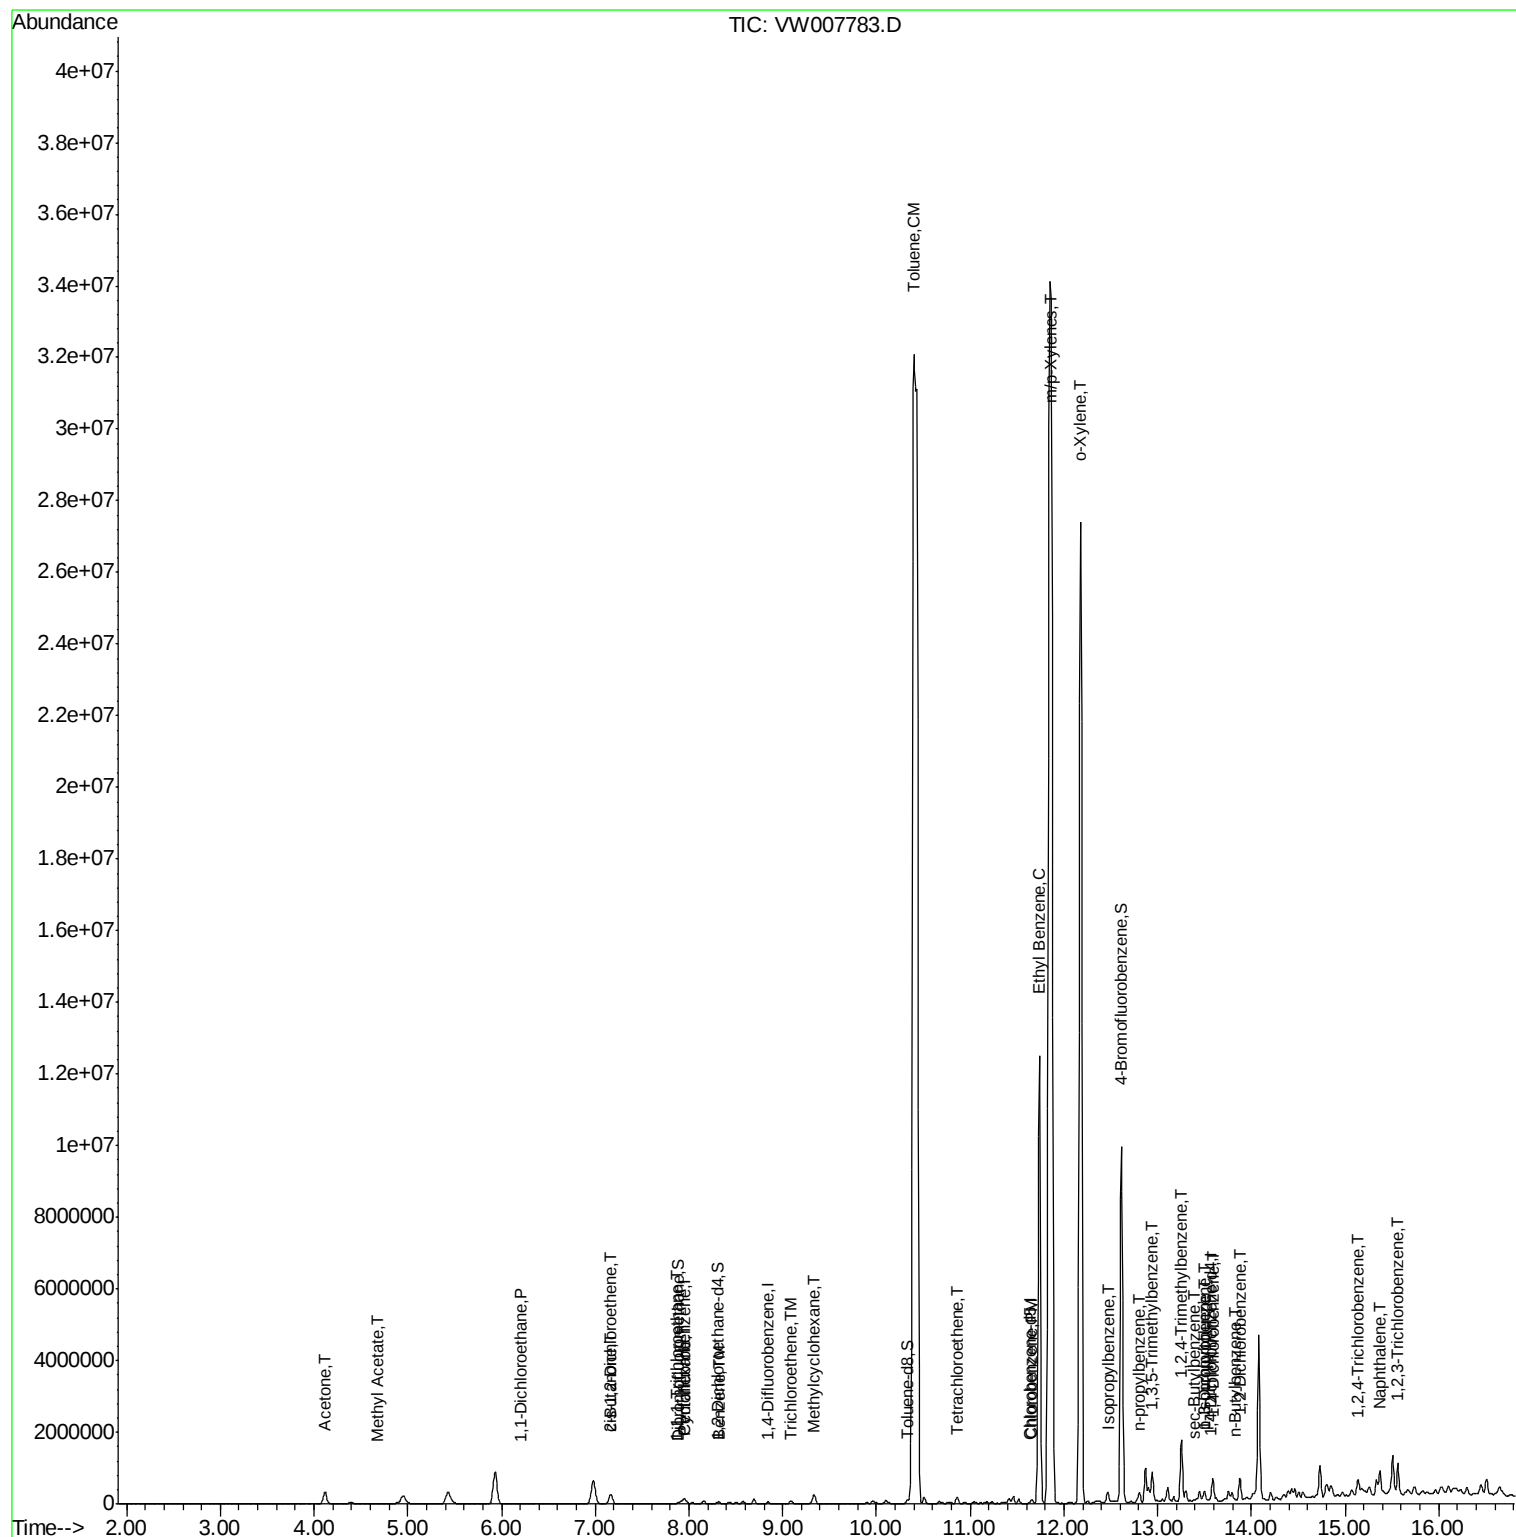



#1





Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 7.95 min Scan# 992
 Delta R.T. 0.01 min
 Lab File: VW007783.D
 Acq: 21 Dec 2018 09:31

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS013-1824-01

Tgt Ion	Ratio	Lower	Upper
168	100		
99	58.8	54.0	81.0

Manual Integrations
 APPROVED




MMDadoda
 12/26/2018 4:33:44 PM

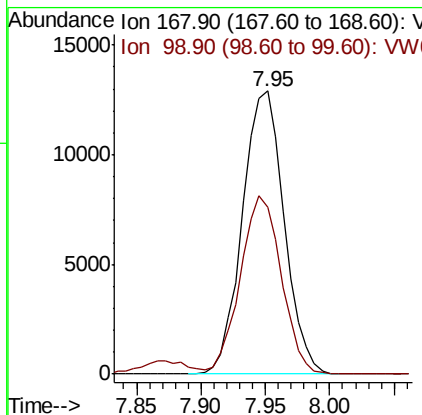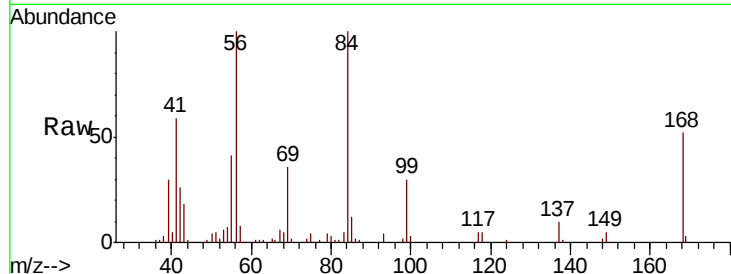


#16

Acetone
 Concen: 9476.429 ug/l
 RT: 4.12 min Scan# 363
 Delta R.T. -0.00 min
 Lab File: VW007783.D
 Acq: 21 Dec 2018 09:31

Tgt Ion	Ratio	Lower	Upper
43	100		
58	29.7	21.2	31.8

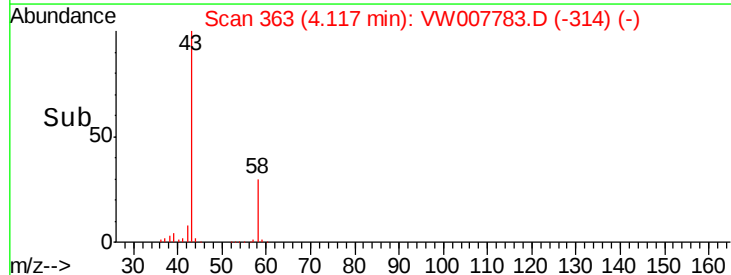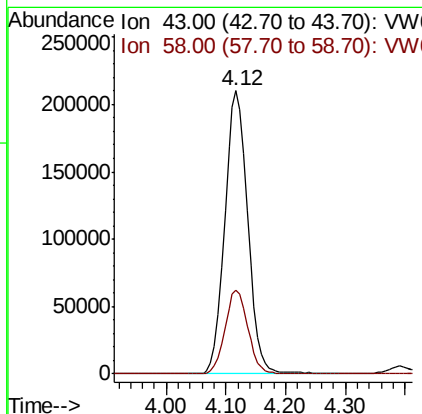



#18

Methyl Acetate

Concen: 59.441 ug/l

RT: 4.67 min Scan# 454

Delta R.T. 0.01 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

P001-SS013-1824-01

Tgt Ion: 43 Resp: 8395

Ion Ratio Lower Upper

43 100





74 26.1 22.7 34.1

Manual Integrations

APPROVED

MMDadoda

12/26/2018 4:33:44 PM

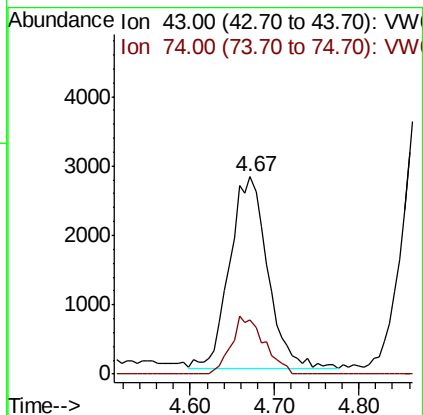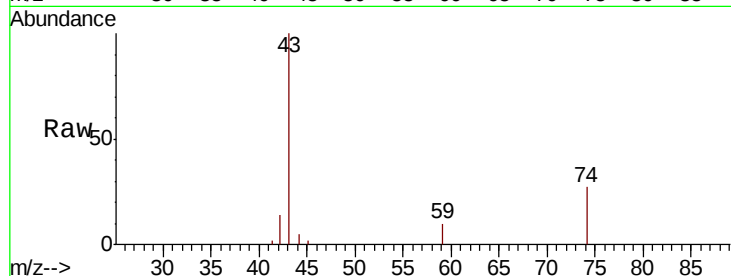

#24

1,1-Dichloroethane

Concen: 2.284 ug/l

RT: 6.21 min Scan# 707

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31




Tgt Ion: 63 Resp: 1178


Ion Ratio Lower Upper

63 100

98 0.0 3.6 10.9#

100 0.0 2.5 7.5#

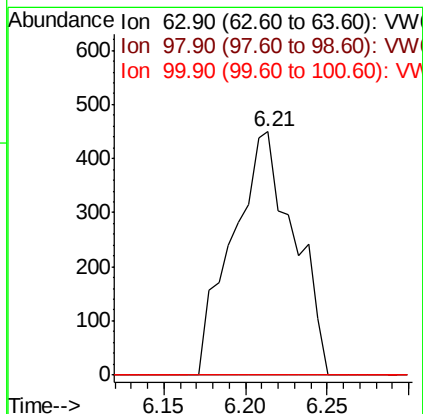



#25

2-Butanone

Concen: 1358.653 ug/l

RT: 7.17 min Scan# 864

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

P001-SS013-1824-01

Tgt Ion: 43 Resp: 94505

Ion Ratio Lower Upper

43 100





72 26.5 24.5 36.7

Manual Integrations

APPROVED

MMDadoda

12/26/2018 4:33:44 PM

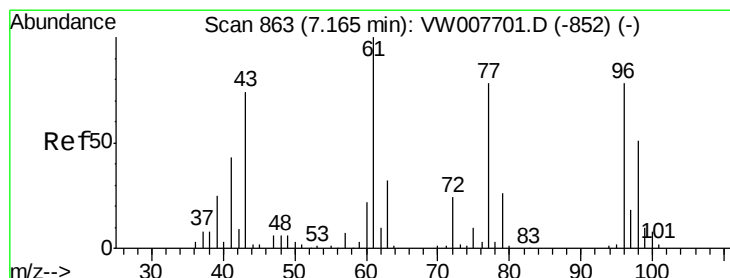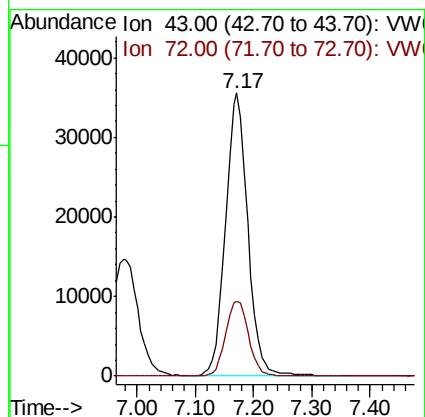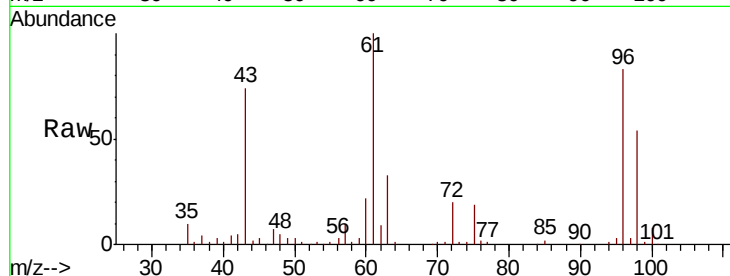

#27

cis-1,2-Dichloroethene

Concen: 332.330 ug/l

RT: 7.17 min Scan# 863

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31




Tgt Ion: 96 Resp: 111162


Ion Ratio Lower Upper

96 100

61 124.8 0.0 271.6

98 65.6 0.0 131.2

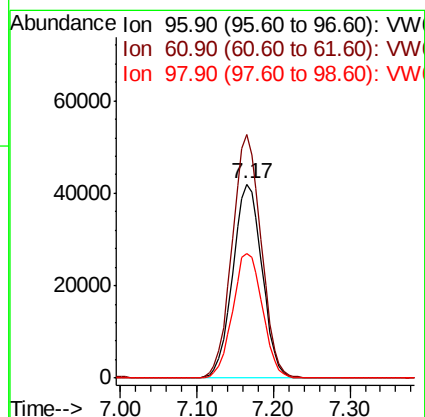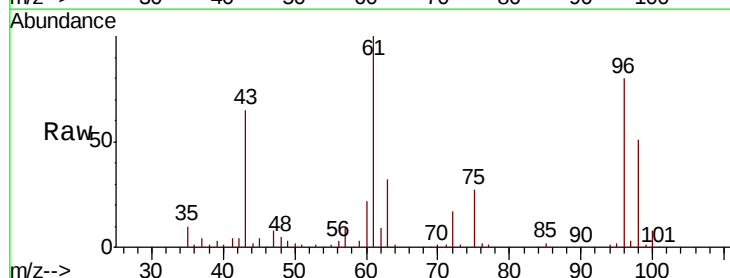







#31
Cyclohexane
Concen: 170.418 ug/l
RT: 7.96 min Scan# 993
Delta R.T. 0.01 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Instrument :
MSVOA_W
ClientSampleId :
P001-SS013-1824-01

Tgt Ion	Ratio	Lower	Upper
56	100		
69	36.3	29.7	44.5
84	93.8	78.9	118.3




Manual Integrations
APPROVED


MMDadoda
12/26/2018 4:33:44 PM

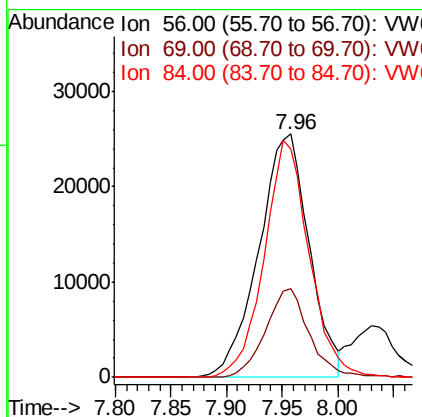

#32
1,1,1-Trichloroethane
Concen: 4.751 ug/l
RT: 7.87 min Scan# 979
Delta R.T. -0.00 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Tgt Ion	Ratio	Lower	Upper
97	100		
99	64.2	50.6	76.0
61	41.8	32.3	48.5

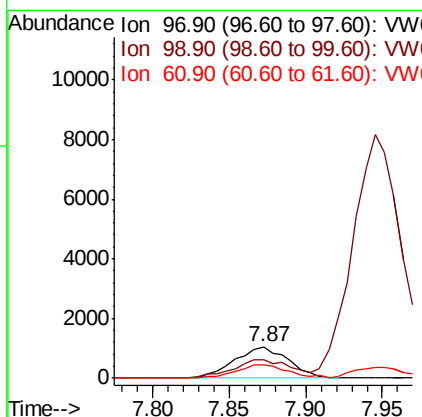



#33

1,2-Dichloroethane-d4

Concen: 77.297 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

P001-SS013-1824-01

Tgt Ion: 65 Resp: 24513

Ion Ratio Lower Upper

65 100


67 49.2 0.0 100.6

Manual Integrations

APPROVED




MMDadoda

12/26/2018 4:33:44 PM



Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

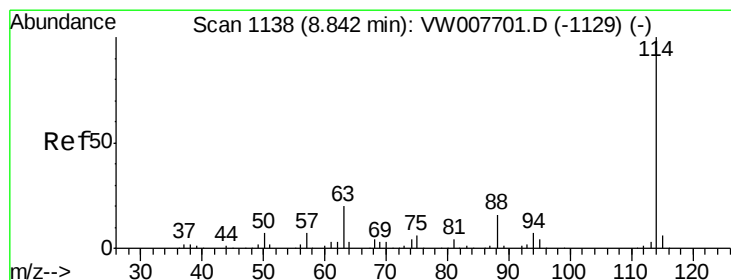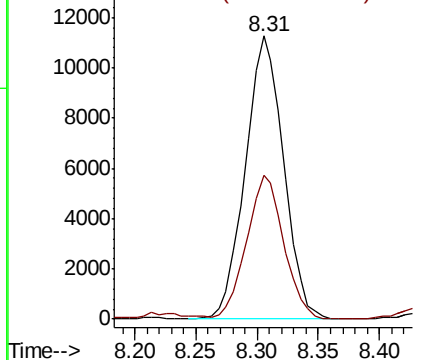

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31


Tgt Ion: 114 Resp: 47740

Ion Ratio Lower Upper

114 100

63 19.9 0.0 40.0



88 16.9 0.0 32.6




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

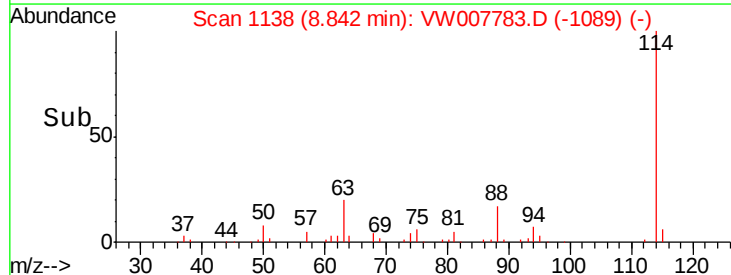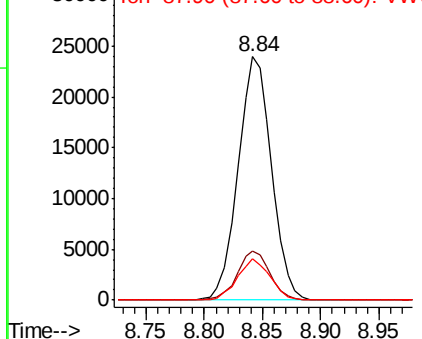



#35

Dibromofluoromethane

Concen: 61.489 ug/l

RT: 7.88 min Scan# 981

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W





ClientSampleId :

P001-SS013-1824-01

Tgt Ion:	113	Resp:	17908
Ion Ratio	Lower	Upper	
113	100		
111	103.5	82.6	124.0
192	19.1	15.5	23.3

Manual Integrations
APPROVED

MMDadoda
12/26/2018 4:33:44 PM

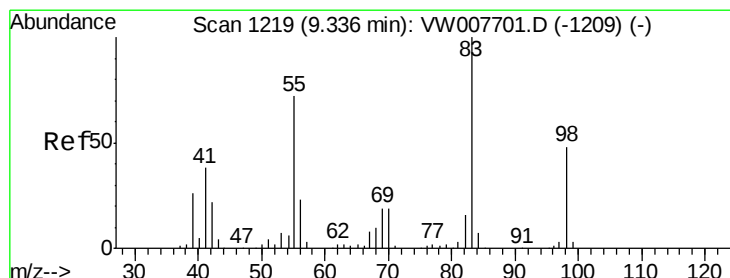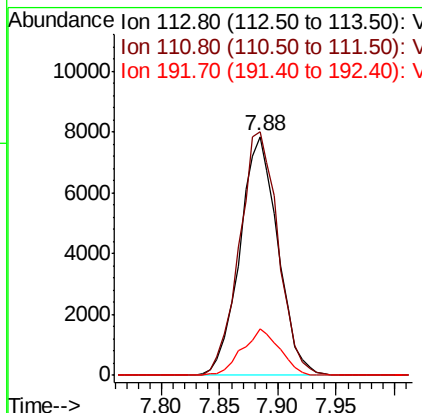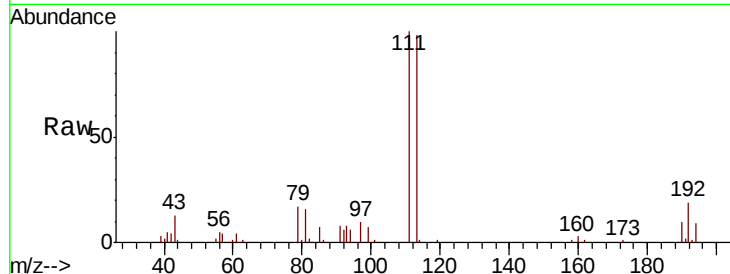

#39

Methylcyclohexane

Concen: 199.197 ug/l




RT: 9.34 min Scan# 1219


Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Tgt Ion:	83	Resp:	114053
Ion Ratio	Lower	Upper	
83	100		
55	75.3	57.2	85.8
98	47.9	38.6	58.0

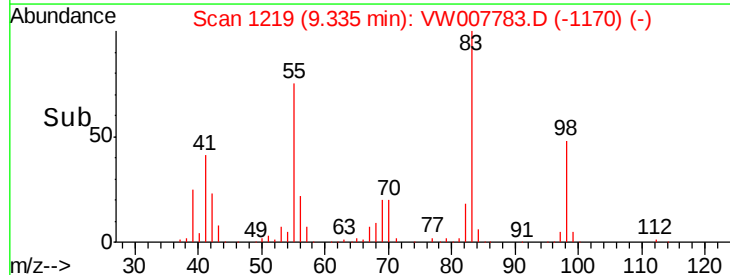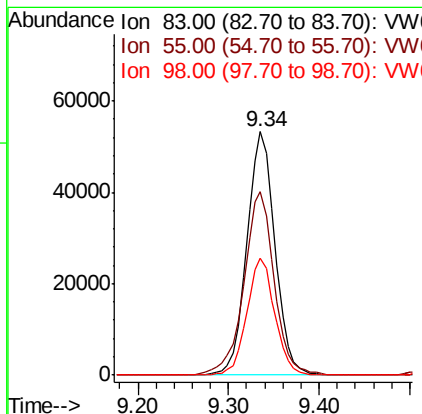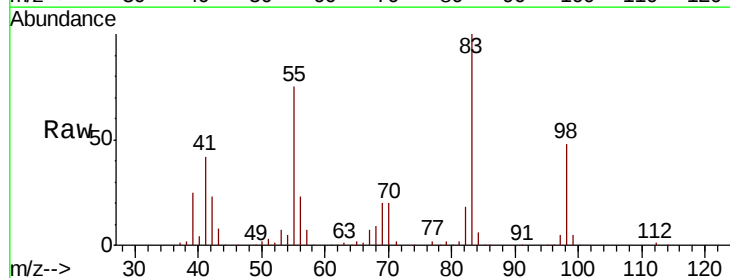



#40

Benzene

Concen: 32.493 ug/l

RT: 8.32 min Scan# 1053

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

P001-SS013-1824-01

Tgt Ion: 78 Resp: 39953

Ion Ratio Lower Upper

78 100





77 25.4 18.7 28.1

Manual Integrations

APPROVED

MMDadoda

12/26/2018 4:33:44 PM

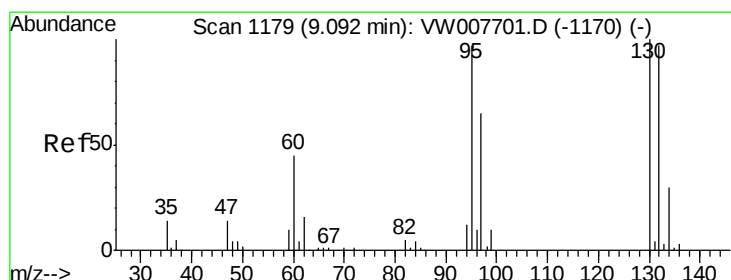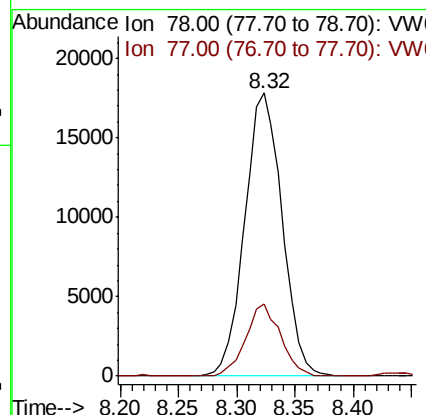

#44

Trichloroethene

Concen: 52.275 ug/l

RT: 9.09 min Scan# 1179

Delta R.T. -0.00 min

Lab File: VW007783.D




Acq: 21 Dec 2018 09:31


Tgt Ion:130 Resp: 19438

Ion Ratio Lower Upper

130 100

95 103.5 0.0 194.8

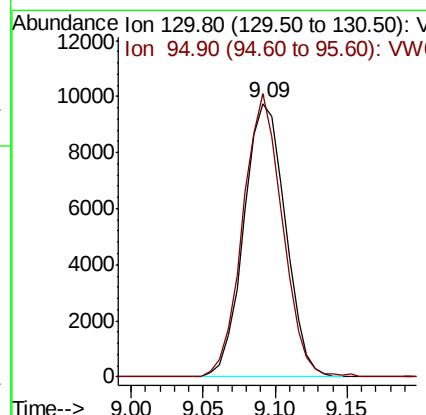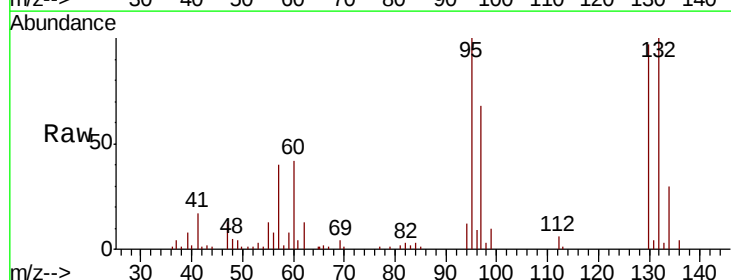



#50

Toluene-d8

Concen: 29.696 ug/l

RT: 10.34 min Scan# 1383

Delta R.T. 0.01 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

P001-SS013-1824-01

Tgt Ion: 98 Resp: 32604





Ion Ratio Lower Upper

98 100

100 53.4 52.2 78.2

Manual Integrations
APPROVED

MMDadoda
12/26/2018 4:33:44 PM

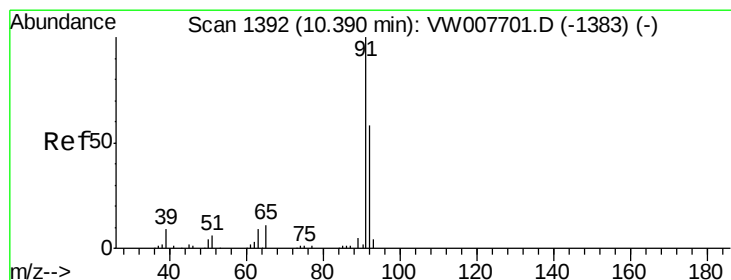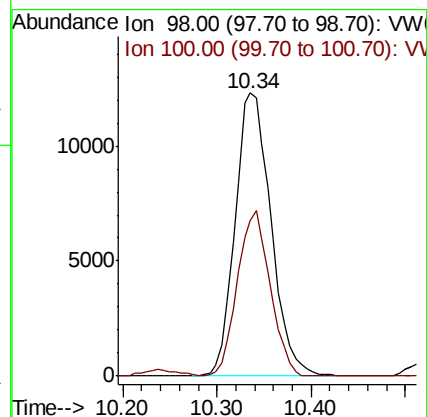

#52

Toluene

Concen: 40133.532 ug/l m

RT: 10.40 min Scan# 1394

Delta R.T. 0.01 min

Lab File: VW007783.D




Acq: 21 Dec 2018 09:31


Tgt Ion: 92 Resp: 33108637

Ion Ratio Lower Upper

92 100

91 0.0 137.0 205.4#

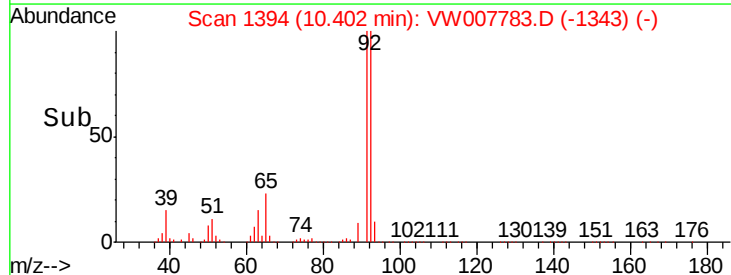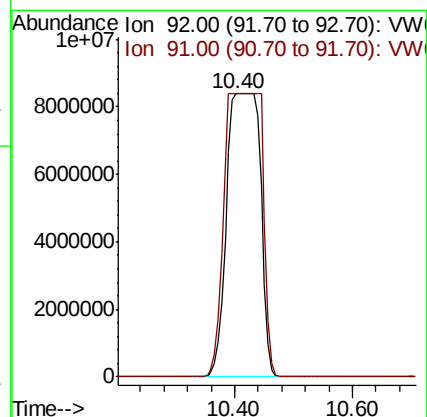

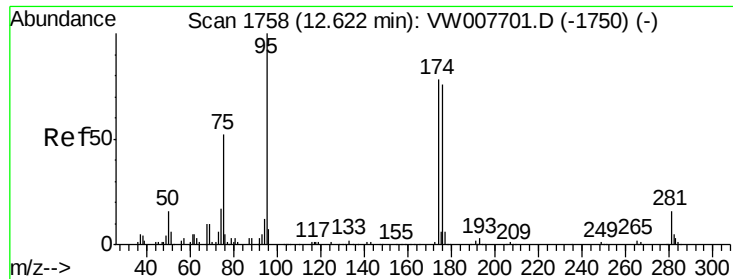

#62

4-Bromofluorobenzene

Concen: 10.550 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W





ClientSampleId :

P001-SS013-1824-01

Tgt Ion:	95	Resp:	4475
Ion Ratio	Lower	Upper	
95	100		
174	113.1	0.0	152.2
176	989.0	0.0	146.8#

Manual Integrations
APPROVED

MMDadoda
12/26/2018 4:33:44 PM

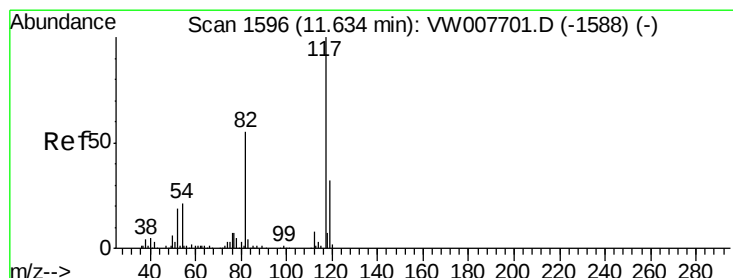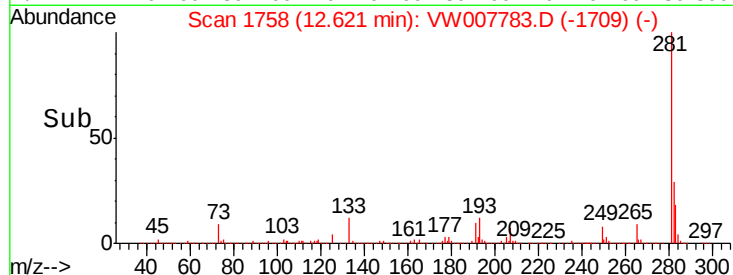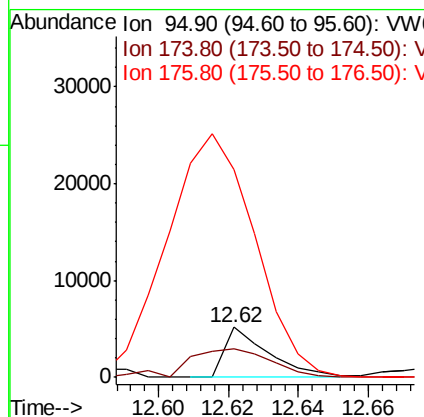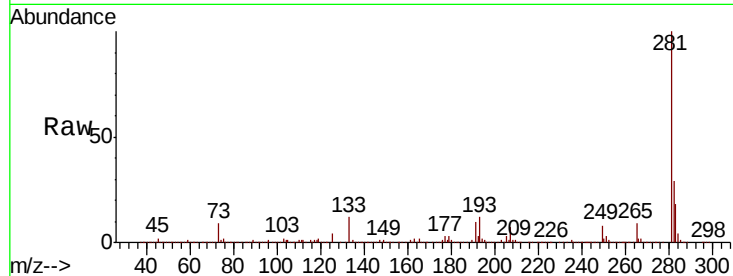

#63

Chlorobenzene-d5

Concen: 50.000 ug/l




RT: 11.63 min Scan# 1596


Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Tgt Ion:	117	Resp:	18117
Ion Ratio	Lower	Upper	
117	100		
82	51.9	44.3	66.5
119	34.1	25.7	38.5

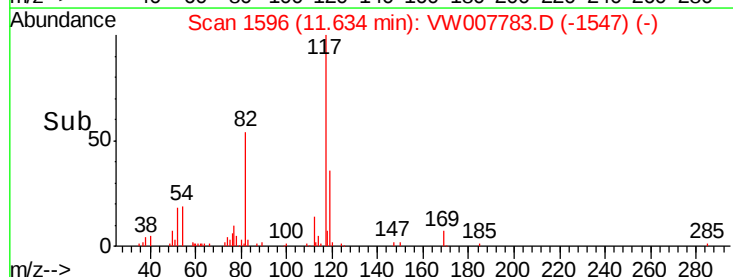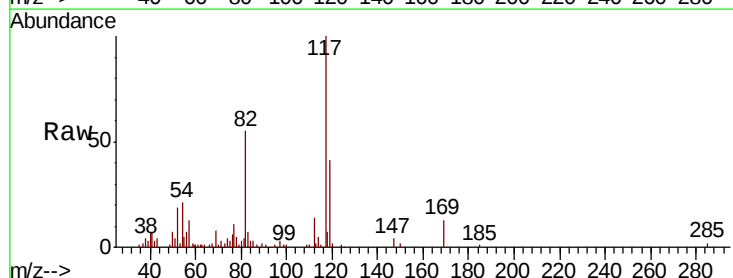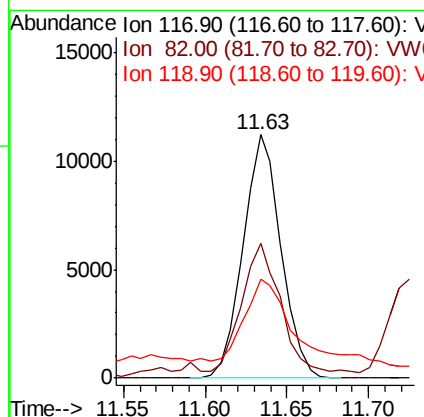







#64
Tetrachloroethene
Concen: 313.092 ug/l
RT: 10.87 min Scan# 1470
Delta R.T. 0.01 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Instrument :
MSVOA_W
ClientSampleId :
P001-SS013-1824-01

Tgt Ion	Ratio	Lower	Upper
164	100		
166	130.3	101.0	151.6
129	100.2	78.7	118.1
131	96.6	79.4	119.0




Manual Integrations
APPROVED


MMDadoda
12/26/2018 4:33:44 PM

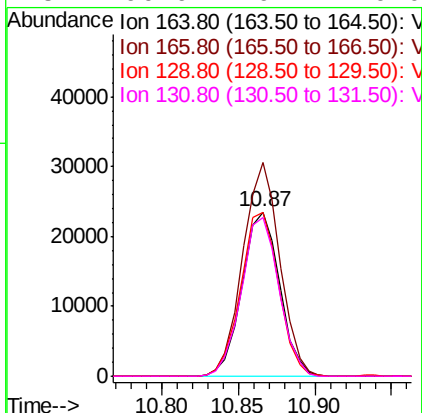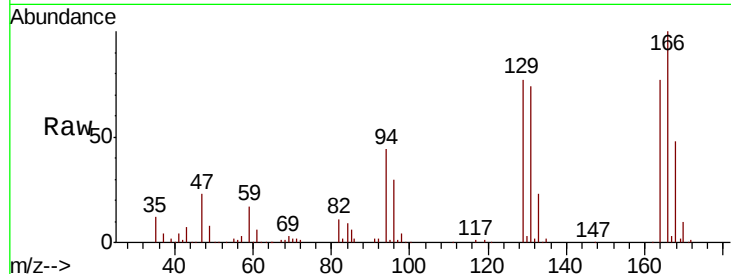

#65
Chlorobenzene
Concen: 136.833 ug/l
RT: 11.66 min Scan# 1601
Delta R.T. 0.01 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Tgt Ion	Ratio	Lower	Upper
112	100		
114	33.3	25.2	37.8

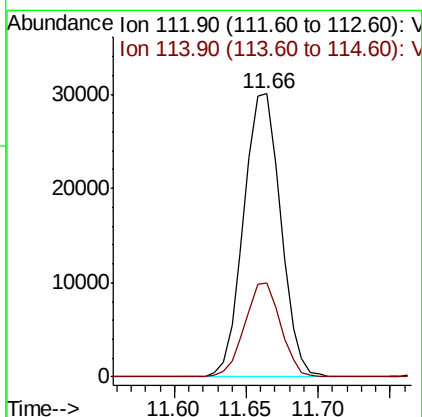







#67
Ethyl Benzene
Concen: 13734.417 ug/l
RT: 11.74 min Scan# 1613
Delta R.T. 0.01 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Instrument :
MSVOA_W
ClientSampleId :
P001-SS013-1824-01

Tgt Ion: 91 Resp: 9241778
Ion Ratio Lower Upper
91 100
106 31.5 25.8 38.8




Manual Integrations
APPROVED


MMDadoda
12/26/2018 4:33:44 PM

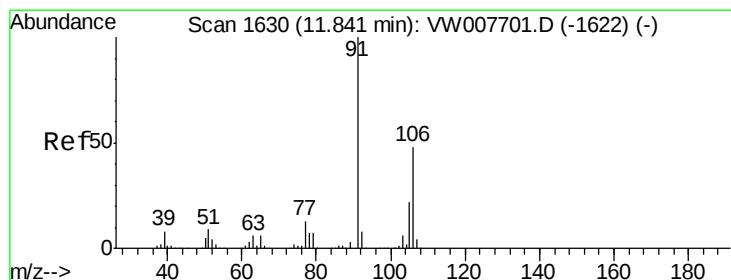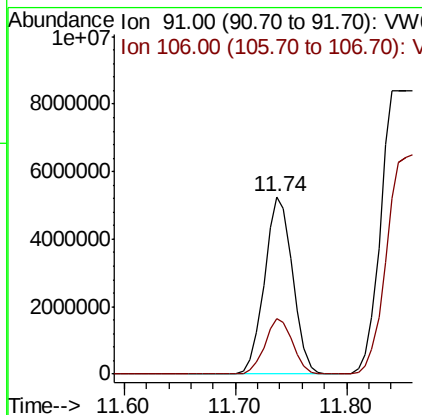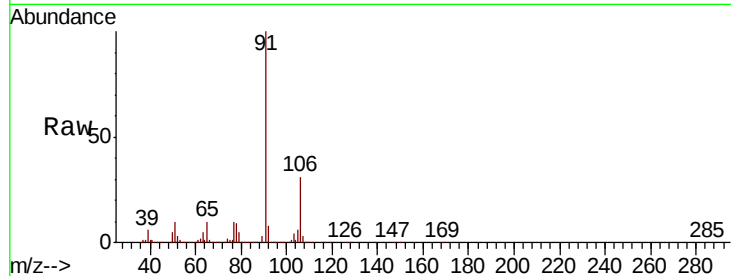

#68
m/p-Xylenes
Concen: 71099.623 ug/l
RT: 11.86 min Scan# 1633
Delta R.T. 0.02 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Tgt Ion: 106 Resp: 18558751
Ion Ratio Lower Upper
106 100
91 0.0 165.2 247.8#

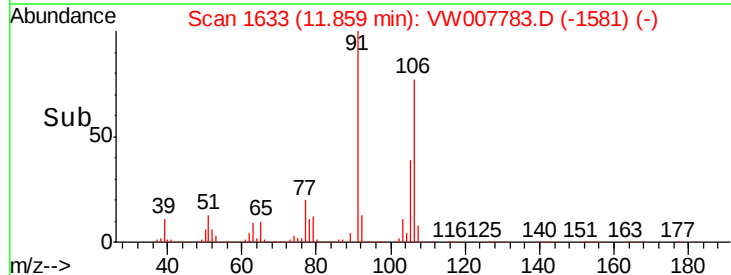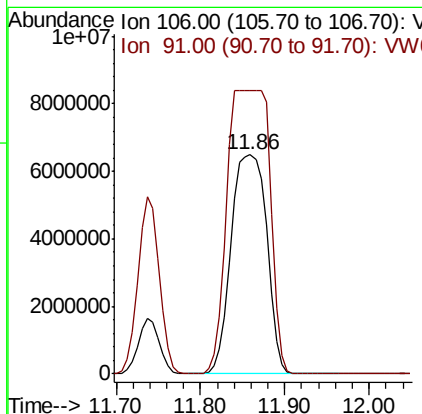







#69
o-Xylene
Concen: 35256.861 ug/l
RT: 12.18 min Scan# 1685
Delta R.T. 0.01 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Instrument :
MSVOA_W
ClientSampleId :
P001-SS013-1824-01

Tgt Ion:106 Resp: 8626546
Ion Ratio Lower Upper
106 100
91 200.4 110.5 331.4




Manual Integrations
APPROVED


MMDadoda
12/26/2018 4:33:44 PM

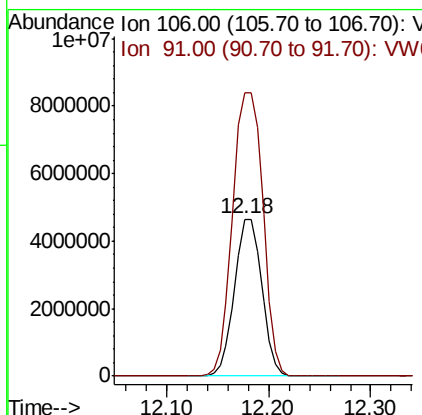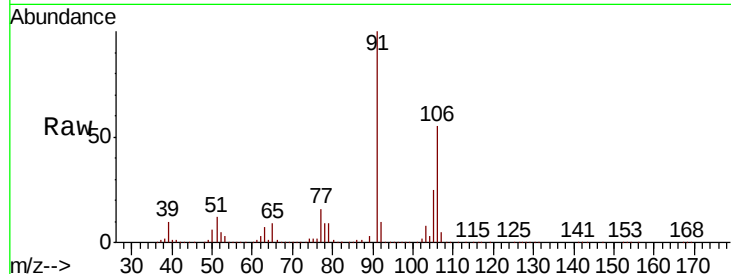

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Tgt Ion:152 Resp: 5761
Ion Ratio Lower Upper
152 100
115 0.0 31.8 95.4#
150 144.0 0.0 350.8

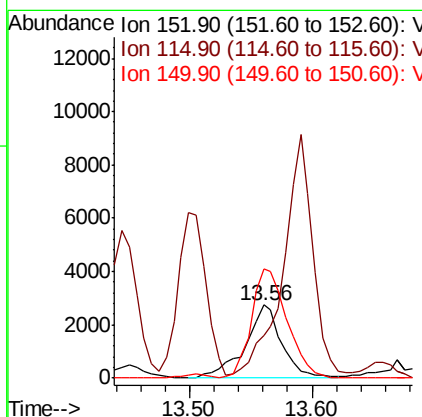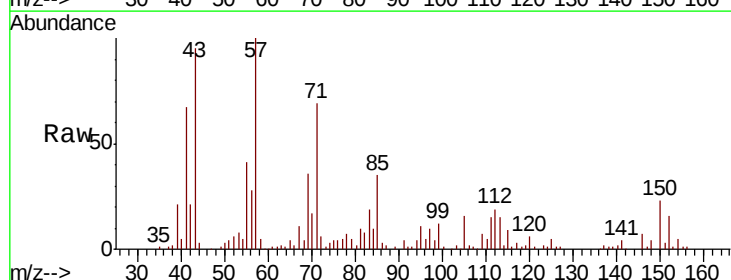

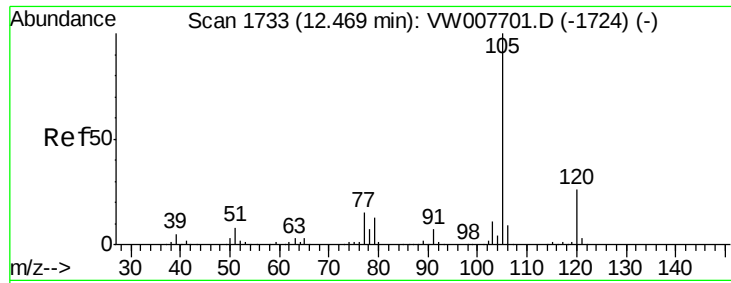

#73

Isopropylbenzene

Concen: 442.086 ug/l

RT: 12.47 min Scan# 1733

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

P001-SS013-1824-01

Tgt Ion: 105 Resp: 192514

Ion Ratio Lower Upper

105 100





120 25.3 13.1 39.3

Manual Integrations

APPROVED

MMDadoda

12/26/2018 4:33:44 PM

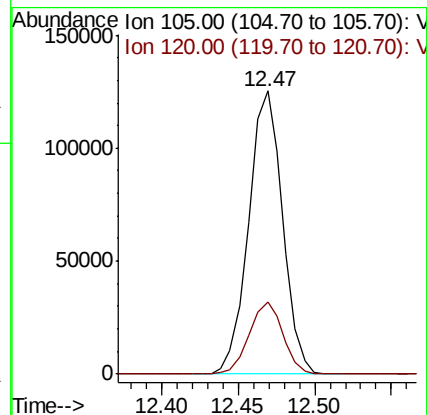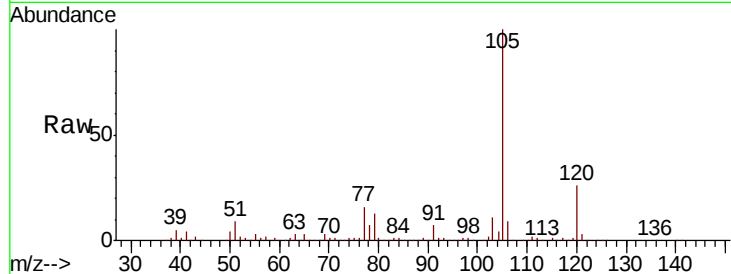

#78

n-propylbenzene

Concen: 437.827 ug/l

RT: 12.81 min Scan# 1789

Delta R.T. -0.00 min

Lab File: VW007783.D




Acq: 21 Dec 2018 09:31


Tgt Ion: 91 Resp: 221940

Ion Ratio Lower Upper

91 100

120 23.5 11.9 35.7

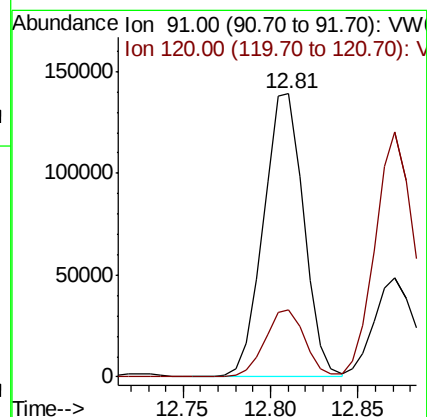







#80
 1,3,5-Trimethylbenzene
 Concen: 933.630 ug/l
 RT: 12.94 min Scan# 1811
 Delta R.T. -0.00 min
 Lab File: VW007783.D
 Acq: 21 Dec 2018 09:31

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS013-1824-01

Tgt Ion:105 Resp: 350692
 Ion Ratio Lower Upper
 105 100
 120 48.9 23.6 70.8




Manual Integrations
 APPROVED


MMDadoda
 12/26/2018 4:33:44 PM

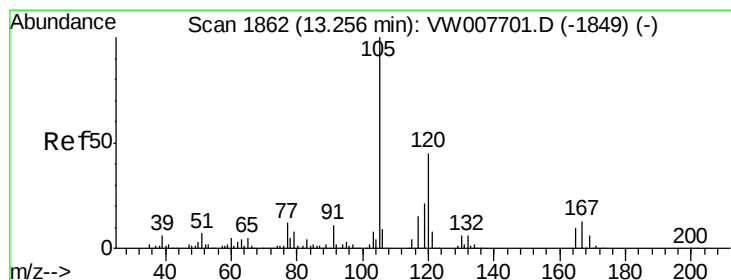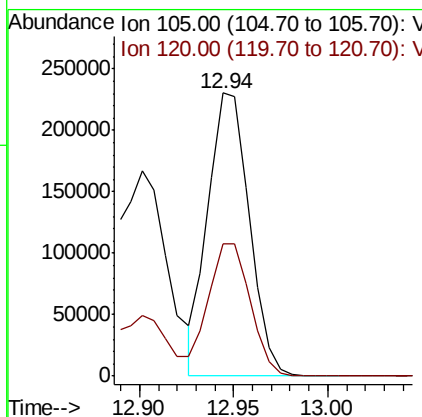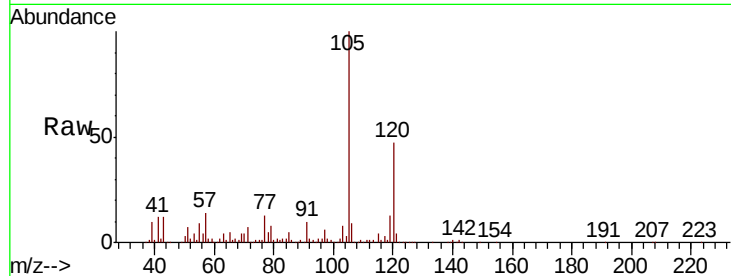

#84
 1,2,4-Trimethylbenzene
 Concen: 2579.558 ug/l
 RT: 13.26 min Scan# 1862
 Delta R.T. -0.00 min
 Lab File: VW007783.D
 Acq: 21 Dec 2018 09:31

Tgt Ion:105 Resp: 977713
 Ion Ratio Lower Upper
 105 100
 120 43.6 22.0 66.0

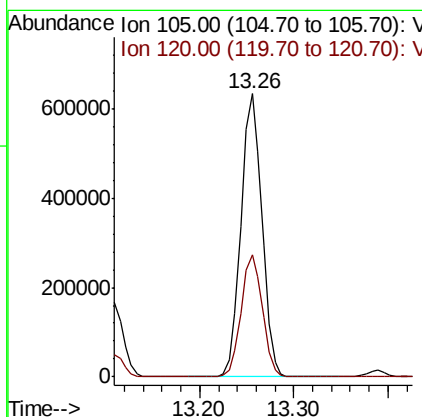

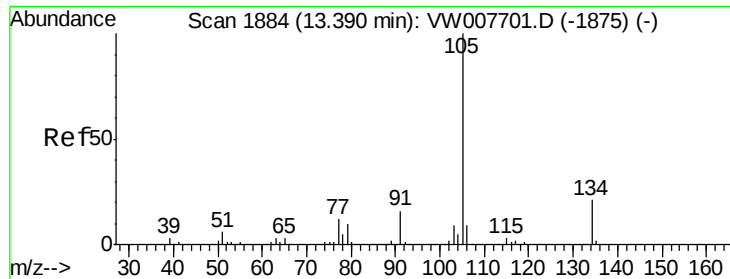

#85

sec-Butylbenzene

Concen: 49.106 ug/l m

RT: 13.39 min Scan# 1884

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

P001-SS013-1824-01

Tgt Ion:105 Resp: 22305





Ion Ratio Lower Upper

105 100

134 0.0 10.2 30.4#

Manual Integrations
APPROVED

MMDadoda
12/26/2018 4:33:44 PM

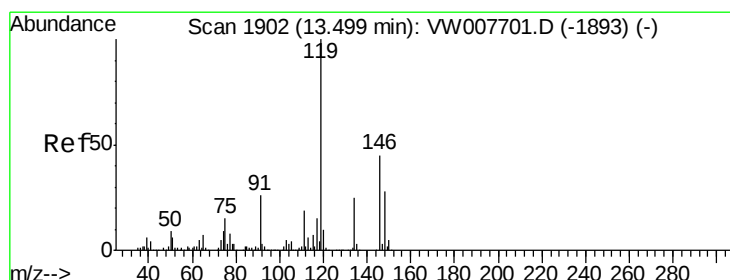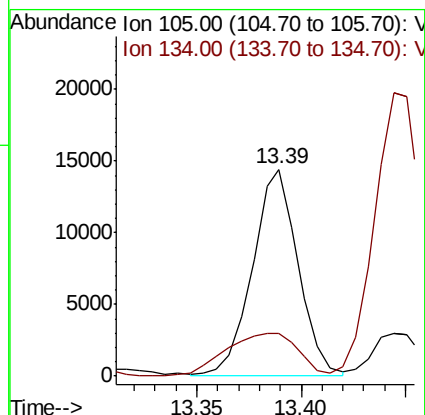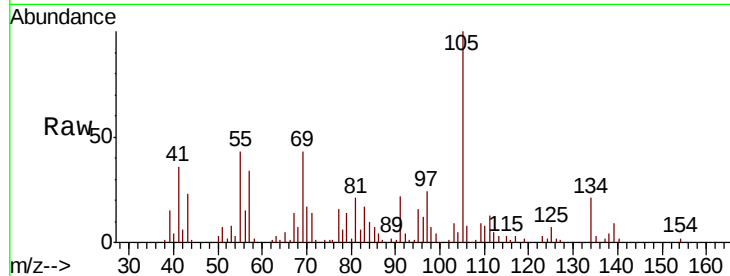

#86

p-Isopropyltoluene

Concen: 319.438 ug/l

RT: 13.50 min Scan# 1902

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31




Tgt Ion:119 Resp: 131937


Ion Ratio Lower Upper

119 100

134 25.5 13.0 39.0

91 25.4 12.8 38.4

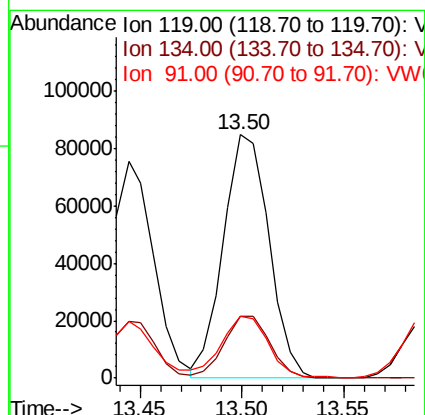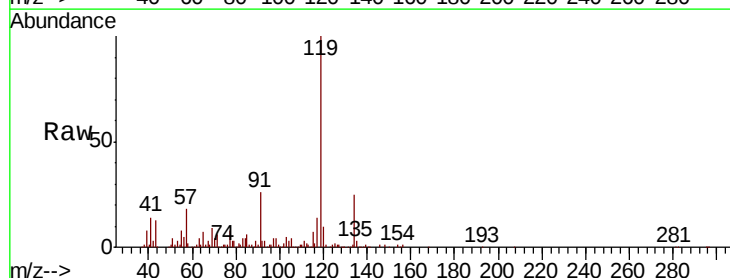



#87

1,3-Dichlorobenzene

Concen: 8.125 ug/l

RT: 13.50 min Scan# 1902

Delta R.T. -0.00 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Instrument :

MSVOA_W





ClientSampleId :

P001-SS013-1824-01

Tgt Ion:	146	Resp:	1610
Ion Ratio	Lower	Upper	
146	100		
111	0.0	21.1	63.4#
148	63.7	32.1	96.5

Manual Integrations
APPROVED

MMDadoda
12/26/2018 4:33:44 PM

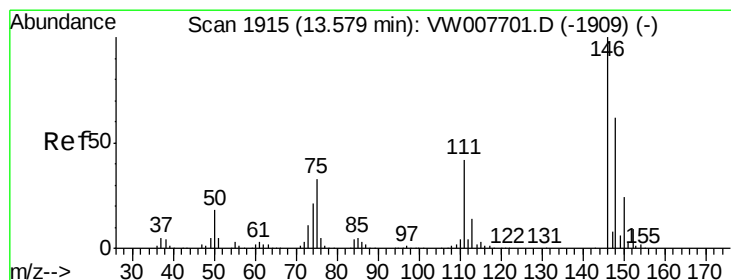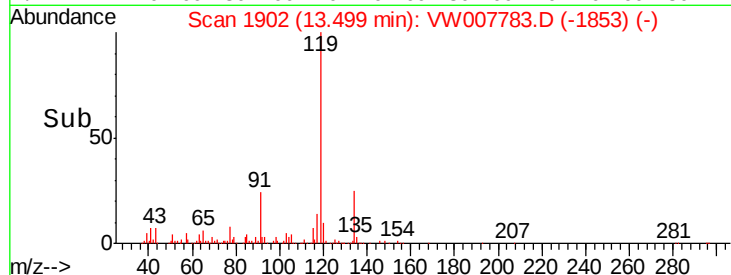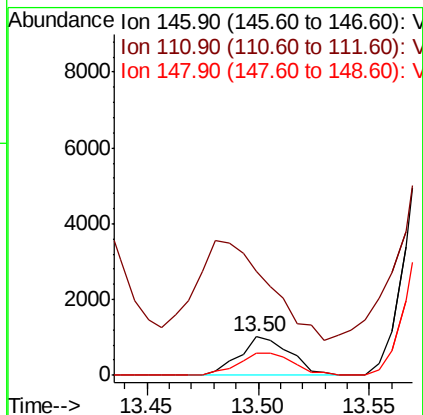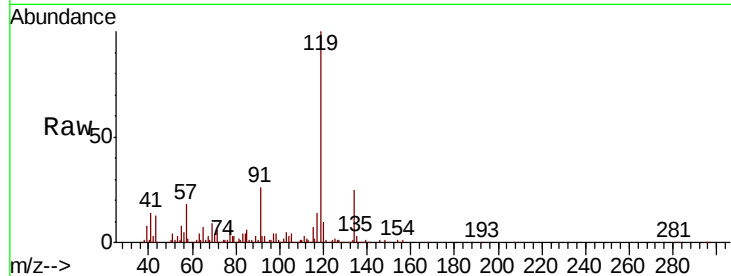

#88

1,4-Dichlorobenzene

Concen: 80.053 ug/l




RT: 13.58 min Scan# 1916


Delta R.T. 0.01 min

Lab File: VW007783.D

Acq: 21 Dec 2018 09:31

Tgt Ion:	146	Resp:	15867
Ion Ratio	Lower	Upper	
146	100		
111	77.3	21.0	63.0#
148	64.0	31.8	95.4

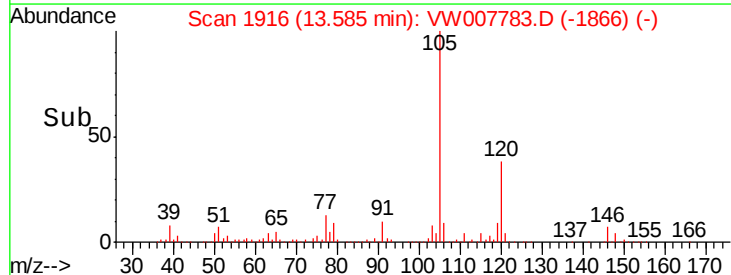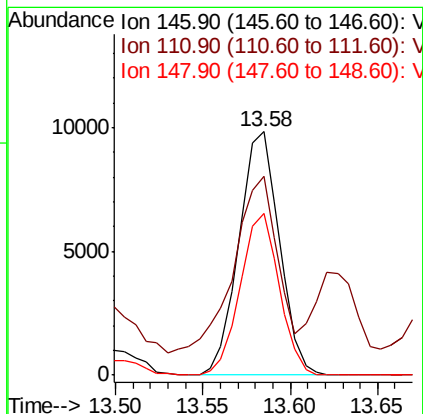







#89
n-Butylbenzene
Concen: 51.609 ug/l
RT: 13.83 min Scan# 1956
Delta R.T. -0.00 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Instrument :
MSVOA_W
ClientSampleId :
P001-SS013-1824-01

Tgt Ion	Ratio	Lower	Upper
91	100		
92	67.4	26.4	79.2
134	0.0	13.7	41.0#




Manual Integrations
APPROVED


MMDadoda
12/26/2018 4:33:44 PM

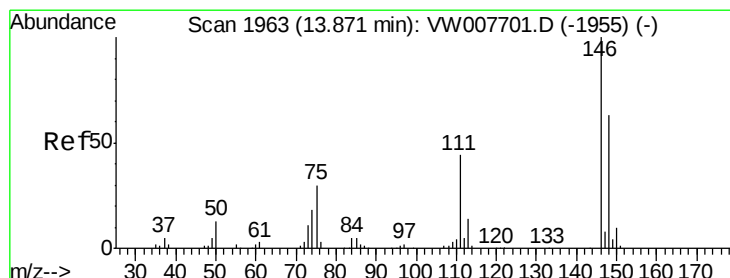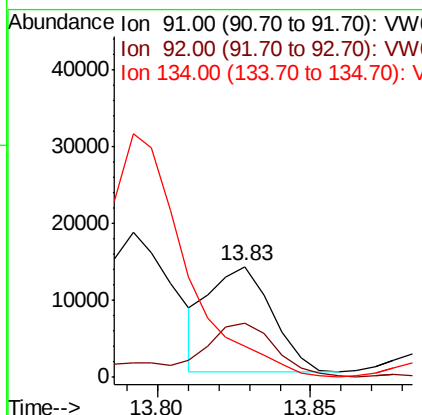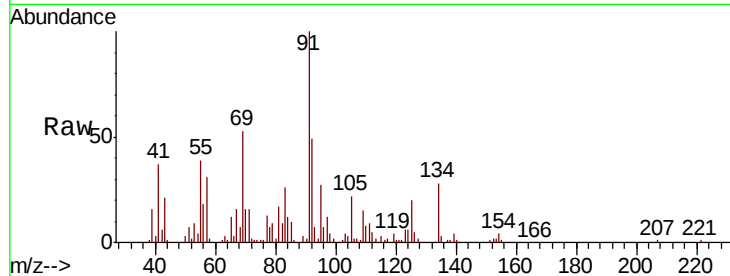

#91
1,2-Dichlorobenzene
Concen: 79.753 ug/l
RT: 13.87 min Scan# 1963
Delta R.T. -0.00 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Tgt Ion	Ratio	Lower	Upper
146	100		
111	114.3	21.7	65.1#
148	62.4	32.1	96.5

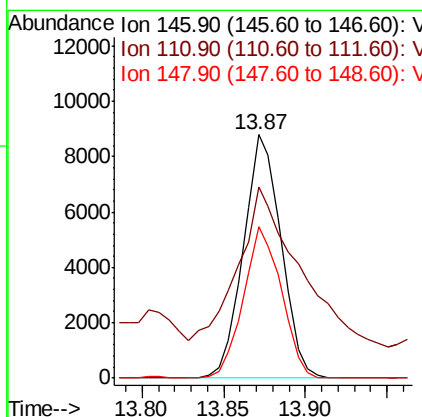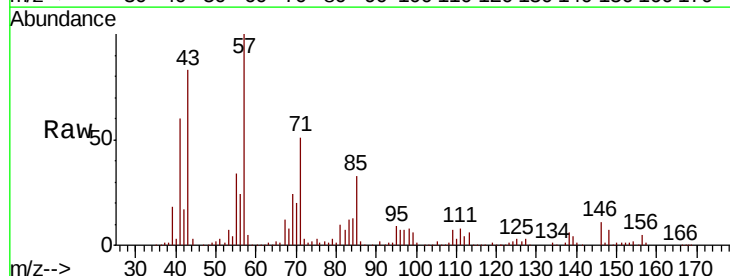







#93
1,2,4-Trichlorobenzene
Concen: 1051.892 ug/l
RT: 15.14 min Scan# 2171
Delta R.T. -0.00 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Instrument :
MSVOA_W
ClientSampleId :
P001-SS013-1824-01

Tgt Ion	Ratio	Resp	Lower	Upper
180	100	129539		
182	96.4	47.5	142.6	
145	55.3	17.5	52.5#	




Manual Integrations
APPROVED


MMDadoda
12/26/2018 4:33:44 PM

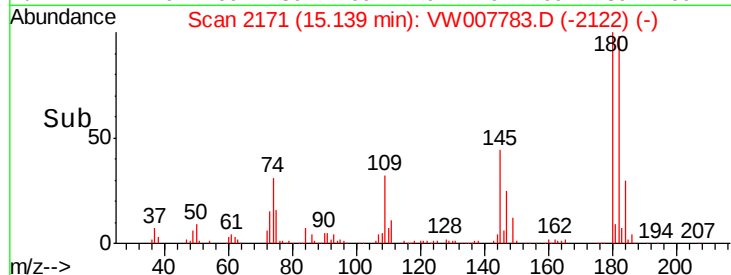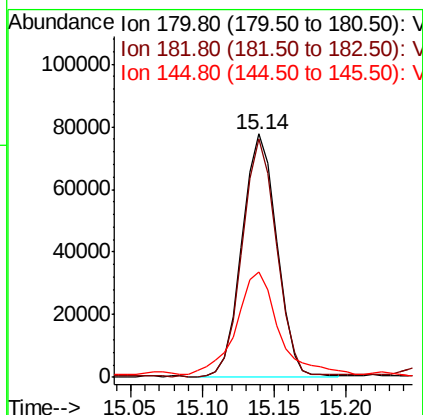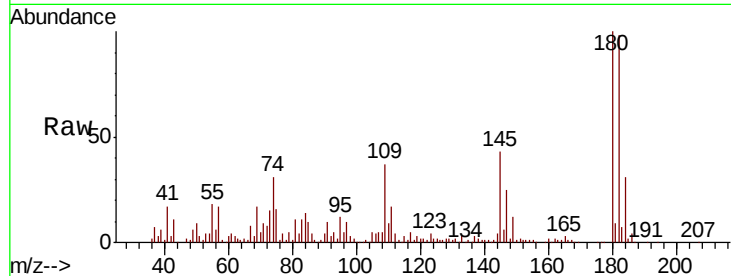

#95
Naphthalene
Concen: 2635.727 ug/l
RT: 15.37 min Scan# 2209
Delta R.T. -0.01 min
Lab File: VW007783.D
Acq: 21 Dec 2018 09:31

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	600105		
127	14.5	10.7	16.1	
129	11.1	8.8	13.2	

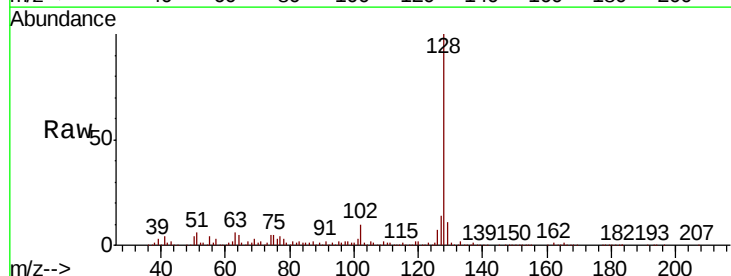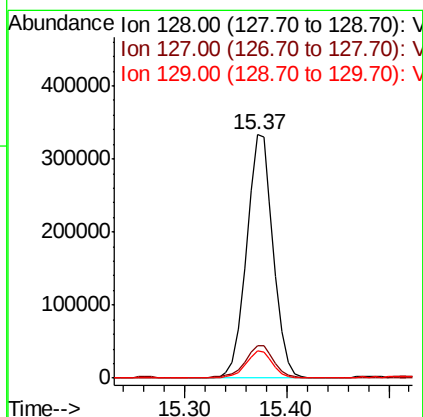



#96
 1,2,3-Trichlorobenzene
 Concen: 370.885 ug/l
 RT: 15.57 min Scan# 2241
 Delta R.T. -0.00 min
 Lab File: VW007783.D
 Acq: 21 Dec 2018 09:31

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS013-1824-01

Tgt Ion	Ratio	Resp	Lower	Upper
180	100	39097		
182	83.3	47.4	142.2	
145	97.1	18.4	55.0	

Manual Integrations
 APPROVED

MMDadoda
 12/26/2018 4:33:44 PM

