


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
Data File : VW021605.D
Acq On : 23 Dec 2021 11:39
Operator : SY/VA
Sample : M5174-01
Misc : 4.70g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBC12

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/24/2021
Supervised By :Mahesh Dadoda 01/02/2022

Quant Time: Dec 24 00:32:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 24 00:28:54 2021
Response via : Initial Calibration

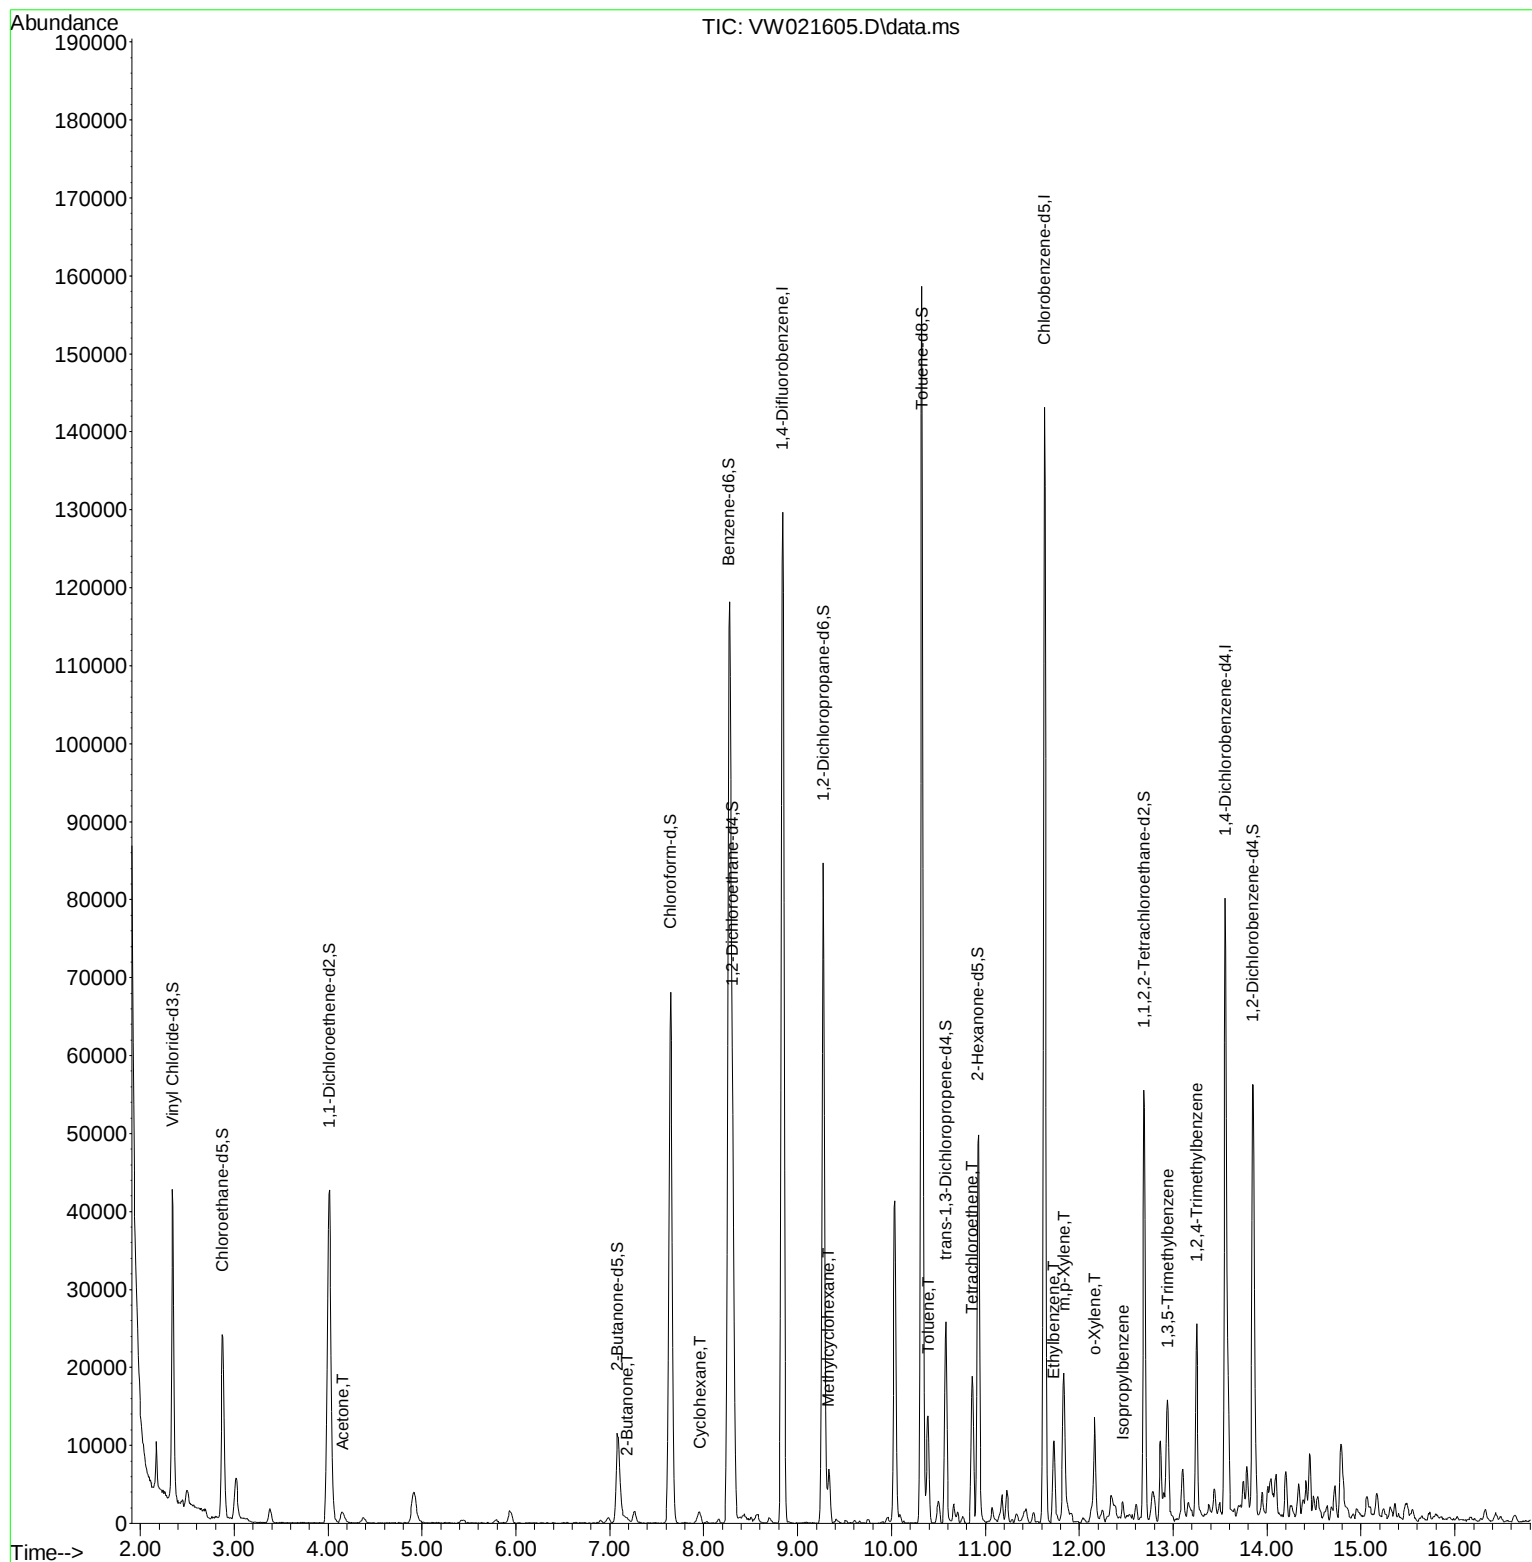




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
 Data File : VW021605.D
 Acq On : 23 Dec 2021 11:39
 Operator : SY/VA
 Sample : M5174-01
 Misc : 4.70g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBC12

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/24/2021
 Supervised By :Mahesh Dadoda 01/02/2022

Quant Time: Dec 24 00:32:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 24 00:28:54 2021
 Response via : Initial Calibration

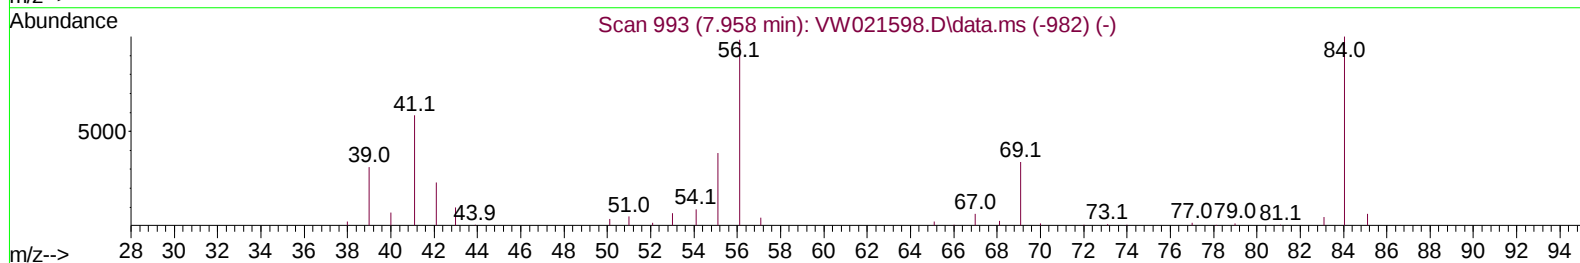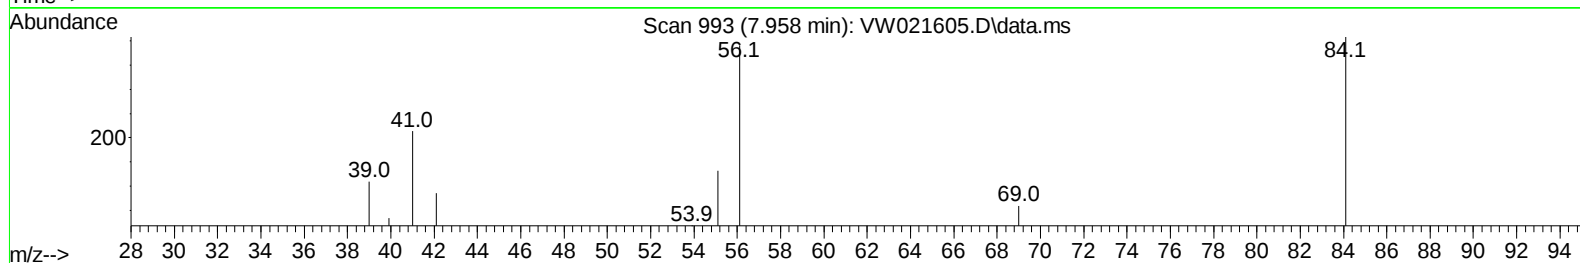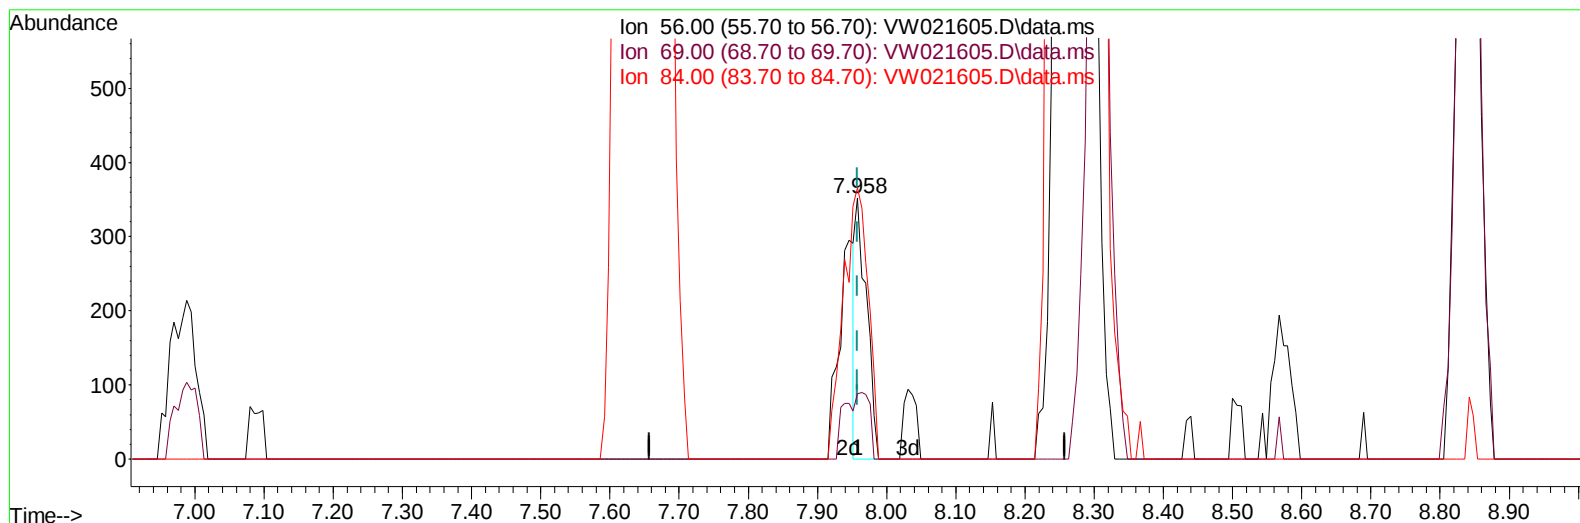

TIC: VW021605.D\data.ms

(29) Cyclohexane (T)

7.958min (0.000) 0.24 ug/L

response 386

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	29.40	32.12
84.00	79.30	235.23#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
Data File : VW021605.D
Acq On : 23 Dec 2021 11:39
Operator : SY/VA
Sample : M5174-01
Misc : 4.70g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBC12

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/24/2021
Supervised By :Mahesh Dadoda 01/02/2022

Quant Time: Dec 24 00:32:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 24 00:28:54 2021
Response via : Initial Calibration

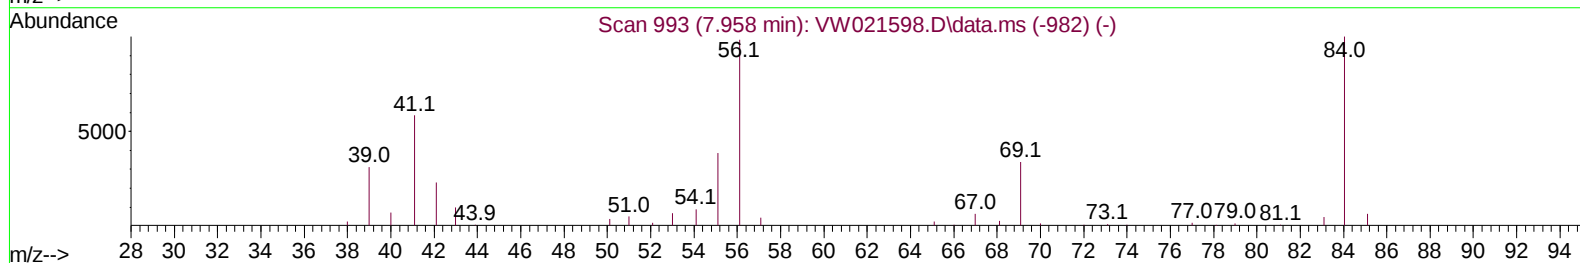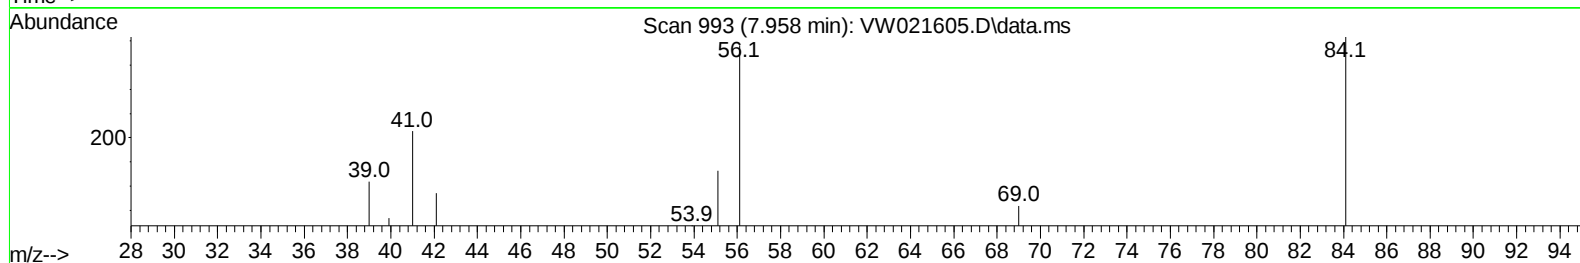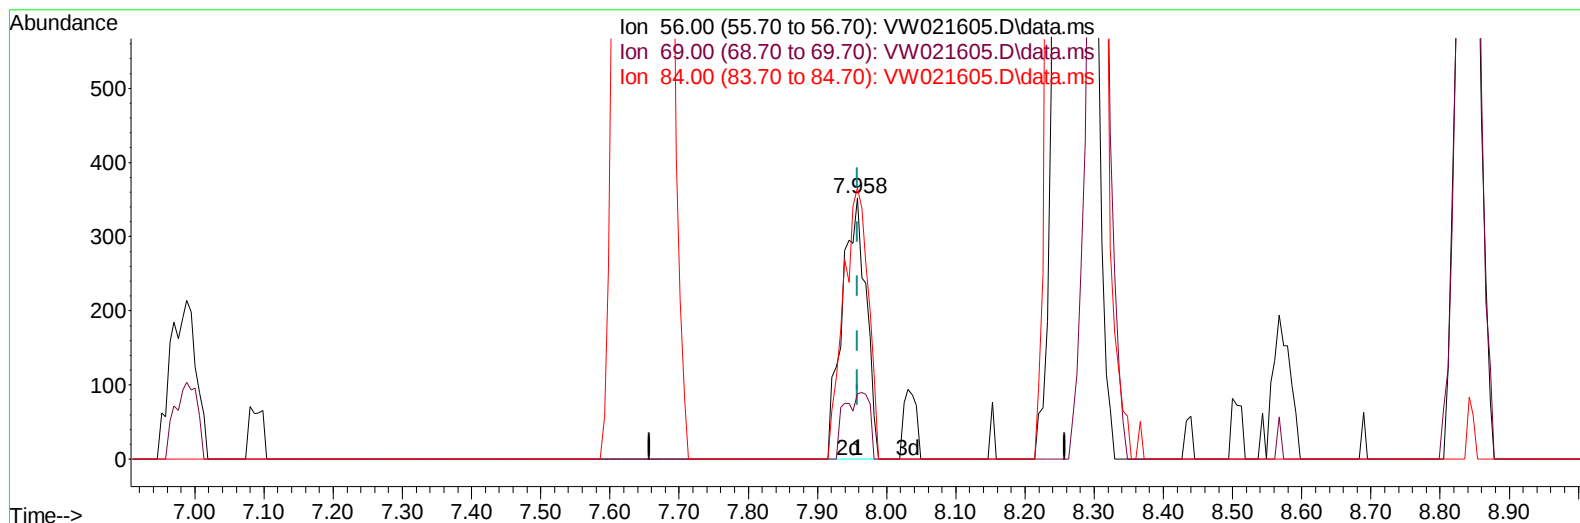

TIC: VW021605.D\data.ms

(29) Cyclohexane (T)

7.958min (0.000) 0.53 ug/L m

response 845

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	29.40	14.67#
84.00	79.30	107.46#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122221\
 Data File : VW021605.D
 Acq On : 23 Dec 2021 11:39
 Operator : SY/VA
 Sample : M5174-01
 Misc : 4.70g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBC12

Manual IntegrationsAPPROVED

Quant Time: Dec 24 00:32:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 24 00:28:54 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/24/2021
 Supervised By :Mahesh Dadoda 01/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	114834	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	80670	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	20393	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	33513	16.024	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	64.080%	
7) Chloroethane-d5	2.873	69	26418	19.108	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.440%	
11) 1,1-Dichloroethene-d2	4.013	63	39748	14.255	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.040%	
21) 2-Butanone-d5	7.080	46	20407	69.221	ug/L	-0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	138.440%#	
24) Chloroform-d	7.647	84	68837	21.510	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.040%	
26) 1,2-Dichloroethane-d4	8.305	65	40088	23.550	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.200%	
32) Benzene-d6	8.269	84	120521	27.256	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	109.040%	
36) 1,2-Dichloropropane-d6	9.275	67	36243	30.562	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	122.240%#	
41) Toluene-d8	10.323	98	100779	22.306	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.240%	
43) trans-1,3-Dichloroprop...	10.579	79	13570	24.852	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	99.400%	
47) 2-Hexanone-d5	10.921	63	16655	94.977	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	189.960%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	25073	24.595	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	98.400%	
66) 1,2-Dichlorobenzene-d4	13.847	152	14825	18.758	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	75.040%	
Target Compounds					Qvalue	
13) Acetone	4.154	43	3167	11.983	ug/L	95
22) 2-Butanone	7.183	43	901	2.611	ug/L	86
29) Cyclohexane	7.958	56	845m	0.526	ug/L	
35) Methylcyclohexane	9.329	83	2719	1.336	ug/L	89
42) Toluene	10.390	91	10522	2.047	ug/L	93
46) Tetrachloroethene	10.860	164	4406	3.760	ug/L	95
52) Ethylbenzene	11.731	91	6895	1.174	ug/L	98
53) m,p-Xylene	11.835	106	5250	2.216	ug/L	86
54) o-Xylene	12.164	106	3451	1.535	ug/L	93
60) Isopropylbenzene	12.463	105	1745	0.630	ug/L	100
62) 1,3,5-Trimethylbenzene	12.945	105	6569	2.786	ug/L	95
63) 1,2,4-Trimethylbenzene	13.249	105	13620	5.855	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed