


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
Data File : VW021607.D
Acq On : 23 Dec 2021 12:27
Operator : SY/VA
Sample : M5174-03
Misc : 5.98g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBC14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/24/2021
Supervised By :Mahesh Dadoda 01/02/2022

Quant Time: Dec 24 00:32:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 24 00:28:54 2021
Response via : Initial Calibration

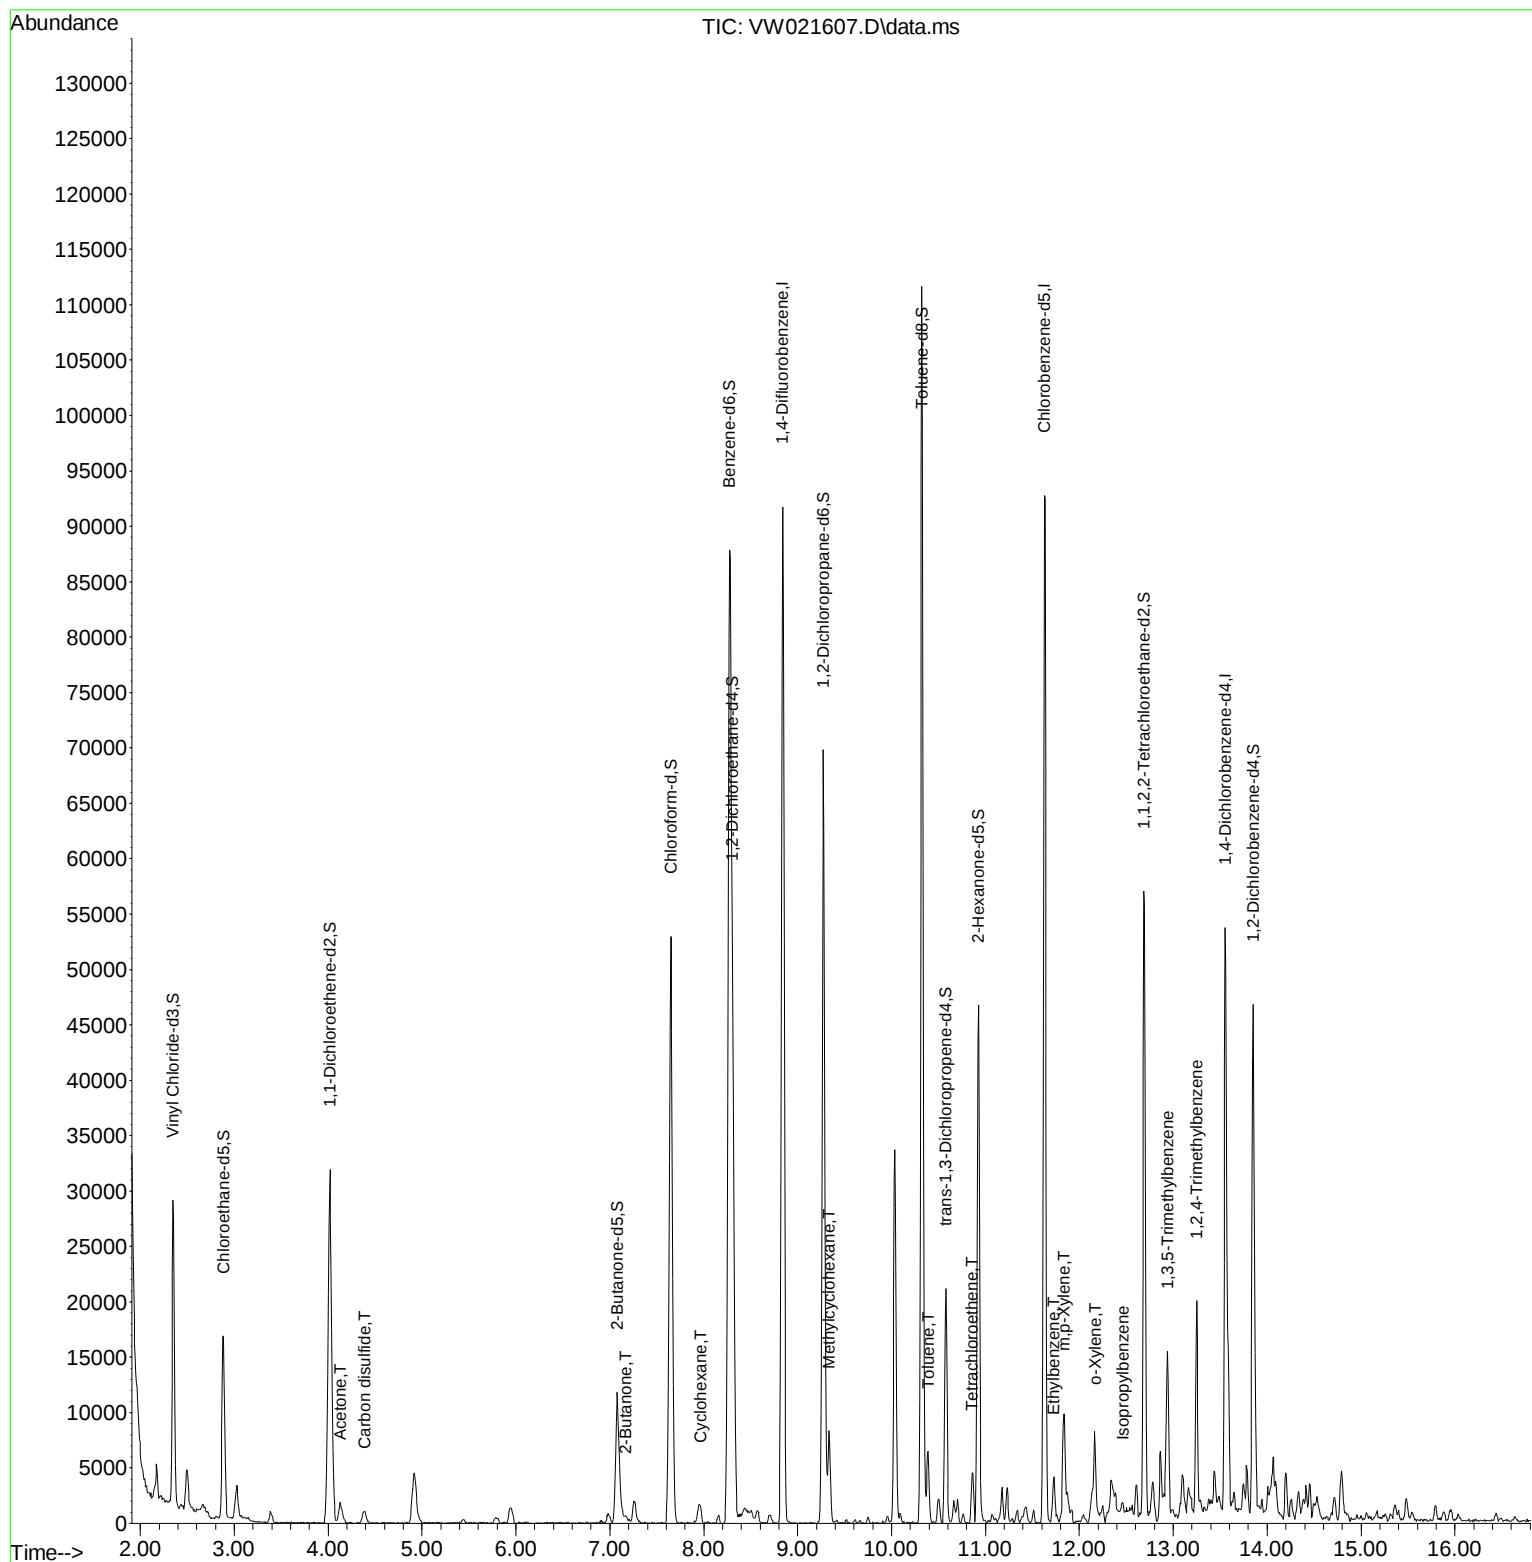




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
 Data File : VW021607.D
 Acq On : 23 Dec 2021 12:27
 Operator : SY/VA
 Sample : M5174-03
 Misc : 5.98g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBC14

Manual IntegrationsAPPROVED

Quant Time: Dec 24 00:32:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 24 00:28:54 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/24/2021
 Supervised By :Mahesh Dadoda 01/02/2022

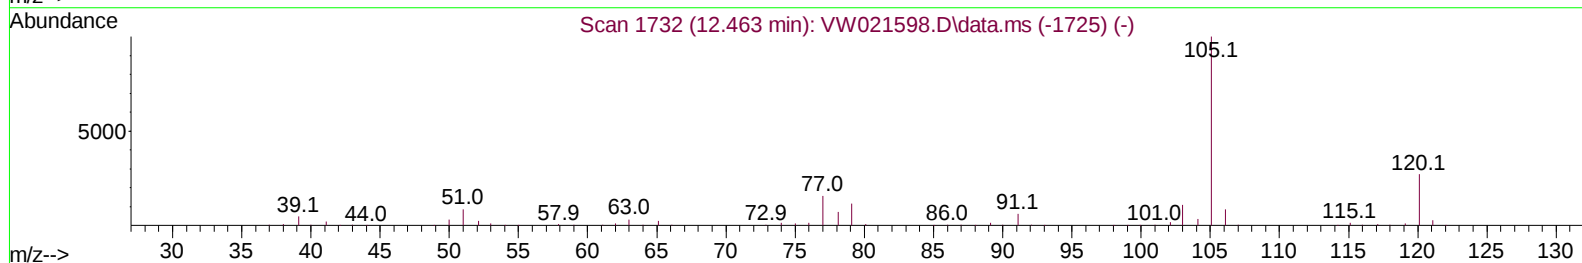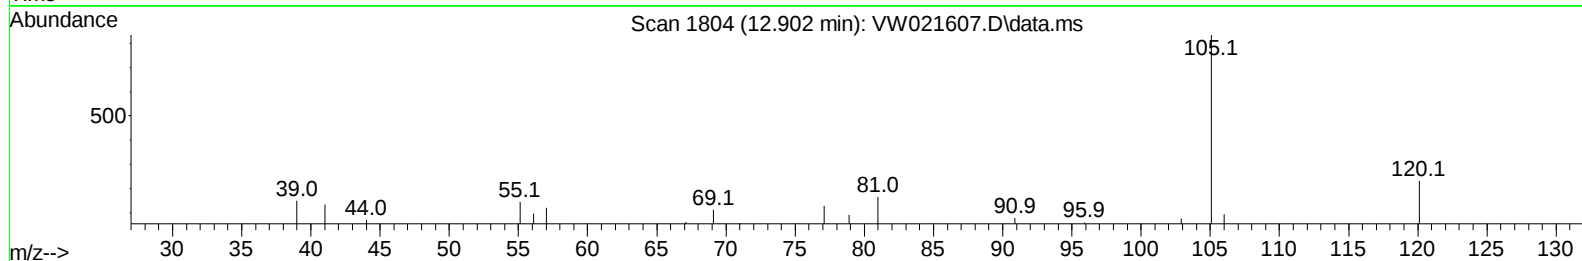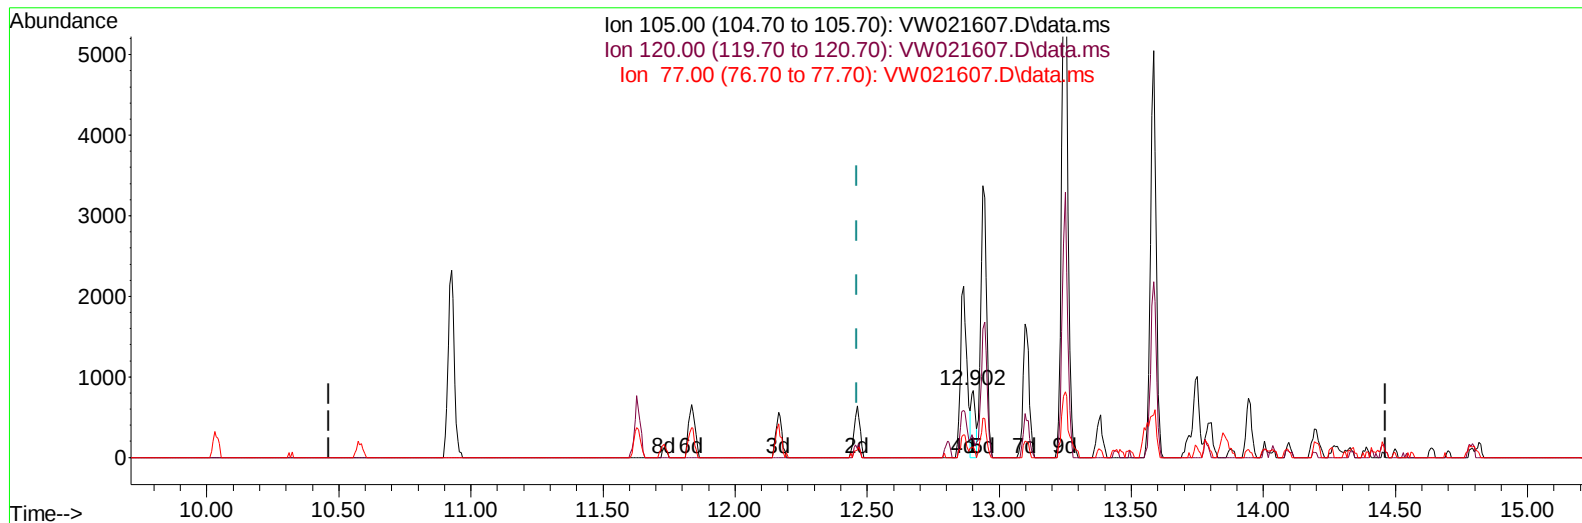

TIC: VW021607.D\data.ms

(60) Isopropylbenzene

12.902min (+ 0.439) 0.46 ug/L

response 925

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	25.10	25.73
77.00	17.30	17.51
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
 Data File : VW021607.D
 Acq On : 23 Dec 2021 12:27
 Operator : SY/VA
 Sample : M5174-03
 Misc : 5.98g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBC14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/24/2021
 Supervised By :Mahesh Dadoda 01/02/2022

Quant Time: Dec 24 00:32:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 24 00:28:54 2021
 Response via : Initial Calibration

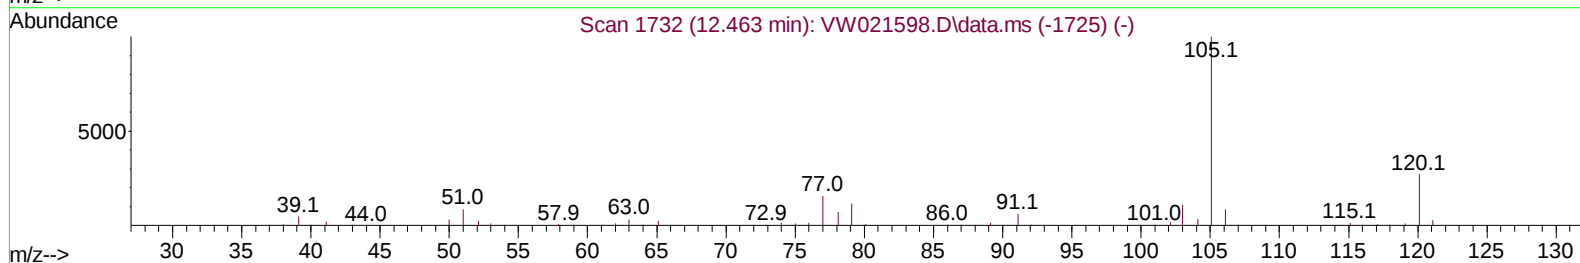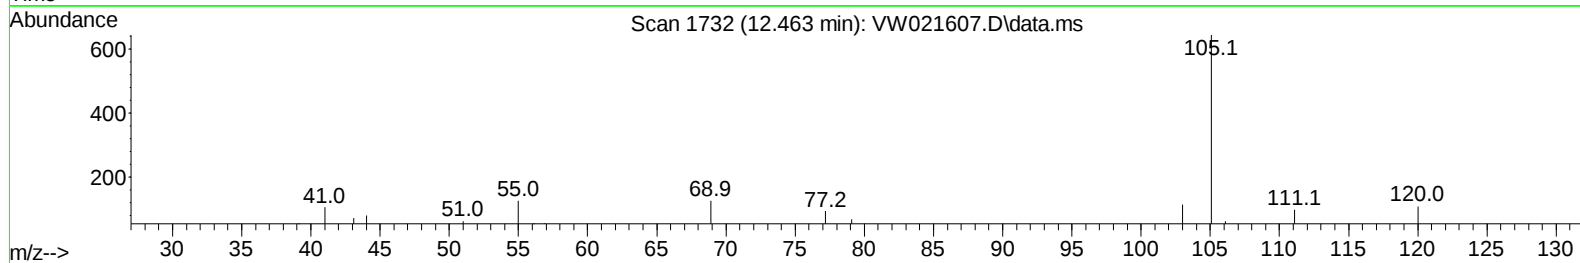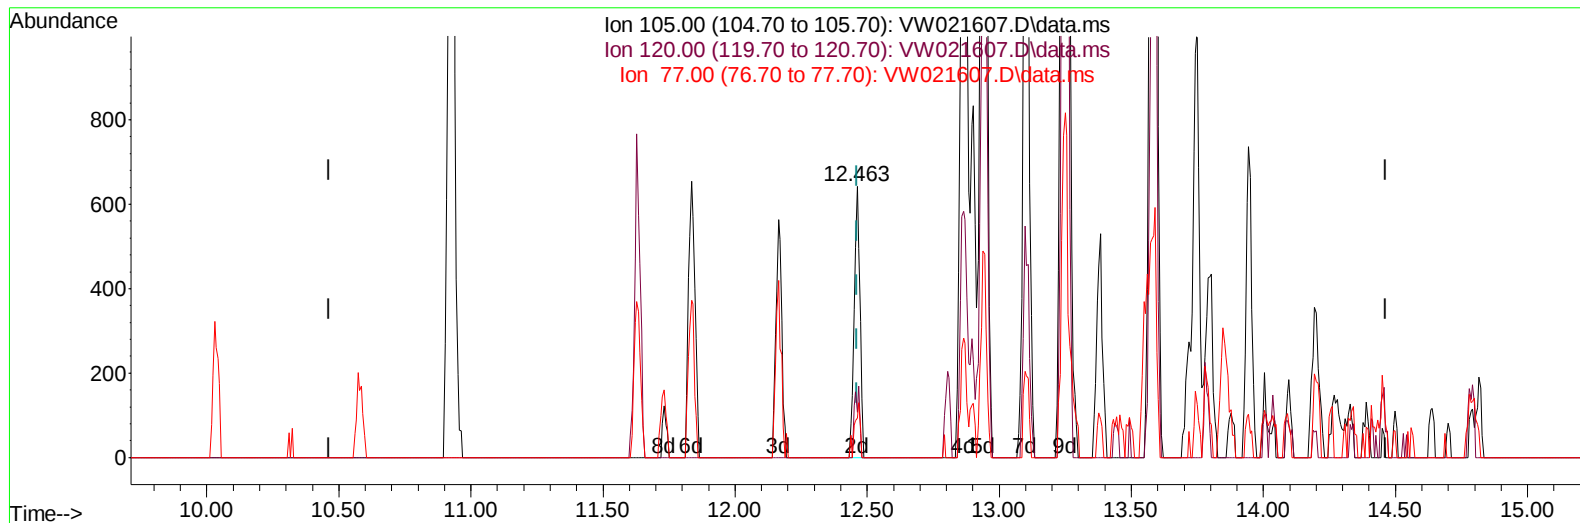

TIC: VW021607.D\data.ms

(60) Isopropylbenzene

12.463min (-0.000) 0.49 ug/L m

response 980

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	25.10	24.29
77.00	17.30	16.53
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122221\
 Data File : VW021607.D
 Acq On : 23 Dec 2021 12:27
 Operator : SY/VA
 Sample : M5174-03
 Misc : 5.98g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBC14

Manual IntegrationsAPPROVED

Quant Time: Dec 24 00:32:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 24 00:28:54 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/24/2021
 Supervised By :Mahesh Dadoda 01/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	76821	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	54305	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	14814	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	24277	17.352	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	69.400%	
7) Chloroethane-d5	2.885	69	17884	19.336	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.360%	
11) 1,1-Dichloroethene-d2	4.019	63	28987	15.540	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.160%	
21) 2-Butanone-d5	7.080	46	19501	98.880	ug/L	-0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	197.760%#	
24) Chloroform-d	7.653	84	52683	24.609	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.440%	
26) 1,2-Dichloroethane-d4	8.305	65	34367	30.179	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	120.720%	
32) Benzene-d6	8.275	84	90747	30.486	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	121.960%	
36) 1,2-Dichloropropane-d6	9.274	67	29082	36.430	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	145.720%#	
41) Toluene-d8	10.323	98	70108	23.052	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	92.200%	
43) trans-1,3-Dichloroprop...	10.579	79	10711	29.140	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	116.560%	
47) 2-Hexanone-d5	10.927	63	15030	127.322	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	254.640%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	25988	37.869	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	151.480%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	11577	20.165	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	80.640%	
Target Compounds						
						Qvalue
13) Acetone	4.129	43	3515	19.881	ug/L	93
14) Carbon disulfide	4.385	76	2358	0.959	ug/L	96
22) 2-Butanone	7.171	43	821	3.556	ug/L	77
29) Cyclohexane	7.964	56	1043	0.965	ug/L #	84
35) Methylcyclohexane	9.335	83	3371	2.461	ug/L	87
42) Toluene	10.390	91	5035	1.455	ug/L	97
46) Tetrachloroethene	10.859	164	1121	1.421	ug/L	90
52) Ethylbenzene	11.731	91	2602	0.658	ug/L	97
53) m,p-Xylene	11.835	106	2569	1.611	ug/L	81
54) o-Xylene	12.170	106	2124	1.403	ug/L	73
60) Isopropylbenzene	12.463	105	980m	0.487	ug/L	
62) 1,3,5-Trimethylbenzene	12.938	105	5298	3.093	ug/L	93
63) 1,2,4-Trimethylbenzene	13.249	105	10681	6.321	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed