

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
 Data File : VW021567.D
 Acq On : 22 Dec 2021 16:53
 Operator : SY/VA
 Sample : VIBLK561
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK561

Quant Time: Dec 23 00:37:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 23 00:34:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	109089	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	109626	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	61903	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	36313	18.277	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.120%
7) Chloroethane-d5	2.873	69	26707	20.334	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.320%
11) 1,1-Dichloroethene-d2	4.007	63	48302	18.236	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.960%
21) 2-Butanone-d5	7.080	46	20660	73.770	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	147.540%#
24) Chloroform-d	7.647	84	77883	25.619	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.480%
26) 1,2-Dichloroethane-d4	8.305	65	44631	27.599	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	8.269	84	149513	24.882	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.520%
36) 1,2-Dichloropropane-d6	9.268	67	42161	26.162	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.640%
41) Toluene-d8	10.323	98	149423	24.337	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.360%
43) trans-1,3-Dichloroprop...	10.579	79	17835	24.036	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.160%
47) 2-Hexanone-d5	10.927	63	16895	70.897	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.800%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	38536	27.817	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	57326	23.895	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.560%
Target Compounds						
13) Acetone	4.153	43	939	3.740	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
Data File : VW021567.D
Acq On : 22 Dec 2021 16:53
Operator : SY/VA
Sample : VIBLK561
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK561

Quant Time: Dec 23 00:37:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 23 00:34:33 2021
Response via : Initial Calibration

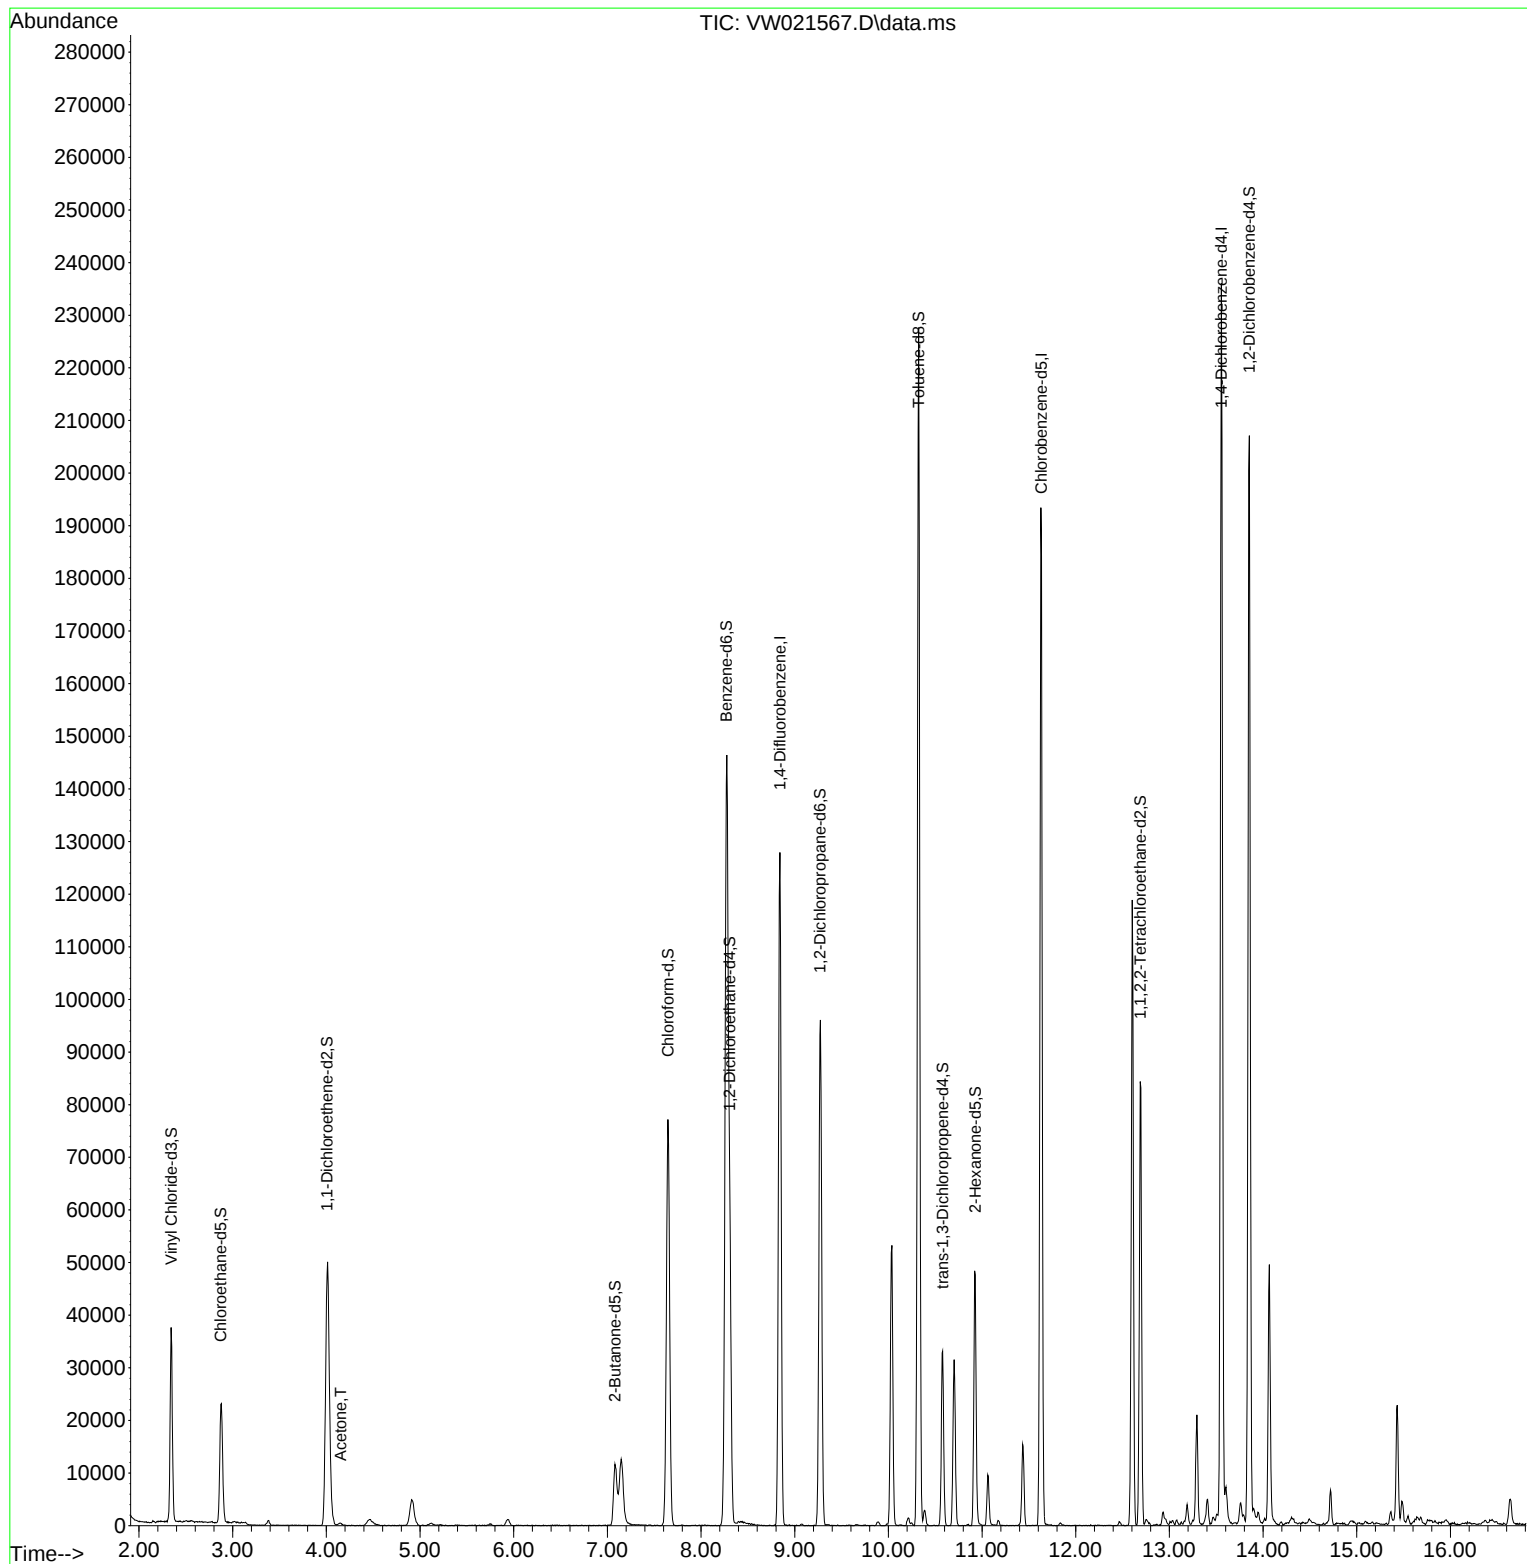

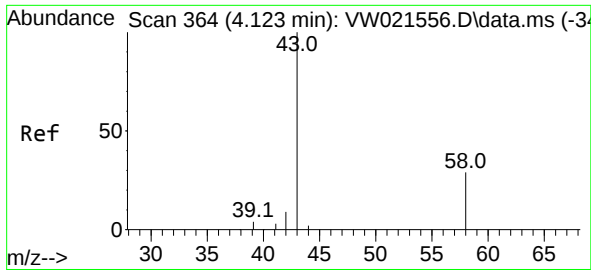

#13
 Acetone
 Concen: 3.740 ug/L
 RT: 4.153 min Scan# 30
 Delta R.T. 0.031 min
 Lab File: VW021567.D
 Acq: 22 Dec 2021 16:53

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK561

Tgt Ion: 43 Resp: 939
 Ion Ratio Lower Upper
 43 100
 58 20.1 0.0 52.8

