

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
 Data File : VW021578.D
 Acq On : 22 Dec 2021 22:06
 Operator : SY/VA
 Sample : VW1222SBL02
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK427

Quant Time: Dec 23 02:56:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 23 02:55:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	116483	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	116838	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	67053	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	46942	22.127	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.520%
7) Chloroethane-d5	2.879	69	29092	20.744	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.960%
11) 1,1-Dichloroethene-d2	4.007	63	55979	19.792	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.160%
21) 2-Butanone-d5	7.098	46	14018	46.876	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.760%
24) Chloroform-d	7.647	84	78741	24.257	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.040%
26) 1,2-Dichloroethane-d4	8.305	65	43303	25.078	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.320%
32) Benzene-d6	8.275	84	157833	24.645	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.560%
36) 1,2-Dichloropropane-d6	9.274	67	43531	25.345	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.360%
41) Toluene-d8	10.323	98	161478	24.677	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.720%
43) trans-1,3-Dichloroprop...	10.579	79	18482	23.370	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.480%
47) 2-Hexanone-d5	10.927	63	12552	49.421	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.840%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	32317	21.888	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	58792	22.624	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.480%
Target Compounds						
16) Methylene chloride	4.915	84	7347	3.817	ug/L	Qvalue 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
Data File : VW021578.D
Acq On : 22 Dec 2021 22:06
Operator : SY/VA
Sample : VW1222SBL02
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK427

Quant Time: Dec 23 02:56:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 23 02:55:43 2021
Response via : Initial Calibration

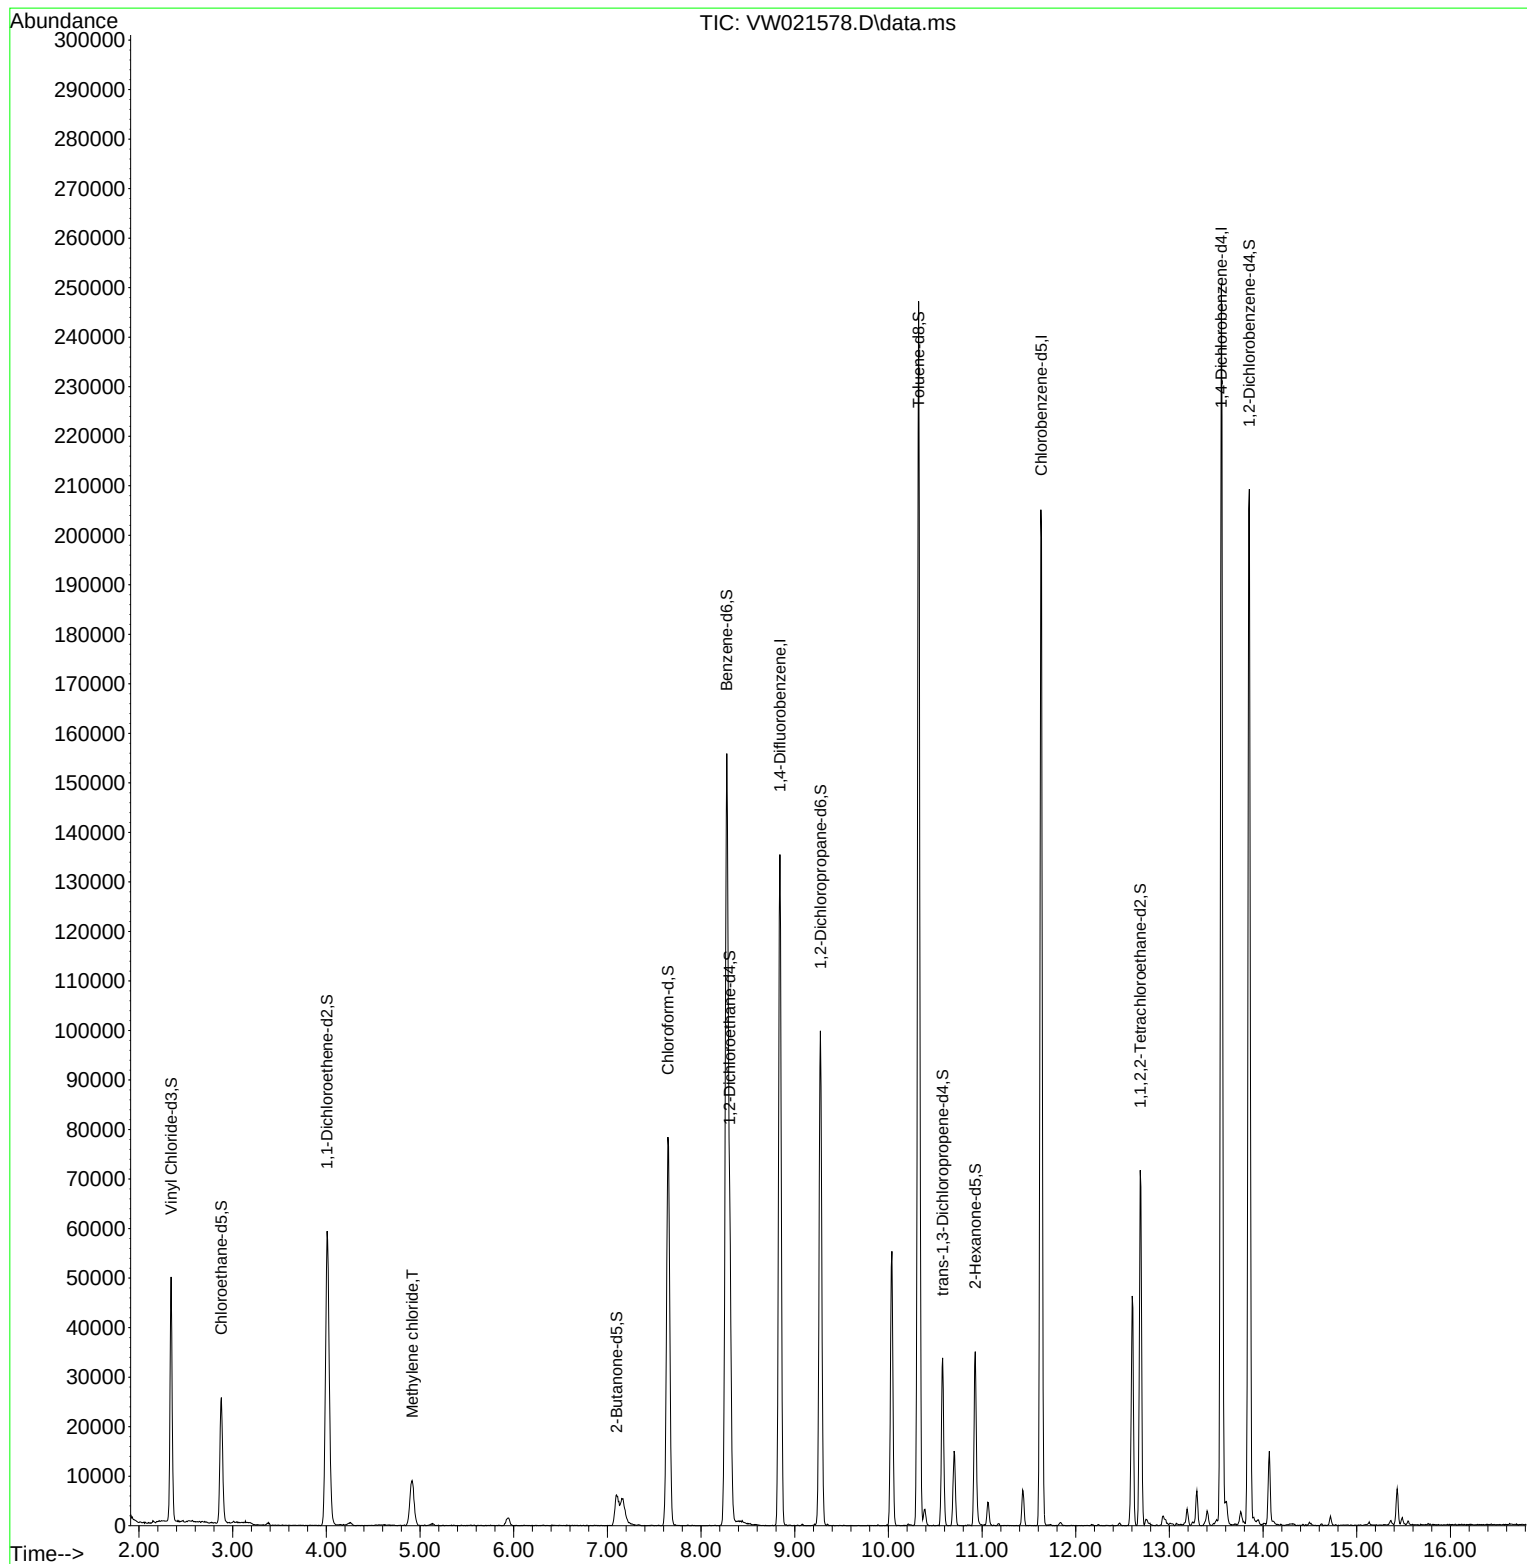

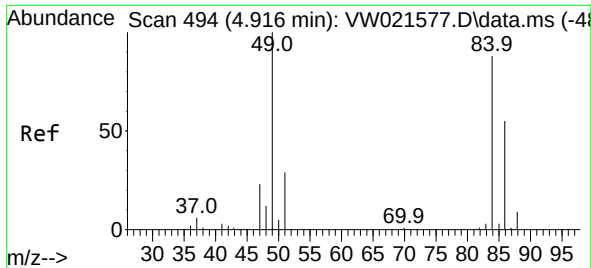

#16

Methylene chloride

Concen: 3.817 ug/L

RT: 4.915 min Scan# 49

Delta R.T. -0.000 min

Lab File: VW021578.D


Acq: 22 Dec 2021 22:06

Instrument :

MSVOA_W

ClientSampleId :

VBLK427

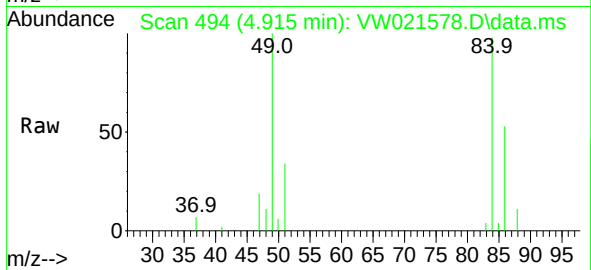

Tgt Ion: 84 Resp: 7347

Ion Ratio Lower Upper

84 100

86 54.7 45.5 84.5

49 102.3 100.5 186.7

