

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
 Data File : VW021630.D
 Acq On : 23 Dec 2021 22:41
 Operator : SY/VA
 Sample : VIBLK566
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK566

Quant Time: Dec 24 01:48:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 24 01:43:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	119098	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	121602	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	66214	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	26770	12.342	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	49.360%
7) Chloroethane-d5	2.885	69	19541	13.628	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.520%
11) 1,1-Dichloroethene-d2	4.019	63	39812	13.767	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.080%
21) 2-Butanone-d5	7.074	46	18193	59.502	ug/L	-0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.000%
24) Chloroform-d	7.653	84	69512	20.944	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.760%
26) 1,2-Dichloroethane-d4	8.305	65	39284	22.251	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.000%
32) Benzene-d6	8.275	84	127659	19.152	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.600%
36) 1,2-Dichloropropane-d6	9.274	67	37733	21.108	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.440%
41) Toluene-d8	10.323	98	121243	17.803	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.200%
43) trans-1,3-Dichloroprop...	10.579	79	14692	17.850	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.400%
47) 2-Hexanone-d5	10.927	63	14177	53.633	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.260%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	34806	22.650	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	50858	19.819	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.280%
Target Compounds						
16) Methylene chloride	4.915	84	10467	5.319	ug/L	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122221\
Data File : VW021630.D
Acq On : 23 Dec 2021 22:41
Operator : SY/VA
Sample : VIBLK566
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK566


Quant Time: Dec 24 01:48:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 24 01:43:02 2021
Response via : Initial Calibration

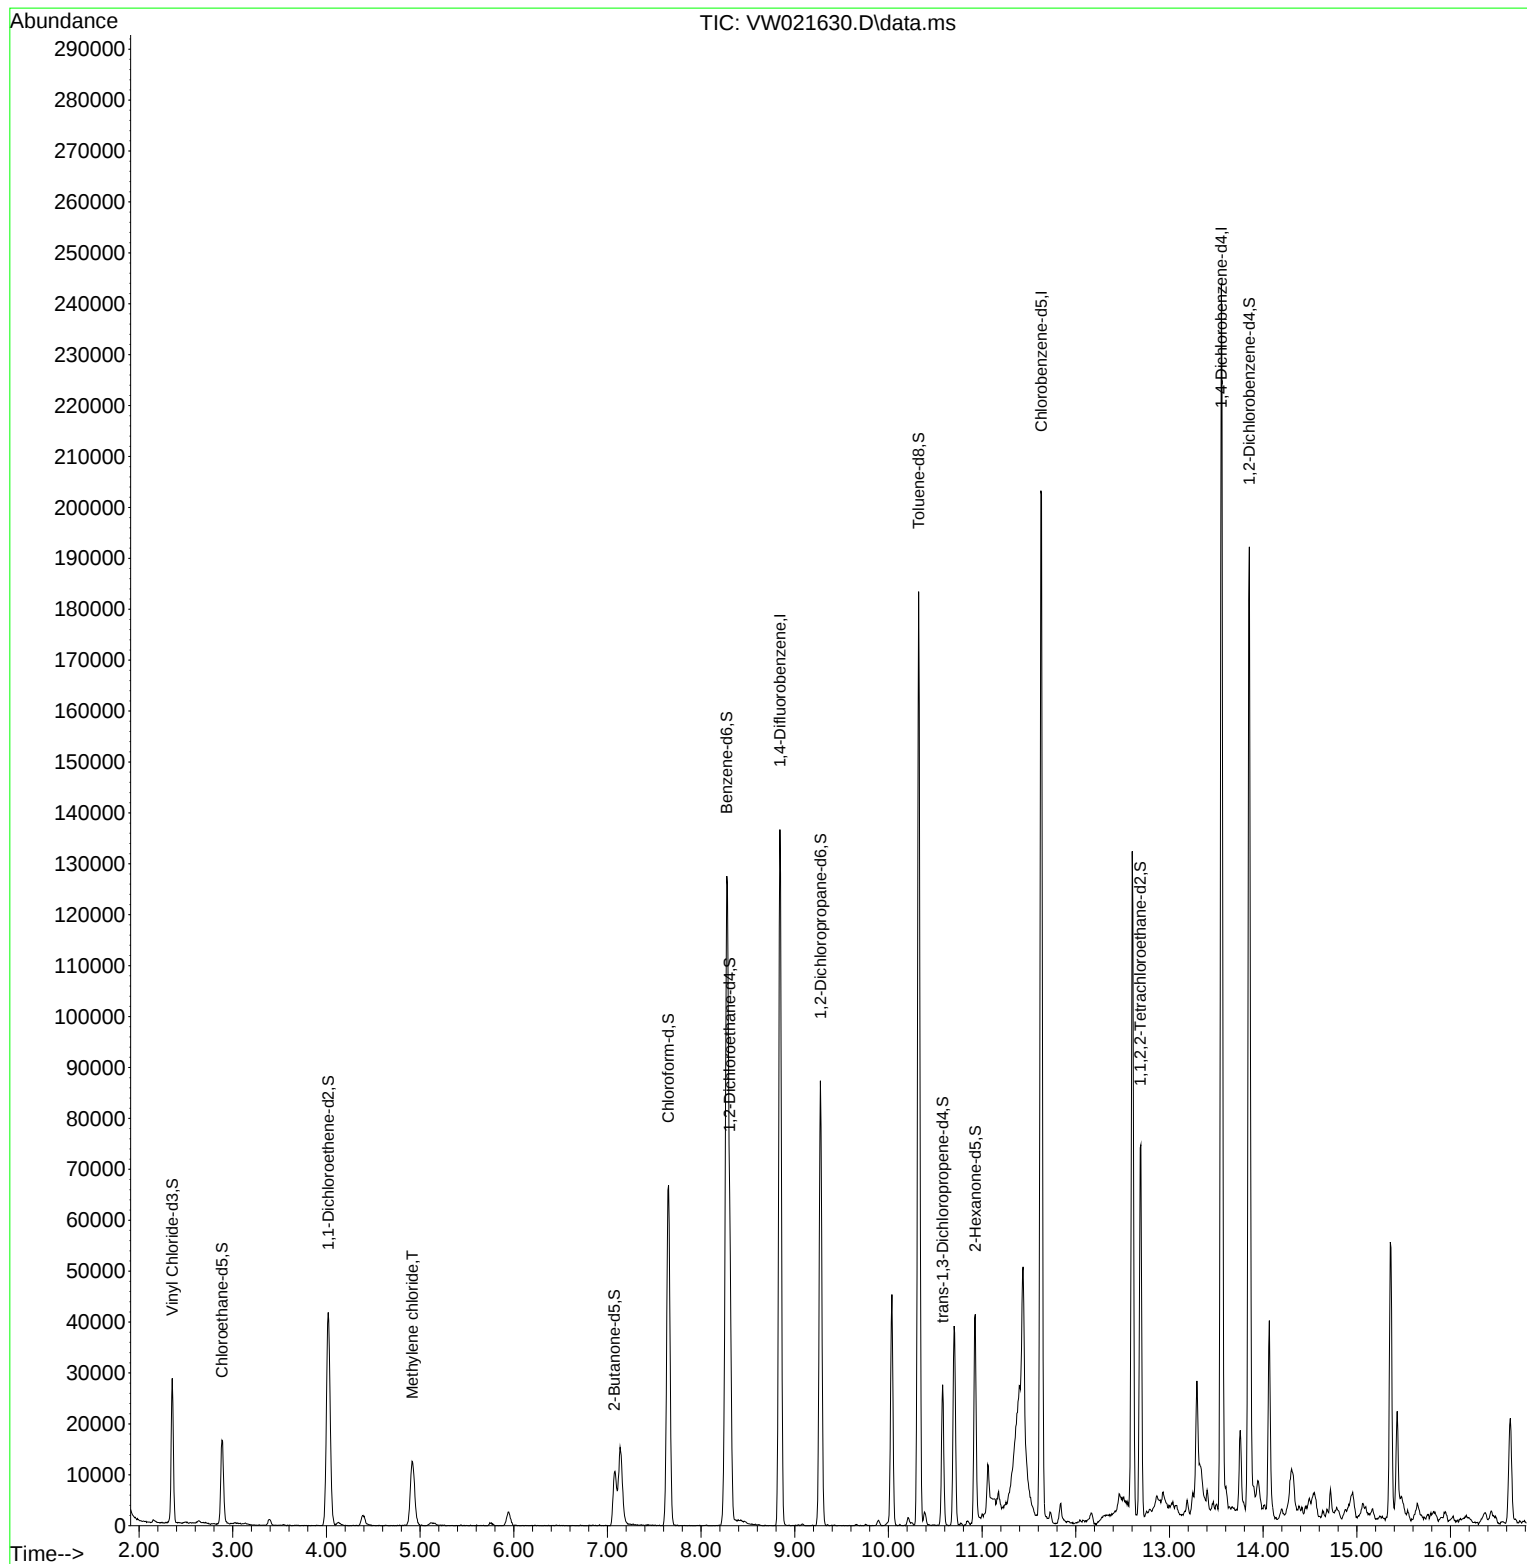

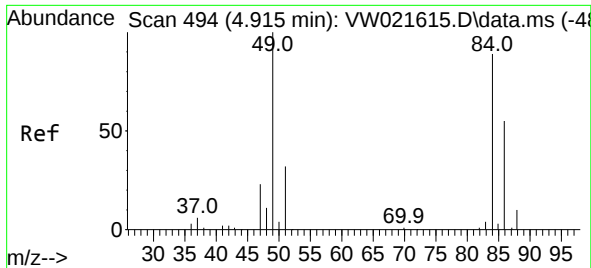

#16
Methylene chloride
Concen: 5.319 ug/L
RT: 4.915 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW021630.D
Acq: 23 Dec 2021 22:41

Instrument :
MSVOA_W
ClientSampleId :
VIBLK566

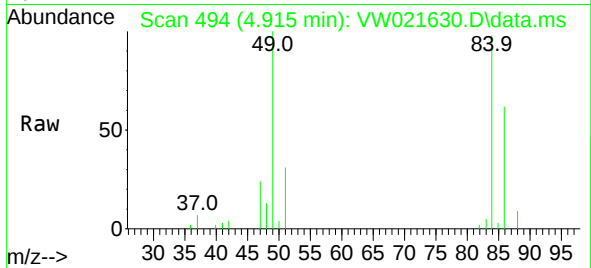

Tgt Ion: 84 Resp: 10467
Ion Ratio Lower Upper
84 100
86 63.2 45.5 84.5
49 102.3 100.5 186.7

