
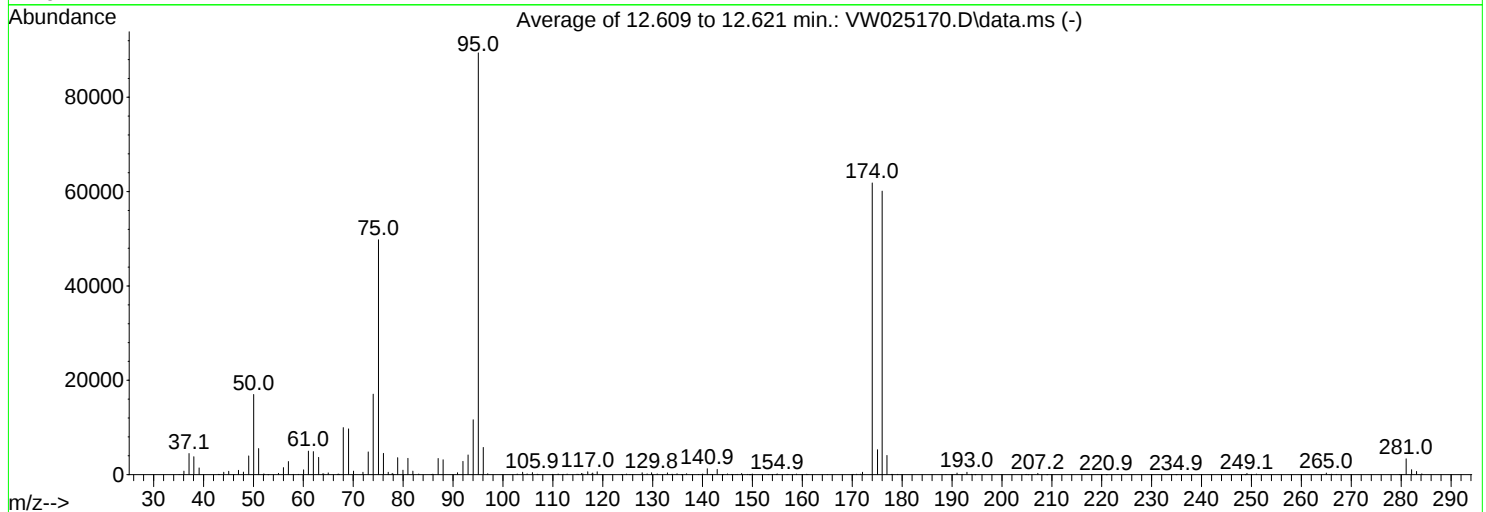


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122222\
 Data File : VW025170.D
 Acq On : 22 Dec 2022 21:31
 Operator : SY/MD
 Sample : BFB466
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB466

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
 Title : SFAM01.0
 Last Update : Fri Dec 23 21:59:05 2022

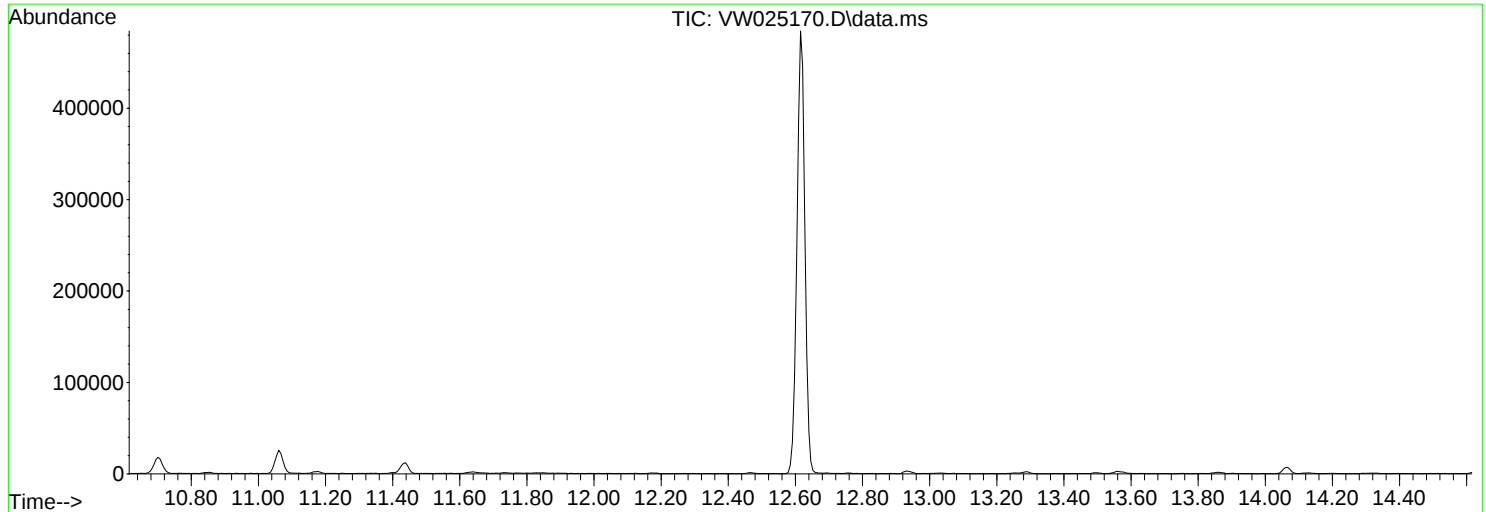

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	16983	PASS
75	95	30	80	55.7	49781	PASS
95	95	100	100	100.0	89419	PASS
96	95	5	9	6.4	5755	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.1	61827	PASS
175	174	5	9	8.5	5281	PASS
176	174	95	105	97.2	60112	PASS
177	176	5	10	6.8	4081	PASS

Scan 1749 (12.567 min): VW025170.D\data.ms
BFB466

m/z	Abundance
40.00	239.0
44.10	84.0
281.00	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

m/z	Abundance
35.10	70.0
36.10	633.0
37.10	4208.0
38.10	3448.0
39.10	1415.0
39.90	229.0
43.00	119.0
44.00	558.0
45.10	700.0
47.00	734.0
48.10	414.0
49.10	3542.0
50.00	15994.0
51.00	5286.0
52.00	187.0
52.90	51.0
55.10	309.0
56.00	1505.0
57.00	2545.0
58.10	62.0
59.00	163.0
60.00	1012.0
61.00	4373.0
62.00	4551.0
63.00	3283.0
63.90	260.0
65.00	466.0
66.80	155.0
68.00	8967.0
69.10	8772.0
70.10	701.0
71.90	527.0
73.00	4566.0
74.00	15356.0
75.10	45312.0
76.00	4127.0
77.00	432.0
77.80	219.0
78.90	3158.0
80.00	959.0
81.00	3079.0
81.90	705.0
83.20	55.0
85.70	121.0
87.00	3185.0
88.00	2683.0
90.80	319.0
92.00	2902.0
93.00	4444.0
94.00	10315.0
95.00	79552.0
96.00	5331.0
97.00	212.0
102.90	186.0
104.10	440.0
104.80	204.0
105.90	292.0
106.80	120.0
107.20	98.0
110.00	119.0
111.10	130.0
112.00	65.0
112.90	121.0
114.90	145.0
115.70	286.0
117.10	453.0
117.80	390.0
118.90	697.0
123.80	65.0
124.80	126.0
125.50	72.0
127.90	344.0
129.00	119.0
129.80	416.0
131.00	186.0
133.00	598.0
134.00	97.0
134.80	303.0
135.80	57.0
136.80	239.0
140.10	99.0
141.00	892.0
141.70	199.0
142.90	932.0
144.00	56.0
145.00	212.0
145.90	123.0
147.00	106.0
147.90	226.0
149.00	102.0
149.90	90.0
154.80	233.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

156.90	107.0
158.90	110.0
160.90	99.0
165.00	70.0
170.10	102.0
171.00	156.0
171.70	283.0
172.20	486.0
174.00	48760.0
175.00	4546.0
176.00	45152.0
176.90	3439.0
177.90	191.0
179.10	114.0
188.80	65.0
191.00	555.0
191.80	71.0
193.10	704.0
194.00	114.0
194.60	52.0
204.70	90.0
205.20	57.0
207.20	326.0
209.00	51.0
220.90	52.0
234.90	58.0
249.10	486.0
250.00	171.0
251.00	267.0
265.00	399.0
266.10	244.0
267.00	138.0
279.70	109.0
281.00	5038.0
282.10	1849.0
283.10	1022.0
284.20	332.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

m/z	Abundance
36.10	970.0
37.10	4932.0
38.10	4132.0
39.10	1571.0
40.00	183.0
43.00	104.0
44.10	612.0
45.00	785.0
47.00	894.0
48.00	689.0
49.00	4546.0
50.10	19128.0
51.10	6325.0
52.20	310.0
55.00	249.0
56.00	1639.0
57.00	3201.0
57.90	97.0
59.00	98.0
60.00	1033.0
61.00	5538.0
62.00	5406.0
63.10	4212.0
64.10	491.0
65.00	344.0
67.00	399.0
68.00	11058.0
69.00	10663.0
70.10	795.0
72.00	589.0
73.00	5486.0
74.00	18744.0
75.00	55632.0
76.10	5016.0
77.10	645.0
77.90	349.0
78.90	4173.0
80.00	982.0
80.90	4092.0
82.00	824.0
83.20	183.0
85.90	140.0
87.00	3535.0
88.00	3666.0
90.90	448.0
92.00	3002.0
93.00	4319.0
94.10	13075.0
95.00	100296.0
96.10	6427.0
97.00	238.0
102.80	162.0
103.90	549.0
104.80	135.0
105.90	502.0
106.90	143.0
109.90	57.0
110.90	149.0
112.00	90.0
112.80	113.0
114.80	166.0
116.00	494.0
116.90	709.0
118.00	576.0
118.90	523.0
124.80	192.0
127.90	452.0
128.80	265.0
129.80	414.0
130.80	164.0
132.90	338.0
133.80	152.0
134.90	172.0
136.90	213.0
139.20	66.0
140.00	156.0
140.90	1443.0
142.90	1202.0
145.00	177.0
146.10	113.0
146.90	105.0
147.80	177.0
149.00	68.0
150.00	152.0
153.20	68.0
155.00	335.0
156.90	136.0
158.90	109.0
161.10	153.0
170.20	117.0
172.00	489.0
174.00	67568.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

175.00	5489.0
176.00	64832.0
177.00	4700.0
178.10	116.0
179.10	110.0
191.00	393.0
192.10	81.0
192.90	576.0
204.90	101.0
207.20	335.0
249.10	227.0
250.80	89.0
251.10	72.0
264.90	435.0
266.10	61.0
267.00	62.0
281.10	3519.0
282.10	812.0
283.10	676.0
284.10	135.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

m/z	Abundance
36.00	686.0
37.10	4261.0
38.00	3850.0
39.10	1344.0
40.00	165.0
43.20	116.0
44.10	604.0
45.10	645.0
46.10	61.0
47.00	1085.0
47.90	582.0
49.10	3810.0
50.10	15826.0
51.10	4988.0
52.00	190.0
54.90	256.0
56.00	1299.0
57.00	2591.0
57.90	75.0
60.10	1031.0
61.00	5095.0
62.00	4660.0
63.00	3541.0
63.90	288.0
65.00	336.0
67.20	222.0
68.00	9887.0
69.00	9654.0
70.00	749.0
72.00	389.0
73.00	4427.0
74.00	17048.0
75.00	48400.0
76.00	4354.0
76.90	420.0
77.70	295.0
78.10	301.0
78.90	3470.0
79.90	945.0
81.00	3228.0
82.00	751.0
83.10	157.0
86.00	139.0
87.00	3524.0
88.00	3081.0
91.00	408.0
92.00	2561.0
93.00	3759.0
94.10	11571.0
95.10	88408.0
96.00	5507.0
96.90	176.0
102.80	77.0
103.90	555.0
104.90	206.0
105.90	577.0
107.00	216.0
111.10	119.0
112.10	87.0
112.90	137.0
115.10	155.0
115.80	395.0
117.00	653.0
118.00	430.0
118.90	579.0
124.90	99.0
125.40	65.0
126.00	64.0
127.90	408.0
129.00	151.0
129.80	419.0
130.90	141.0
133.00	151.0
133.80	64.0
135.00	181.0
136.00	63.0
136.70	198.0
140.00	116.0
140.90	1411.0
142.00	124.0
143.00	1278.0
145.00	165.0
145.90	123.0
146.70	78.0
147.90	285.0
149.40	54.0
150.00	124.0
153.10	57.0
154.00	72.0
154.90	195.0
157.10	190.0
158.80	168.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

160.90	174.0
170.80	120.0
171.90	543.0
174.00	69152.0
175.10	5807.0
176.00	70352.0
177.00	4104.0
178.10	85.0
191.00	106.0
192.20	94.0
193.00	250.0
193.90	60.0
204.90	85.0
207.10	144.0
248.70	55.0
249.20	97.0
265.10	186.0
265.70	91.0
281.10	1659.0
282.20	551.0
283.10	387.0
284.00	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466