
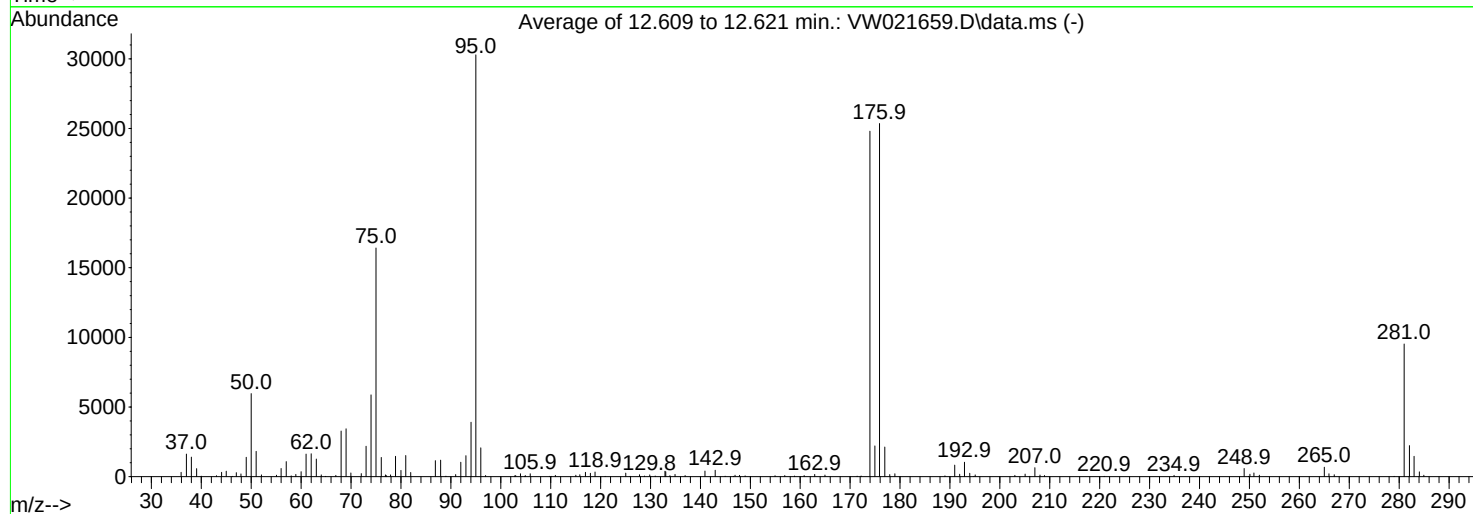


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122721\
Data File : VW021659.D
Acq On : 27 Dec 2021 10:01
Operator : SY/VA
Sample : BFB489
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB489

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Title : SFAM01.0
Last Update : Tue Dec 28 00:40:13 2021

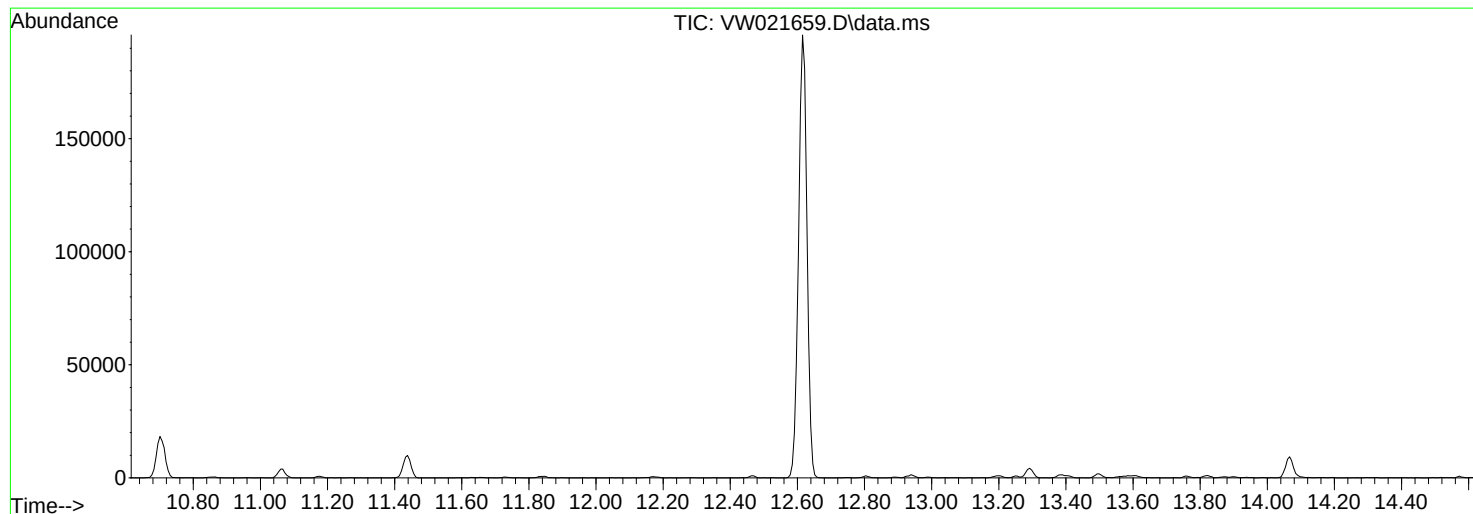

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	5965	PASS
75	95	30	80	54.2	16422	PASS
95	95	100	100	100.0	30288	PASS
96	95	5	9	6.8	2073	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.9	24800	PASS
175	174	5	9	8.9	2211	PASS
176	174	95	105	102.3	25360	PASS
177	176	5	10	8.4	2131	PASS

Scan 1750 (12.573 min): VW021659.D\data.ms
BFB489

m/z	Abundance
73.00	52.0
193.00	74.0
281.00	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB489

m/z	Abundance
36.00	267.0
37.00	1431.0
38.00	1203.0
39.10	576.0
43.00	80.0
44.00	316.0
45.00	465.0
46.20	55.0
47.00	296.0
47.90	177.0
49.00	1269.0
50.00	5107.0
51.00	1581.0
52.20	114.0
55.10	97.0
56.00	456.0
57.00	897.0
58.00	92.0
58.90	207.0
60.00	318.0
61.00	1431.0
62.00	1396.0
63.00	1063.0
64.00	132.0
67.00	60.0
68.00	2984.0
69.00	2699.0
70.00	220.0
72.10	207.0
73.00	2474.0
74.00	5007.0
75.00	14033.0
76.10	1266.0
76.90	172.0
77.90	127.0
78.90	1177.0
80.00	379.0
80.90	1232.0
81.90	219.0
86.90	957.0
88.00	956.0
89.10	55.0
91.00	112.0
92.00	943.0
93.00	1207.0
94.10	3121.0
95.00	24840.0
96.00	1761.0
102.80	160.0
104.00	196.0
104.80	115.0
105.90	163.0
109.80	73.0
110.10	84.0
111.00	101.0
115.10	125.0
115.90	138.0
116.90	284.0
118.00	223.0
118.90	358.0
120.90	59.0
125.00	391.0
125.90	76.0
127.80	110.0
128.80	66.0
129.90	104.0
132.90	1185.0
135.00	219.0
136.90	55.0
140.80	340.0
142.90	308.0
144.90	60.0
146.90	164.0
147.90	89.0
148.90	107.0
155.00	60.0
156.90	79.0
158.90	51.0
160.80	168.0
162.90	202.0
165.00	206.0
173.90	20528.0
175.00	1689.0
175.90	19760.0
177.00	1886.0
178.00	177.0
179.00	288.0
189.00	100.0
190.90	1195.0
192.00	247.0
192.90	1718.0
193.90	394.0

Instrument :
MSVOA_W
ClientSampleId :
BFB489

195.10	180.0
203.00	168.0
205.00	228.0
206.00	61.0
207.00	906.0
208.10	170.0
208.90	96.0
220.90	86.0
235.00	133.0
248.90	885.0
250.10	270.0
250.90	377.0
252.00	169.0
265.00	1007.0
266.00	241.0
267.00	165.0
281.00	14008.0
282.10	2792.0
283.00	2003.0
284.00	500.0
285.00	141.0

Instrument :
MSVOA_W
ClientSampleId :
BFB489

m/z	Abundance
36.00	358.0
37.00	1736.0
38.00	1525.0
39.00	614.0
40.00	56.0
43.10	75.0
44.00	299.0
45.00	350.0
47.00	279.0
48.00	222.0
49.00	1564.0
50.00	6729.0
51.00	2018.0
52.00	137.0
55.10	122.0
56.00	632.0
57.00	1167.0
58.00	78.0
59.00	170.0
60.00	372.0
61.00	1734.0
62.00	1899.0
63.10	1369.0
64.00	108.0
67.00	112.0
68.00	3751.0
69.00	3932.0
70.00	286.0
72.00	186.0
73.00	2356.0
74.00	6497.0
75.00	18008.0
76.00	1447.0
76.90	205.0
77.80	148.0
78.90	1787.0
80.00	501.0
81.00	1626.0
81.90	340.0
86.90	1314.0
87.90	1333.0
90.90	189.0
92.00	1142.0
93.00	1653.0
94.00	4378.0
95.00	33192.0
96.00	2432.0
97.00	96.0
103.00	161.0
104.00	260.0
105.00	127.0
105.90	250.0
110.90	75.0
115.00	105.0
115.80	157.0
117.00	319.0
117.90	304.0
118.90	331.0
125.10	241.0
127.70	144.0
128.80	72.0
129.80	115.0
131.00	87.0
133.10	655.0
133.90	146.0
134.90	122.0
136.90	91.0
140.90	456.0
142.90	480.0
145.00	55.0
147.00	97.0
147.90	103.0
149.00	74.0
155.00	63.0
156.90	70.0
158.80	82.0
160.80	72.0
162.90	178.0
164.90	83.0
171.50	55.0
172.20	147.0
173.90	27208.0
175.00	2359.0
175.90	26856.0
176.90	2300.0
178.00	168.0
178.90	198.0
189.00	67.0
191.00	943.0
191.90	194.0
192.90	977.0
194.00	277.0

Instrument :
MSVOA_W
ClientSampleId :
BFB489

195.00	205.0
203.00	109.0
205.10	234.0
207.00	658.0
208.00	126.0
208.90	62.0
234.80	139.0
249.00	561.0
250.00	149.0
250.90	309.0
252.00	72.0
265.00	682.0
265.90	239.0
267.00	164.0
279.00	58.0
281.00	9462.0
282.00	2864.0
283.00	1398.0
284.10	382.0
284.90	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB489

m/z	Abundance
35.90	290.0
37.00	1687.0
38.00	1466.0
39.00	539.0
40.00	60.0
43.10	62.0
44.10	316.0
45.00	361.0
47.00	276.0
48.00	197.0
49.00	1338.0
50.00	6060.0
51.00	1848.0
51.90	111.0
54.90	105.0
56.00	685.0
57.00	1185.0
59.00	93.0
60.00	391.0
61.00	1697.0
62.00	1645.0
63.00	1367.0
64.10	144.0
64.90	55.0
66.90	95.0
68.00	3097.0
69.00	3667.0
69.90	294.0
72.10	273.0
73.00	1889.0
74.00	6103.0
75.00	17224.0
76.00	1439.0
77.10	191.0
78.00	120.0
78.90	1430.0
80.00	458.0
80.90	1707.0
82.00	338.0
86.90	1169.0
88.00	1253.0
88.90	64.0
91.00	156.0
92.00	1018.0
93.00	1640.0
94.00	4208.0
95.00	32832.0
96.00	2025.0
96.90	135.0
103.00	73.0
103.90	177.0
104.90	73.0
105.90	200.0
110.90	97.0
115.00	74.0
115.90	124.0
116.90	320.0
118.00	189.0
118.90	297.0
125.00	127.0
127.90	148.0
129.80	162.0
130.90	67.0
133.00	397.0
133.90	69.0
134.80	139.0
137.00	91.0
141.00	427.0
143.00	578.0
146.60	68.0
147.00	65.0
147.80	87.0
154.90	69.0
156.90	90.0
162.90	95.0
165.10	56.0
171.30	62.0
174.00	26664.0
174.90	2585.0
175.90	29464.0
176.90	2206.0
177.80	102.0
179.00	150.0
191.00	336.0
192.00	82.0
193.00	644.0
194.00	66.0
194.80	55.0
204.90	85.0
207.10	362.0
207.90	58.0
209.00	85.0

Instrument :
MSVOA_W
ClientSampleId :
BFB489

248.90	312.0
249.80	83.0
250.20	87.0
251.00	101.0
252.00	59.0
264.90	340.0
265.90	142.0
267.00	100.0
281.00	5324.0
281.90	1045.0
283.00	976.0
284.00	147.0
284.90	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB489