

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122722\
 Data File : VW025208.D
 Acq On : 27 Dec 2022 10:31
 Operator : SY/MD
 Sample : VW1227SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK452

Quant Time: Dec 28 00:52:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 28 00:52:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	593230	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	512368	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	240622	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	149037	21.794	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.160%
7) Chloroethane-d5	2.885	69	106410	24.098	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.400%
11) 1,1-Dichloroethene-d2	4.013	63	264486	17.654	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.600%
21) 2-Butanone-d5	7.074	46	82427	48.011	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.020%
24) Chloroform-d	7.647	84	345578	22.568	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.280%
26) 1,2-Dichloroethane-d4	8.305	65	175761	22.633	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.520%
32) Benzene-d6	8.275	84	758671	25.249	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.000%
36) 1,2-Dichloropropane-d6	9.274	67	223254	25.535	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.160%
41) Toluene-d8	10.323	98	676450	24.830	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.320%
43) trans-1,3-Dichloroprop...	10.579	79	85512	23.154	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.600%
47) 2-Hexanone-d5	10.920	63	66489	51.833	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.660%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	156155	24.186	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	206632	25.335	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.360%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	17422	2.095	ug/L	# 8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122722\
Data File : VW025208.D
Acq On : 27 Dec 2022 10:31
Operator : SY/MD
Sample : VW1227SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK452

Quant Time: Dec 28 00:52:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 28 00:52:08 2022
Response via : Initial Calibration

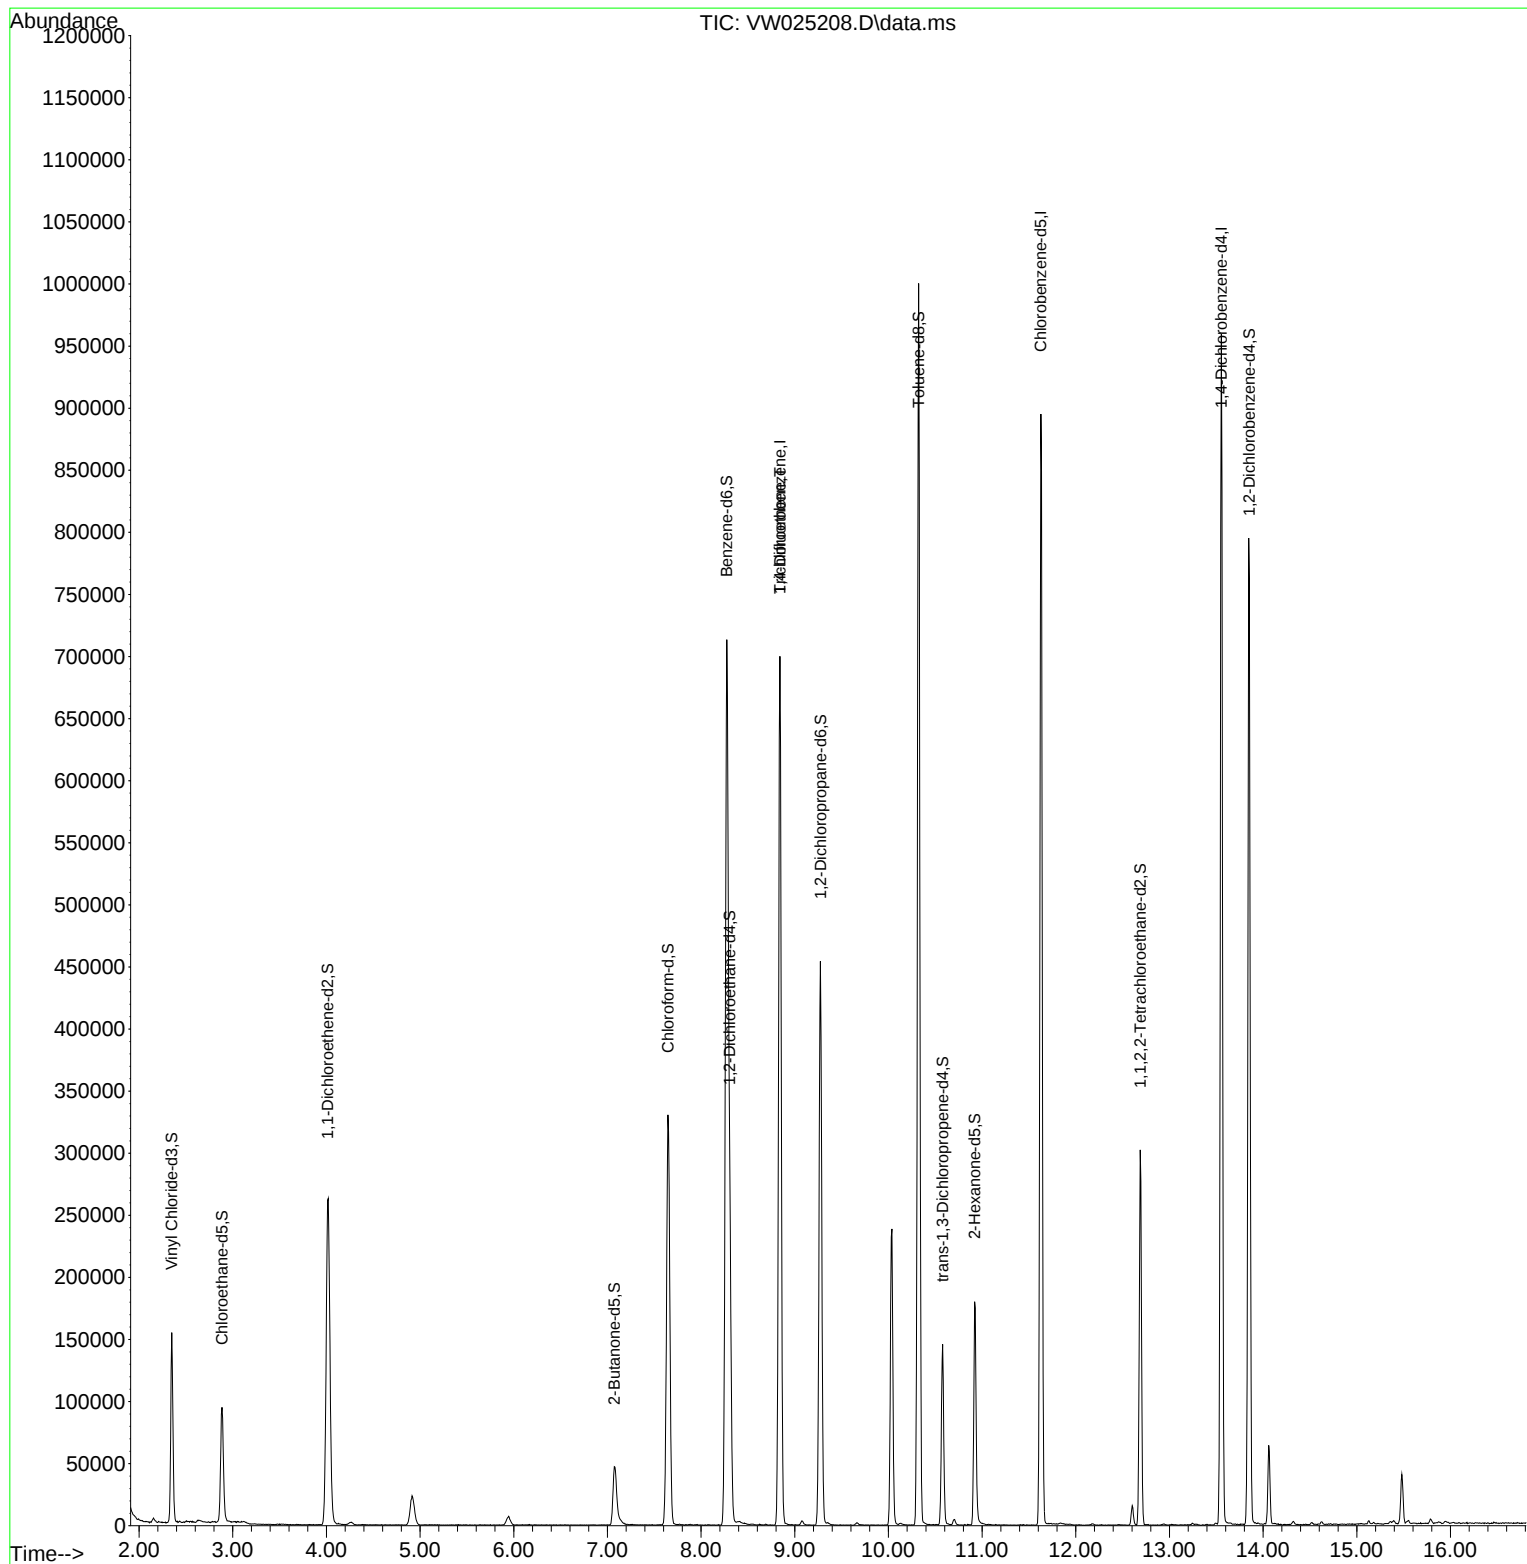

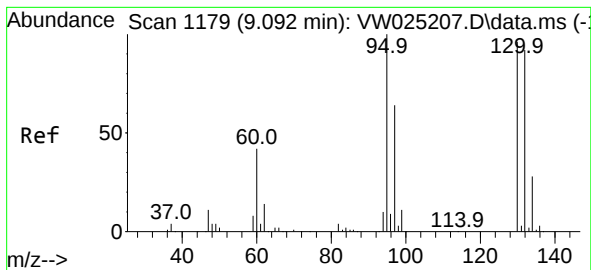

#34

Trichloroethene

Concen: 2.095 ug/L

RT: 8.842 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW025208.D


Acq: 27 Dec 2022 10:31

Instrument :

MSVOA_W

ClientSampleId :

VBLK452

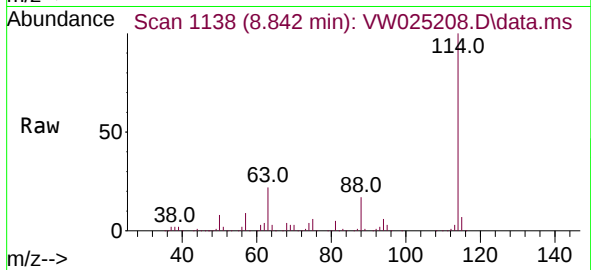

Tgt Ion: 95 Resp: 17422

Ion Ratio Lower Upper

95 100

97 0.0 44.3 82.3#

132 0.0 63.0 117.0#

130 0.0 63.4 117.8#

