

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122724\
 Data File : VW031548.D
 Acq On : 27 Dec 2024 13:42
 Operator : SY/MD
 Sample : P5333-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 27 22:22:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 27 22:18:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	505653	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	446590	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	213739	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	160759	21.130	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.520%
7) Chloroethane-d5	2.893	69	142600	25.338	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.360%
11) 1,1-Dichloroethene-d2	4.015	65	73766	20.440	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.760%
21) 2-Butanone-d5	7.100	46	80155	55.943	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.880%
24) Chloroform-d	7.648	84	348083	25.124	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.480%
26) 1,2-Dichloroethane-d4	8.569	65	40	0.006	ug/L	0.26
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.270	84	680110	23.760	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.040%
36) 1,2-Dichloropropane-d6	9.270	67	209624	25.128	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.520%
41) Toluene-d8	10.319	98	618111	23.212	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.840%
43) trans-1,3-Dichloroprop...	10.575	79	76638	19.924	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.680%
47) 2-Hexanone-d5	10.922	63	61812	55.096	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	156112	29.804	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	119.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	210278	26.501	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.000%
Target Compounds					Qvalue	
25) Chloroform	7.673	83	4571	0.371	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122724\
Data File : VW031548.D
Acq On : 27 Dec 2024 13:42
Operator : SY/MD
Sample : P5333-10
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 27 22:22:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 27 22:18:12 2024
Response via : Initial Calibration

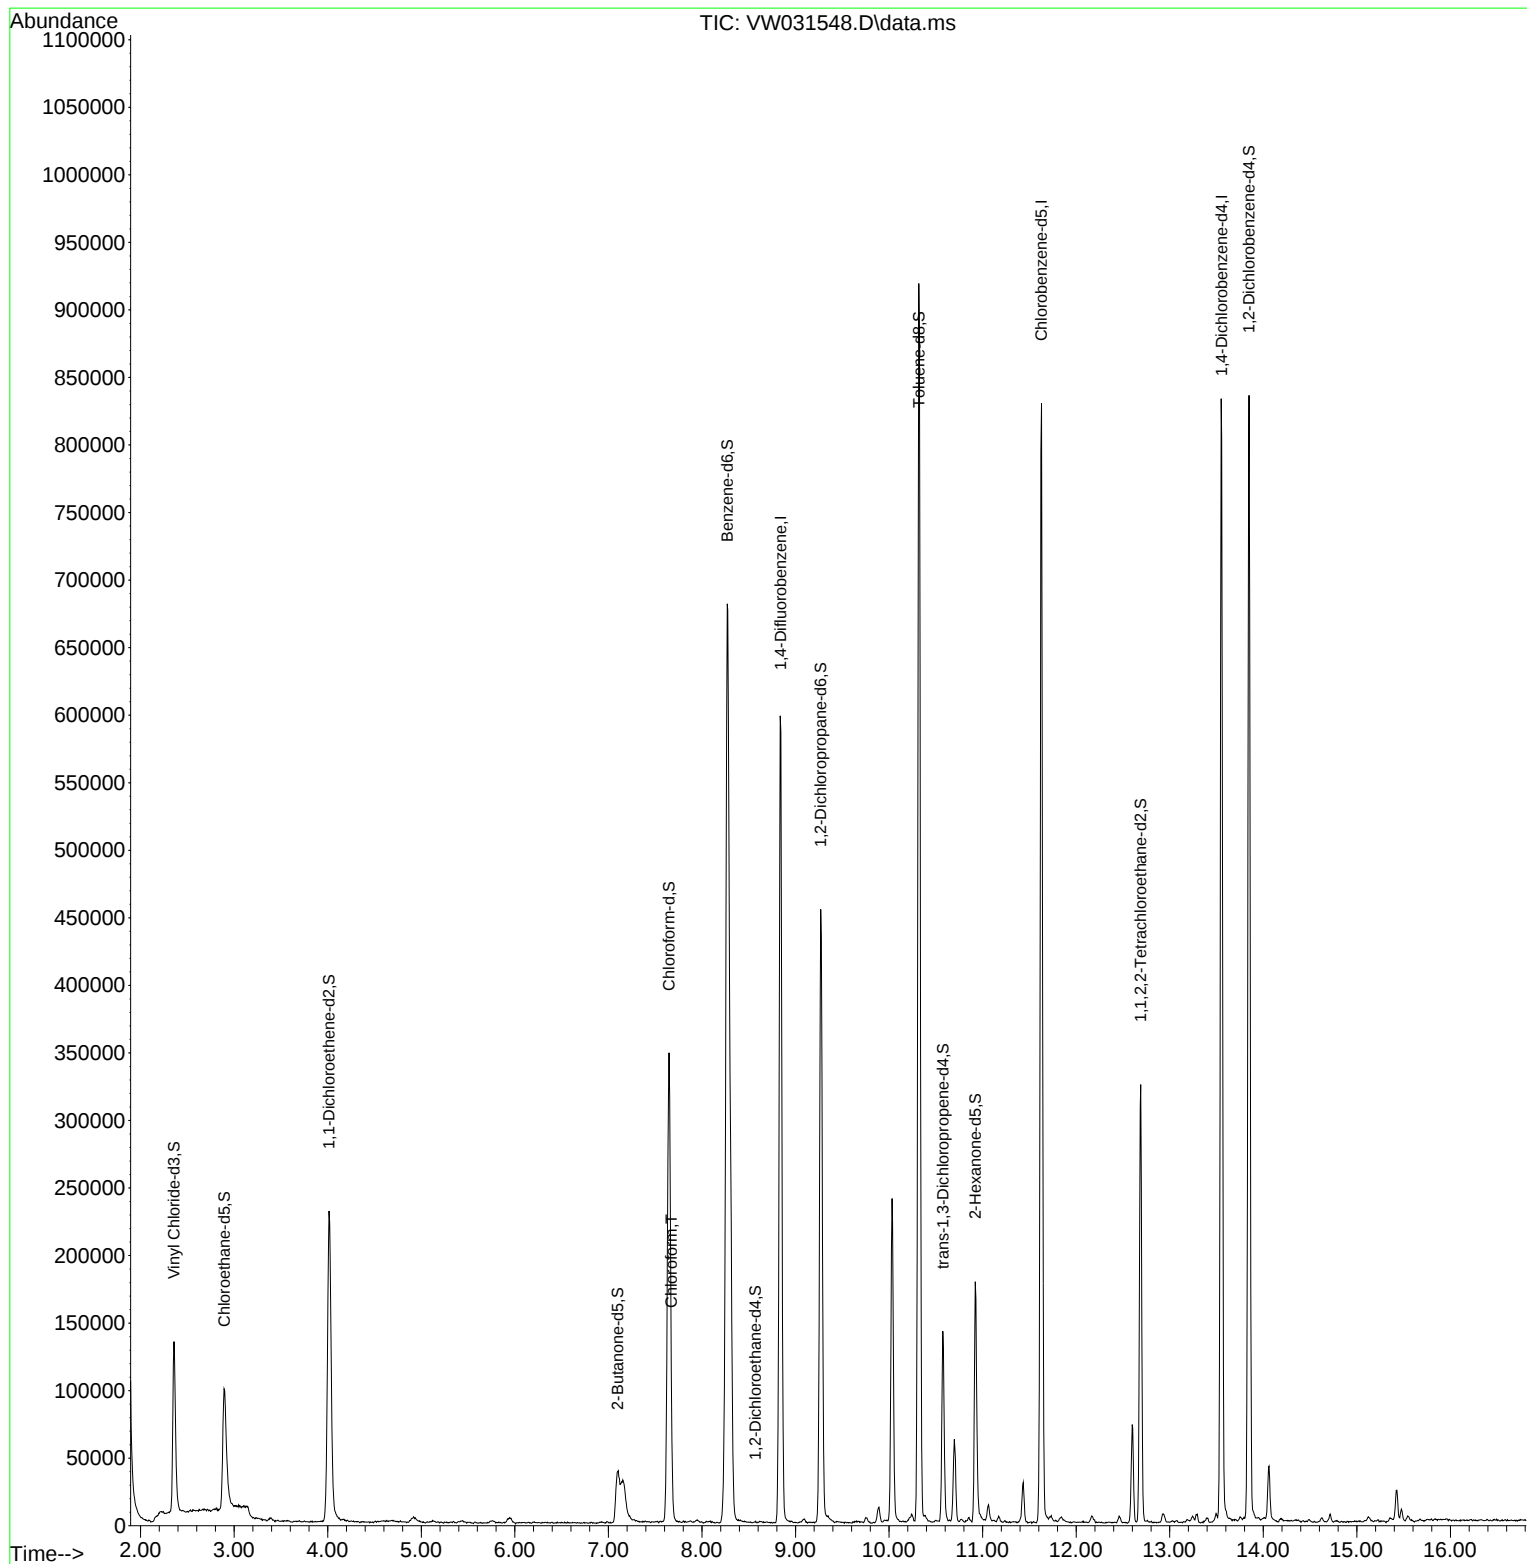

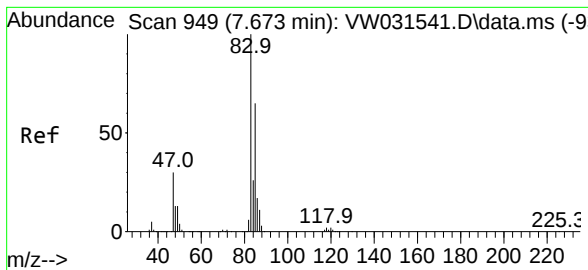

#25
 Chloroform
 Concen: 0.371 ug/L
 RT: 7.673 min Scan# 94
 Delta R.T. -0.000 min
 Lab File: VW031548.D
 Acq: 27 Dec 2024 13:42

Instrument :
 MSVOA_W
 ClientSampleId :

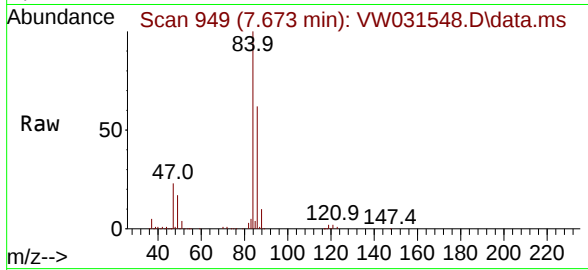

Tgt Ion: 83 Resp: 4571
 Ion Ratio Lower Upper
 83 100
 85 77.1 46.1 85.5

