

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122724\
 Data File : VW031551.D
 Acq On : 27 Dec 2024 15:12
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 27 22:23:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 27 22:18:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	482572	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	421851	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	209985	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	155010	21.349	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.400%
7) Chloroethane-d5	2.893	69	135732	25.271	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.080%
11) 1,1-Dichloroethene-d2	4.015	65	68990	20.031	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.120%
21) 2-Butanone-d5	7.099	46	76390	55.865	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.740%
24) Chloroform-d	7.642	84	328400	24.837	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.360%
26) 1,2-Dichloroethane-d4	8.301	65	179067	26.967	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.880%
32) Benzene-d6	8.270	84	636565	23.543	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.160%
36) 1,2-Dichloropropane-d6	9.270	67	196246	24.904	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.600%
41) Toluene-d8	10.318	98	582292	23.149	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.600%
43) trans-1,3-Dichloroprop...	10.575	79	74401	20.476	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.920%
47) 2-Hexanone-d5	10.922	63	62365	58.849	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.700%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	151090	30.537	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	122.160%#
66) 1,2-Dichlorobenzene-d4	13.848	152	207981	26.680	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.720%
Target Compounds						Qvalue
25) Chloroform	7.666	83	6270	0.533	ug/L	86
39) cis-1,3-Dichloropropene	10.032	75	6514	0.593	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122724\
Data File : VW031551.D
Acq On : 27 Dec 2024 15:12
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 27 22:23:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 27 22:18:12 2024
Response via : Initial Calibration




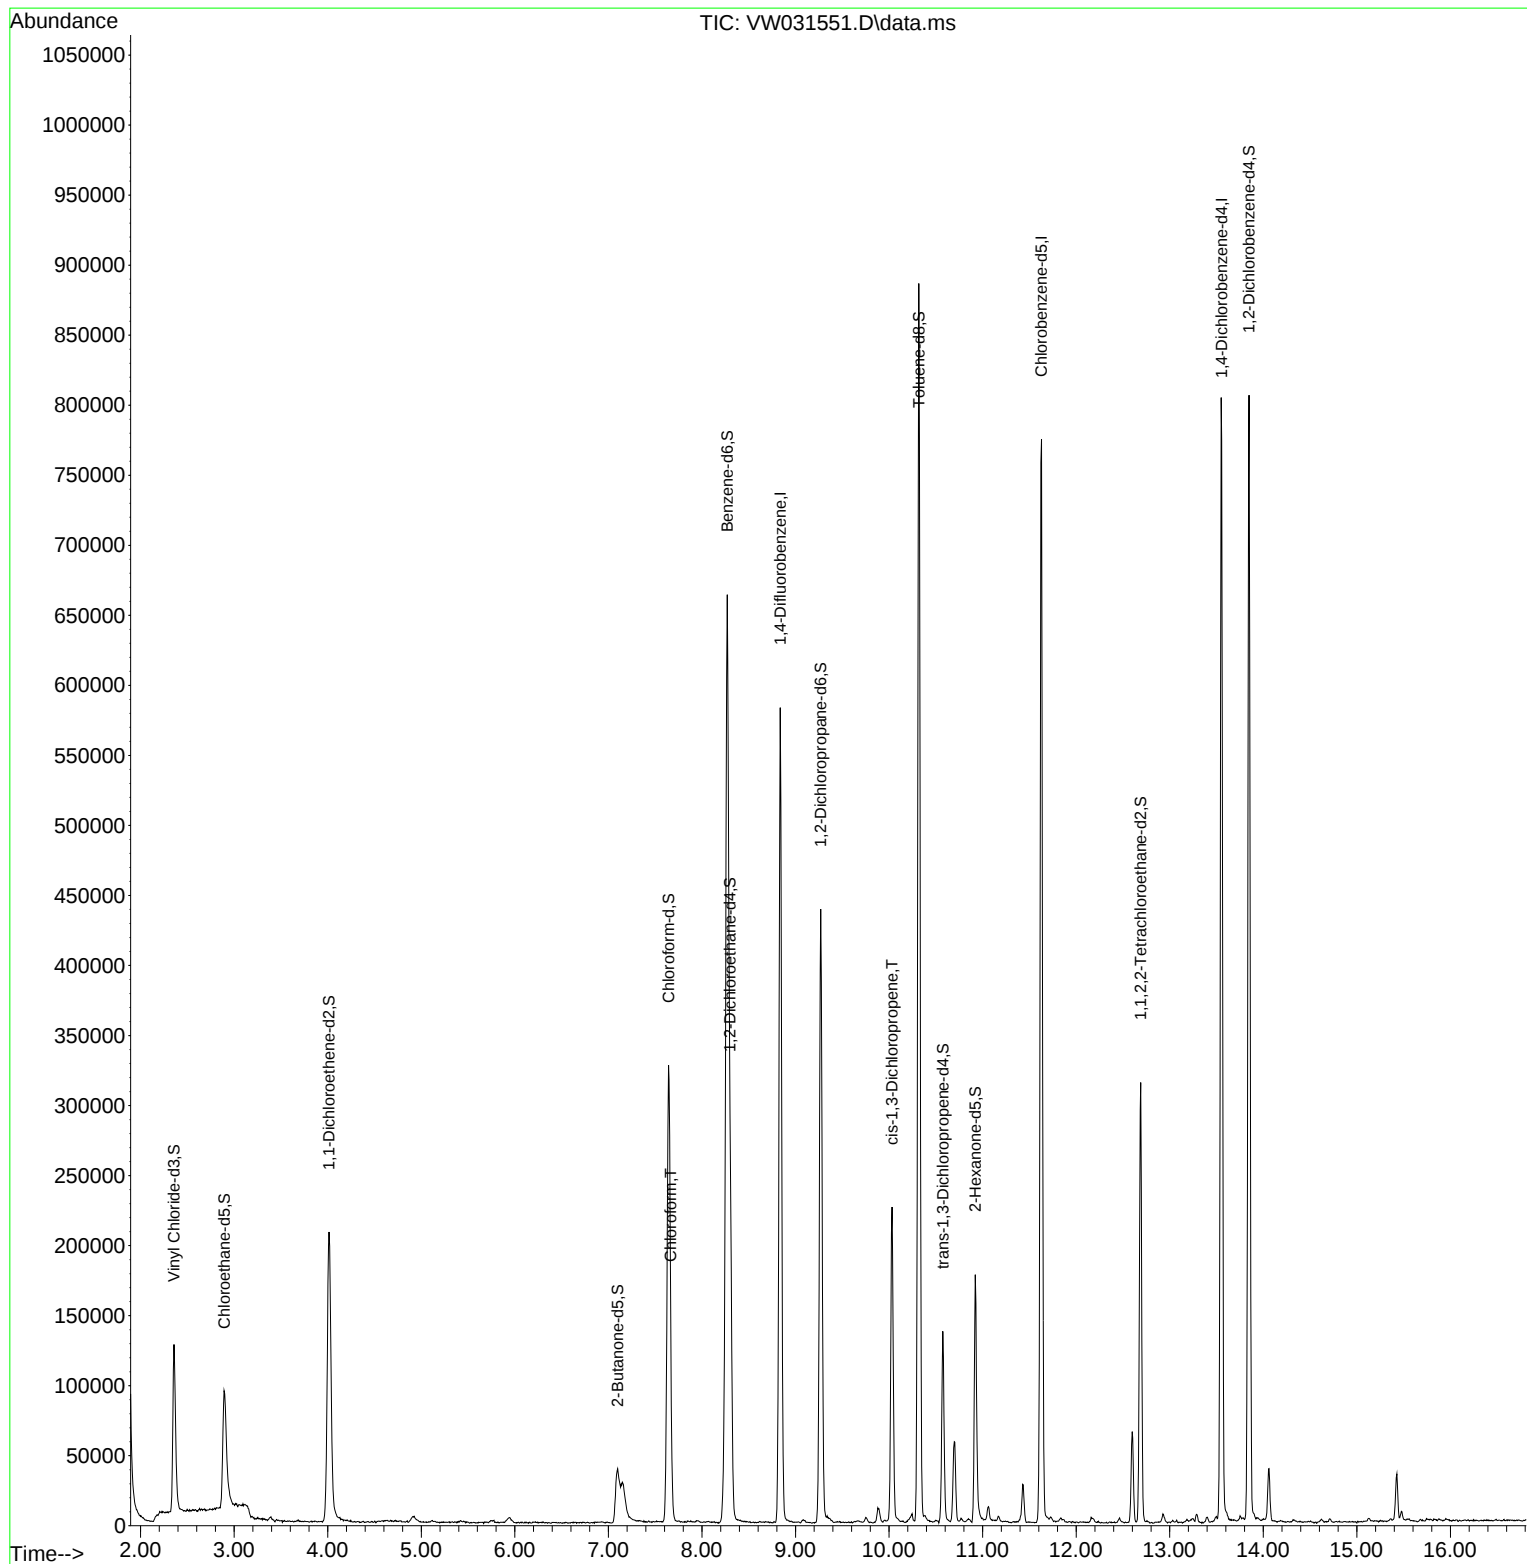


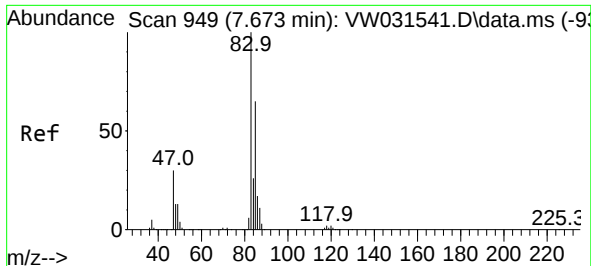

#25
Chloroform
Concen: 0.533 ug/L
RT: 7.666 min Scan# 94
Delta R.T. -0.006 min
Lab File: VW031551.D
Acq: 27 Dec 2024 15:12

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 83 Resp: 6270
Ion Ratio Lower Upper
83 100
85 77.3 46.1 85.5

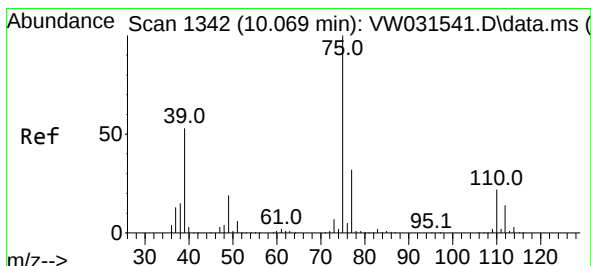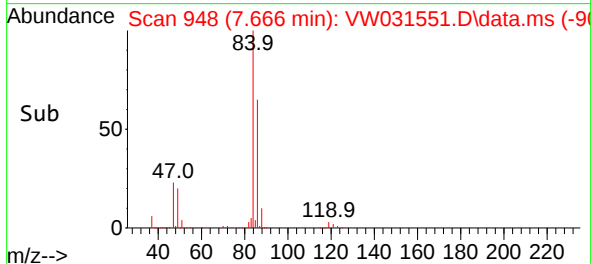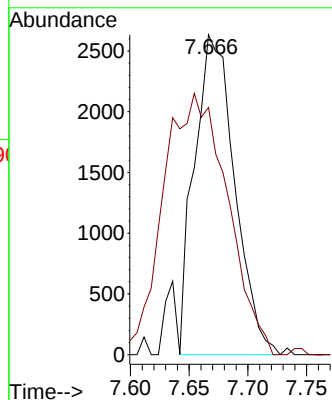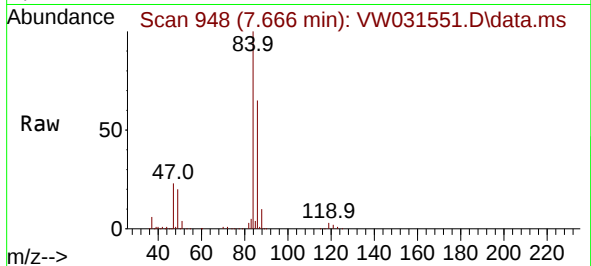

#39
cis-1,3-Dichloropropene
Concen: 0.593 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.037 min
Lab File: VW031551.D
Acq: 27 Dec 2024 15:12

Tgt Ion: 75 Resp: 6514
Ion Ratio Lower Upper
75 100
77 39.8 21.8 40.4

