
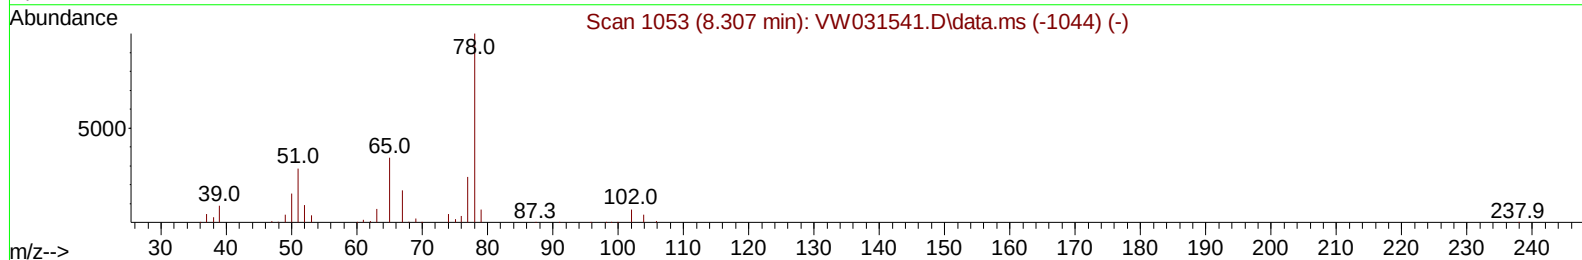
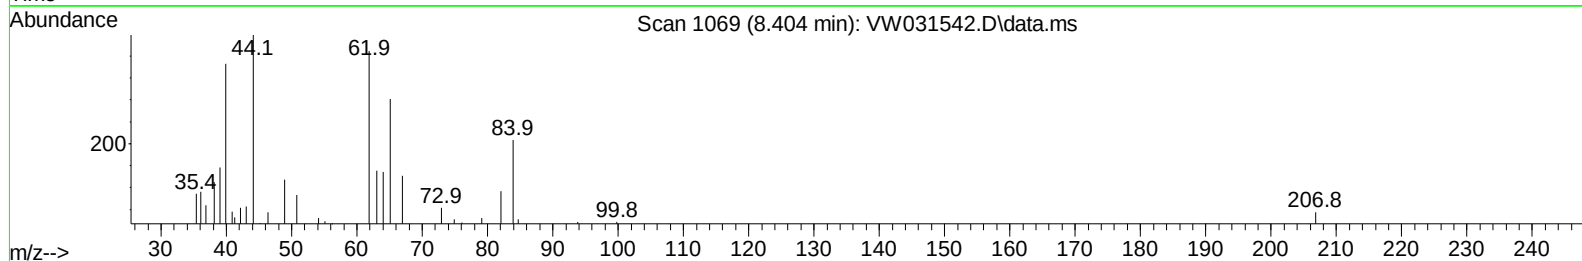


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122724\
Data File : VW031542.D
Acq On : 27 Dec 2024 11:11
Operator : SY/MD
Sample : VW1228SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 22:58:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 27 22:18:12 2024
Response via : Initial Calibration

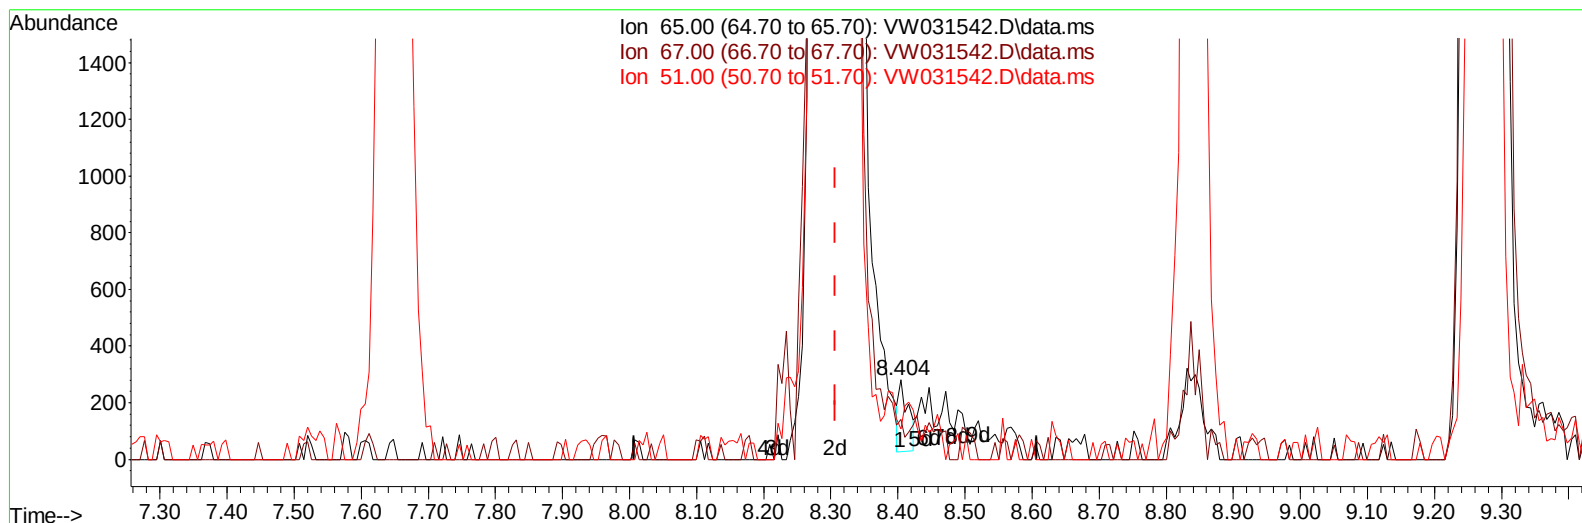

TIC: VW031542.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.404min (+ 0.097) 0.03 ug/L

response 245

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	57.55
51.00	108.10	131.43
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122724\
Data File : VW031542.D
Acq On : 27 Dec 2024 11:11
Operator : SY/MD
Sample : VW1228SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 22:58:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 27 22:18:12 2024
Response via : Initial Calibration

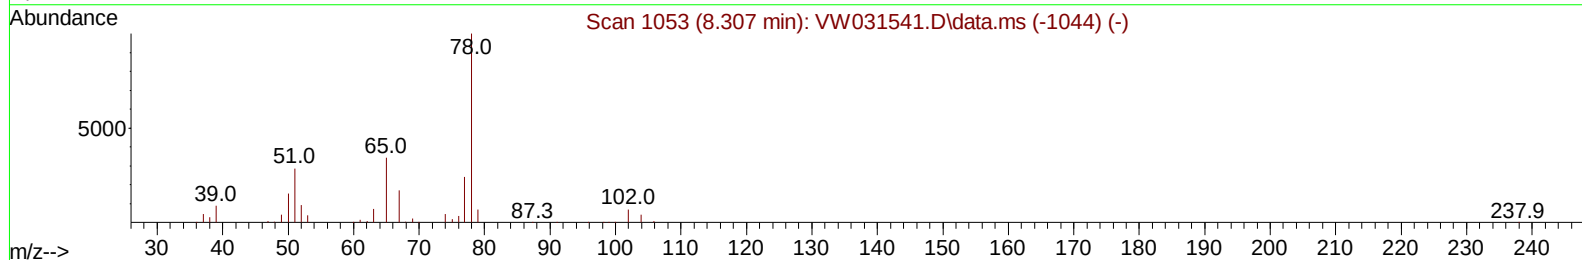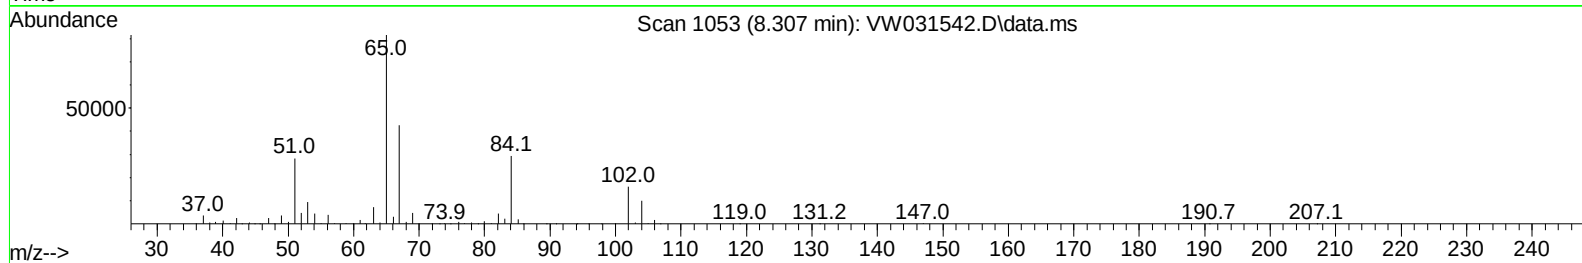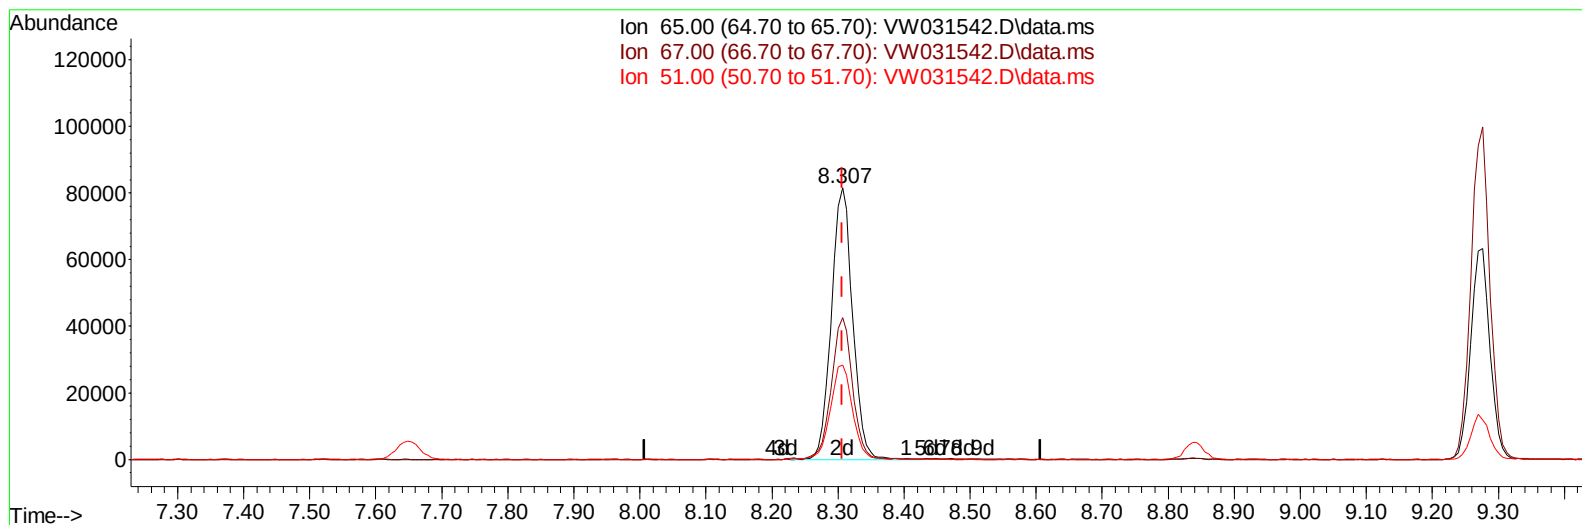

TIC: VW031542.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 25.24 ug/L m

response 182046

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.08#
51.00	108.10	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122724\
 Data File : VW031542.D
 Acq On : 27 Dec 2024 11:11
 Operator : SY/MD
 Sample : VW1228SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 22:58:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 27 22:18:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	524112	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	461236	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	230465	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	158903	20.150	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.600%	
7) Chloroethane-d5	2.899	69	140917	24.157	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.640%	
11) 1,1-Dichloroethene-d2	4.021	65	71602	19.142	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	76.560%	
21) 2-Butanone-d5	7.099	46	74929	50.454	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.900%	
24) Chloroform-d	7.648	84	340015	23.678	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	94.720%	
26) 1,2-Dichloroethane-d4	8.307	65	182046m	25.242	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	100.960%	
32) Benzene-d6	8.276	84	666760	22.554	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.200%	
36) 1,2-Dichloropropane-d6	9.276	67	199866	23.197	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.800%	
41) Toluene-d8	10.318	98	592735	21.552	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	86.200%	
43) trans-1,3-Dichloroprop...	10.574	79	75833	19.088	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	76.360%	
47) 2-Hexanone-d5	10.922	63	56904	49.111	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.220%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	146685	27.115	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.480%	
66) 1,2-Dichlorobenzene-d4	13.848	152	206485	24.134	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.520%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122724\
Data File : VW031542.D
Acq On : 27 Dec 2024 11:11
Operator : SY/MD
Sample : VW1228SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 22:58:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 27 22:18:12 2024
Response via : Initial Calibration

