




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122921\
 Data File : VW021690.D
 Acq On : 29 Dec 2021 14:56
 Operator : SY/VA
 Sample : M5171-15RE
 Misc : 6.22g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB1RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/30/2021
 Supervised By :Mahesh Dadoda 12/30/2021

Quant Time: Dec 30 01:19:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 30 01:18:20 2021
 Response via : Initial Calibration

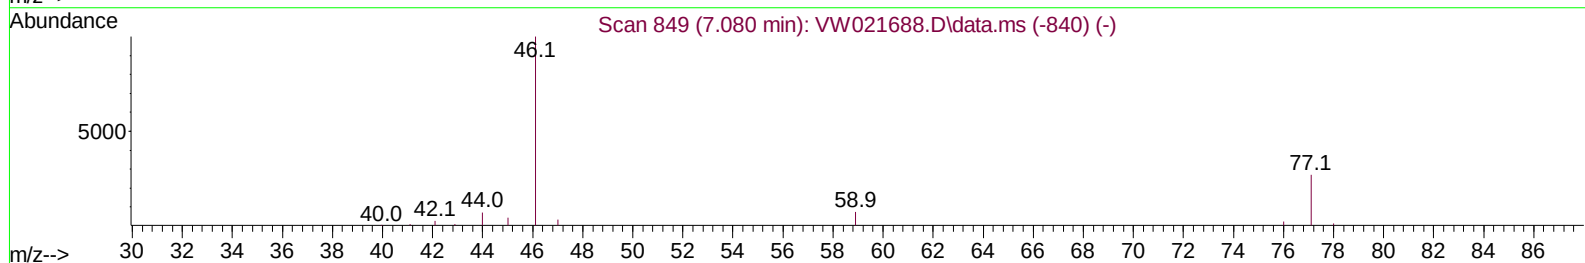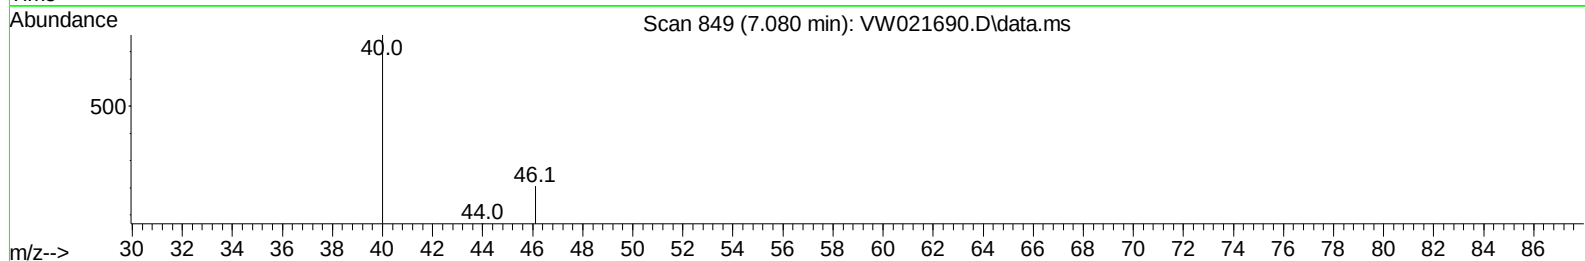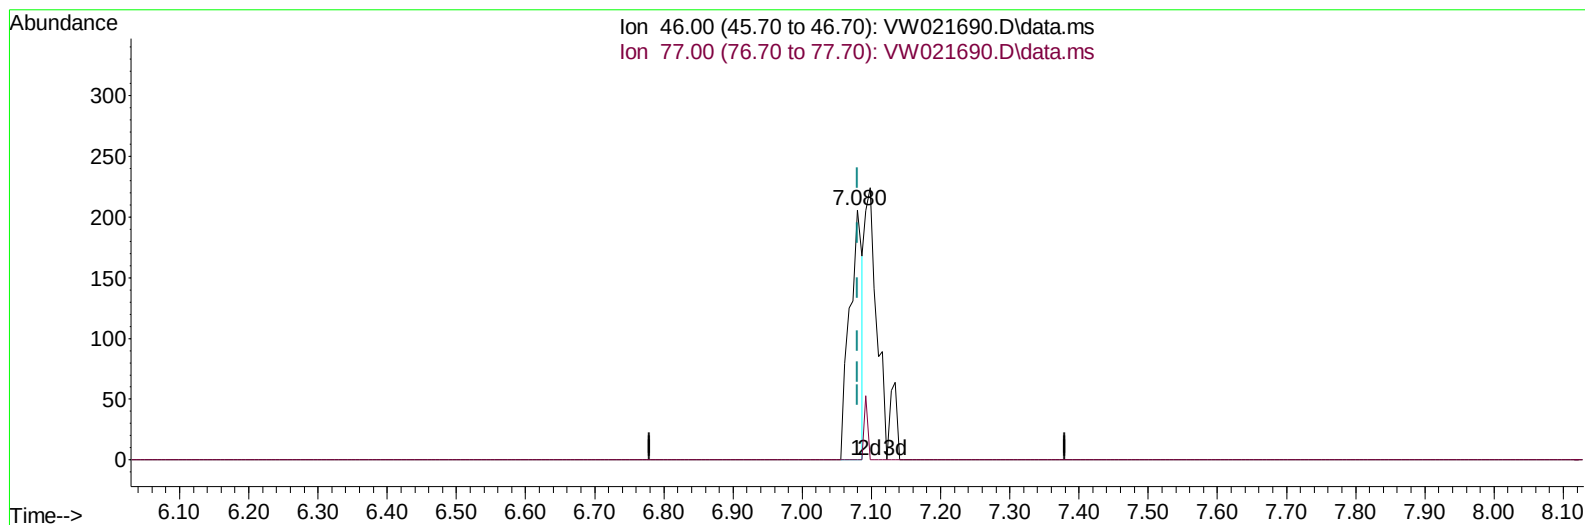

TIC: VW021690.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (-0.000) 19.11 ug/L

response 259

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122921\
 Data File : VW021690.D
 Acq On : 29 Dec 2021 14:56
 Operator : SY/VA
 Sample : M5171-15RE
 Misc : 6.22g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB1RE

Manual IntegrationsAPPROVED

Quant Time: Dec 30 01:19:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 30 01:18:20 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/30/2021
 Supervised By :Mahesh Dadoda 12/30/2021

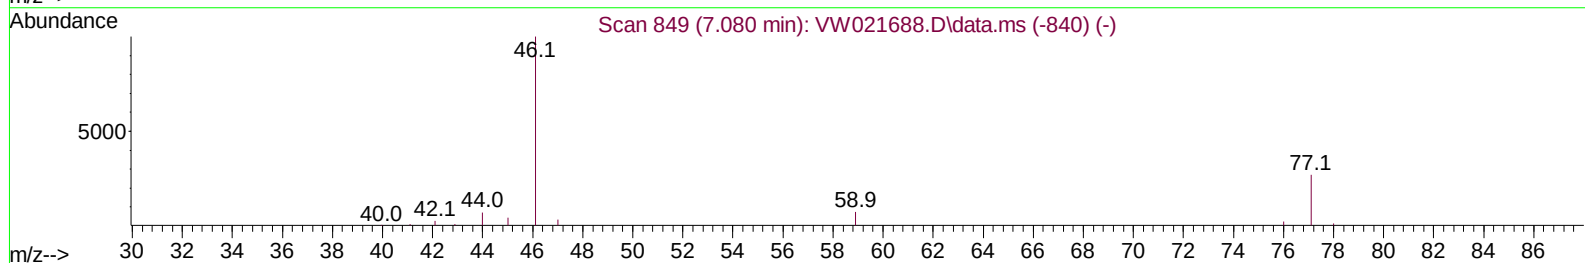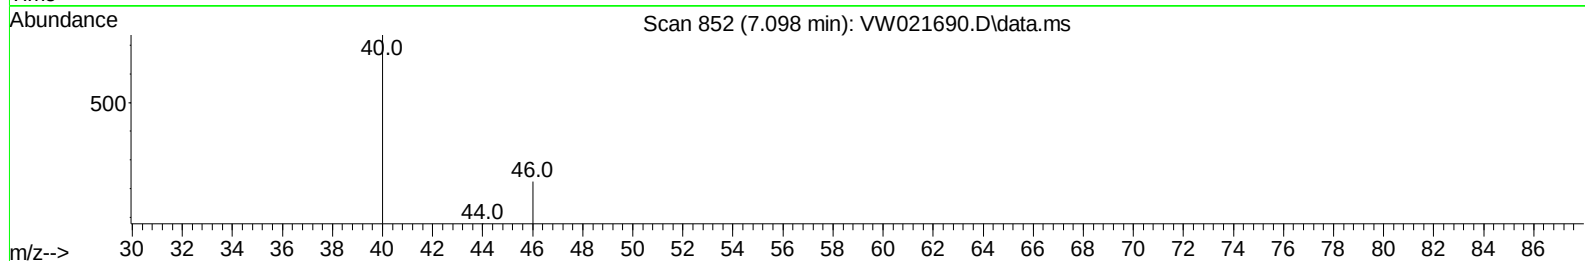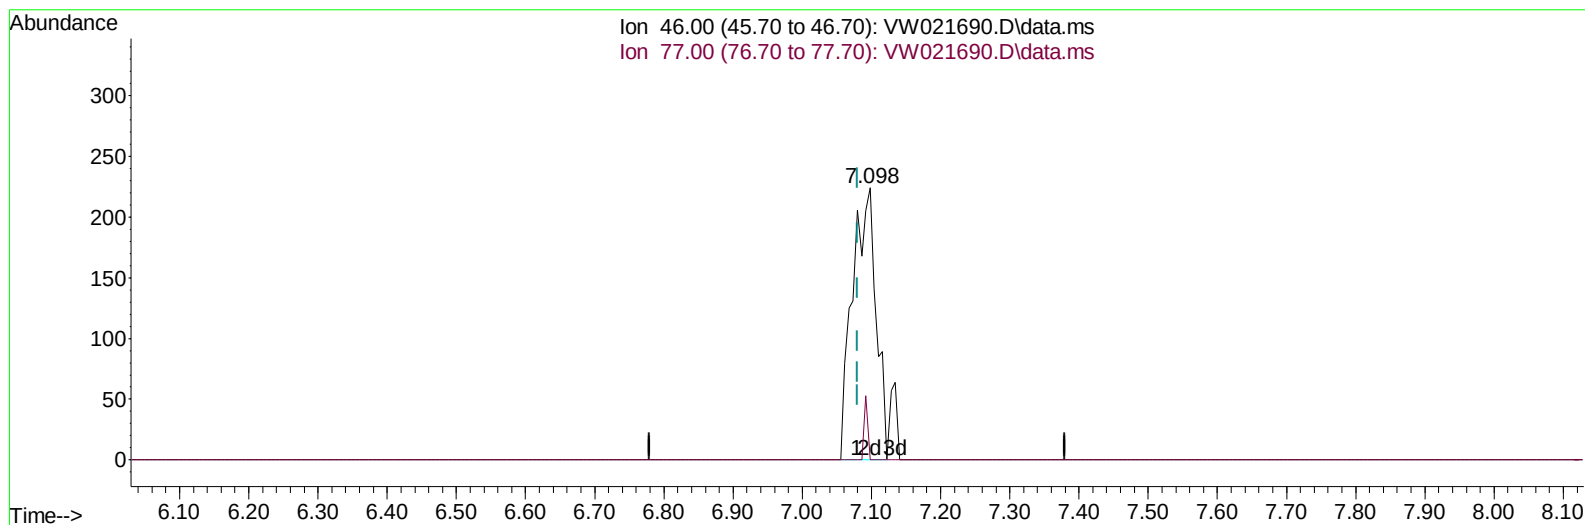

TIC: VW021690.D\data.ms

(21) 2-Butanone-d5 (S)

7.098min (+ 0.018) 39.26 ug/L m

response 532

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122921\
 Data File : VW021690.D
 Acq On : 29 Dec 2021 14:56
 Operator : SY/VA
 Sample : M5171-15RE
 Misc : 6.22g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLB1RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/30/2021
 Supervised By :Mahesh Dadoda 12/30/2021

Quant Time: Dec 30 01:19:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 30 01:18:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	4698	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	4375	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	2010	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	2572	27.767	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	111.080%	
7) Chloroethane-d5	2.897	69	1419	22.745	ug/L	0.02
Spiked Amount 25.000	Range 30	- 150	Recovery	=	90.960%	
11) 1,1-Dichloroethene-d2	4.031	63	2620	19.328	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	77.320%	
21) 2-Butanone-d5	7.098	46	532m	39.257	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	78.520%	
24) Chloroform-d	7.647	84	3494	23.809	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.240%	
26) 1,2-Dichloroethane-d4	8.305	65	1891	24.403	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.600%	
32) Benzene-d6	8.281	84	6090	23.443	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	93.760%	
36) 1,2-Dichloropropane-d6	9.274	67	1890	26.819	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	107.280%	
41) Toluene-d8	10.323	98	5535	21.385	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	85.520%	
43) trans-1,3-Dichloroprop...	10.579	79	788	22.980	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.920%	
47) 2-Hexanone-d5	10.927	63	221	20.678	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	41.360%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	1342	23.099	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	92.400%	
66) 1,2-Dichlorobenzene-d4	13.847	152	1862	24.225	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.880%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122921\
Data File : VW021690.D
Acq On : 29 Dec 2021 14:56
Operator : SY/VA
Sample : M5171-15RE
Misc : 6.22g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLB1RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/30/2021
Supervised By :Mahesh Dadoda 12/30/2021

Quant Time: Dec 30 01:19:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 30 01:18:20 2021
Response via : Initial Calibration

