

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122921\
 Data File : VW021691.D
 Acq On : 29 Dec 2021 15:20
 Operator : SY/VA
 Sample : VIBLK573
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK573

Quant Time: Dec 30 01:19:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 30 01:18:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	80288	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	80739	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	45998	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	41411	26.160	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.640%
7) Chloroethane-d5	2.879	69	26861	25.193	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.760%
11) 1,1-Dichloroethene-d2	4.013	63	39345	16.984	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.920%
21) 2-Butanone-d5	7.074	46	12044	52.004	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.000%
24) Chloroform-d	7.647	84	58213	23.211	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.840%
26) 1,2-Dichloroethane-d4	8.305	65	31857	24.055	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.240%
32) Benzene-d6	8.275	84	111903	23.342	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.360%
36) 1,2-Dichloropropane-d6	9.274	67	30567	23.504	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.000%
41) Toluene-d8	10.323	98	110470	23.127	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.520%
43) trans-1,3-Dichloroprop...	10.579	79	14419	22.785	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.120%
47) 2-Hexanone-d5	10.927	63	9833	49.854	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.700%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	26086	24.330	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	42287	24.040	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.160%
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	6894	4.810	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122921\
Data File : VW021691.D
Acq On : 29 Dec 2021 15:20
Operator : SY/VA
Sample : VIBLK573
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK573

Quant Time: Dec 30 01:19:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 30 01:18:20 2021
Response via : Initial Calibration

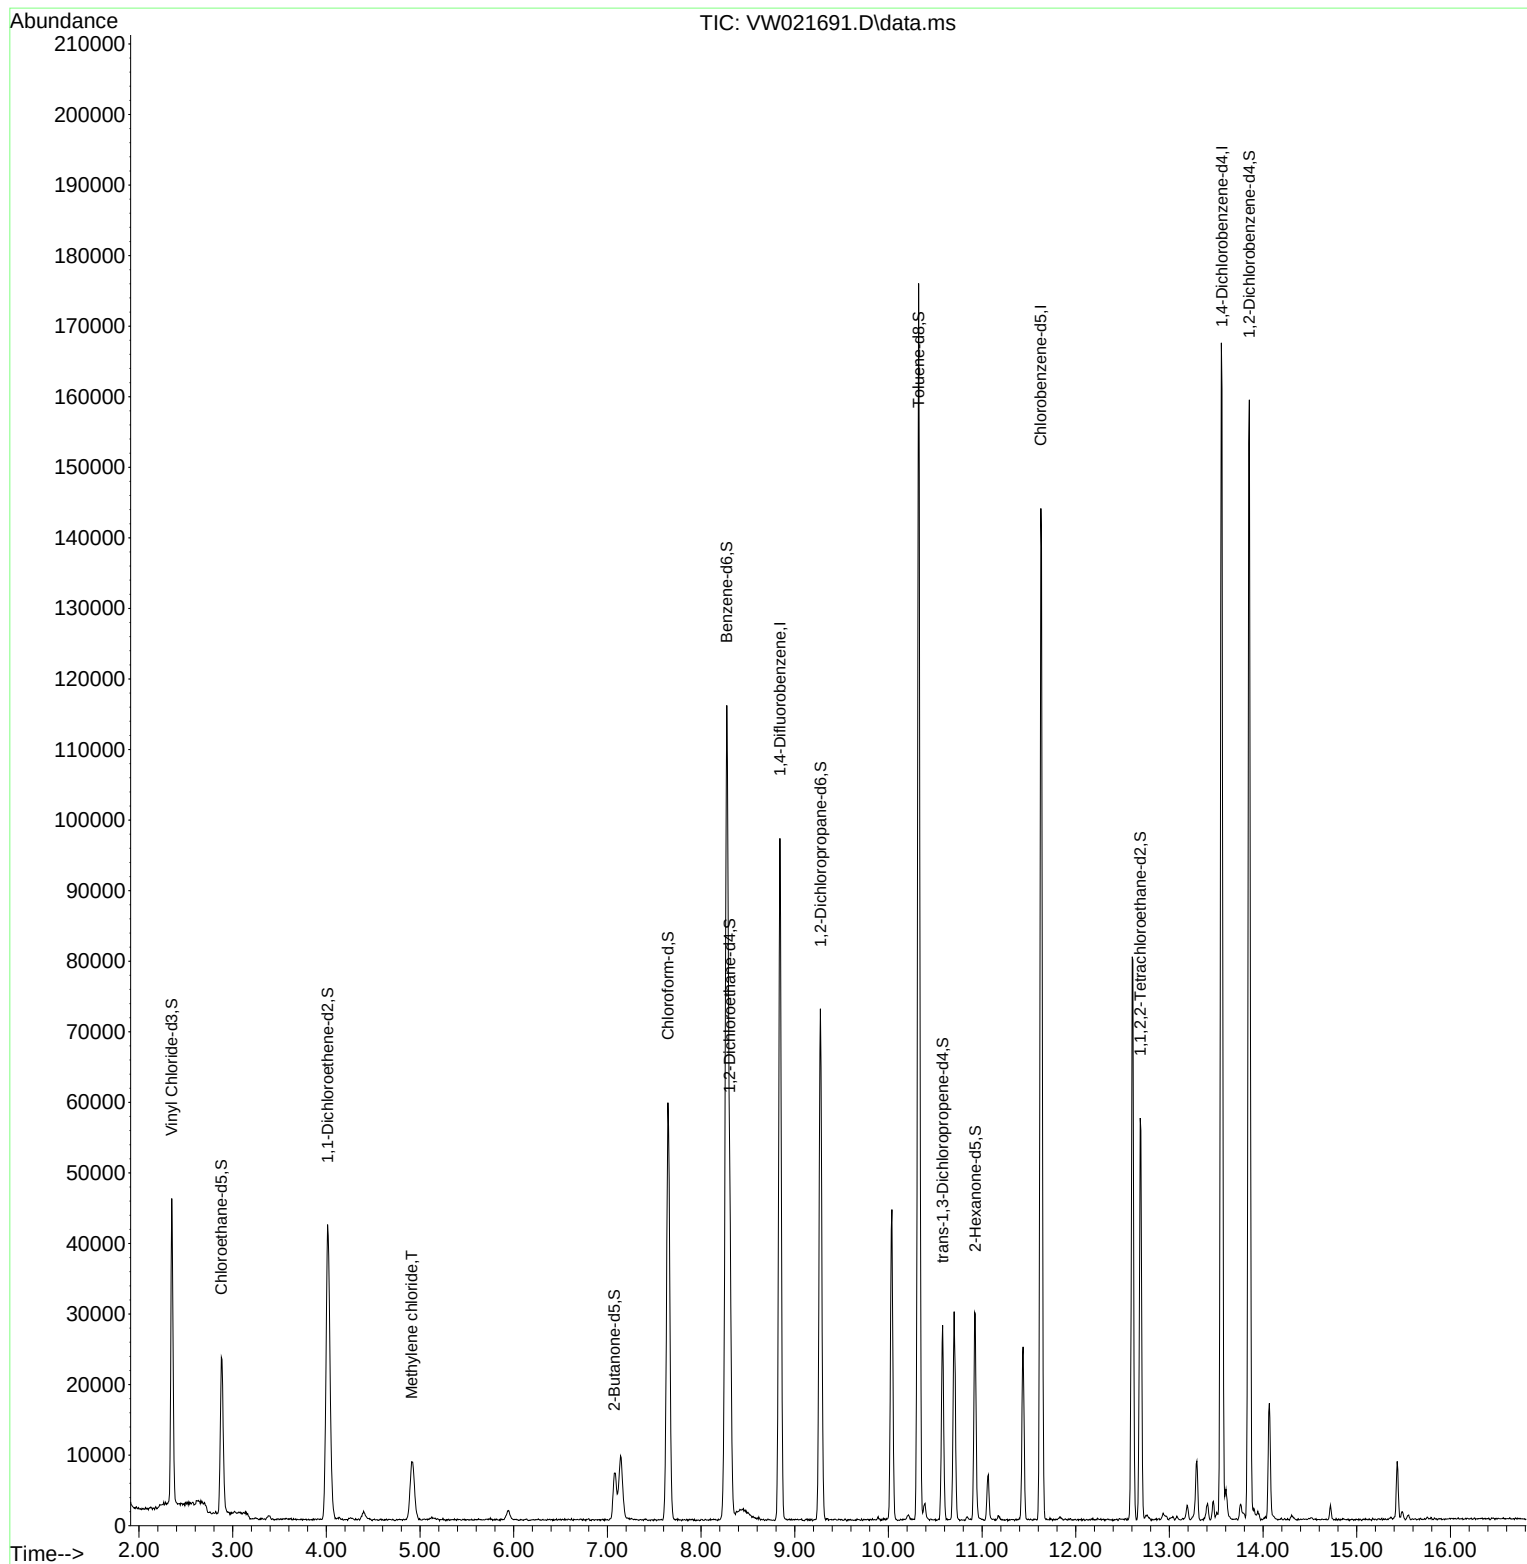

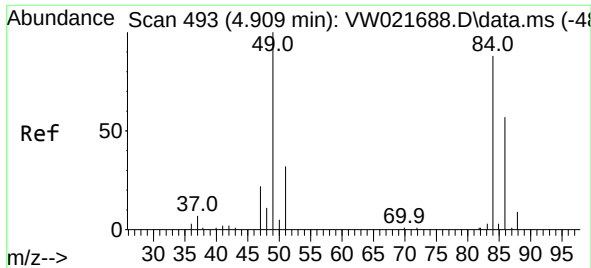

#16

Methylene chloride

Concen: 4.810 ug/L

RT: 4.909 min Scan# 49

Delta R.T. 0.000 min

Lab File: VW021691.D


Acq: 29 Dec 2021 15:20

Instrument :

MSVOA_W

ClientSampleId :

VIBLK573

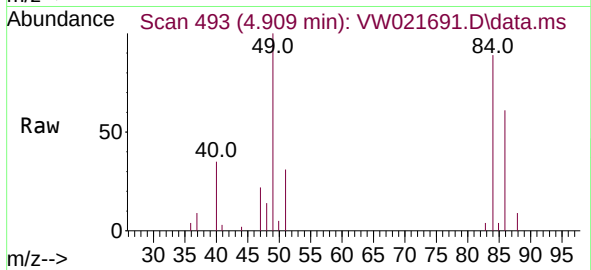

Tgt Ion: 84 Resp: 6894

Ion Ratio Lower Upper

84 100

86 69.2 45.5 84.5

49 112.9 100.5 186.7

