




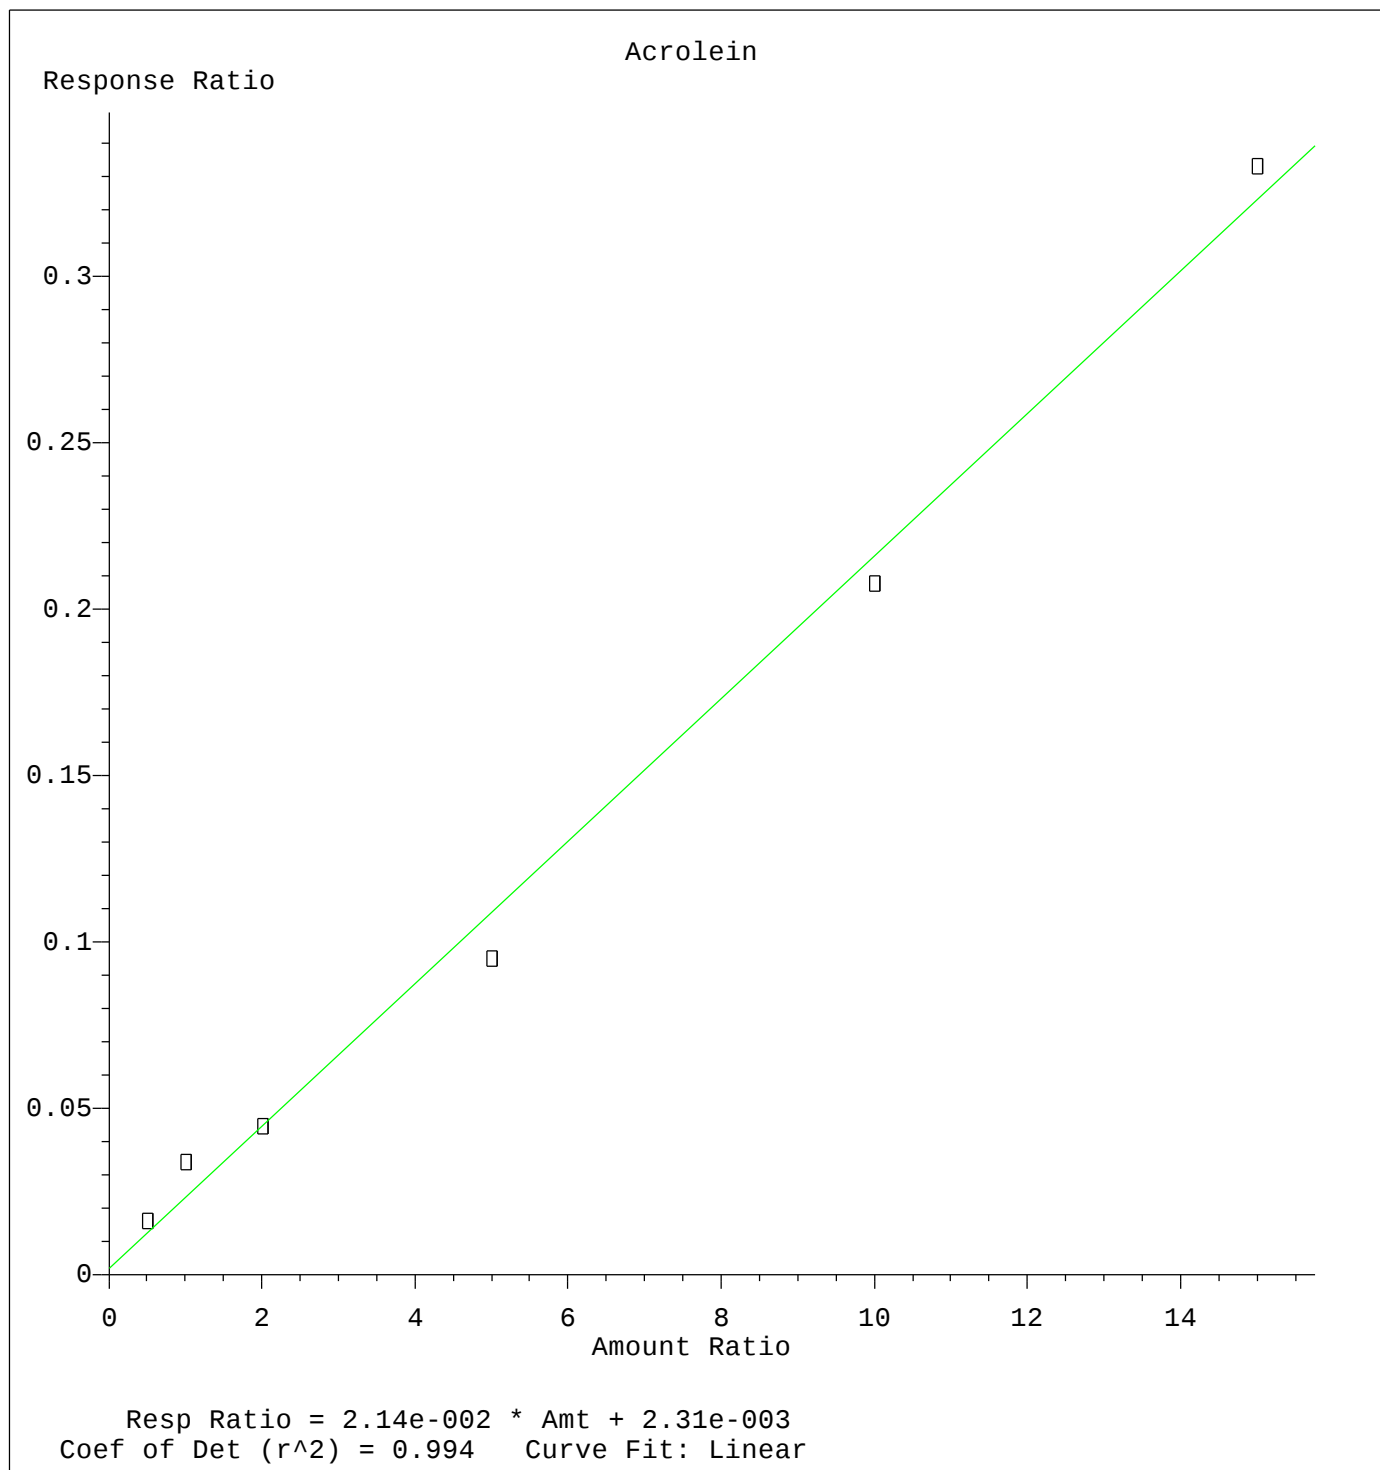

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019

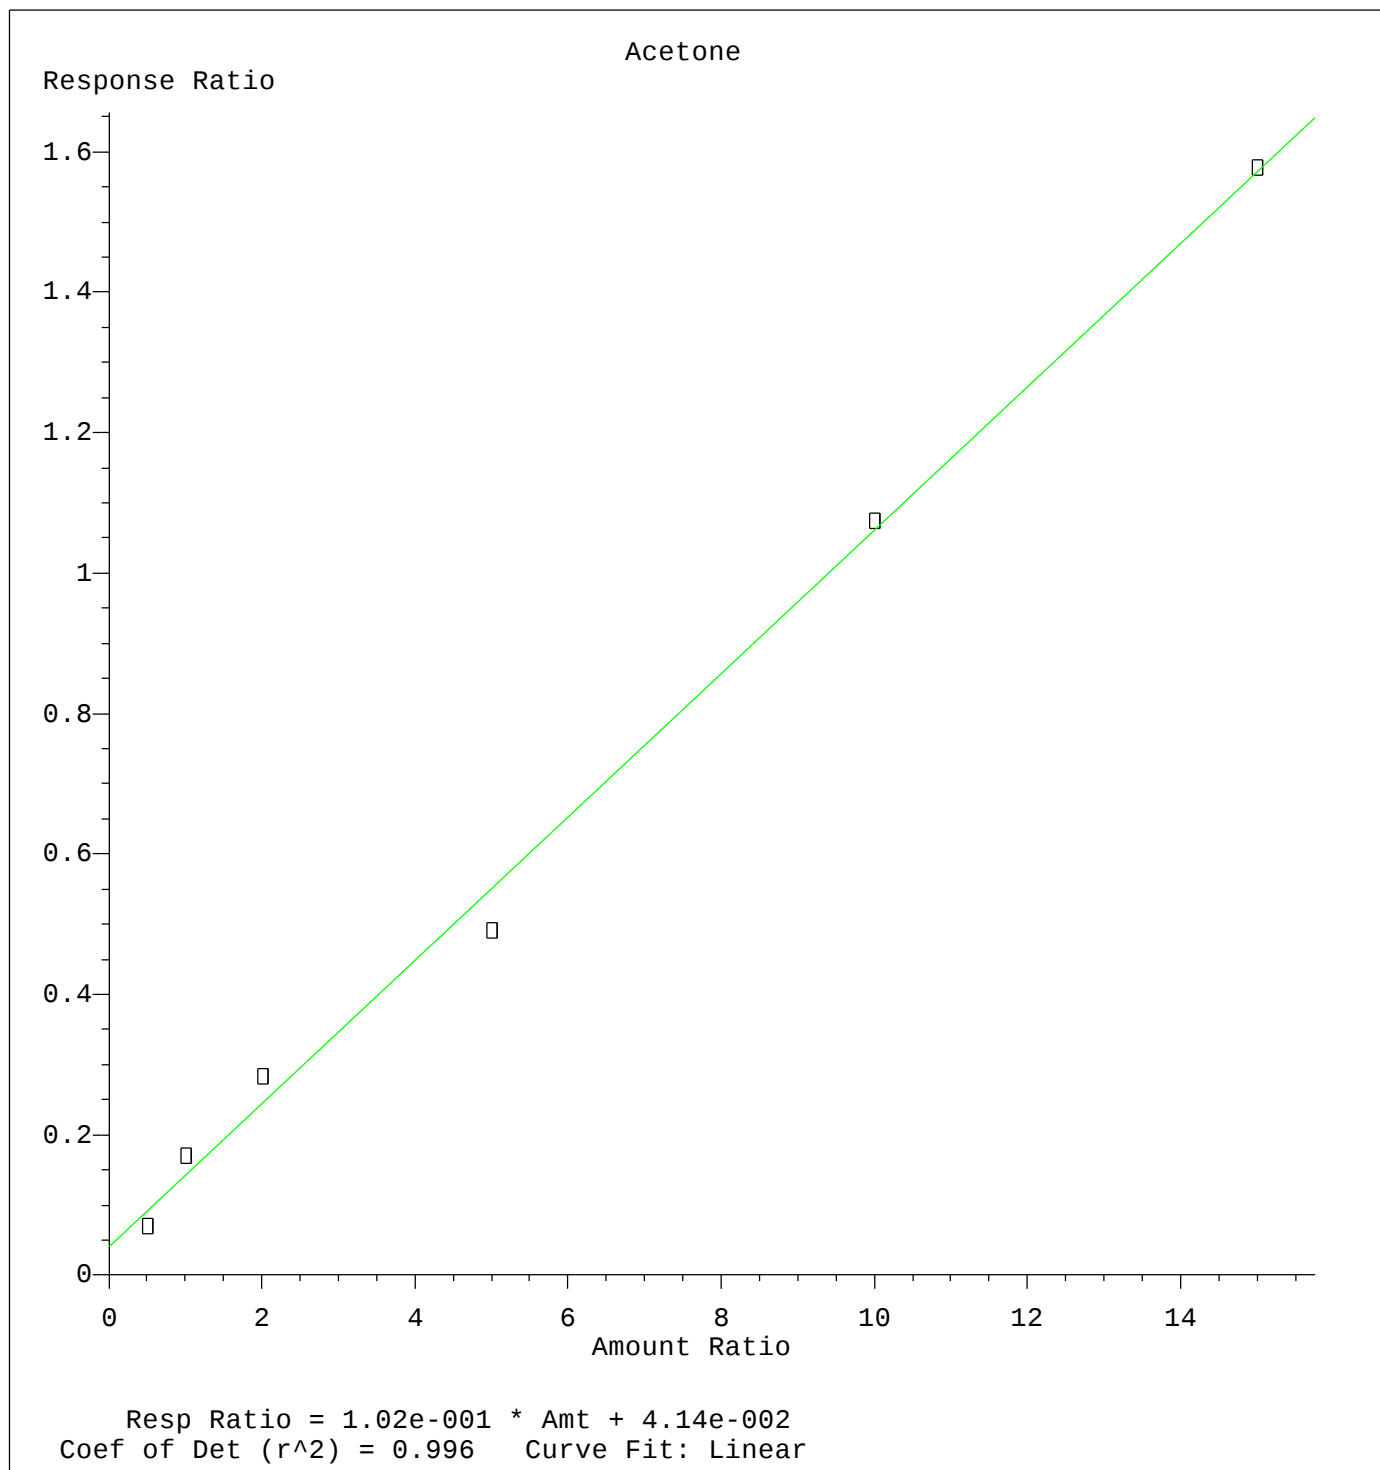


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019

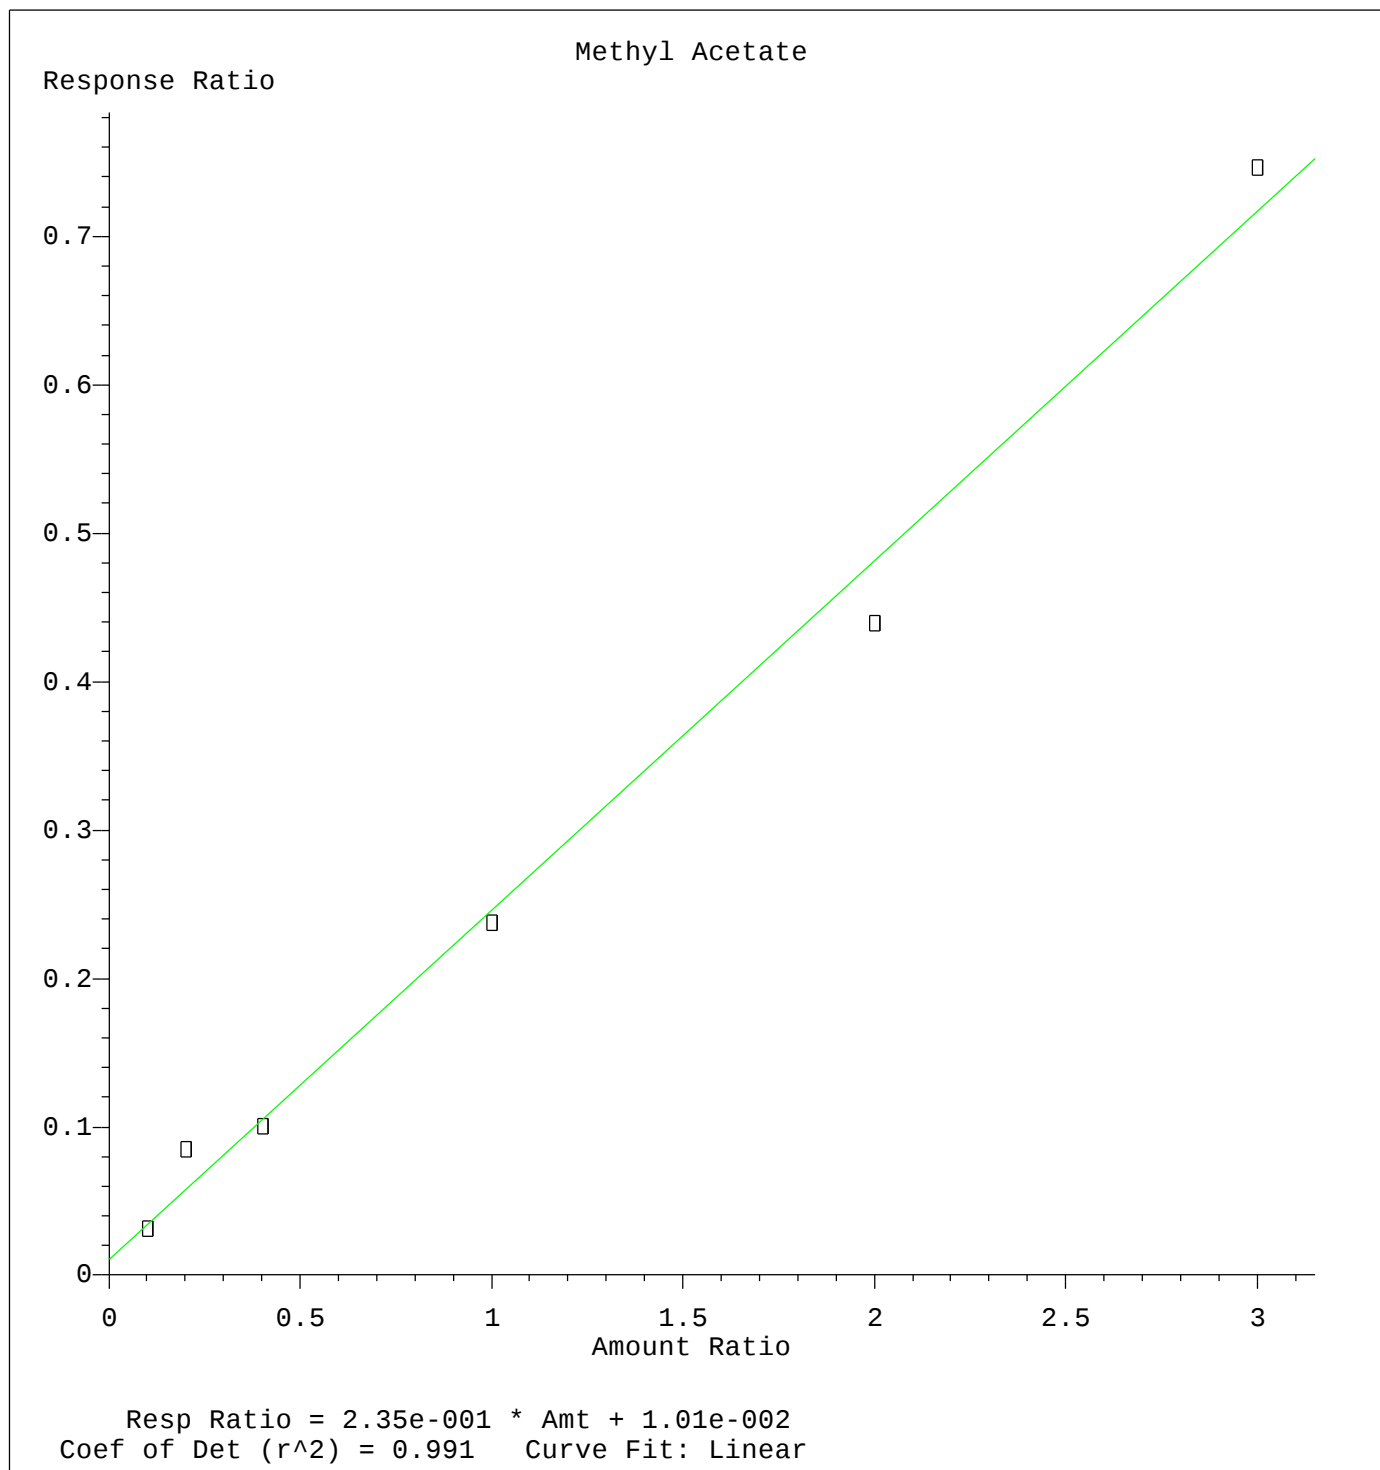

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019

Methylene Chloride

Response Ratio

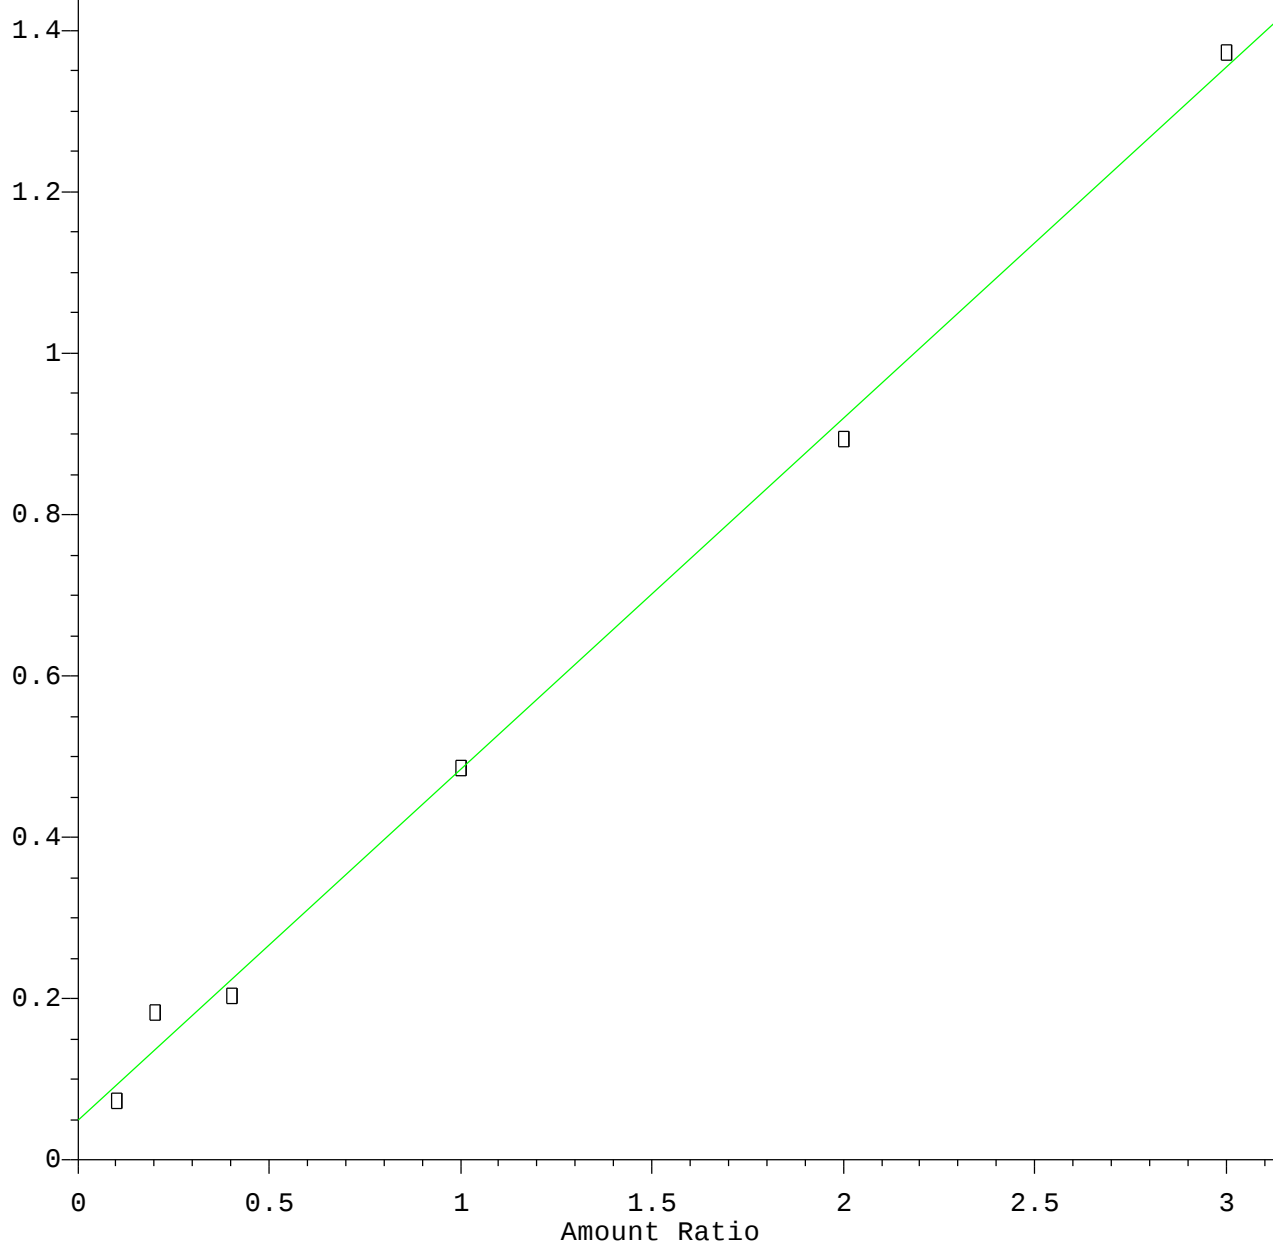


Resp Ratio = $4.35 \times 10^{-1} \times \text{Amt} + 4.89 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019


2-Butanone

Response Ratio

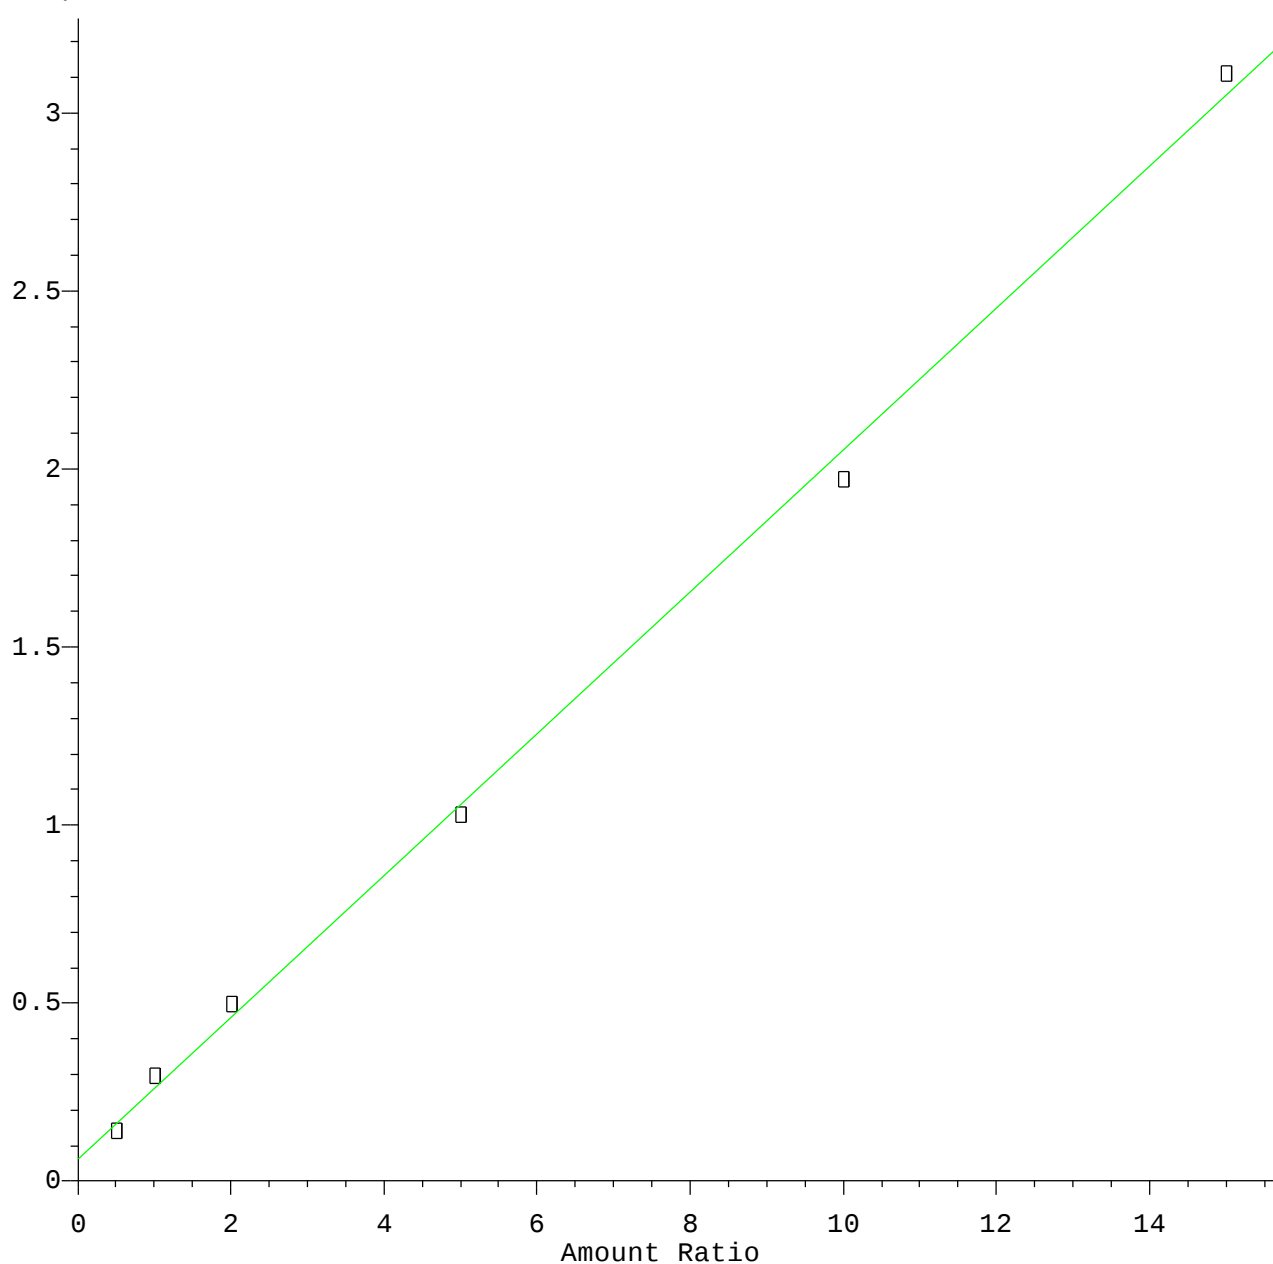


Resp Ratio = $1.99 \times 10^{-1} \times \text{Amt} + 5.99 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019

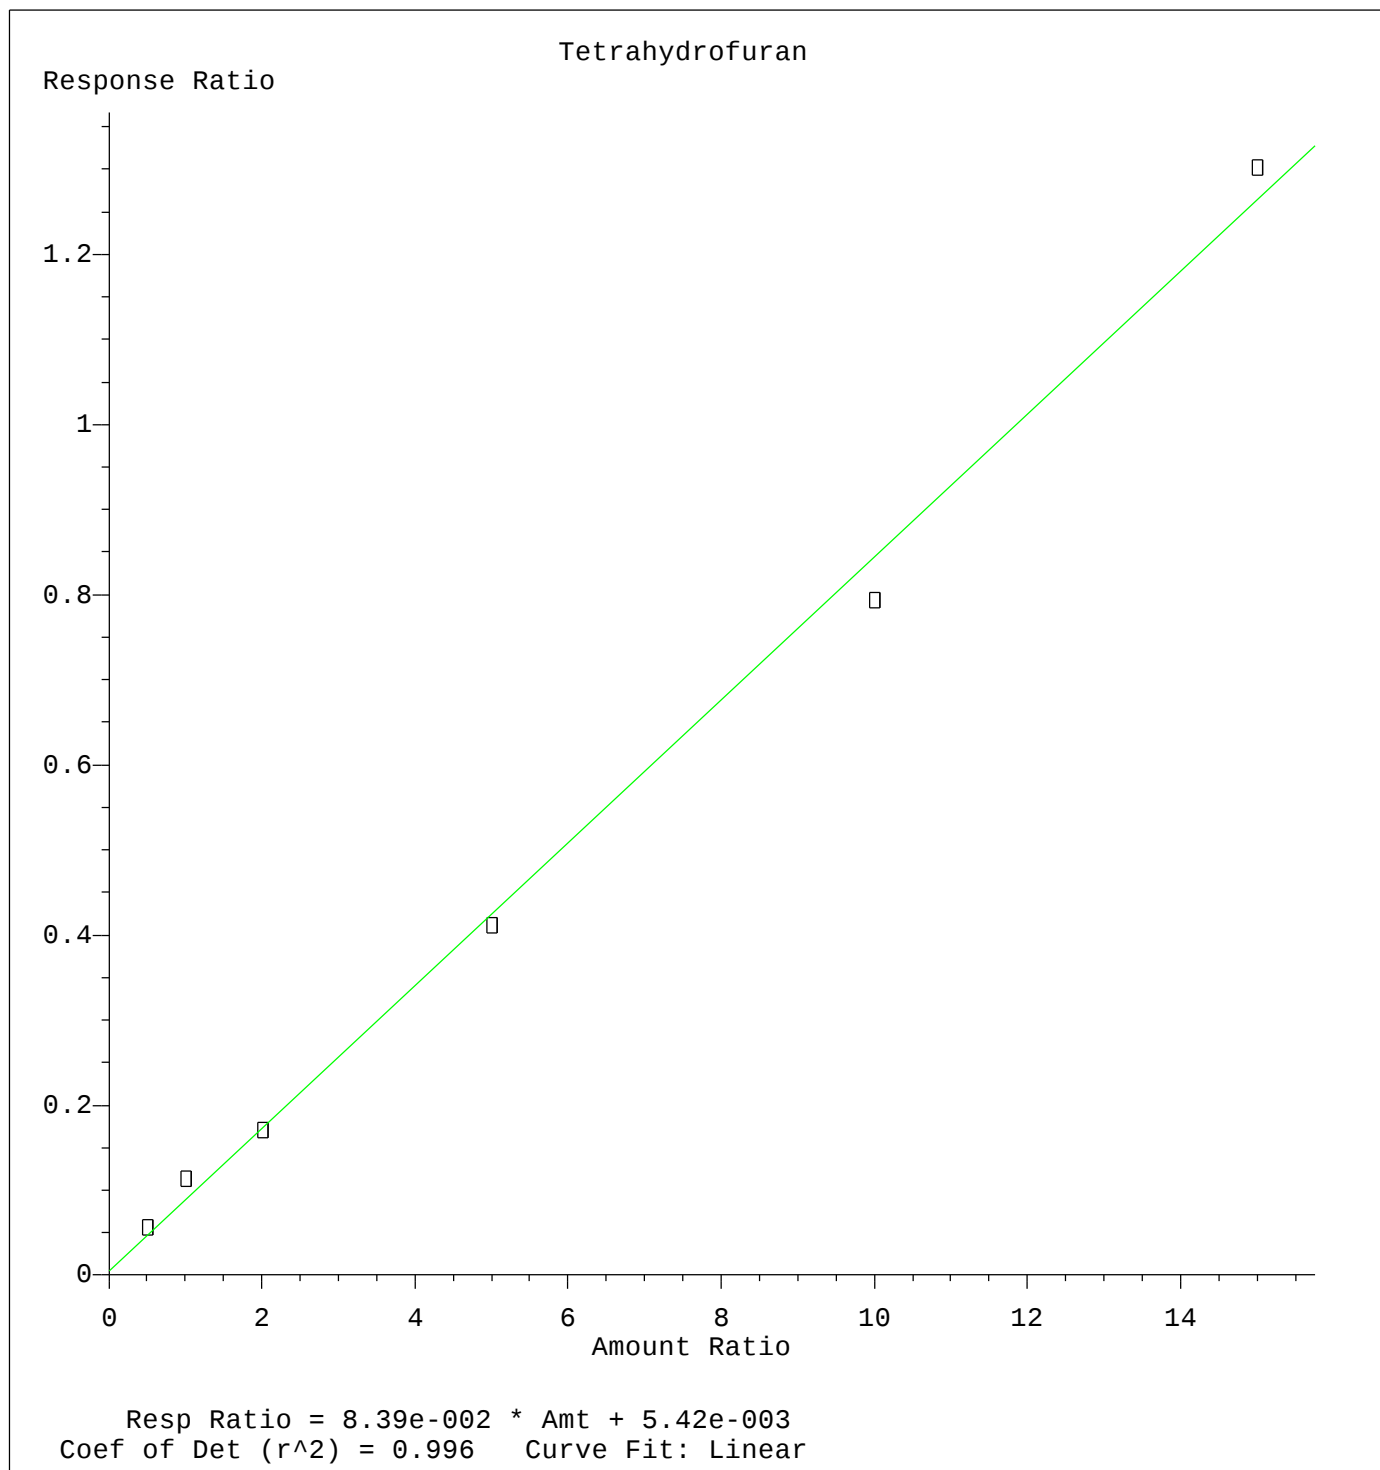


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019

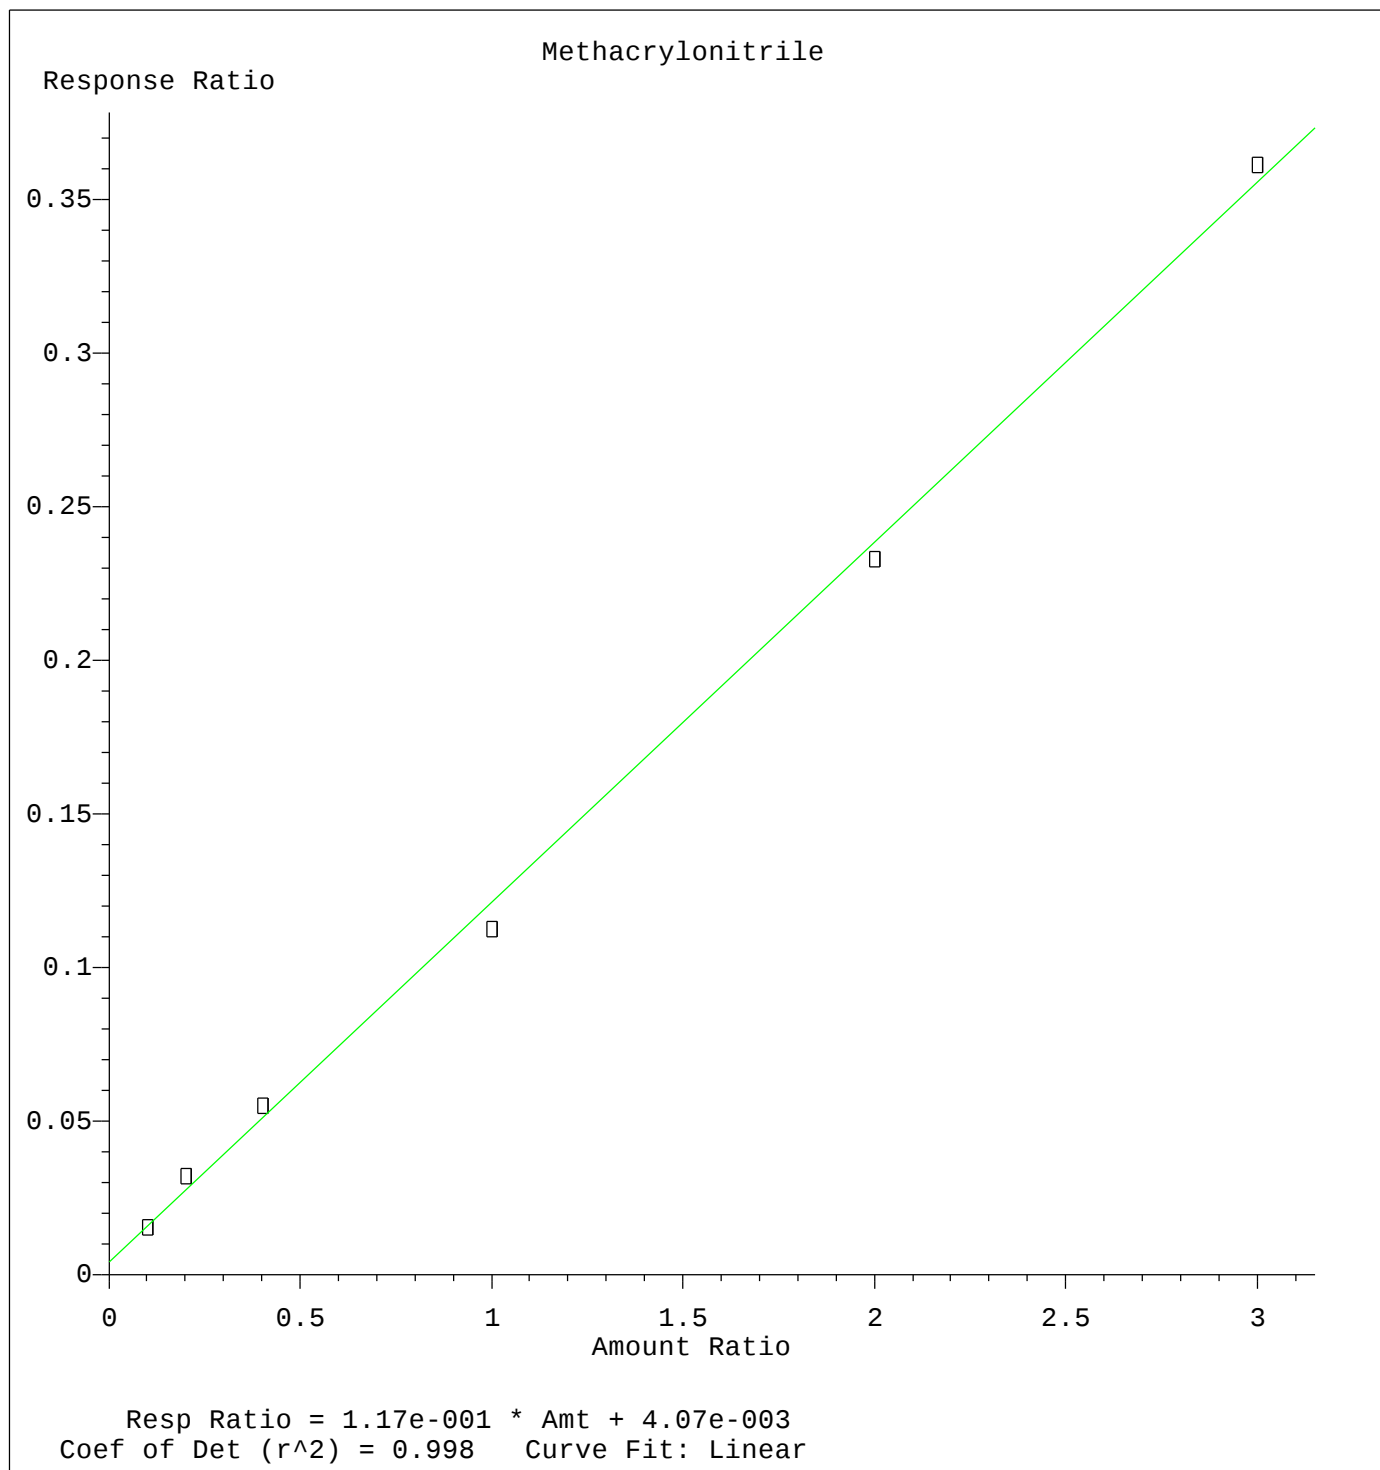

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019


4-Methyl-2-Pentanone

Response Ratio

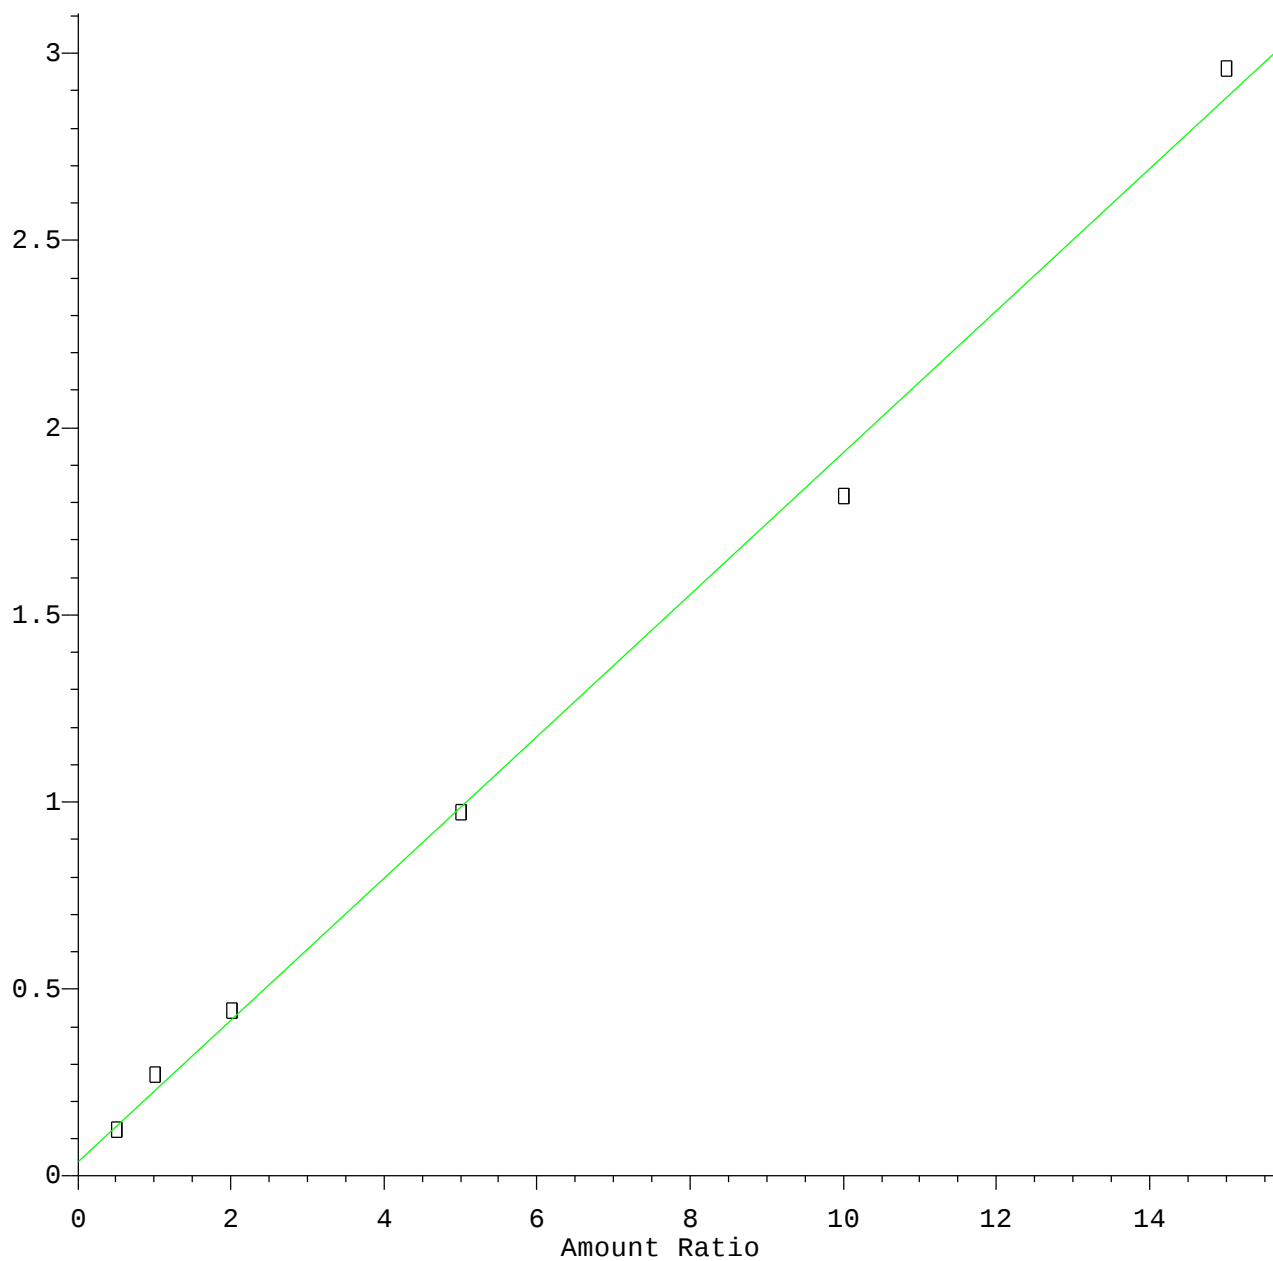

Resp Ratio = $1.89 \times 10^{-1} \times \text{Amt} + 3.84 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019

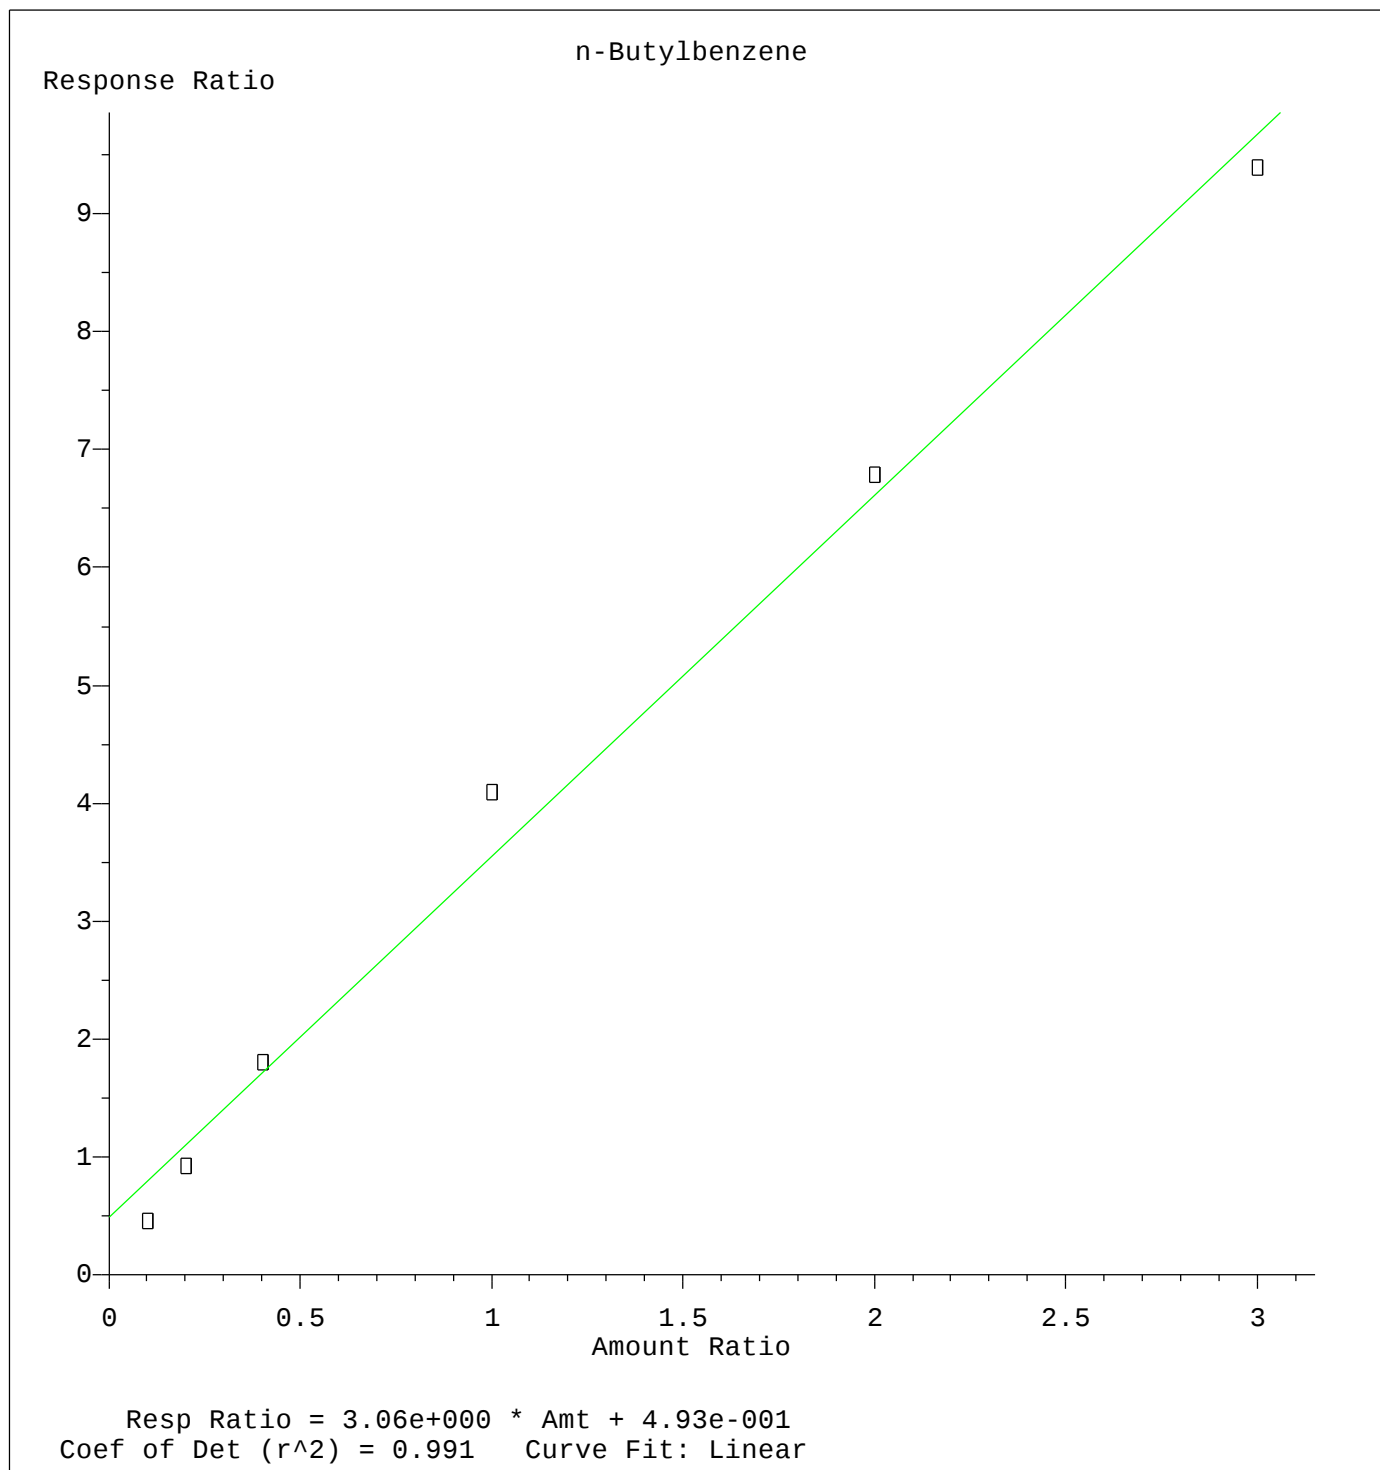

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Calibration Table Last Updated: Fri Jan 04 03:27:18 2019