

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF010719\
 Data File : VF061276.D
 Acq On : 7 Jan 2019 13:45
 Operator : VA/AP
 Sample : K1010-01
 Misc : 6.45g/5mL/MSVOA-F/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 OK-03-010419

Manual Integrations
 APPROVED

MMDadoda
 1/8/2019 12:58:08 PM

Quant Time: Jan 08 00:36:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 04 03:27:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.84	168	205628	50.00	ug/l	-0.04
34) 1,4-Difluorobenzene	5.57	114	362755	50.00	ug/l	-0.03
63) Chlorobenzene-d5	9.75	117	293506	50.00	ug/l	-0.03
72) 1,4-Dichlorobenzene-d4	12.53	152	126708	50.00	ug/l	-0.02
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.82	65	128777	49.34	ug/l	-0.03
Spiked Amount 50.000			Recovery	=	98.68%	
35) Dibromofluoromethane	4.09	113	139296	49.91	ug/l	-0.03
Spiked Amount 50.000			Recovery	=	99.82%	
50) Toluene-d8	7.53	98	339548	41.00	ug/l	-0.03
Spiked Amount 50.000			Recovery	=	82.00%	
62) 4-Bromofluorobenzene	11.39	95	146331	39.88	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	79.76%	
Target Compounds						
16) Acetone	2.23	43	15574	16.845	ug/l	94
20) Methylene Chloride	2.17	84	17823m	4.343	ug/l	
52) Toluene	7.59	92	6488	1.025	ug/l	100
68) m/p-Xylenes	10.11	106	6146	1.535	ug/l	97
95) Naphthalene	14.44	128	22742	4.125	ug/l #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF010719\
Data File : VF061276.D
Acq On : 7 Jan 2019 13:45
Operator : VA/AP
Sample : K1010-01
Misc : 6.45g/5mL/MSVOA-F/SOIL
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_F
ClientSampleId :
OK-03-010419

Manual Integrations
APPROVED

MMDadoda
1/8/2019 12:58:08 PM

Quant Time: Jan 08 00:36:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F010319S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 04 03:27:18 2019
Response via : Initial Calibration

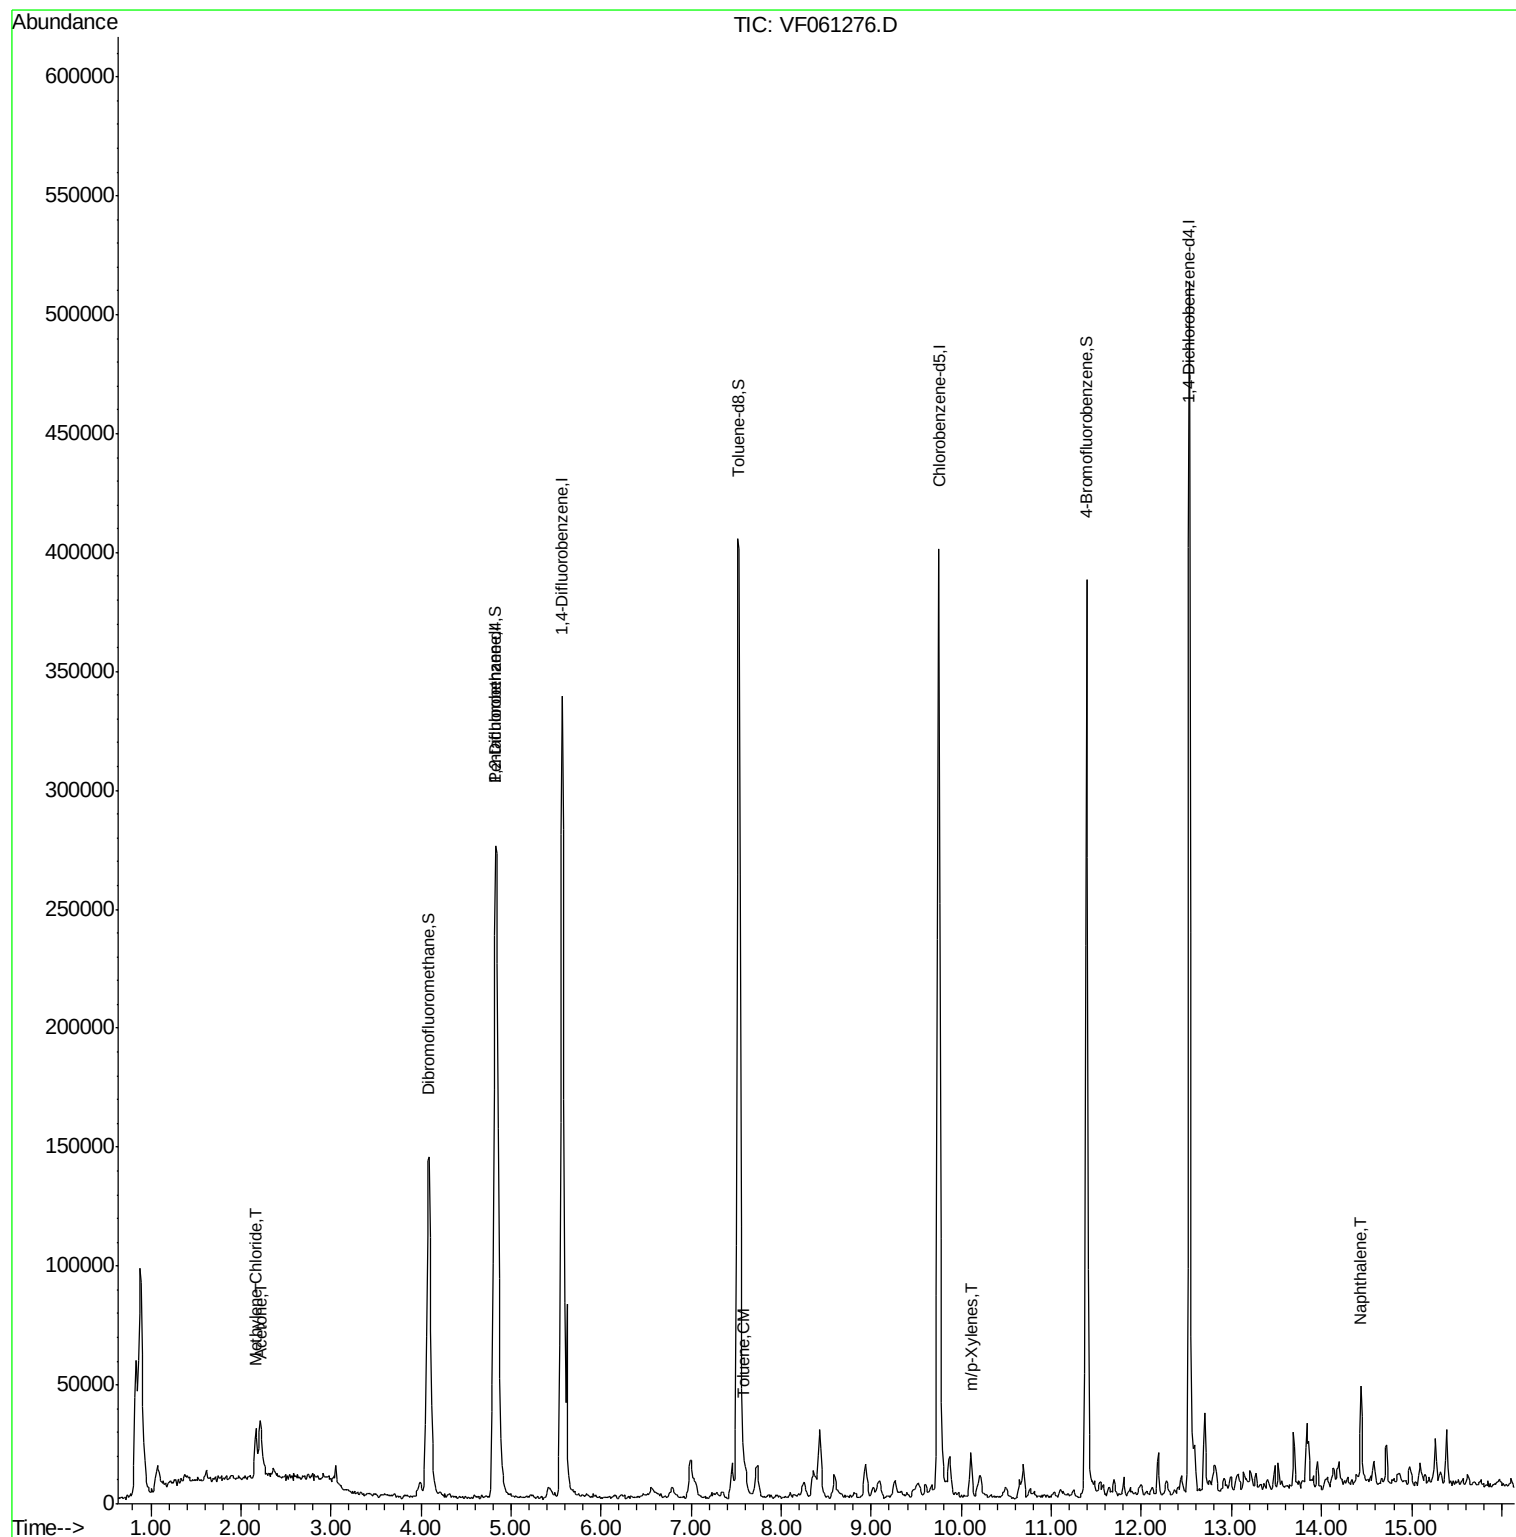

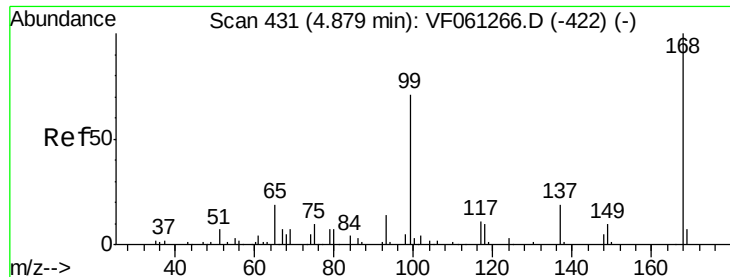

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.84 min Scan# 427

Delta R.T. -0.04 min

Lab File: VF061276.D

Acq: 7 Jan 2019 13:45

Instrument :

MSVOA_F

ClientSampleId :

OK-03-010419

Tot Ion:168 Resp: 205628

Ion Ratio Lower Upper

168 100


99 65.9 57.0 85.6

Manual Integrations

APPROVED

MMDadoda

1/8/2019 12:58:08 PM

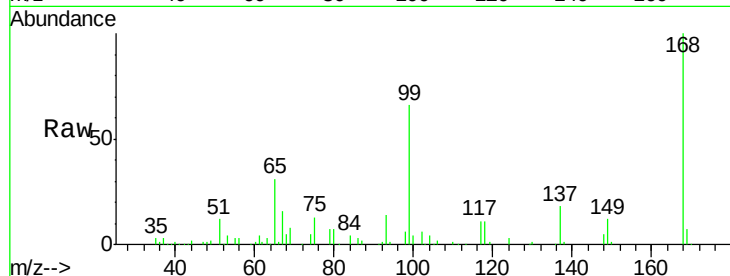

Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

4.84



60000

40000

20000

0

Time-->

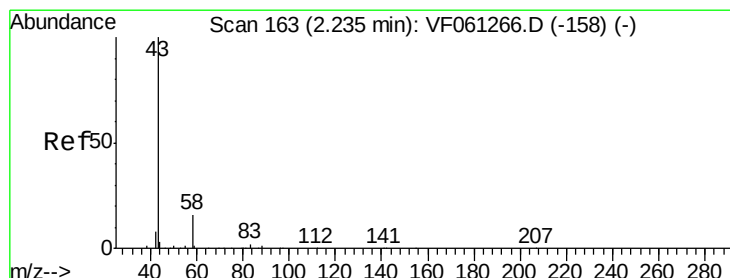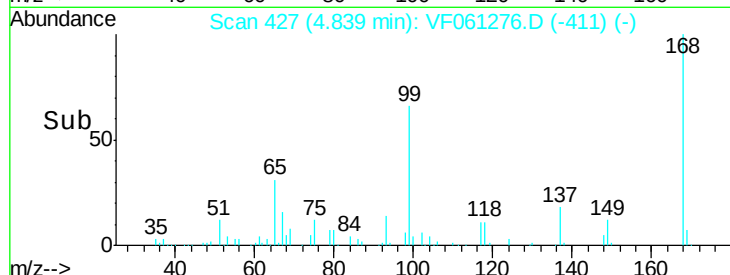

#16

Acetone

Concen: 16.845 ug/l

RT: 2.23 min Scan# 162

Delta R.T. -0.01 min

Lab File: VF061276.D


Acq: 7 Jan 2019 13:45

Tgt Ion: 43 Resp: 15574

Ion Ratio Lower Upper

43 100

58 18.7 13.0 19.4

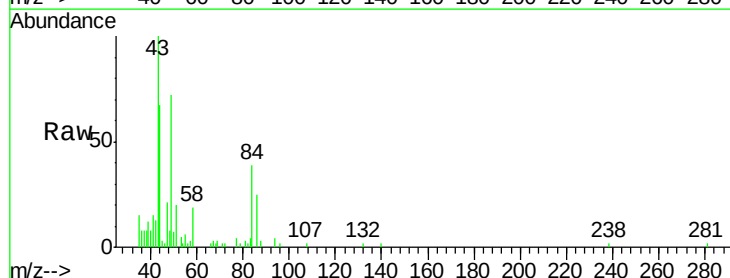

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0

2.23


6000


4000

2000

0

Time-->

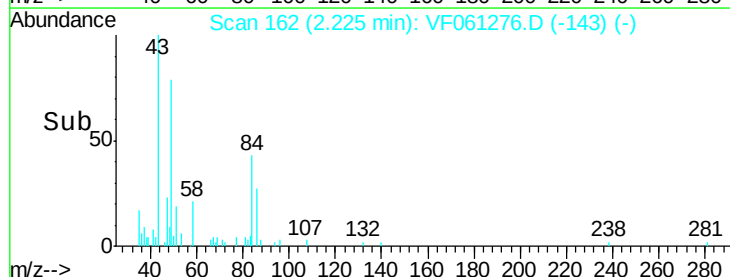

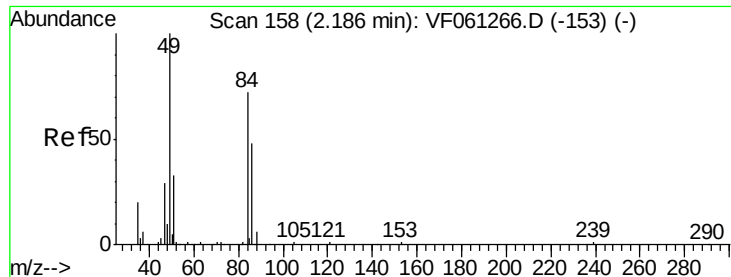





#20
Methylene Chloride
Concen: 4.343 ug/l m
RT: 2.17 min Scan# 156
Delta R.T. -0.02 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Instrument :
MSVOA_F
ClientSampleId :
OK-03-010419

Tot Ion	Ratio	Lower	Upper
84	100		
49	154.3	112.9	169.3
51	51.3	37.9	56.9
86	65.4	53.8	80.8




Manual Integrations
APPROVED


MMDadoda
1/8/2019 12:58:08 PM

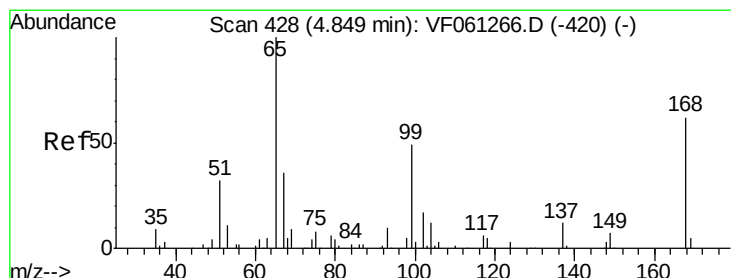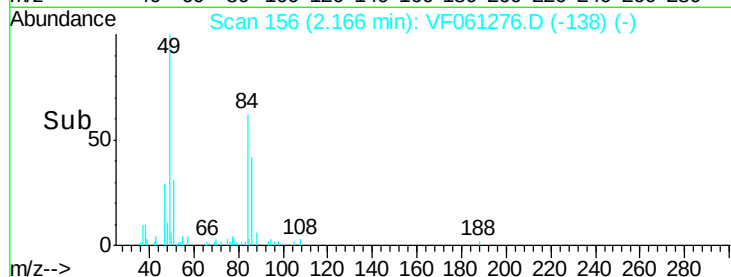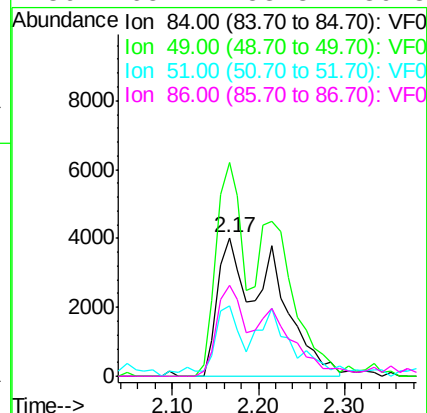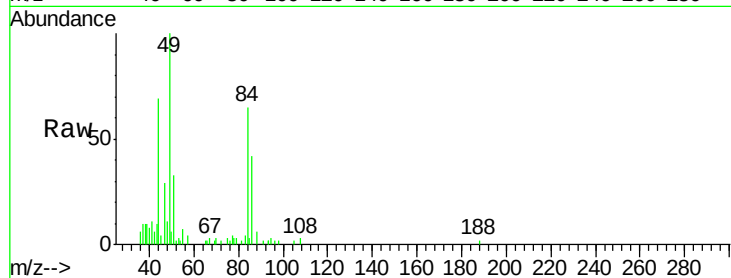

#33
1,2-Dichloroethane-d4
Concen: 49.336 ug/l
RT: 4.82 min Scan# 425
Delta R.T. -0.03 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Tgt Ion	Ratio	Lower	Upper
65	100		
67	48.7	0.0	90.4

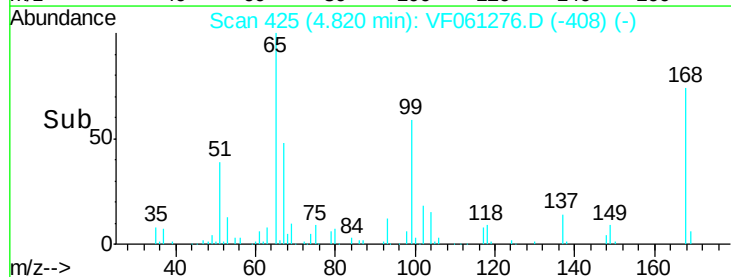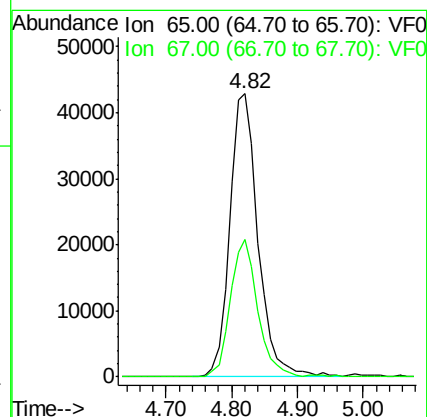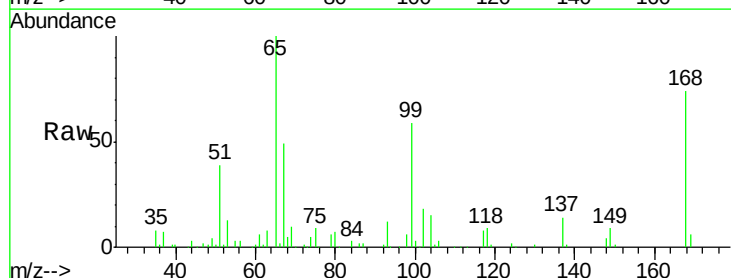

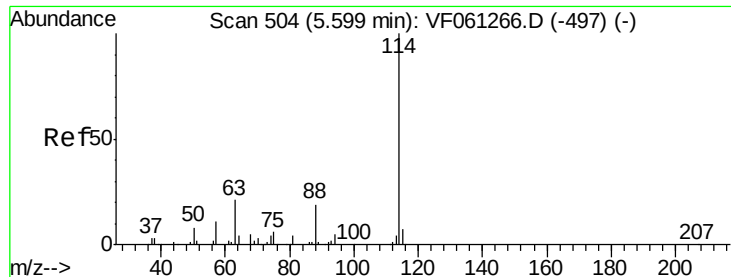

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.57 min Scan# 501

Delta R.T. -0.03 min

Lab File: VF061276.D

Acq: 7 Jan 2019 13:45

Instrument :

MSVOA_F


ClientSampleId :

OK-03-010419

Tot Ion	Ratio	Resp	Lower	Upper
114	100	362755		
63	21.6		0.0	41.8
88	20.1		0.0	38.4

Manual Integrations
APPROVED




MMDadoda
1/8/2019 12:58:08 PM

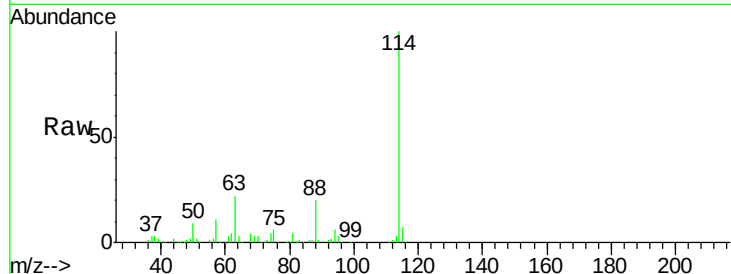

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

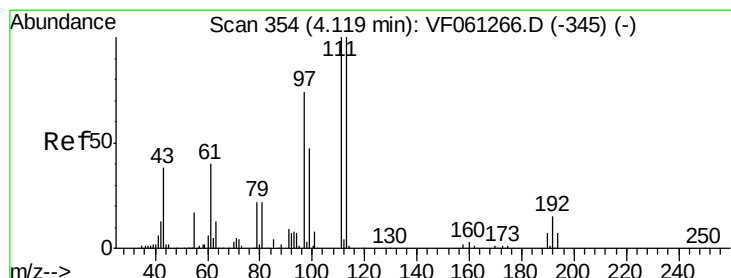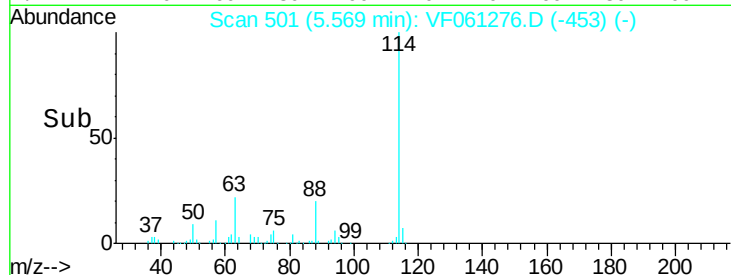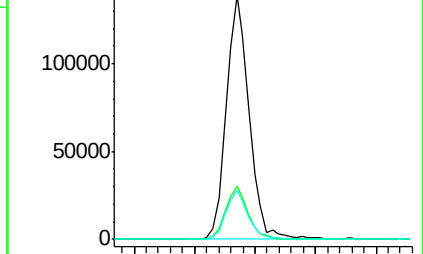

#35

Dibromofluoromethane

Concen: 49.911 ug/l


RT: 4.09 min Scan# 351

Delta R.T. -0.03 min

Lab File: VF061276.D

Acq: 7 Jan 2019 13:45



Tgt Ion	Ratio	Resp	Lower	Upper
113	100	139296		
111	100.4		79.8	119.6
192	16.6		11.9	17.9

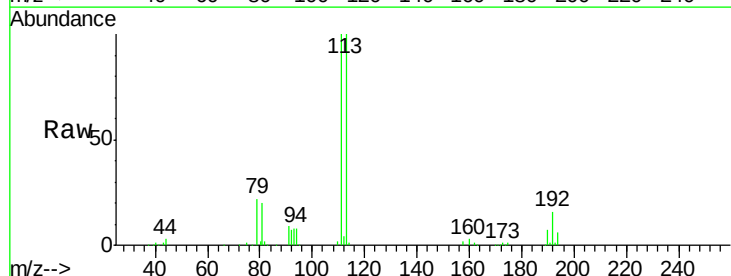


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

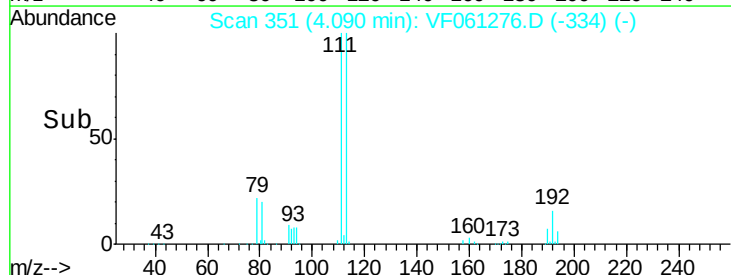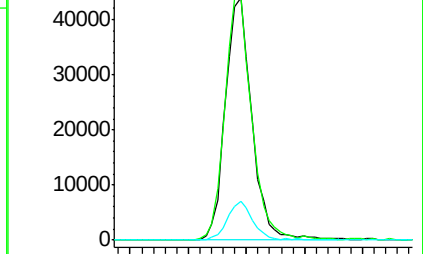

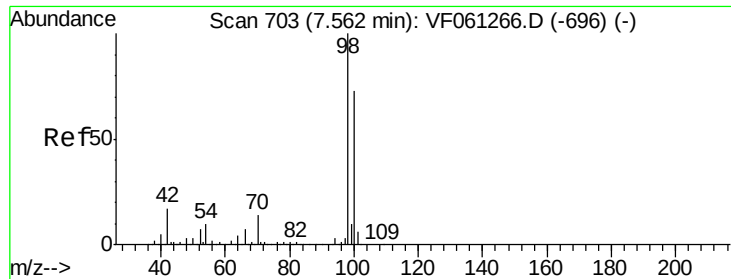





#50
Toluene-d8
Concen: 40.999 ug/l
RT: 7.53 min Scan# 700
Delta R.T. -0.03 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Instrument :
MSVOA_F
ClientSampleId :
OK-03-010419

Tot Ion: 98 Resp: 339548
Ion Ratio Lower Upper
98 100
100 68.5 58.1 87.1




Manual Integrations
APPROVED


MMDadoda
1/8/2019 12:58:08 PM

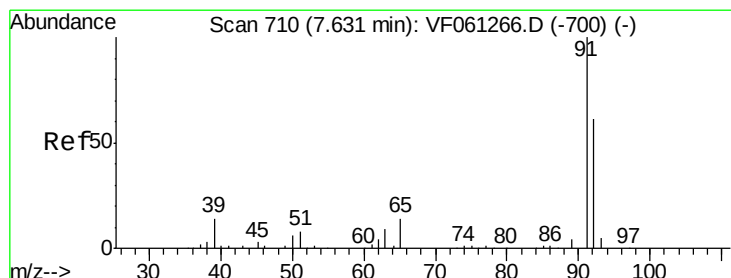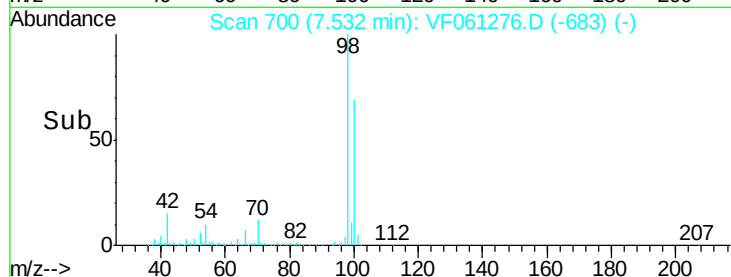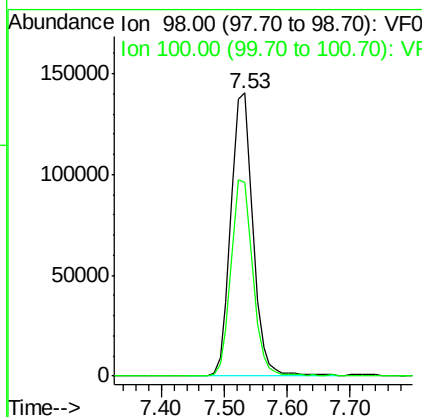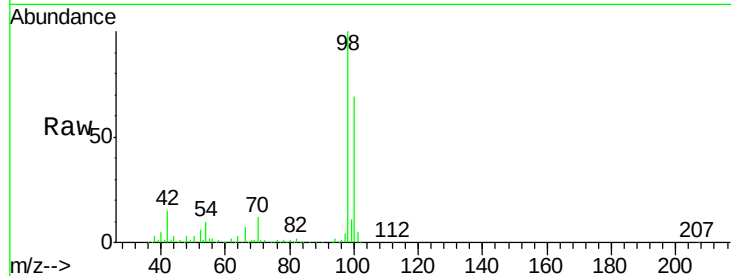

#52
Toluene
Concen: 1.025 ug/l
RT: 7.59 min Scan# 706
Delta R.T. -0.04 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Tgt Ion: 92 Resp: 6488
Ion Ratio Lower Upper
92 100
91 162.8 130.5 195.7

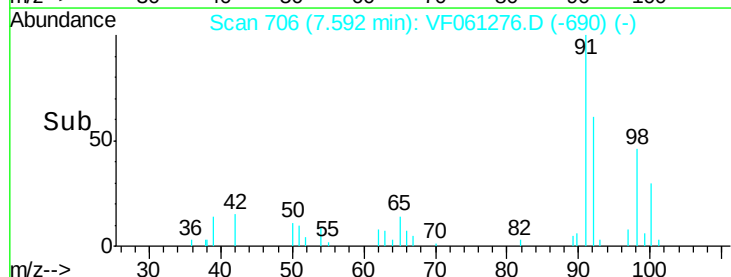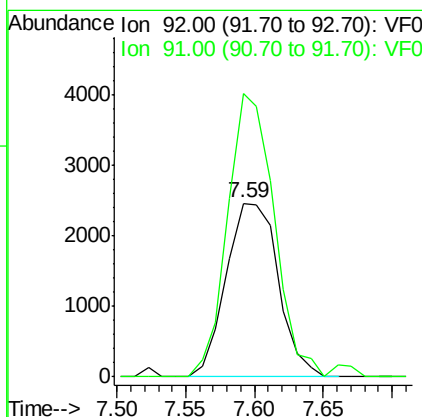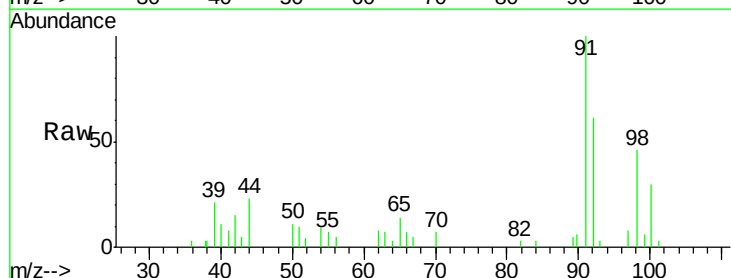

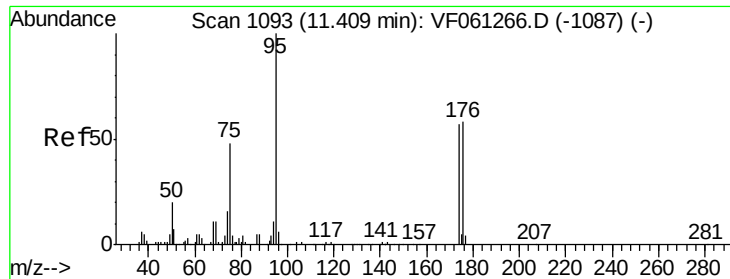





#62
4-Bromofluorobenzene
Concen: 39.877 ug/l
RT: 11.39 min Scan# 1091
Delta R.T. -0.02 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Instrument :
MSVOA_F
ClientSampleId :
OK-03-010419

Tot Ion	Ratio	Resp	Lower	Upper
95	100	146331		
174	66.5	0.0	113.2	
176	65.4	0.0	115.6	




Manual Integrations
APPROVED


MMDadoda
1/8/2019 12:58:08 PM

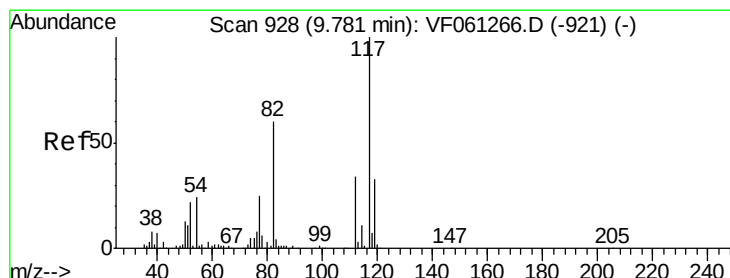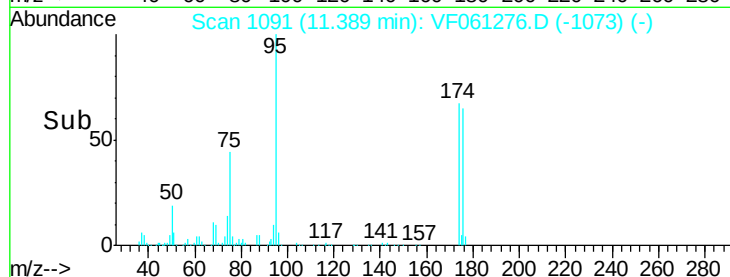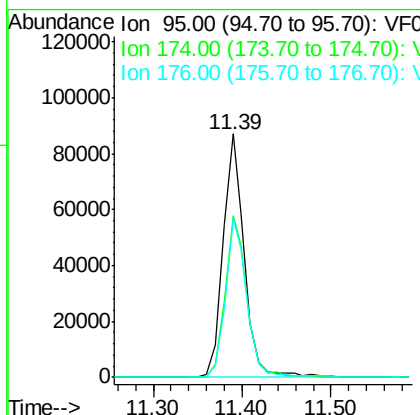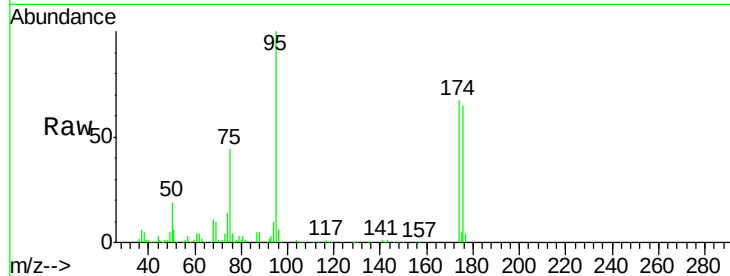

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.75 min Scan# 925
Delta R.T. -0.03 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Tgt Ion	Ratio	Resp	Lower	Upper
117	100	293506		
82	60.0	47.8	71.6	
119	32.9	26.1	39.1	

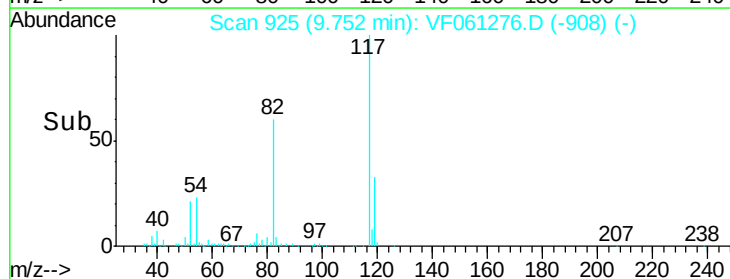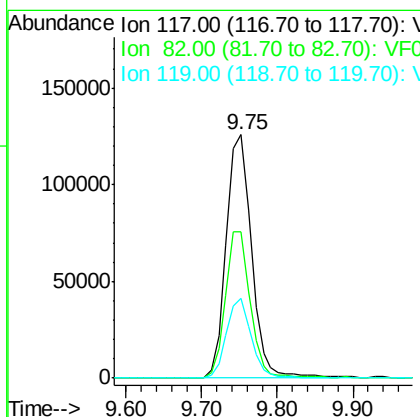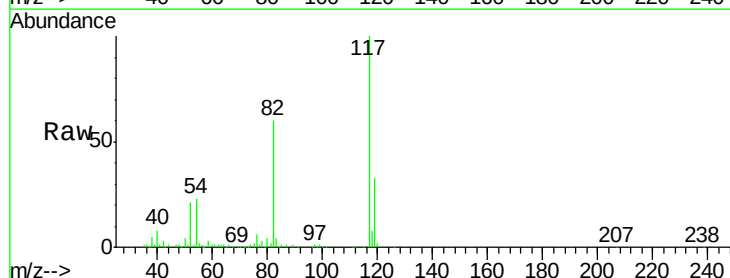

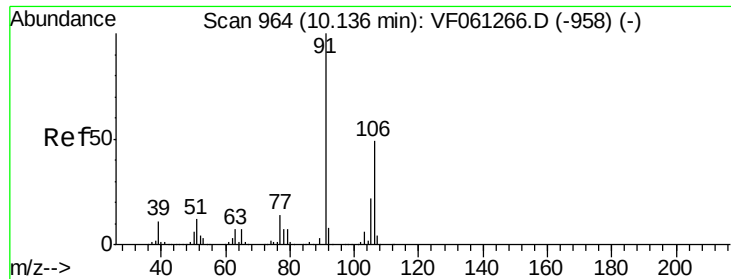





#68
m/p-Xvlenes
Concen: 1.535 ug/l
RT: 10.11 min Scan# 961
Delta R.T. -0.03 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Instrument :
MSVOA_F
ClientSampleId :
OK-03-010419

Tot Ion:106 Resp: 6146
Ion Ratio Lower Upper
106 100
91 201.1 164.8 247.2




Manual Integrations
APPROVED


MMDadoda
1/8/2019 12:58:08 PM

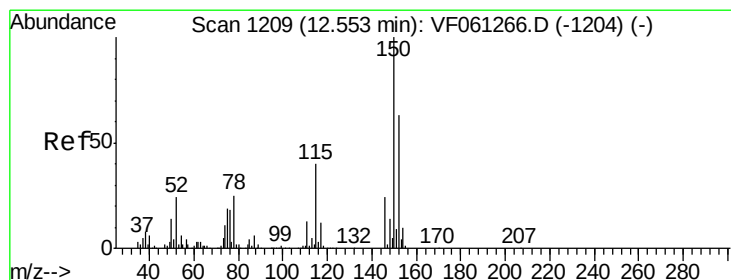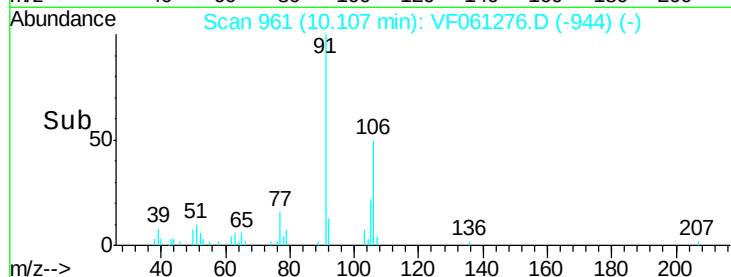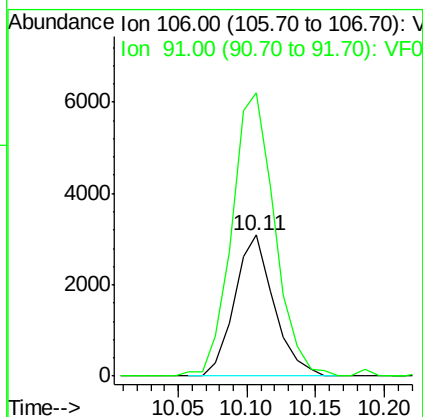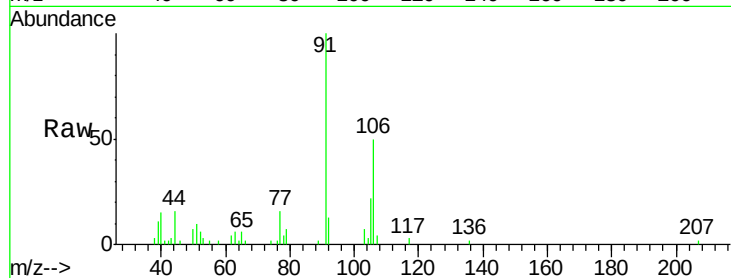

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.53 min Scan# 1207
Delta R.T. -0.02 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Tgt Ion:152 Resp: 126708
Ion Ratio Lower Upper
152 100
115 56.0 31.6 94.7
150 152.3 0.0 320.2

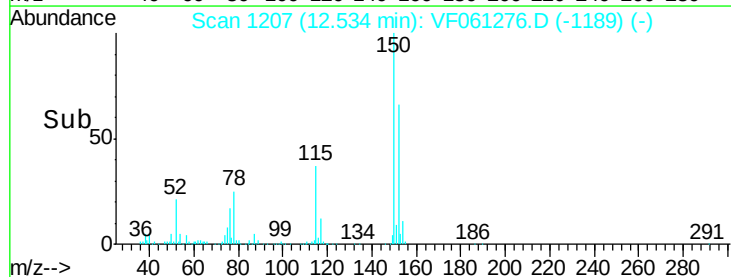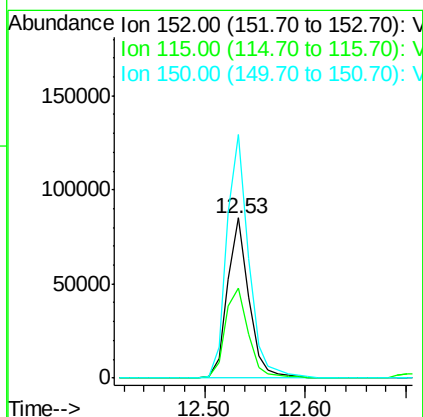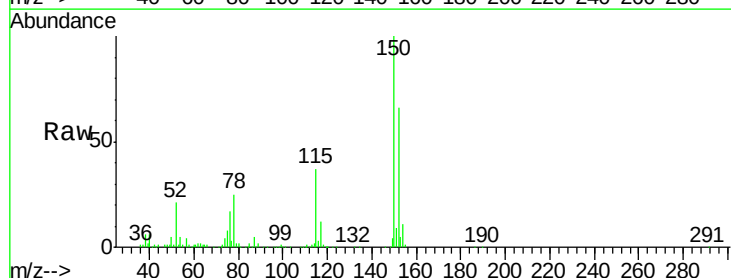

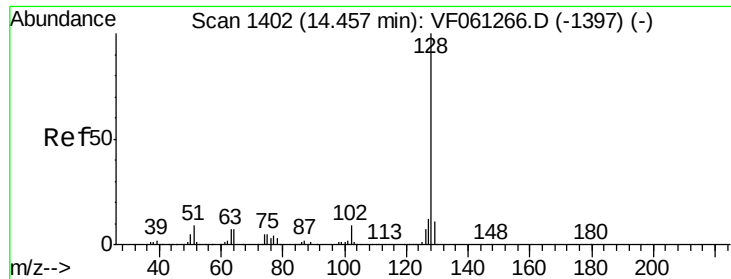

#95
Naphthalene
Concen: 4.125 ug/l
RT: 14.44 min Scan# 1400
Delta R.T. -0.02 min
Lab File: VF061276.D
Acq: 7 Jan 2019 13:45

Instrument :
MSVOA_F
ClientSampleId :
OK-03-010419

Tot Ion	Ratio	Resp	Lower	Upper
128	100	22742		
127	14.8		9.8	14.6#
129	12.4		9.0	13.4

Manual Integrations
APPROVED

MMDadoda
1/8/2019 12:58:08 PM

