


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF011019\
Data File : VF061337.D
Acq On : 10 Jan 2019 10:47
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010819S.M
Title : SW846 8260
Last Update : Wed Jan 09 07:13:51 2019

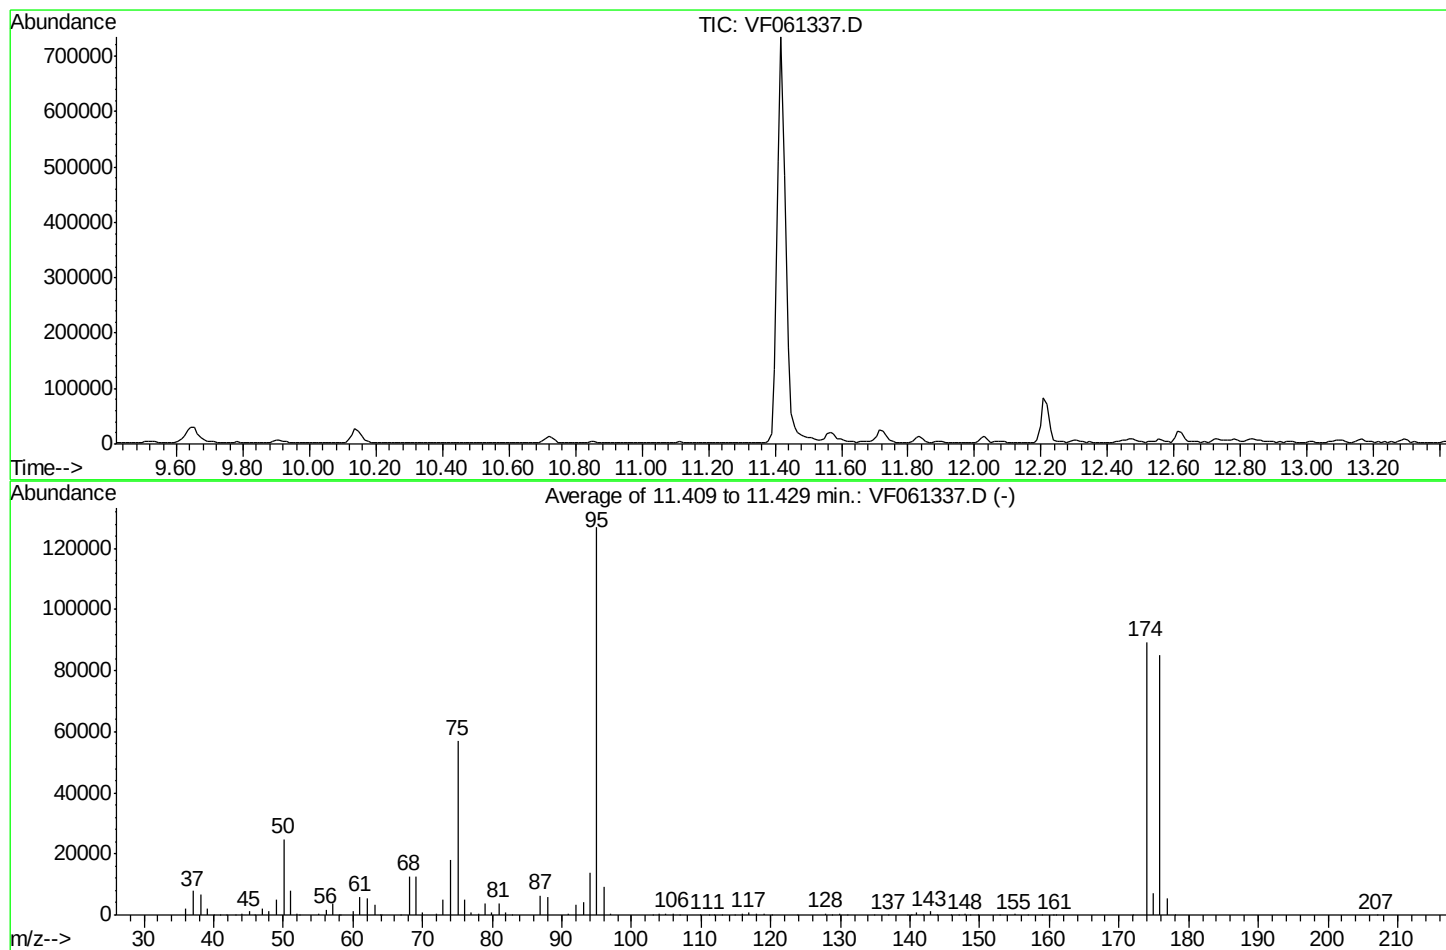

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1087

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	24853	PASS
75	95	30	60	45.0	57128	PASS
95	95	100	100	100.0	126968	PASS
96	95	5	9	7.1	9048	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.3	89317	PASS
175	174	5	9	7.9	7018	PASS
176	174	95	101	95.4	85200	PASS
177	176	5	9	6.6	5635	PASS