


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF011119\
Data File : VF061360.D
Acq On : 11 Jan 2019 10:21
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F010819S.M
Title : SW846 8260
Last Update : Wed Jan 09 07:13:51 2019

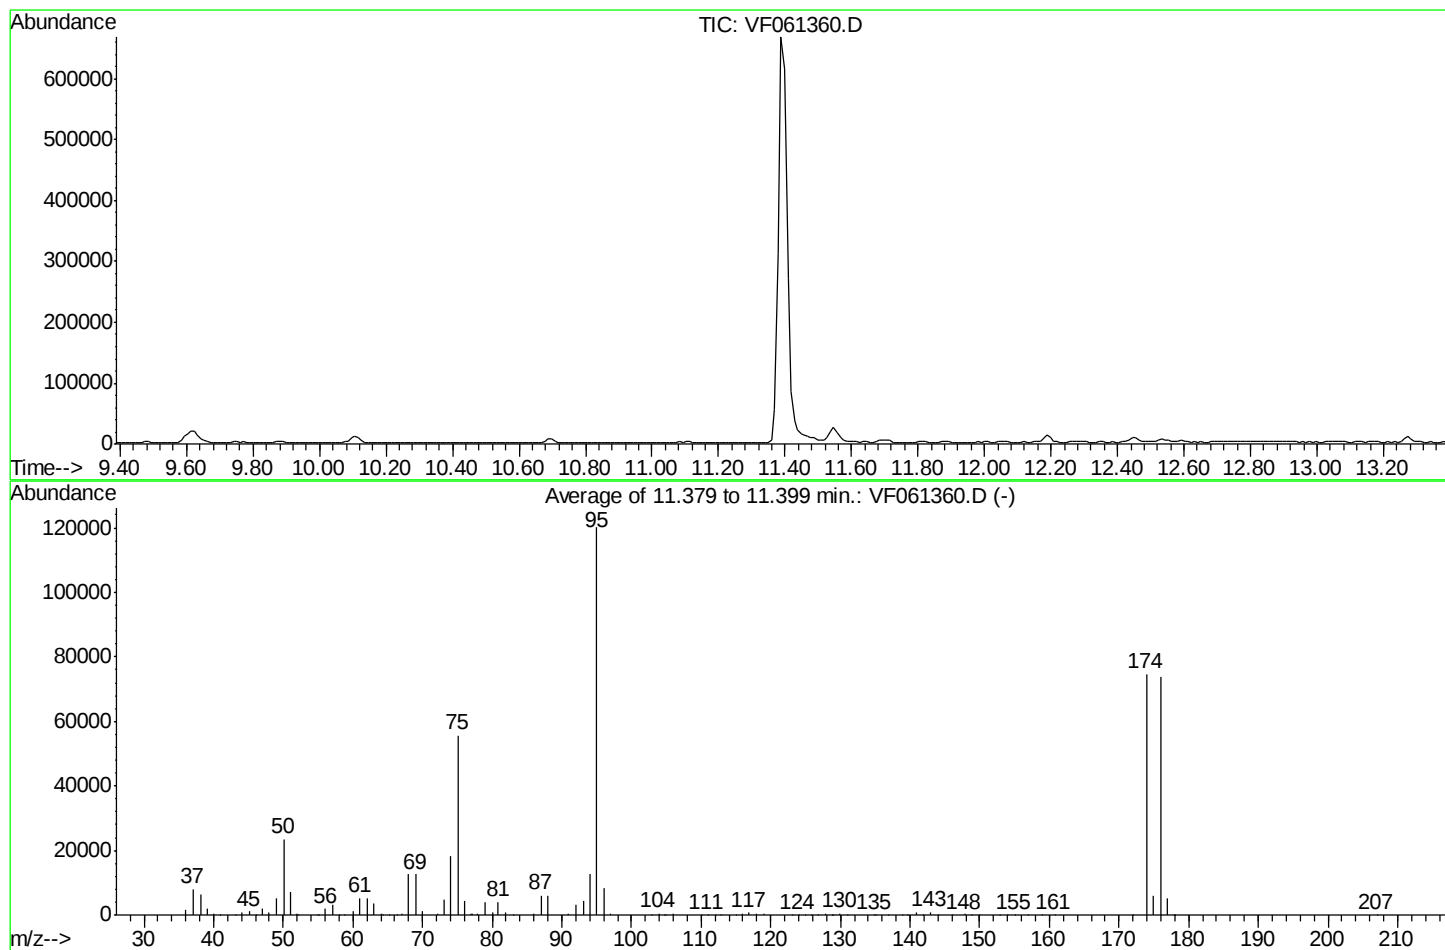

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	23616	PASS
75	95	30	60	46.3	55624	PASS
95	95	100	100	100.0	120160	PASS
96	95	5	9	6.8	8220	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	62.1	74640	PASS
175	174	5	9	7.9	5898	PASS
176	174	95	101	99.0	73906	PASS
177	176	5	9	6.8	5001	PASS