


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF011819\
 Data File : VF061451.D
 Acq On : 18 Jan 2019 10:05
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
 Title : SW846 8260
 Last Update : Wed Jan 16 04:51:59 2019

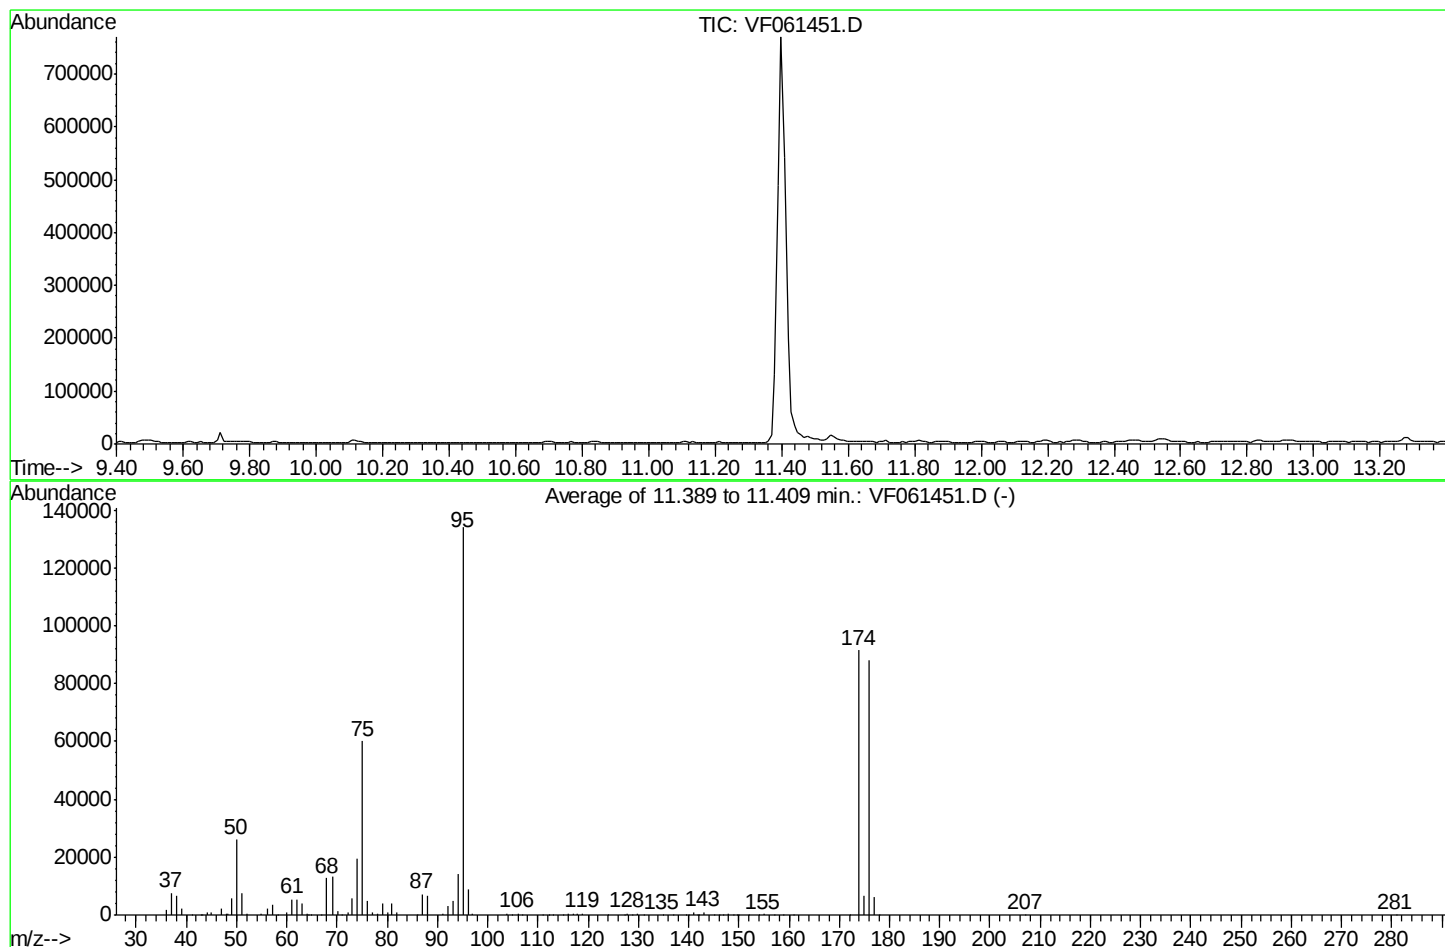

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	25938	PASS
75	95	30	60	44.8	60069	PASS
95	95	100	100	100.0	134002	PASS
96	95	5	9	6.7	8969	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.3	91546	PASS
175	174	5	9	7.4	6753	PASS
176	174	95	101	96.0	87861	PASS
177	176	5	9	7.0	6111	PASS