


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF012119\
Data File : VF061467.D
Acq On : 21 Jan 2019 10:26
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
Title : SW846 8260
Last Update : Wed Jan 16 04:51:59 2019

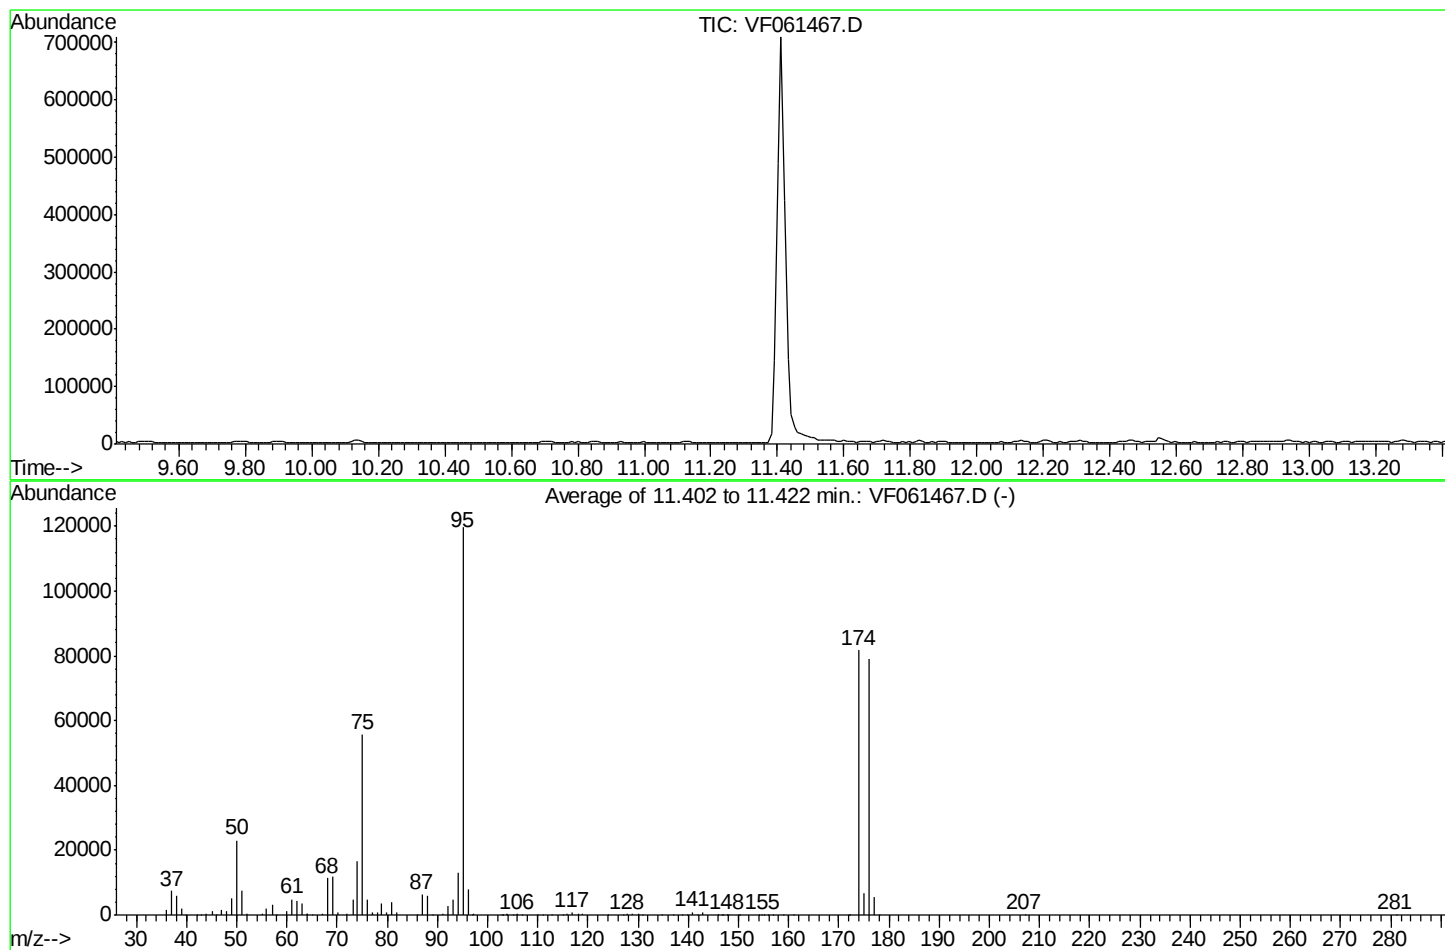

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	22998	PASS
75	95	30	60	46.5	55608	PASS
95	95	100	100	100.0	119674	PASS
96	95	5	9	6.7	8001	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.2	81645	PASS
175	174	5	9	8.0	6554	PASS
176	174	95	101	96.8	79010	PASS
177	176	5	9	6.8	5412	PASS