


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF012419\
Data File : VF061491.D
Acq On : 24 Jan 2019 10:17
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
Title : SW846 8260
Last Update : Wed Jan 16 04:51:59 2019

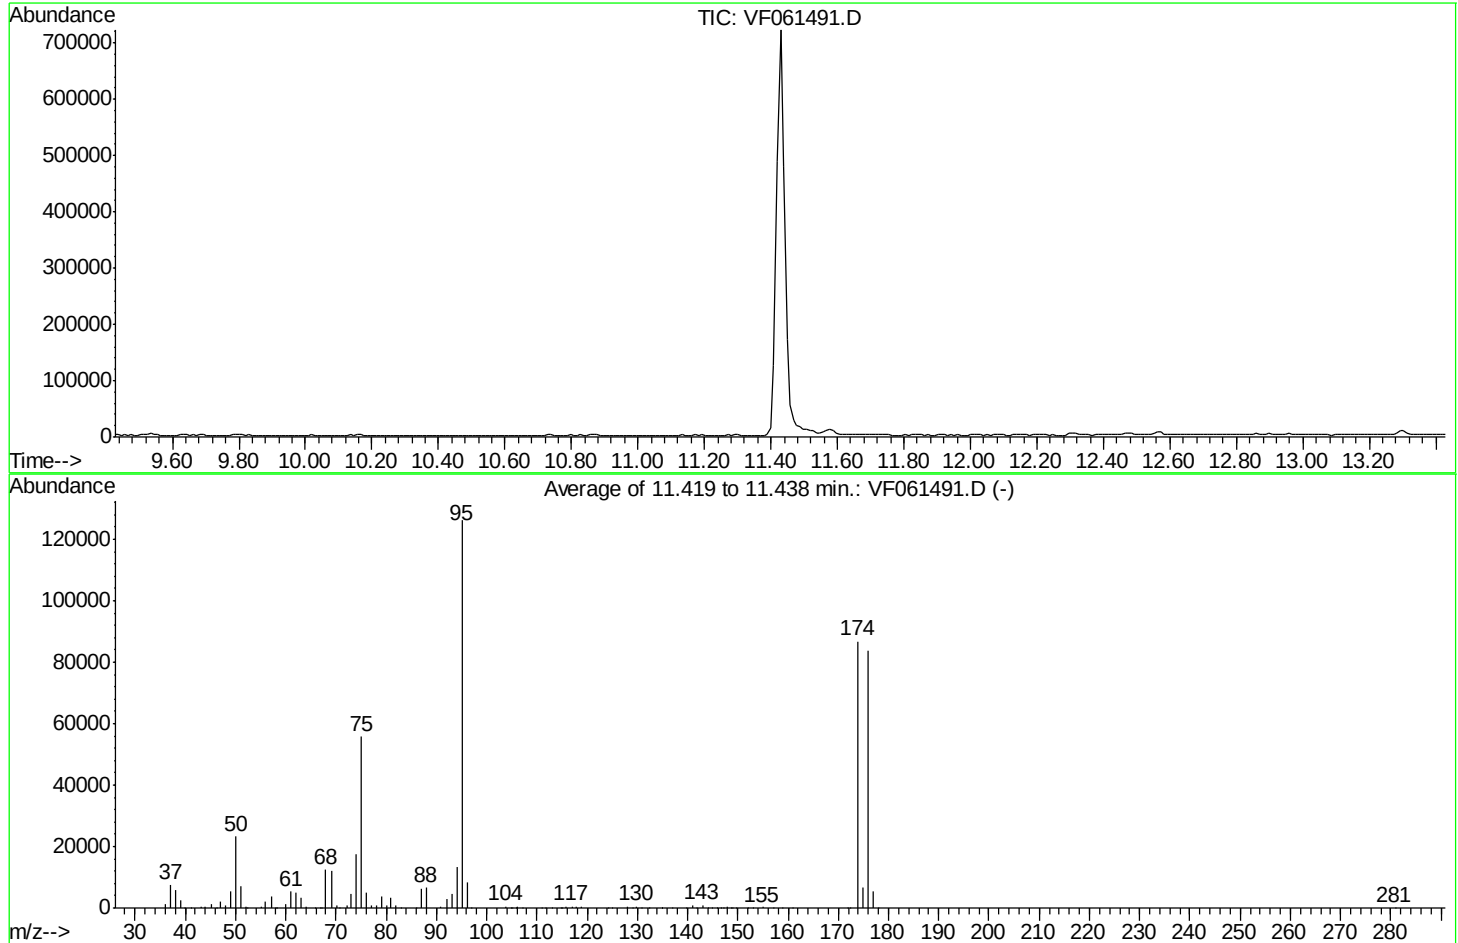

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	23208	PASS
75	95	30	60	44.1	55698	PASS
95	95	100	100	100.0	126186	PASS
96	95	5	9	6.8	8536	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.8	86874	PASS
175	174	5	9	7.5	6556	PASS
176	174	95	101	96.2	83592	PASS
177	176	5	9	6.6	5525	PASS