


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF012519\
Data File : VF061513.D
Acq On : 25 Jan 2019 10:41
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
Title : SW846 8260
Last Update : Wed Jan 16 04:51:59 2019

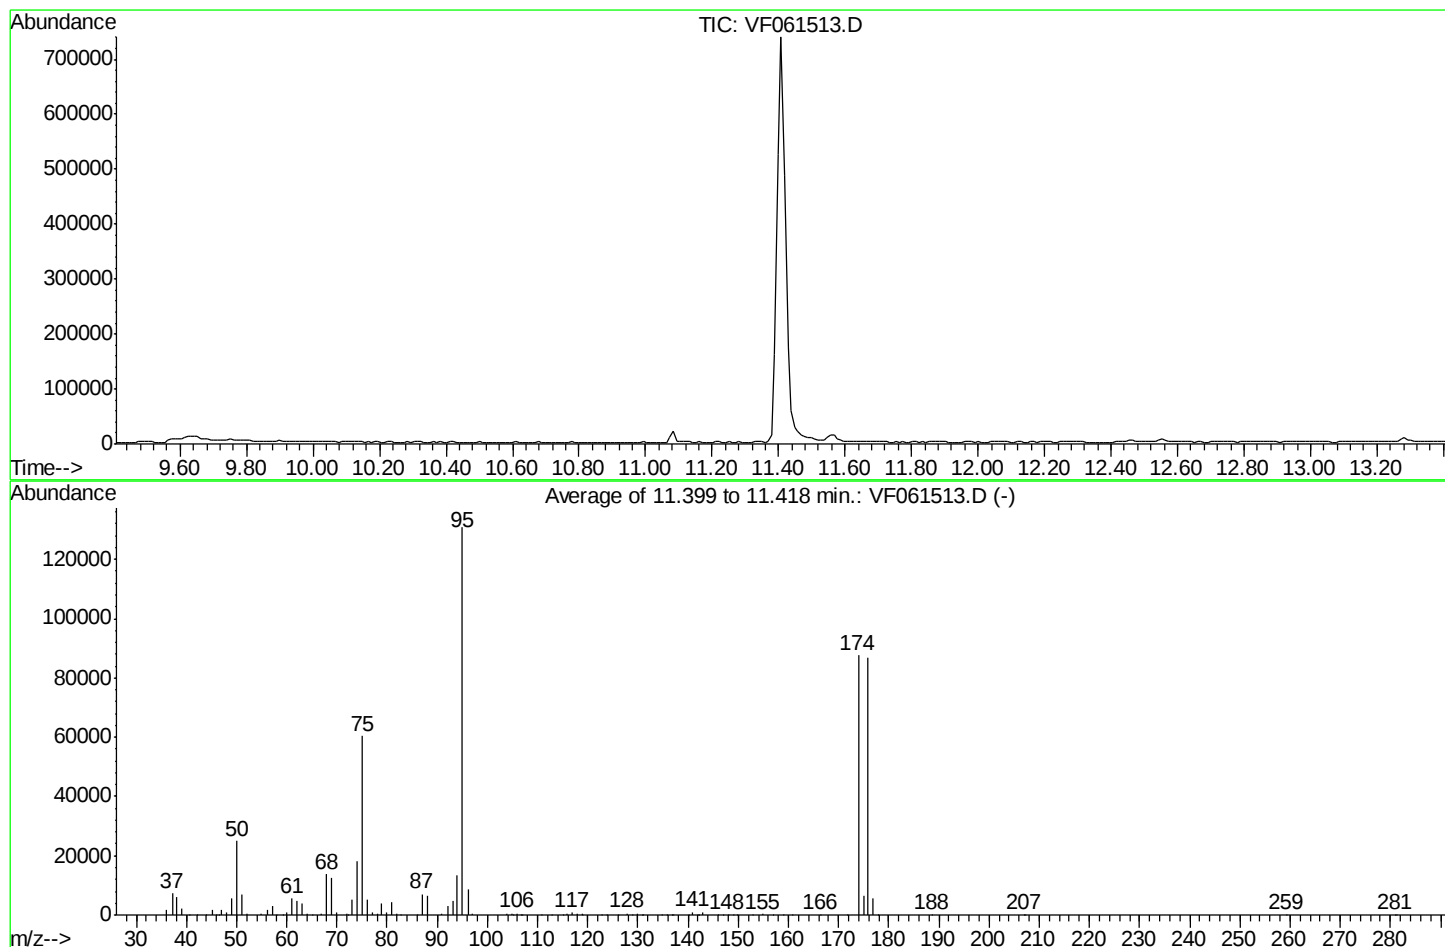

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	24898	PASS
75	95	30	60	46.1	60288	PASS
95	95	100	100	100.0	130826	PASS
96	95	5	9	6.7	8769	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.9	87520	PASS
175	174	5	9	7.5	6532	PASS
176	174	95	101	99.1	86768	PASS
177	176	5	9	6.5	5638	PASS