

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF012819\
 Data File : VF061539.D
 Acq On : 28 Jan 2019 14:10
 Operator : VA/AP
 Sample : K1011-11
 Misc : 6.68g/5mL/MSVOA-F/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 OR-01-012519-B

Manual Integrations
 APPROVED

MMDadoda
 1/29/2019 12:19:10 PM

Quant Time: Jan 29 04:40:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 16 04:51:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.86	168	221312	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.60	114	390288	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.77	117	328474	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.54	152	143774	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.84	65	121593	44.50	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.00%	
35) Dibromofluoromethane	4.11	113	147267	47.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.64%	
50) Toluene-d8	7.54	98	340736	40.38	ug/l	0.00
Spiked Amount 50.000			Recovery	=	80.76%	
62) 4-Bromofluorobenzene	11.41	95	144536	36.66	ug/l	0.00
Spiked Amount 50.000			Recovery	=	73.32%	
Target Compounds						
16) Acetone	2.24	43	36623	66.812	ug/l	94
20) Methylene Chloride	2.18	84	19119m	8.828	ug/l	
25) 2-Butanone	4.33	43	6070	6.659	ug/l	95
52) Toluene	7.61	92	17333	2.614	ug/l	83
68) m/p-Xylenes	10.13	106	7356	1.676	ug/l	100
95) Naphthalene	14.46	128	8437	1.372	ug/l #	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF012819\
Data File : VF061539.D
Acq On : 28 Jan 2019 14:10
Operator : VA/AP
Sample : K1011-11
Misc : 6.68g/5mL/MSVOA-F/SOIL
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_F
ClientSampleId :
OR-01-012519-B

Manual Integrations
APPROVED

MMDadoda
1/29/2019 12:19:10 PM

Quant Time: Jan 29 04:40:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
Quant Title : SW846 8260
QLast Update : Wed Jan 16 04:51:59 2019
Response via : Initial Calibration

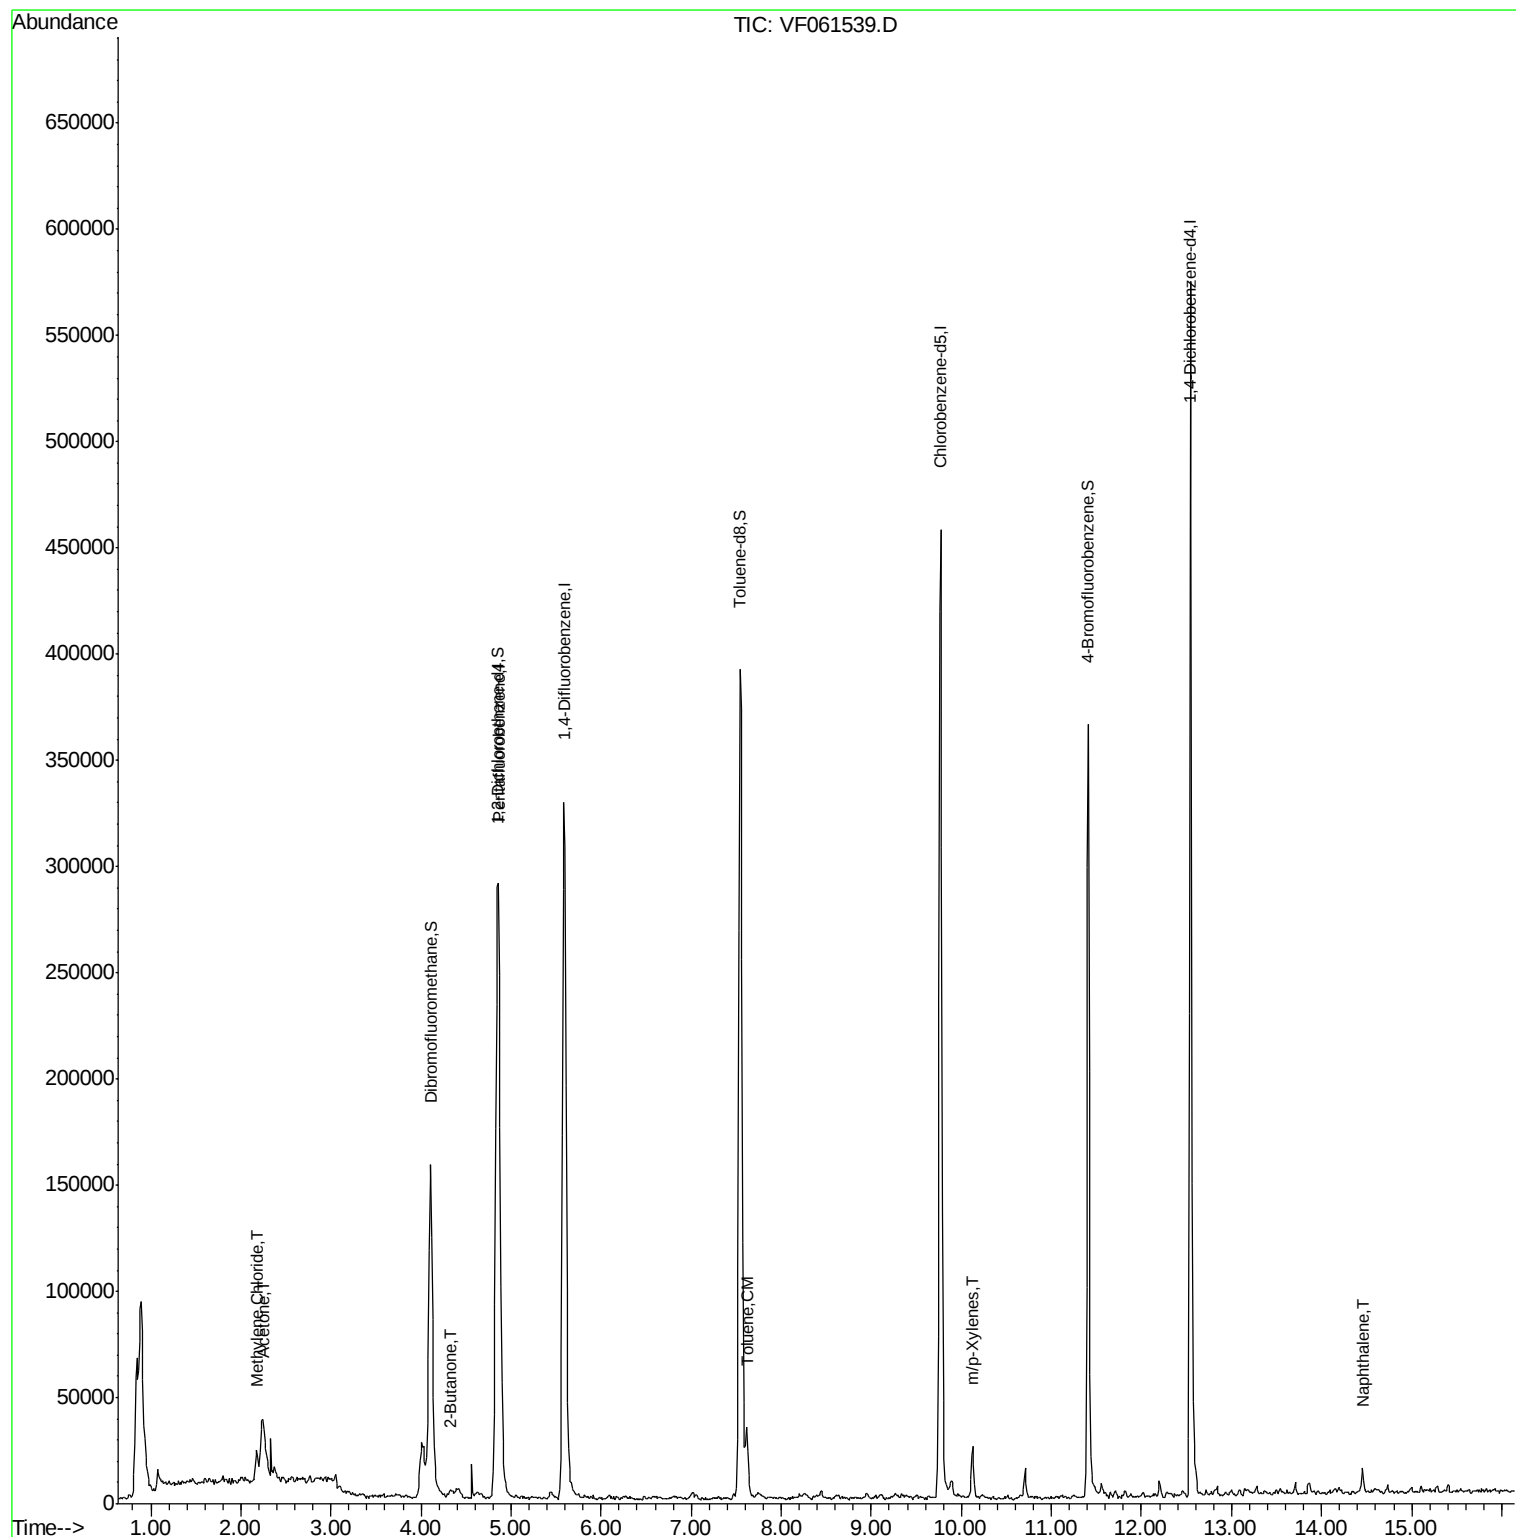

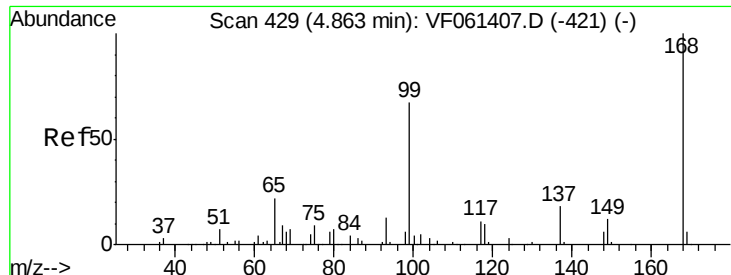

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.86 min Scan# 429

Delta R.T. -0.00 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10

Instrument :

MSVOA_F

ClientSampleId :

OR-01-012519-B

Tot Ion:168 Resp: 221312

Ion Ratio Lower Upper

168 100


99 66.4 53.5 80.3

Manual Integrations

APPROVED

MMDadoda

1/29/2019 12:19:10 PM

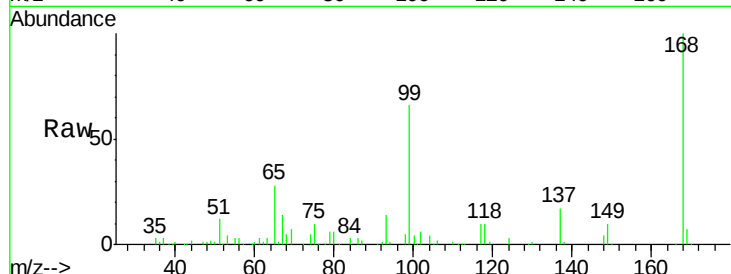

Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

4.86

80000



60000

40000

20000

0

Time-->

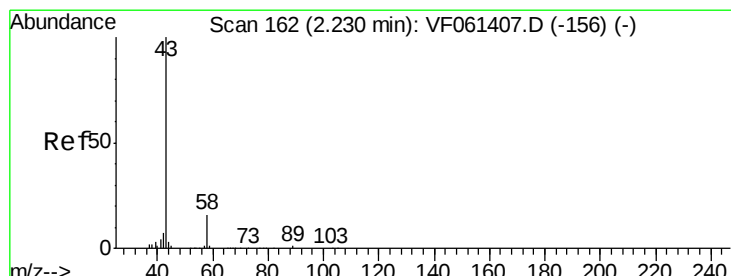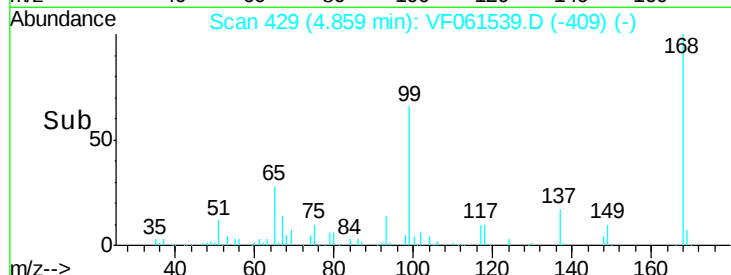

#16

Acetone

Concen: 66.812 ug/l

RT: 2.24 min Scan# 163

Delta R.T. 0.01 min

Lab File: VF061539.D


Acq: 28 Jan 2019 14:10

Tgt Ion: 43 Resp: 36623

Ion Ratio Lower Upper

43 100

58 19.0 13.3 19.9

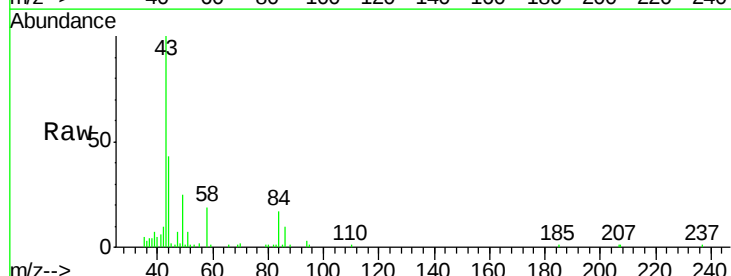

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0


15000


10000

5000

0

Time-->

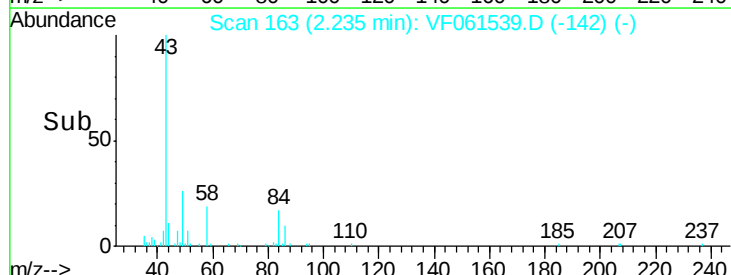

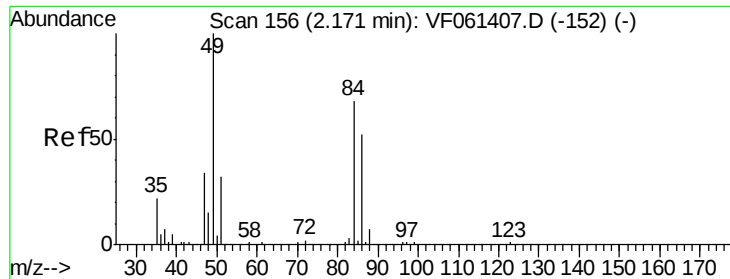

#20

Methylene Chloride

Concen: 8.828 ug/l

RT: 2.18 min Scan# 157

Delta R.T. 0.01 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10

Instrument :

MSVOA_F





ClientSampleId :

OR-01-012519-B

Tot Ion:	84	Resp:	19119
Ion	Ratio	Lower	Upper
84	100		
49	125.6	120.0	180.0
51	34.0	38.6	58.0#
86	49.5	61.0	91.6#

Manual Integrations
APPROVED

MMDadoda
1/29/2019 12:19:10 PM

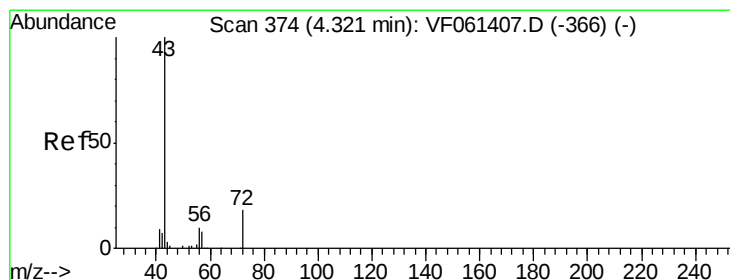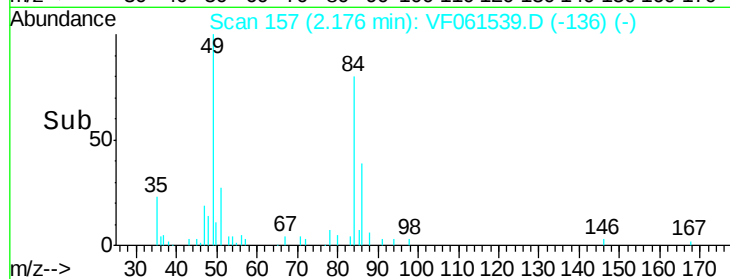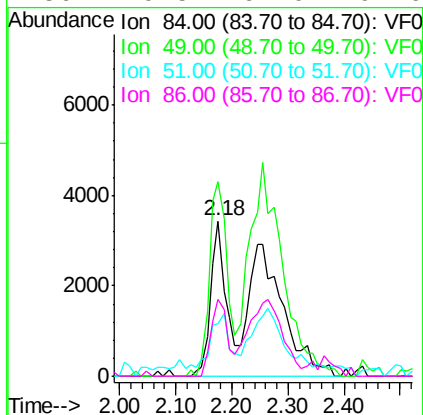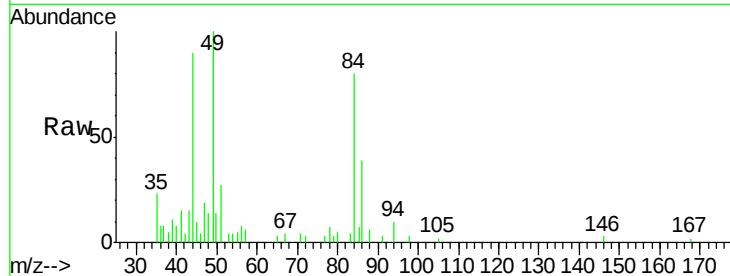

#25

2-Butanone

Concen: 6.659 ug/l




RT: 4.33 min Scan# 375


Delta R.T. 0.01 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10

Tgt Ion:	43	Resp:	6070
Ion	Ratio	Lower	Upper
43	100		
72	17.2	15.8	23.6

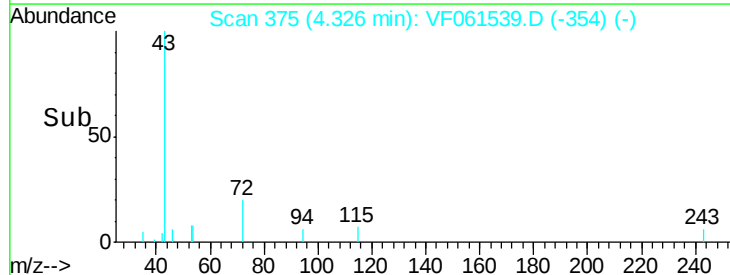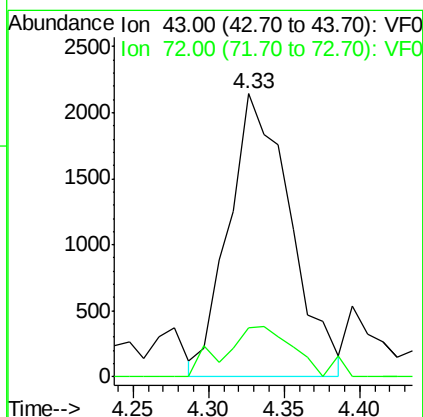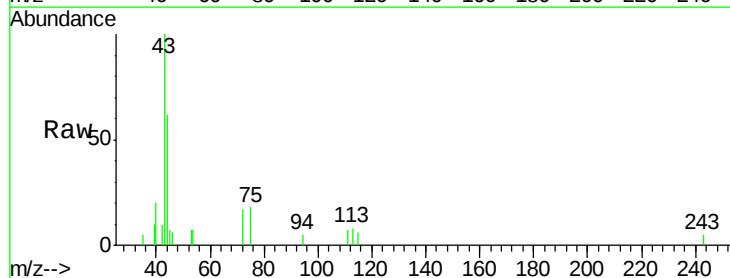

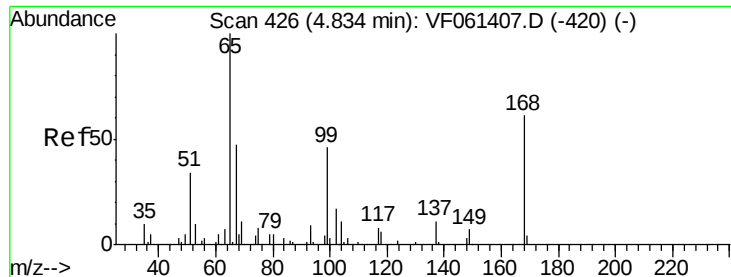

#33

1,2-Dichloroethane-d4

Concen: 44.501 ug/l

RT: 4.84 min Scan# 427

Delta R.T. 0.01 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10

Instrument :

MSVOA_F

ClientSampleId :

OR-01-012519-B

Tot Ion: 65 Resp: 121593

Ion Ratio Lower Upper

65 100





67 52.8 0.0 99.8

Manual Integrations

APPROVED

MMDadoda

1/29/2019 12:19:10 PM

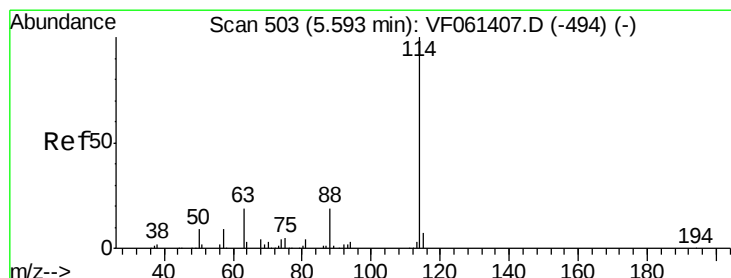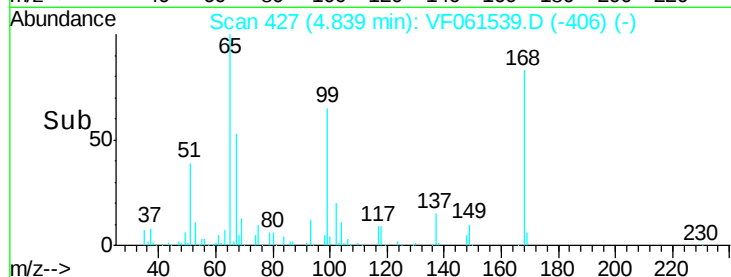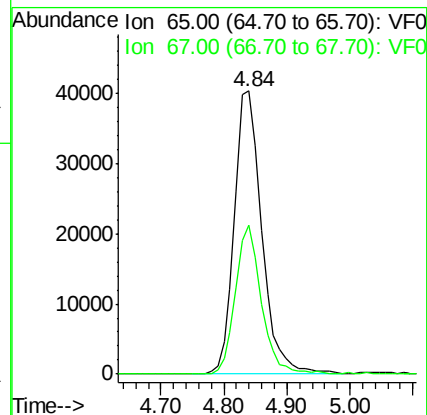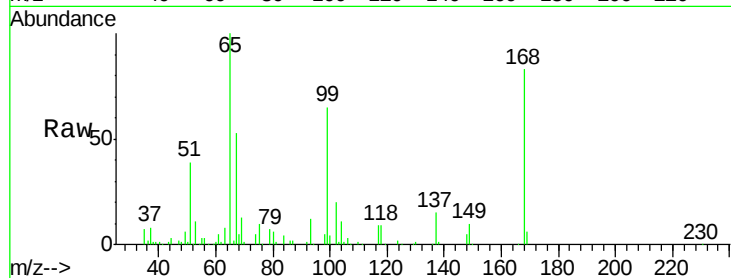

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.60 min Scan# 504

Delta R.T. 0.01 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10




Tgt Ion: 114 Resp: 390288


Ion Ratio Lower Upper

114 100

63 19.7 0.0 39.0

88 18.7 0.0 37.4

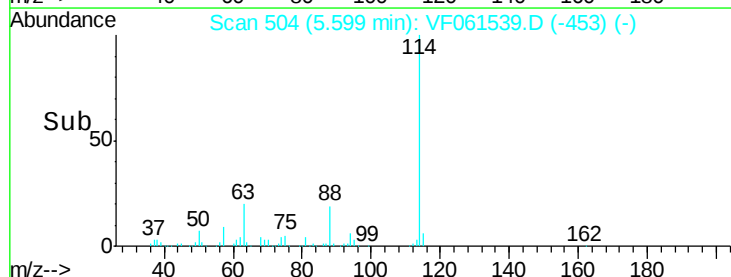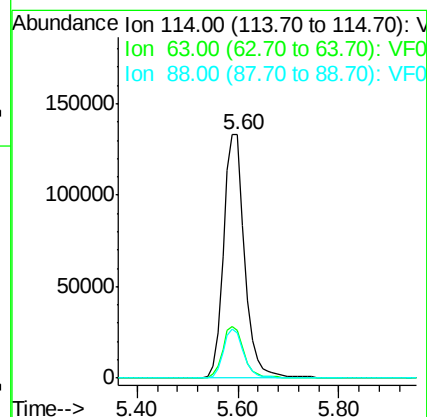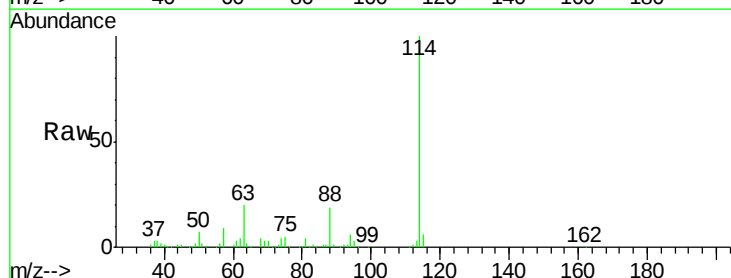

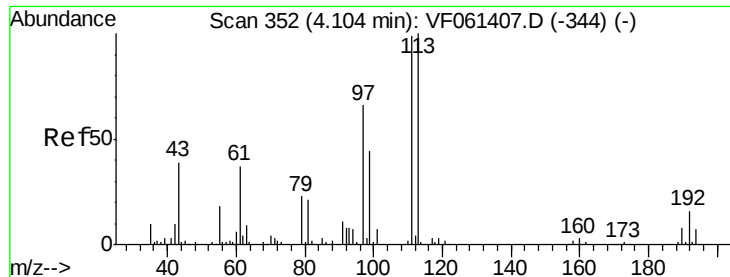





#35
Dibromofluoromethane
Concen: 47.818 ug/l
RT: 4.11 min Scan# 353
Delta R.T. 0.01 min
Lab File: VF061539.D
Acq: 28 Jan 2019 14:10

Instrument :
MSVOA_F
ClientSampleId :
OR-01-012519-B

Tot Ion	Ion	Ratio	Resp	Lower	Upper
113	100		147267		
111	98.8	79.4	119.0		
192	17.0	12.4	18.6		




Manual Integrations
APPROVED


MMDadoda
1/29/2019 12:19:10 PM

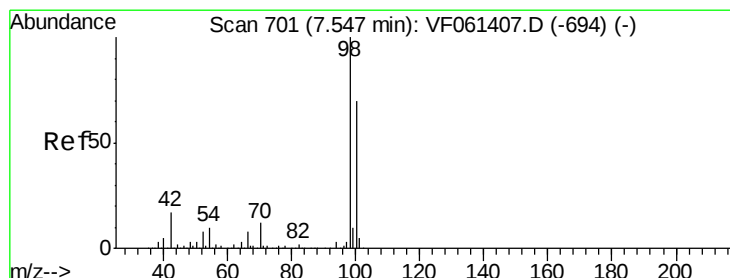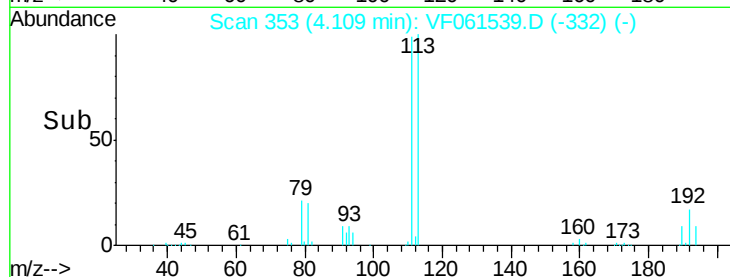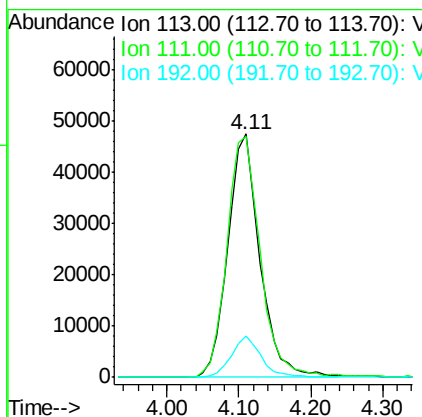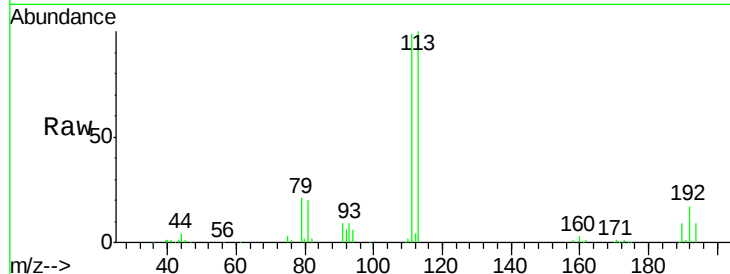

#50
Toluene-d8
Concen: 40.382 ug/l
RT: 7.54 min Scan# 701
Delta R.T. -0.00 min
Lab File: VF061539.D
Acq: 28 Jan 2019 14:10

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
98	100		340736		
100	70.5	55.6	83.4		

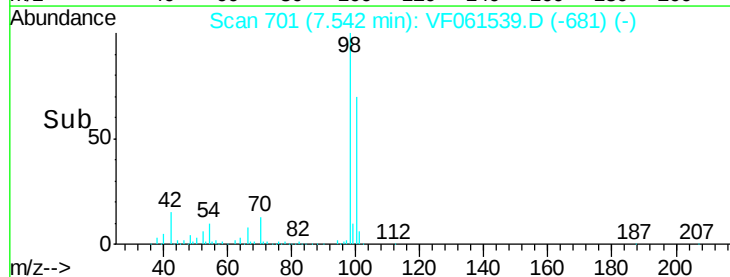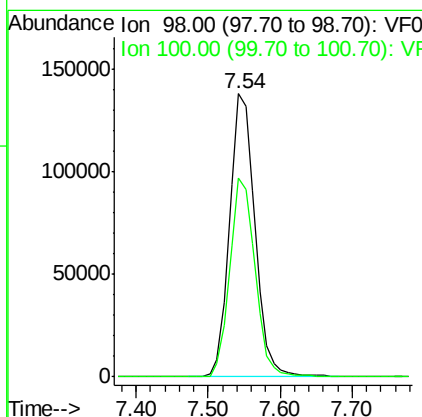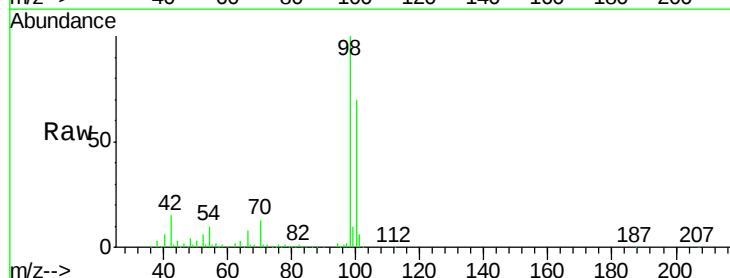

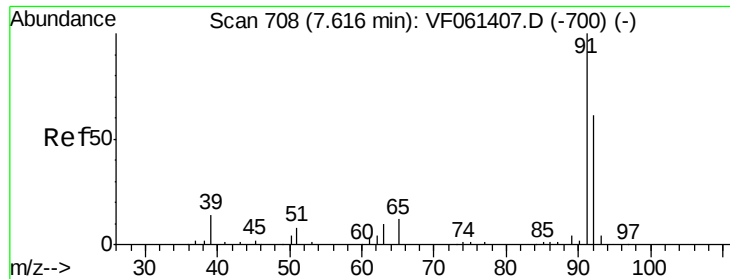

#52

Toluene

Concen: 2.614 ug/l

RT: 7.61 min Scan# 708

Delta R.T. -0.00 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10

Instrument :

MSVOA_F

ClientSampleId :

OR-01-012519-B

Tot Ion: 92 Resp: 17333

Ion Ratio Lower Upper

92 100


91 141.5 131.2 196.8

Manual Integrations

APPROVED




MMDadoda

1/29/2019 12:19:10 PM

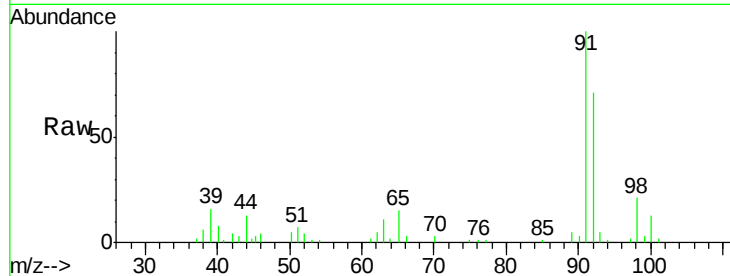

Abundance Ion 92.00 (91.70 to 92.70): VF0

Ion 91.00 (90.70 to 91.70): VF0

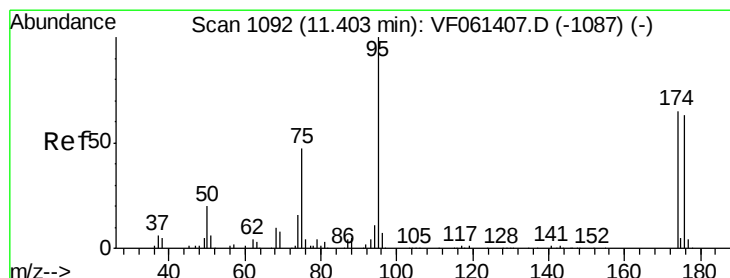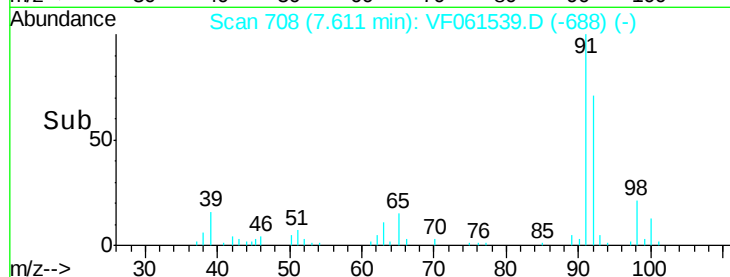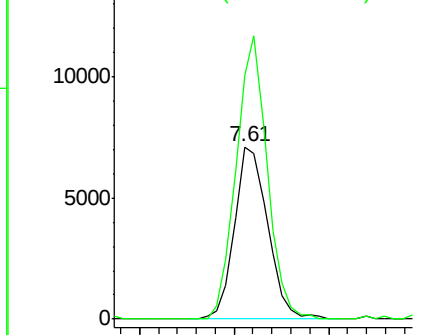

#62

4-Bromofluorobenzene

Concen: 36.662 ug/l

RT: 11.41 min Scan# 1093

Delta R.T. 0.01 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10


Tgt Ion: 95 Resp: 144536

Ion Ratio Lower Upper

95 100

174 72.1 0.0 130.4



176 67.0 0.0 126.2

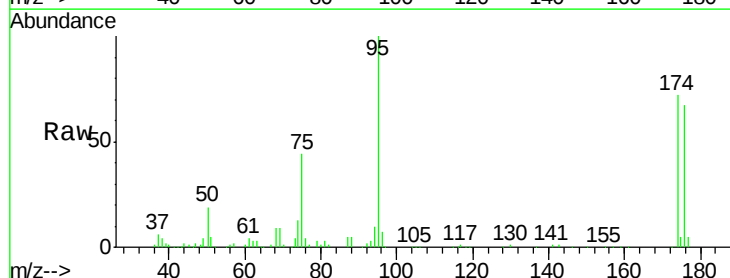


Abundance Ion 95.00 (94.70 to 95.70): VF0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

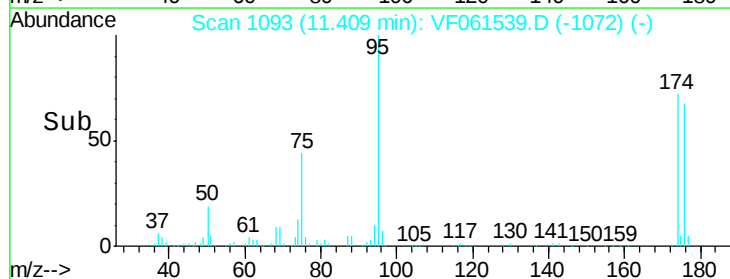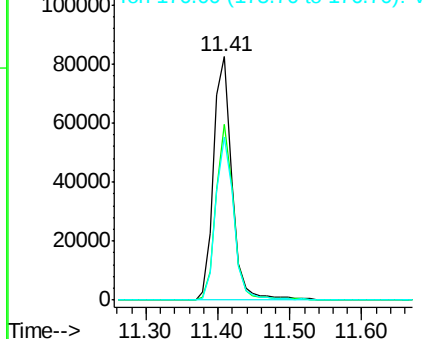

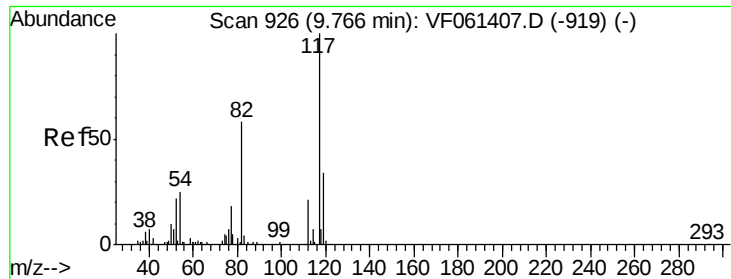





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.77 min Scan# 927
Delta R.T. 0.01 min
Lab File: VF061539.D
Acq: 28 Jan 2019 14:10

Instrument :
MSVOA_F
ClientSampleId :
OR-01-012519-B

Tot Ion	Ratio	Resp	Lower	Upper
117	100	328474		
82	59.7		46.4	69.6
119	33.0		27.2	40.8




Manual Integrations
APPROVED


MMDadoda
1/29/2019 12:19:10 PM

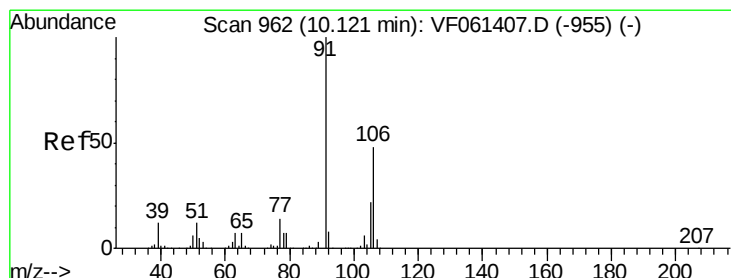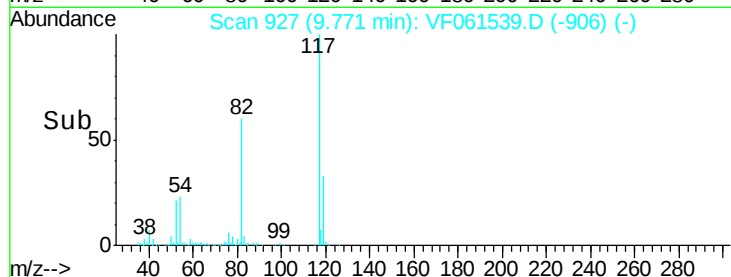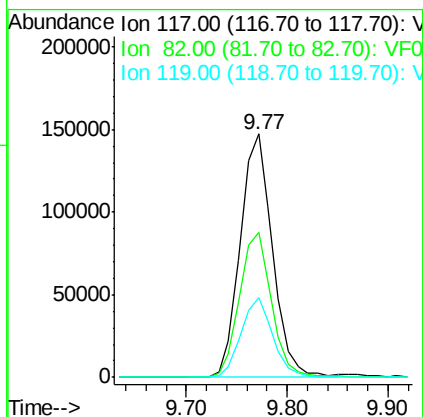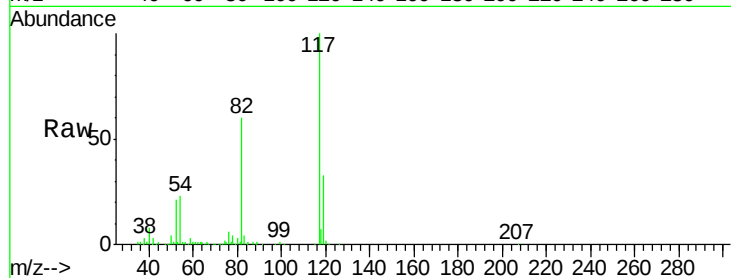

#68
m/p-Xylenes
Concen: 1.676 ug/l
RT: 10.13 min Scan# 963
Delta R.T. 0.01 min
Lab File: VF061539.D
Acq: 28 Jan 2019 14:10

Tgt Ion	Ratio	Resp	Lower	Upper
106	100	7356		
91	207.6		166.2	249.4

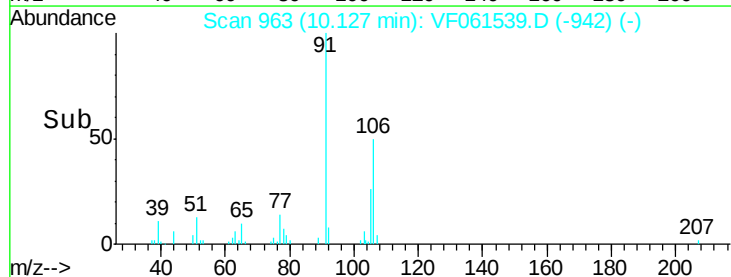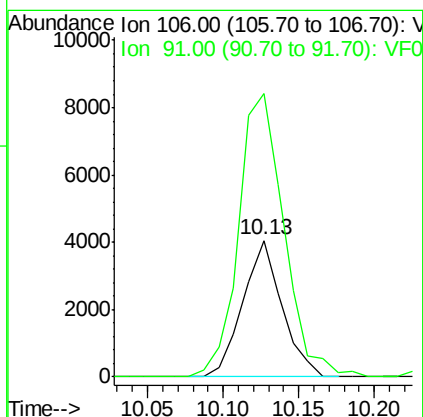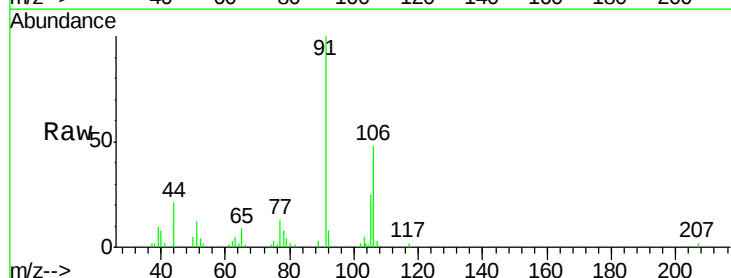

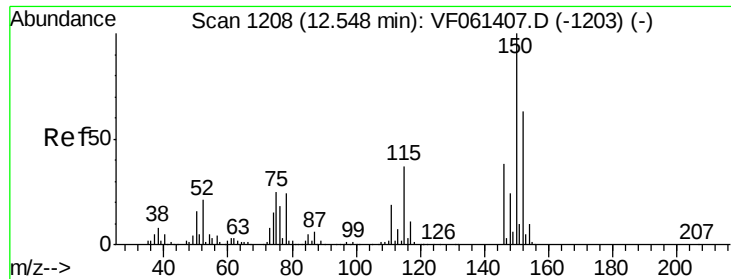

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.54 min Scan# 1208

Delta R.T. -0.00 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10

Instrument :

MSVOA_F

ClientSampleId :

OR-01-012519-B

Tot Ion:152 Resp: 143774

Ion Ratio Lower Upper

152 100


115 66.1 30.0 90.0

150 157.9 0.0 321.4




Manual Integrations
APPROVED

MMDadoda

1/29/2019 12:19:10 PM

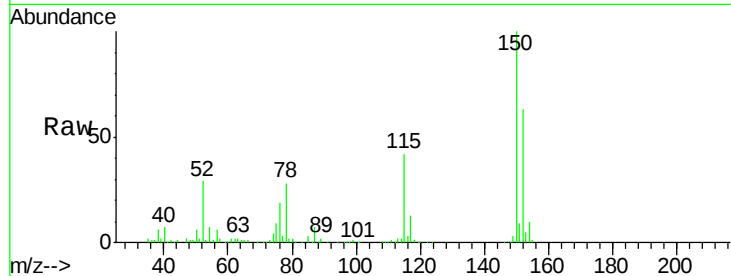

Abundance Ion 152.00 (151.70 to 152.70): V
Ion 115.00 (114.70 to 115.70): V
Ion 150.00 (149.70 to 150.70): V

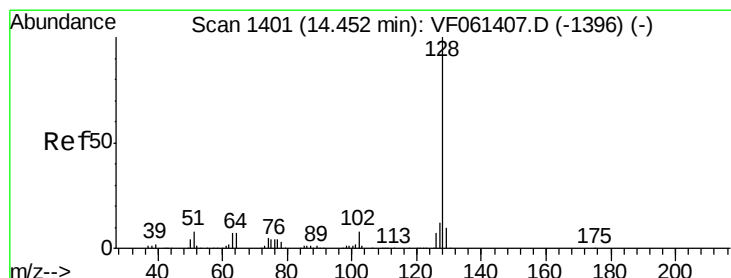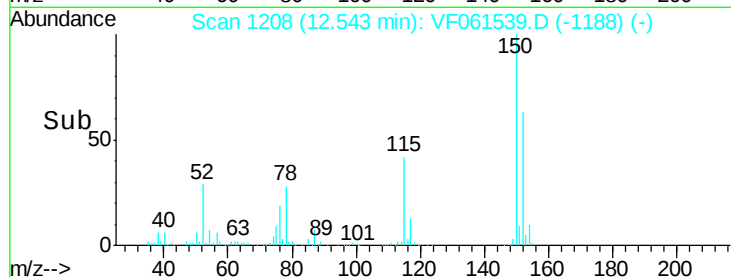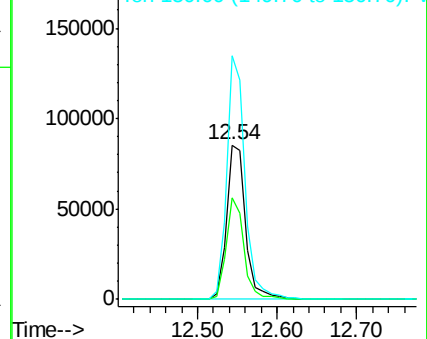

#95

Naphthalene

Concen: 1.372 ug/l

RT: 14.46 min Scan# 1402

Delta R.T. 0.01 min

Lab File: VF061539.D

Acq: 28 Jan 2019 14:10


Tgt Ion:128 Resp: 8437

Ion Ratio Lower Upper

128 100

127 6.0 9.5 14.3#

129 15.4 8.4 12.6#

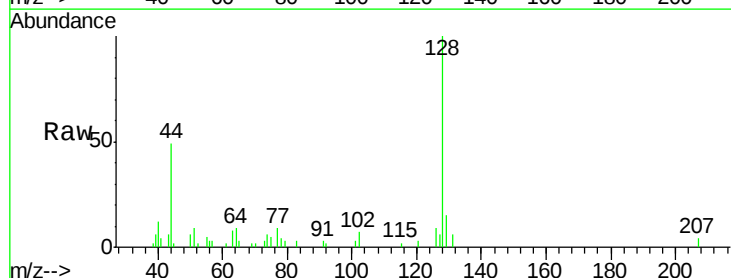

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

