


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF020719\
Data File : VF061541.D
Acq On : 7 Feb 2019 12:48
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
Title : SW846 8260
Last Update : Wed Jan 16 04:51:59 2019

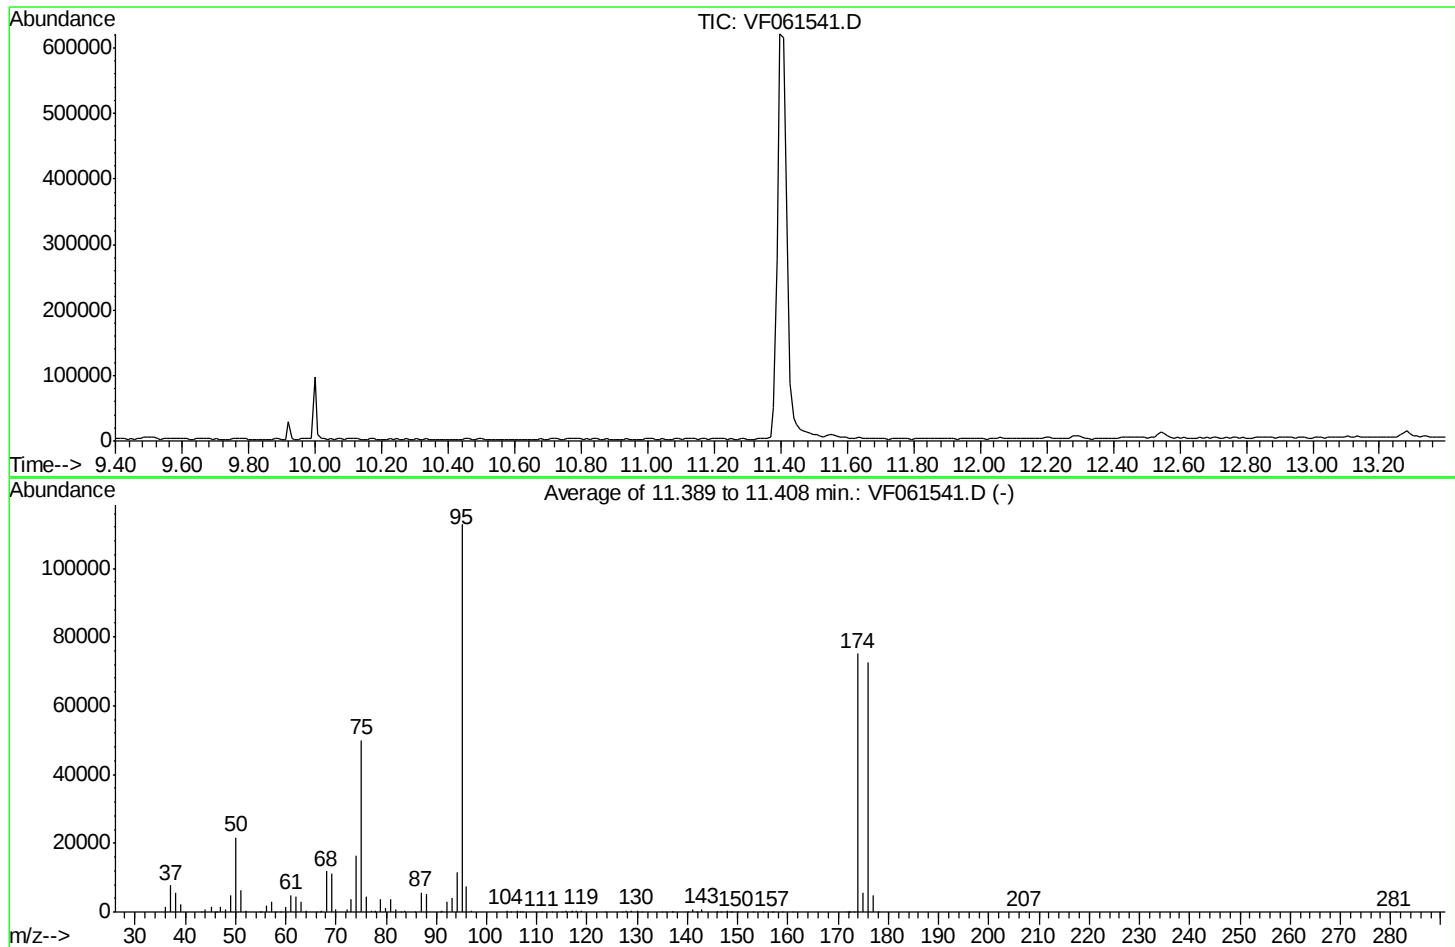

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	21652	PASS
75	95	30	60	44.4	50050	PASS
95	95	100	100	100.0	112800	PASS
96	95	5	9	6.7	7534	PASS
173	174	0.00	2	0.2	150	PASS
174	95	50	100	66.6	75165	PASS
175	174	5	9	7.6	5731	PASS
176	174	95	101	96.9	72813	PASS
177	176	5	9	6.9	4989	PASS