


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF021119\
 Data File : VF061580.D
 Acq On : 11 Feb 2019 10:33
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
 Title : SW846 8260
 Last Update : Wed Jan 16 04:51:59 2019

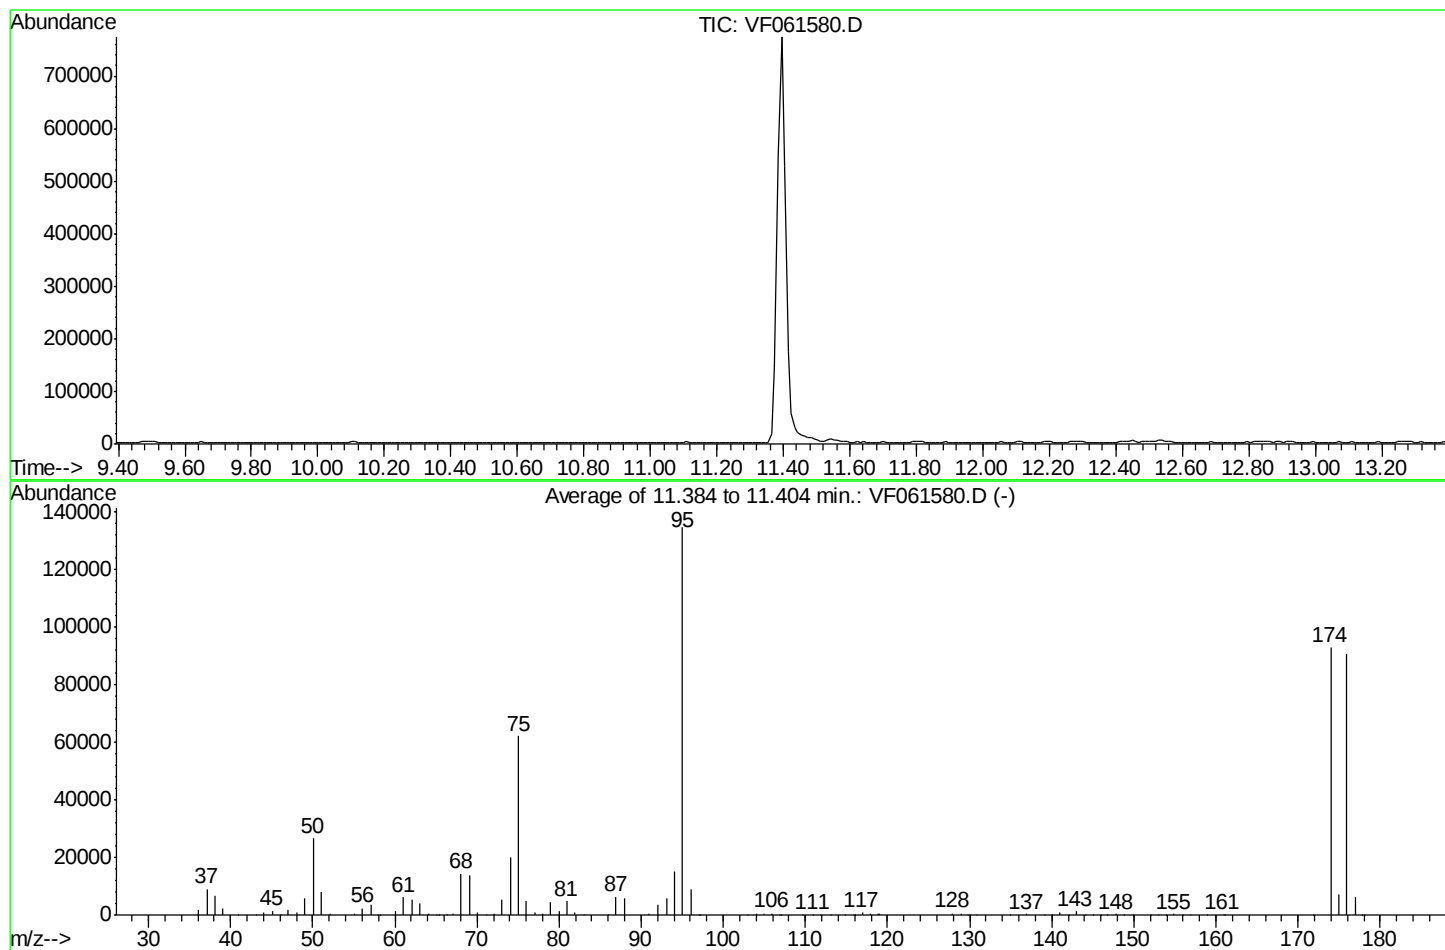

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1084

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	26568	PASS
75	95	30	60	46.2	62144	PASS
95	95	100	100	100.0	134610	PASS
96	95	5	9	6.8	9123	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.0	92861	PASS
175	174	5	9	7.7	7139	PASS
176	174	95	101	97.5	90514	PASS
177	176	5	9	6.7	6065	PASS