

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF021219\
 Data File : VF061615.D
 Acq On : 12 Feb 2019 18:11
 Operator : VA/AP
 Sample : K1343-17
 Misc : 6.45g/5mL/MSVOA-F/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 JC-02-021119-I

Quant Time: Feb 13 03:20:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 16 04:51:59 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.86	168	95253	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.59	114	147543	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.78	117	109898	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.55	152	36781	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.84	65	41749	35.50	ug/l	0.00
Spiked Amount 50.000			Recovery	=	71.00%	
35) Dibromofluoromethane	4.11	113	49601	42.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	85.20%	
50) Toluene-d8	7.55	98	121838	38.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	76.40%	
62) 4-Bromofluorobenzene	11.40	95	42942	28.81	ug/l	0.00
Spiked Amount 50.000			Recovery	=	57.62%	
Target Compounds						
16) Acetone	2.24	43	8346	35.376	ug/l #	91
20) Methylene Chloride	2.17	84	6889m	7.094	ug/l	
84) 1,2,4-Trimethylbenzene	12.20	105	6370	2.562	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF021219\
Data File : VF061615.D
Acq On : 12 Feb 2019 18:11
Operator : VA/AP
Sample : K1343-17
Misc : 6.45g/5mL/MSVOA-F/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
JC-02-021119-I

Quant Time: Feb 13 03:20:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
Quant Title : SW846 8260
QLast Update : Wed Jan 16 04:51:59 2019
Response via : Initial Calibration

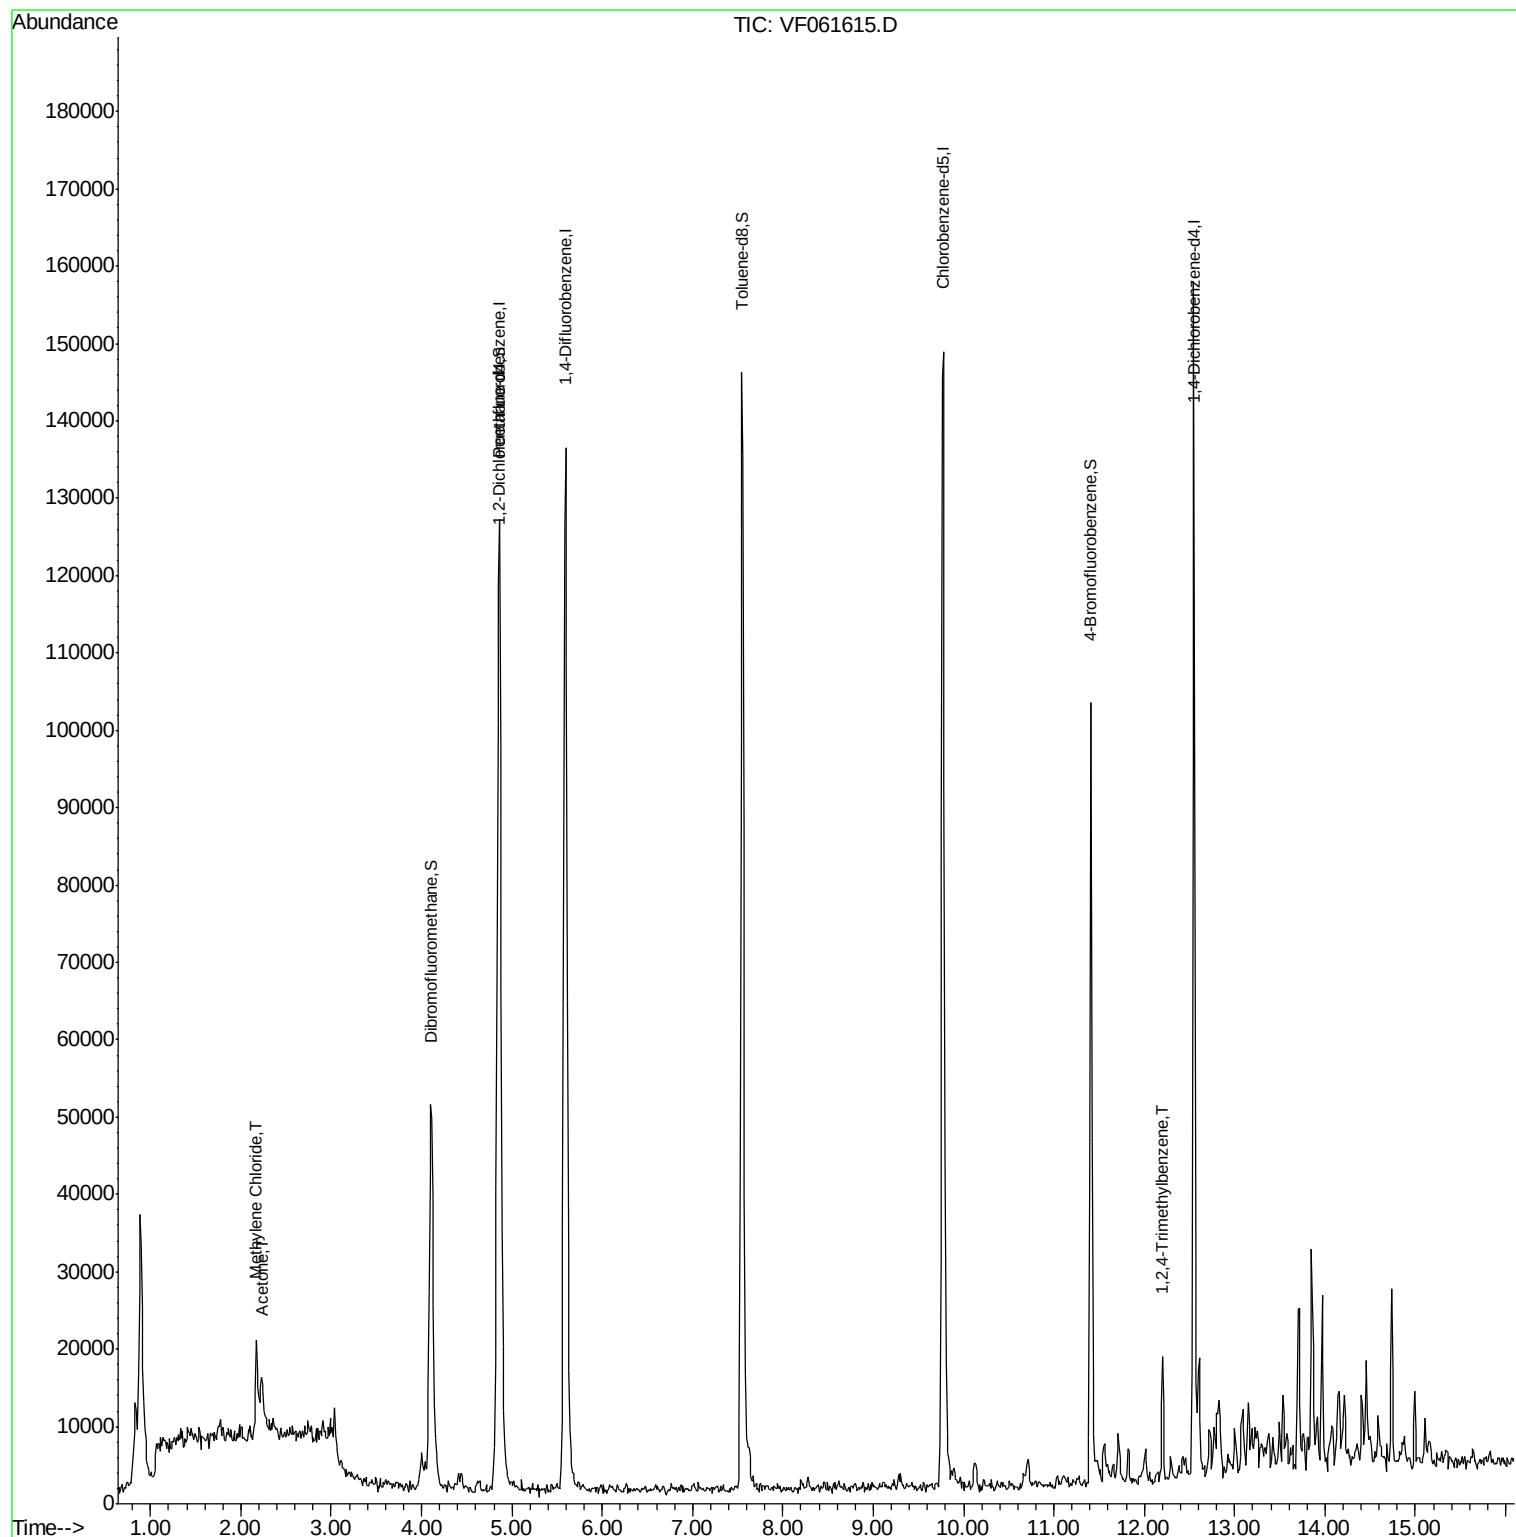

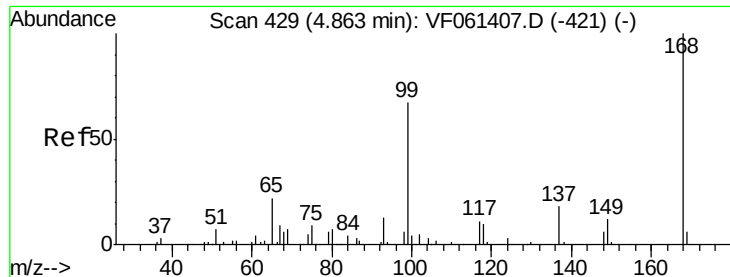

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.86 min Scan# 429

Delta R.T. 0.00 min

Lab File: VF061615.D

Acq: 12 Feb 2019 18:11

Instrument :

MSVOA_F

ClientSampleId :


JC-02-021119-I

Tot Ion:168 Resp: 95253

Ion Ratio Lower Upper

168 100

99 65.6 53.5 80.3

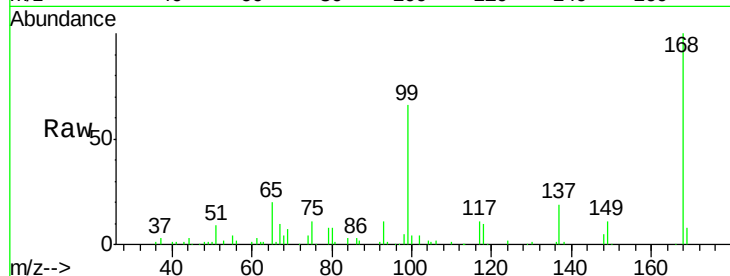

Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

4.86

30000



20000

10000

0

Time-->

4.70 4.80 4.90 5.00 5.10

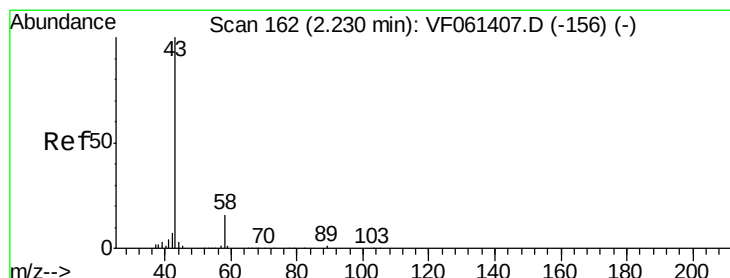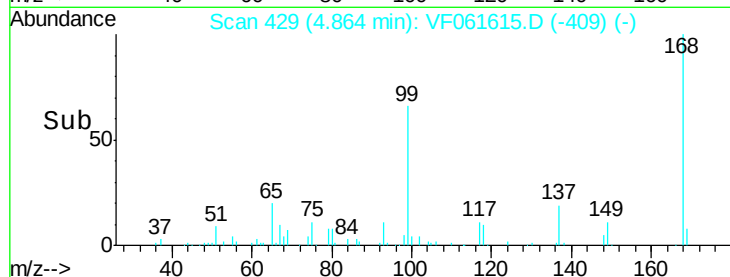

#16

Acetone

Concen: 35.376 ug/l

RT: 2.24 min Scan# 163

Delta R.T. 0.01 min

Lab File: VF061615.D


Acq: 12 Feb 2019 18:11

Tgt Ion: 43 Resp: 8346

Ion Ratio Lower Upper

43 100

58 20.7 13.3 19.9#

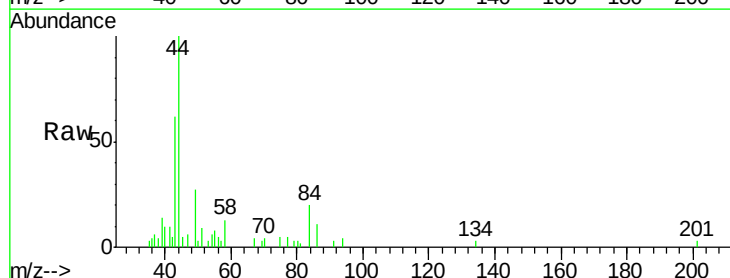

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0

2.24

3000

2500

2000

1500


1000


500

0

Time-->

2.10 2.20 2.30




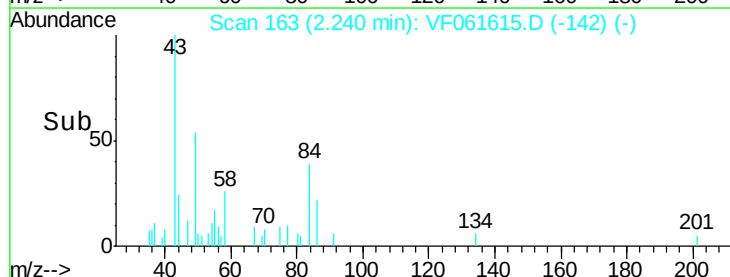


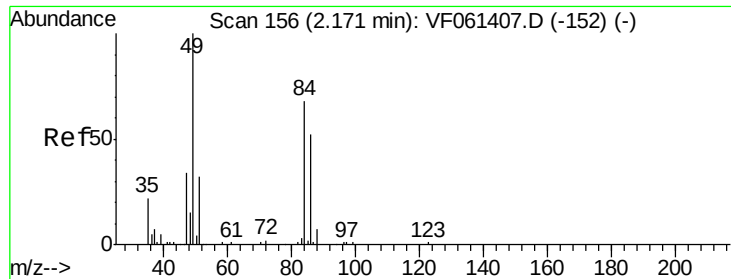

#20
Methylene Chloride
Concen: 7.094 ug/l m
RT: 2.17 min Scan# 156
Delta R.T. 0.00 min
Lab File: VF061615.D
Acq: 12 Feb 2019 18:11




Instrument :
MSVOA_F
ClientSampleId :
JC-02-021119-I


Tot Ion: 84 Resp: 6889
Ion Ratio Lower Upper
84 100
49 138.7 120.0 180.0
51 42.2 38.6 58.0
86 67.1 61.0 91.6

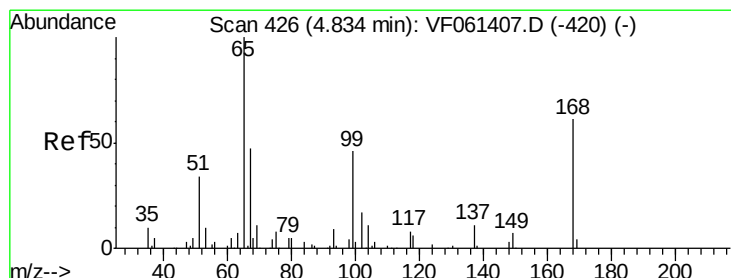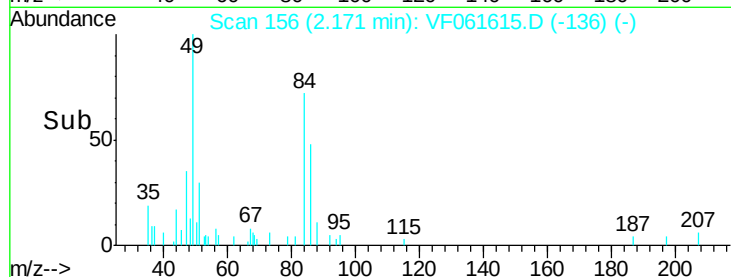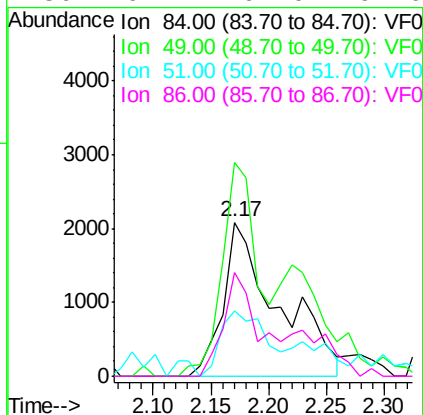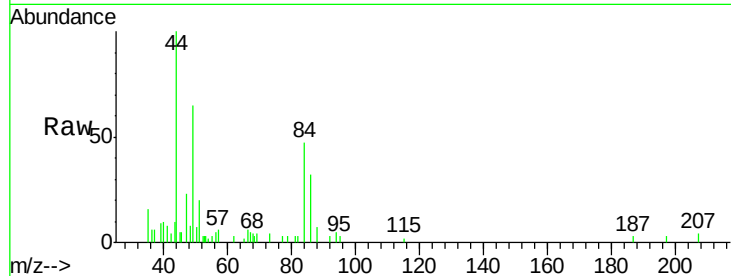

#33
1,2-Dichloroethane-d4
Concen: 35.500 ug/l
RT: 4.84 min Scan# 427
Delta R.T. 0.01 min
Lab File: VF061615.D
Acq: 12 Feb 2019 18:11

Tgt Ion: 65 Resp: 41749
Ion Ratio Lower Upper
65 100
67 50.5 0.0 99.8

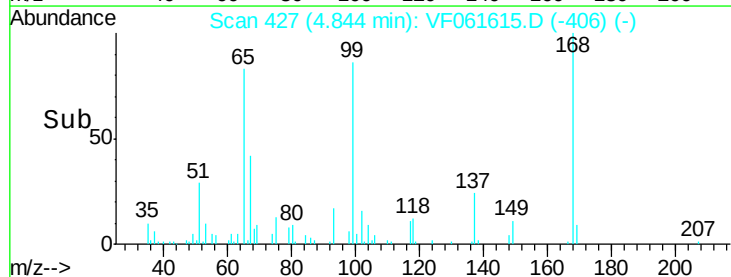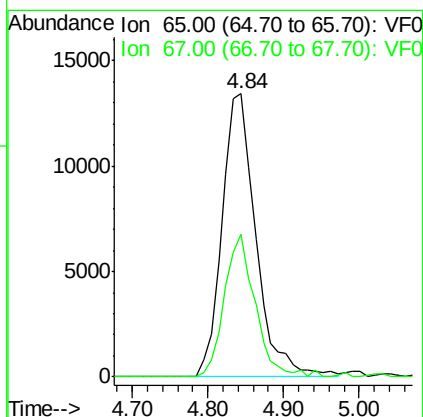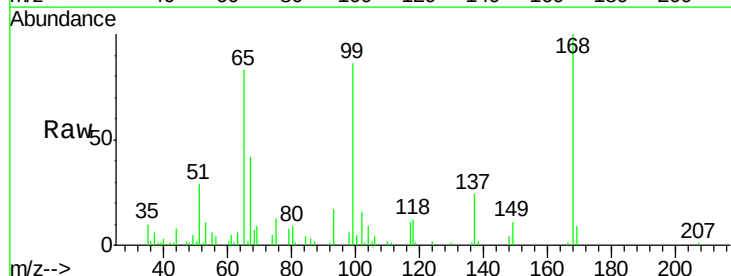

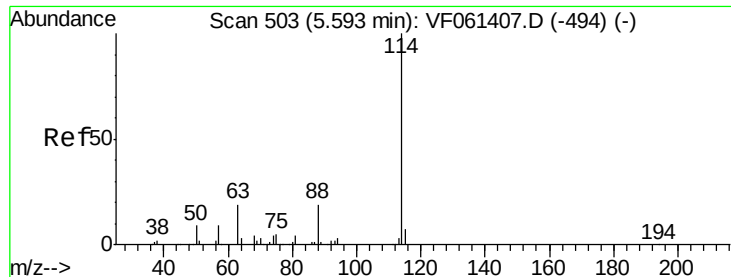

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.59 min Scan# 503

Delta R.T. 0.00 min

Lab File: VF061615.D

Acq: 12 Feb 2019 18:11

Instrument :

MSVOA_F

ClientSampleId :

JC-02-021119-I


Tot Ion:114 Resp: 147543

Ion Ratio Lower Upper

114 100

63 20.3 0.0 39.0




88 19.3 0.0 37.4

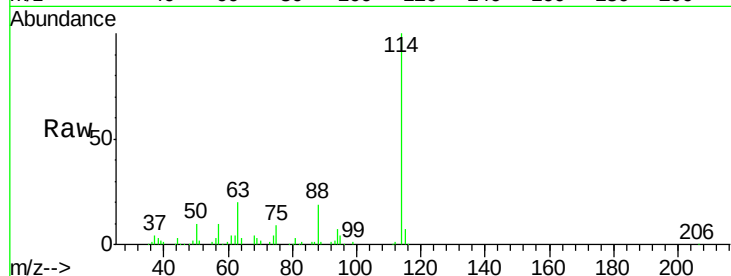

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

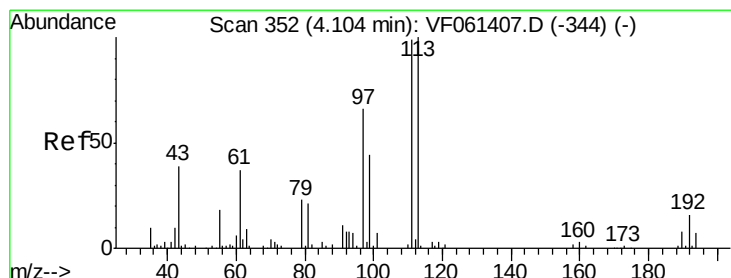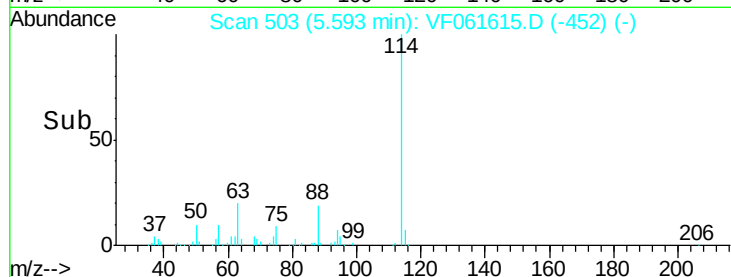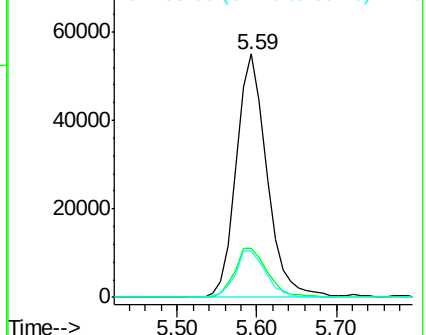

#35

Dibromofluoromethane

Concen: 42.604 ug/l

RT: 4.11 min Scan# 353

Delta R.T. 0.01 min

Lab File: VF061615.D

Acq: 12 Feb 2019 18:11


Tgt Ion:113 Resp: 49601

Ion Ratio Lower Upper

113 100

111 103.8 79.4 119.0



192 14.1 12.4 18.6

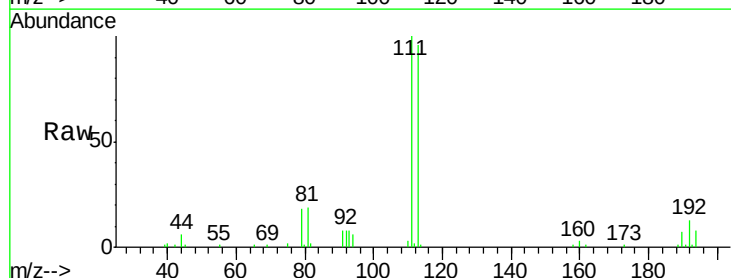


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V



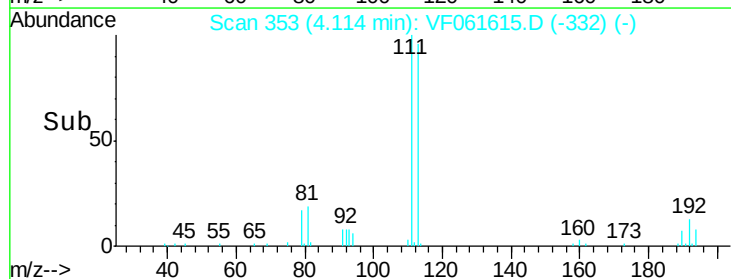
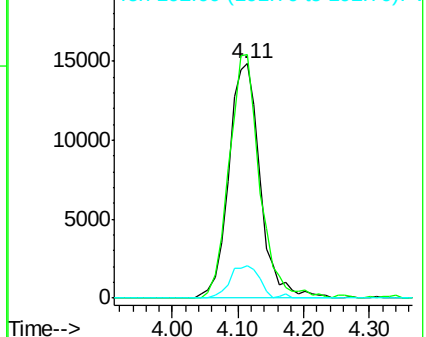


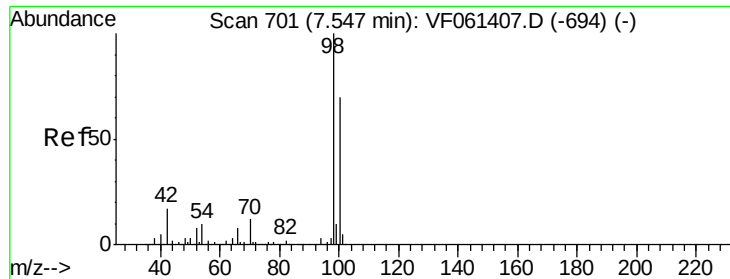

#50
Toluene-d8
Concen: 38.196 ug/l
RT: 7.55 min Scan# 701
Delta R.T. 0.00 min
Lab File: VF061615.D
Acq: 12 Feb 2019 18:11




Instrument :
MSVOA_F
ClientSampleId :
JC-02-021119-I


Tot Ion: 98 Resp: 121838
Ion Ratio Lower Upper
98 100
100 72.4 55.6 83.4

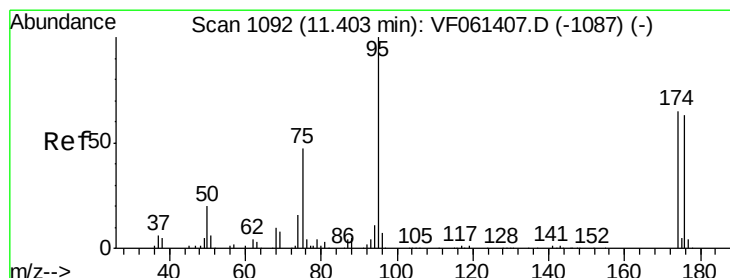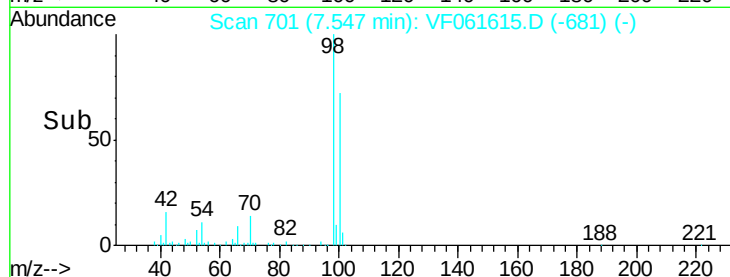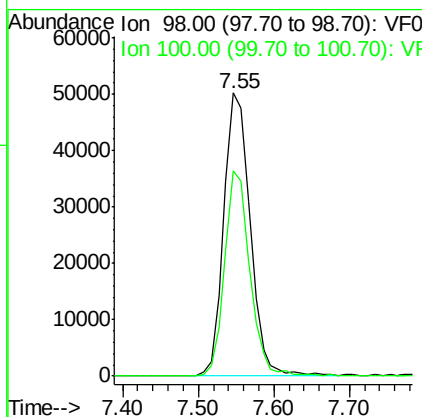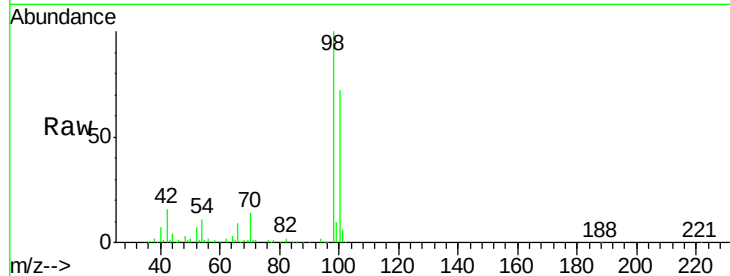

#62
4-Bromofluorobenzene
Concen: 28.813 ug/l
RT: 11.40 min Scan# 1092
Delta R.T. 0.00 min
Lab File: VF061615.D
Acq: 12 Feb 2019 18:11

Tgt Ion: 95 Resp: 42942
Ion Ratio Lower Upper
95 100
174 55.2 0.0 130.4
176 59.6 0.0 126.2


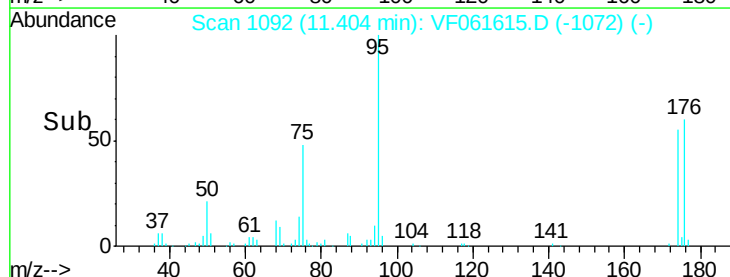
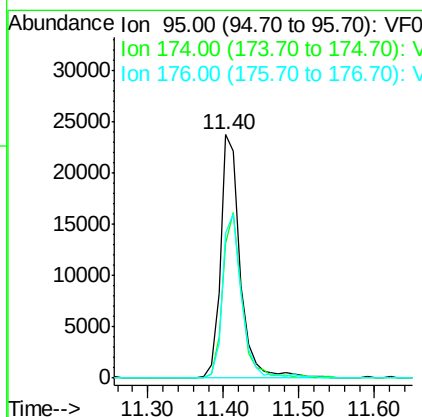
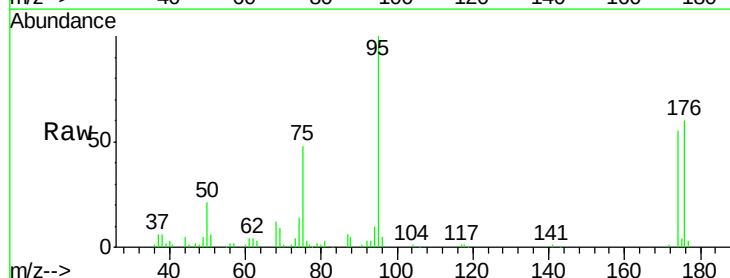


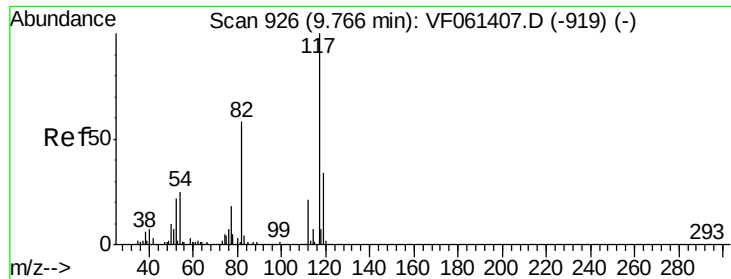

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.78 min Scan# 927
Delta R.T. 0.01 min
Lab File: VF061615.D
Acq: 12 Feb 2019 18:11




Instrument :
MSVOA_F
ClientSampleId :
JC-02-021119-I


Tot Ion	Ratio	Lower	Upper
117	100		
82	54.0	46.4	69.6
119	33.9	27.2	40.8

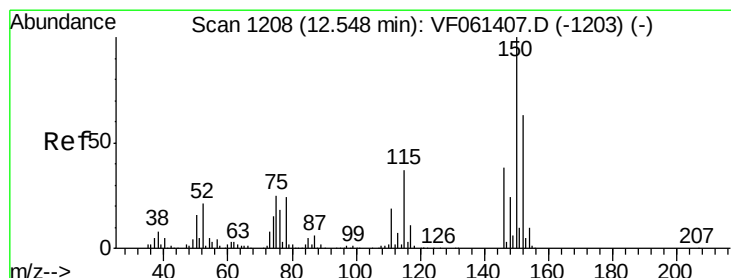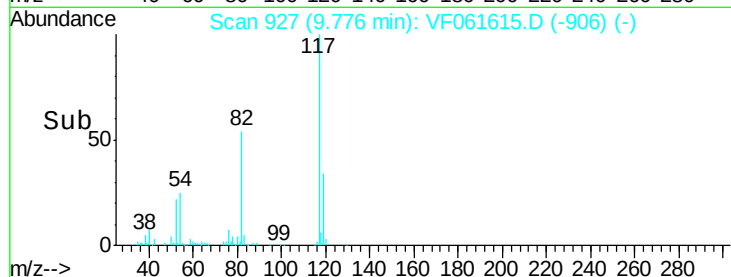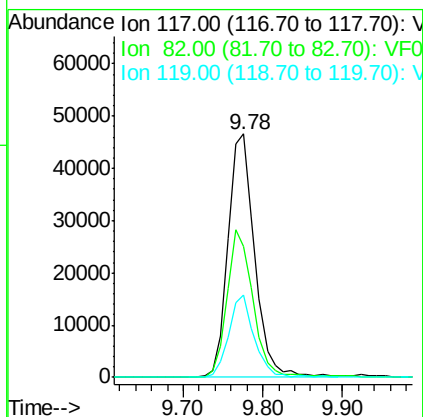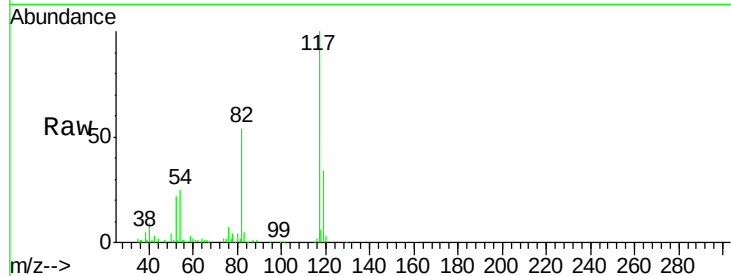

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.55 min Scan# 1208
Delta R.T. 0.00 min
Lab File: VF061615.D
Acq: 12 Feb 2019 18:11

Tgt Ion	Ratio	Lower	Upper
152	100		
115	58.9	30.0	90.0
150	155.6	0.0	321.4

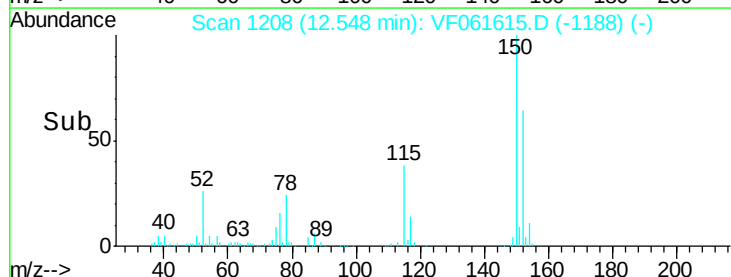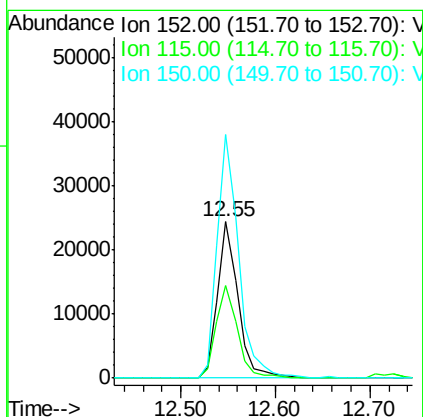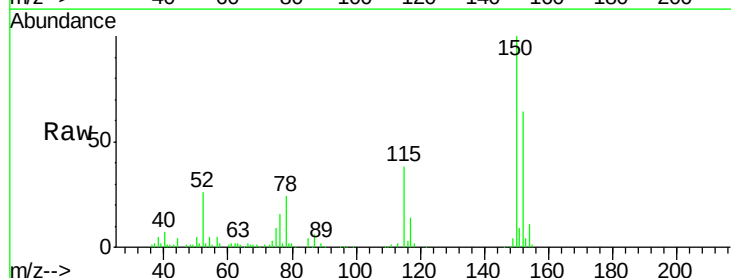

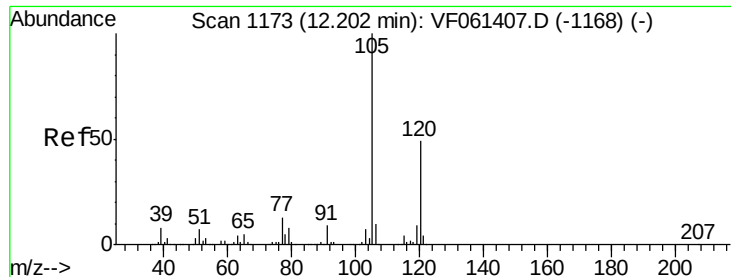

#84
 1,2,4-Trimethylbenzene
 Concen: 2.562 ug/l
 RT: 12.20 min Scan# 1173
 Delta R.T. 0.00 min
 Lab File: VF061615.D
 Acq: 12 Feb 2019 18:11

Instrument :
 MSVOA_F
 ClientSampleId :
 JC-02-021119-I

Tot Ion:105 Resp: 6370
 Ion Ratio Lower Upper
 105 100
 120 48.8 24.9 74.6

