


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF021219\
Data File : VF061602.D
Acq On : 12 Feb 2019 10:15
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F011519S.M
Title : SW846 8260
Last Update : Wed Jan 16 04:51:59 2019

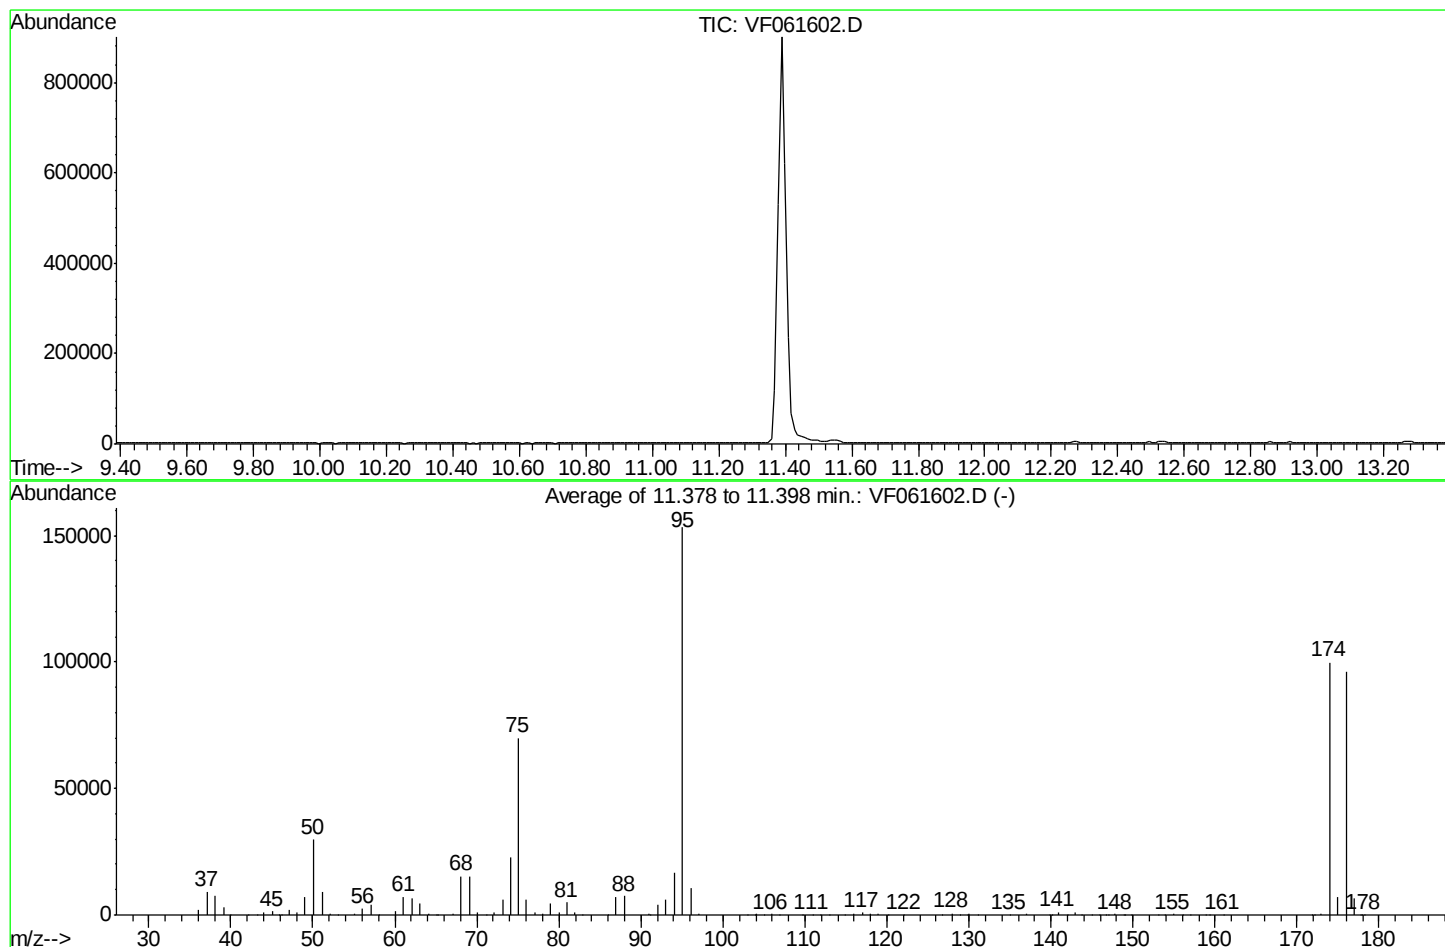

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	29818	PASS
75	95	30	60	45.7	70024	PASS
95	95	100	100	100.0	153226	PASS
96	95	5	9	6.9	10551	PASS
173	174	0.00	2	0.6	611	PASS
174	95	50	100	65.2	99853	PASS
175	174	5	9	7.1	7084	PASS
176	174	95	101	96.5	96344	PASS
177	176	5	9	6.9	6627	PASS