


Data Path : Z:\voasrv\HPCHEM1\MSVOA_F\Data\VF021419\
 Data File : VF061631.D
 Acq On : 14 Feb 2019 9:42
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
 Title : SW846 8260
 Last Update : Thu Feb 14 03:27:56 2019

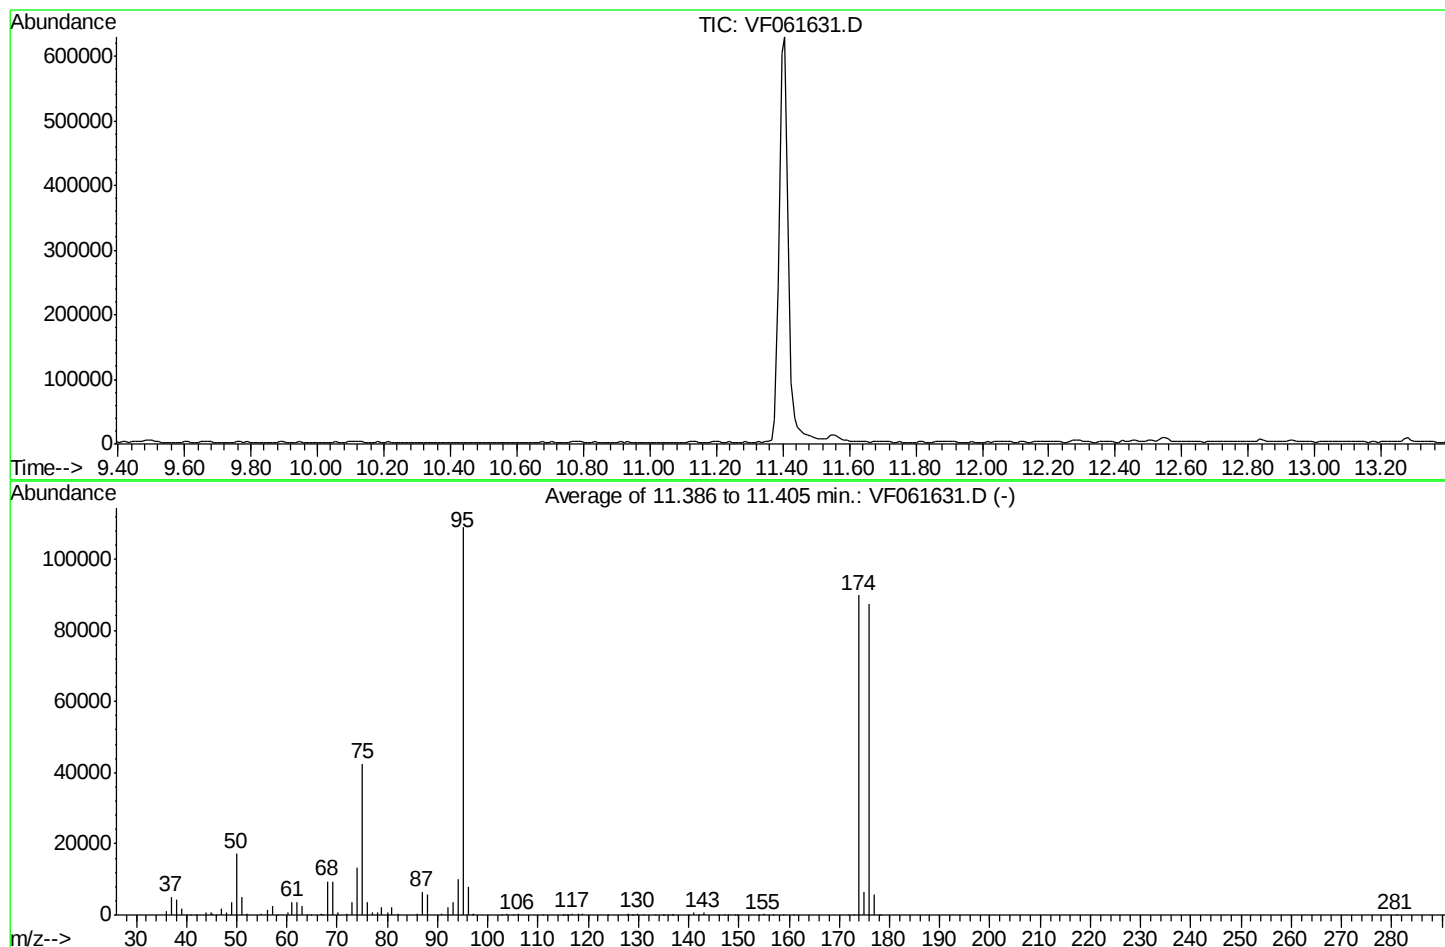

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	17175	PASS
75	95	30	60	39.0	42461	PASS
95	95	100	100	100.0	108936	PASS
96	95	5	9	7.2	7809	PASS
173	174	0.00	2	0.1	55	PASS
174	95	50	100	82.5	89821	PASS
175	174	5	9	7.1	6376	PASS
176	174	95	101	97.2	87344	PASS
177	176	5	9	6.5	5683	PASS