

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF022119\
 Data File : VF061702.D
 Acq On : 21 Feb 2019 17:08
 Operator : VA/AP
 Sample : K1537-01
 Misc : 9.54g/5mL/MSVOA-F/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 DRUM-1-2

Quant Time: Feb 22 03:29:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 14 03:27:56 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-4.89
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-5.61
63) Chlorobenzene-d5	9.79	117	84	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.56
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
35) Dibromofluoromethane	4.13	113	67	0.00	ug/l	0.00
Spiked Amount	50.000		Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
62) 4-Bromofluorobenzene	11.26	95	60	0.00	ug/l	-0.16
Spiked Amount	50.000		Recovery	=	0.00%	
Target Compounds						
68) m/p-Xylenes	9.98	106	62	57.150	ug/l #	1
70) Styrene	10.79	104	66	40.302	ug/l #	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF022119\
Data File : VF061702.D
Acq On : 21 Feb 2019 17:08
Operator : VA/AP
Sample : K1537-01
Misc : 9.54g/5mL/MSVOA-F/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
DRUM-1-2

Quant Time: Feb 22 03:29:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
Quant Title : SW846 8260
QLast Update : Thu Feb 14 03:27:56 2019
Response via : Initial Calibration

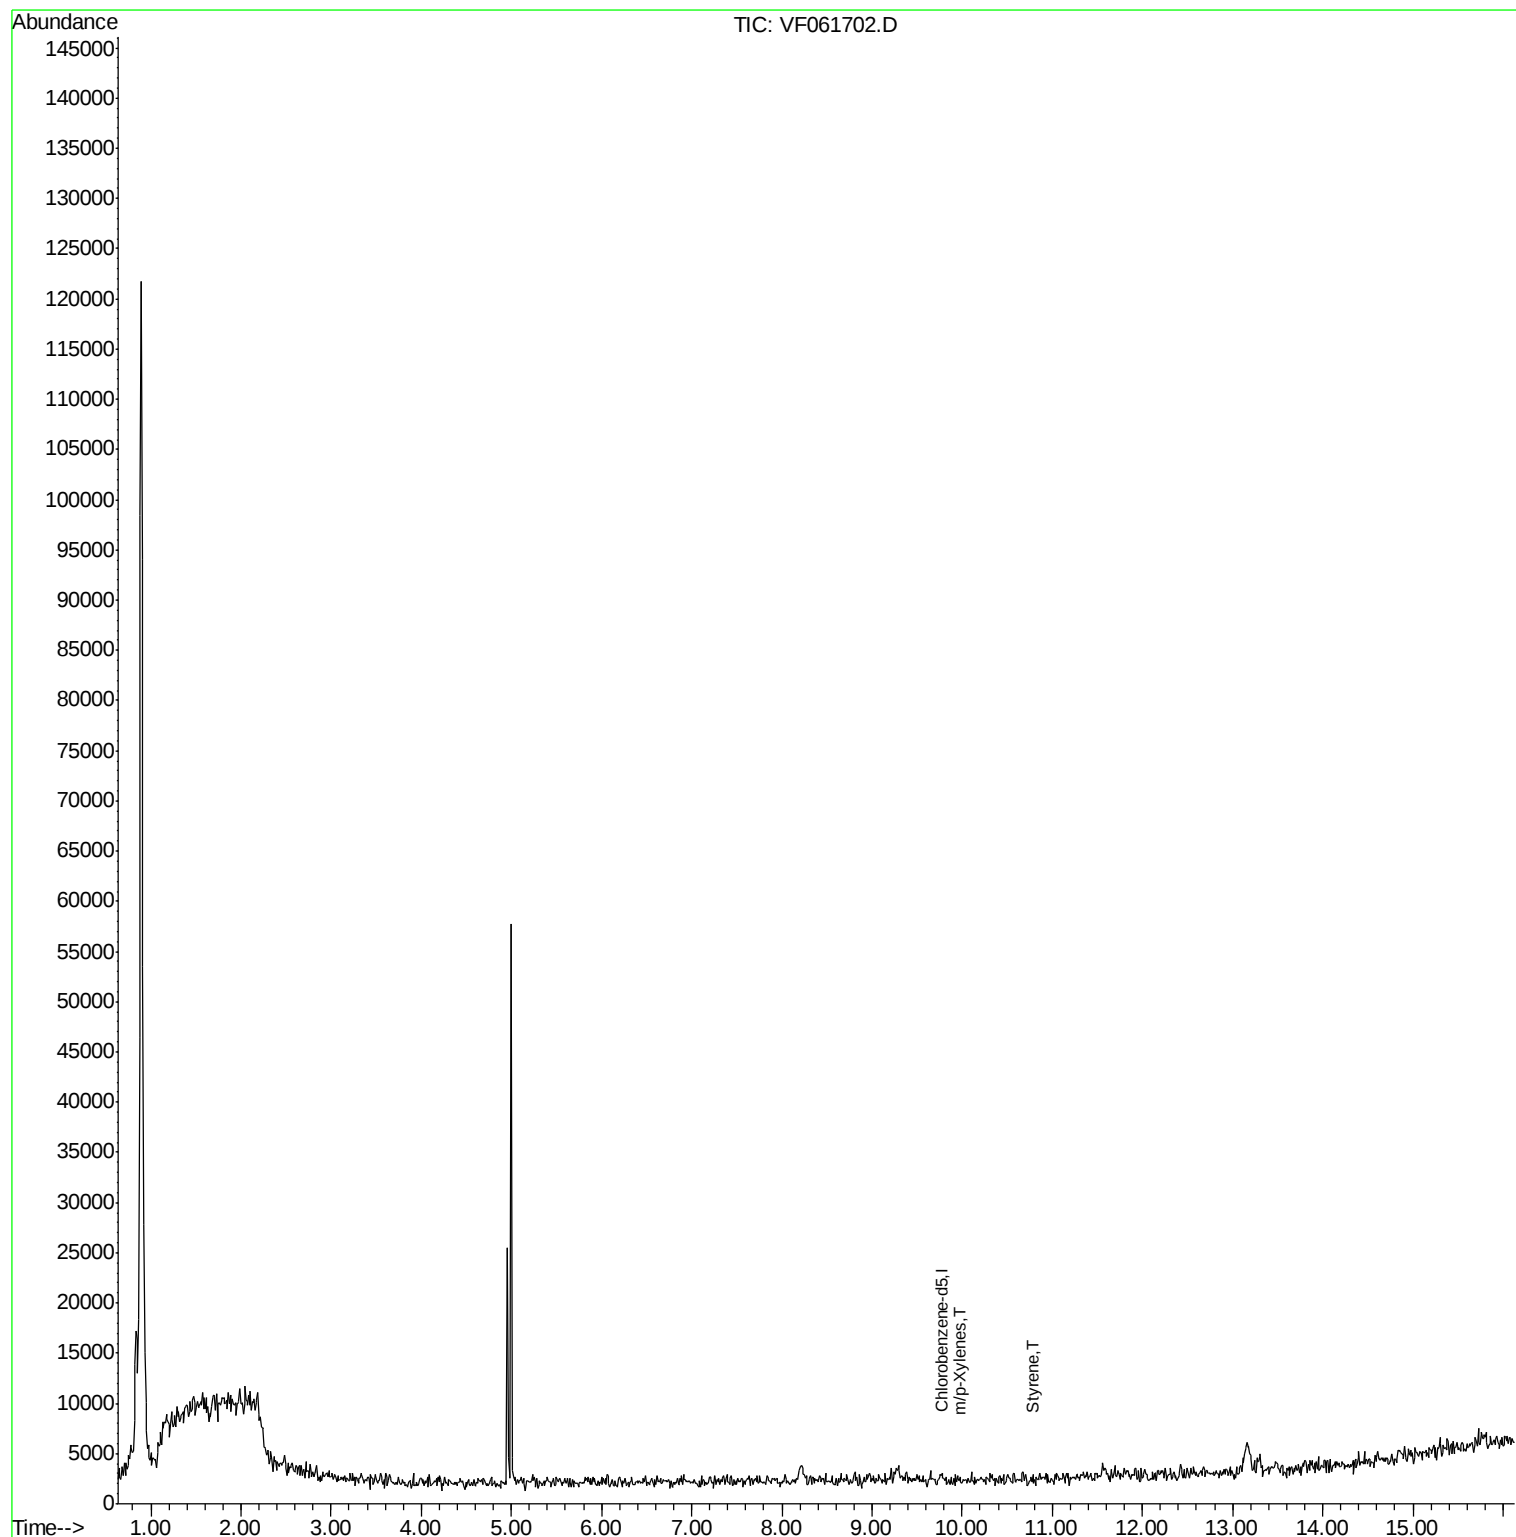

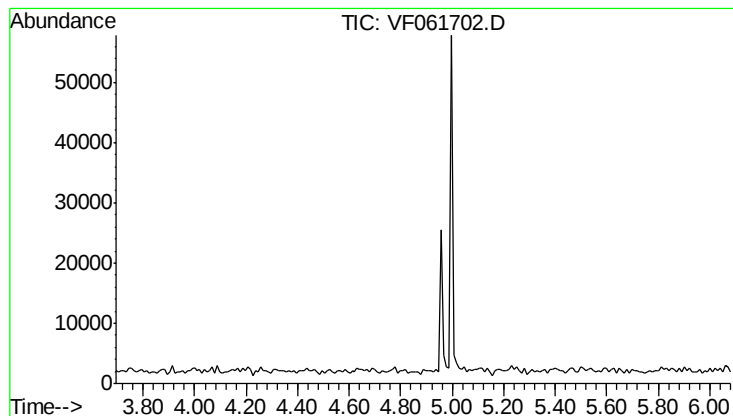

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 4.89 min

Lab File: VF061702.D

Acq: 21 Feb 2019 17:08

Tot Ion: 168

Sig Exp Ratio

168 100



99 43.6

Instrument :

MSVOA_F

ClientSampleId :

DRUM-1-2

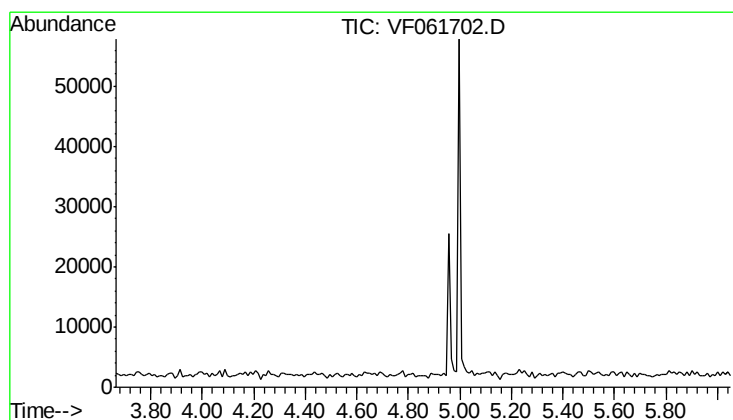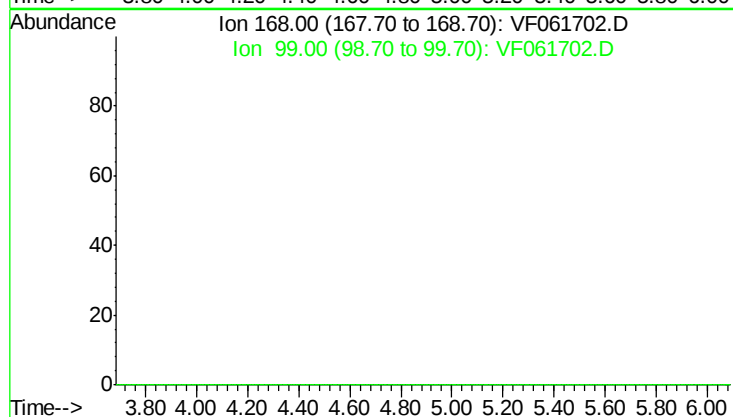

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 4.86 min

Lab File: VF061702.D


Acq: 21 Feb 2019 17:08


Tgt Ion: 65

Sig Exp Ratio

65 100

67 52.0

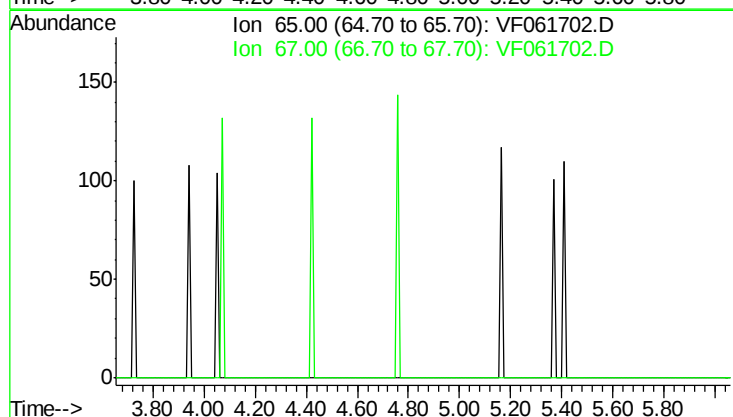

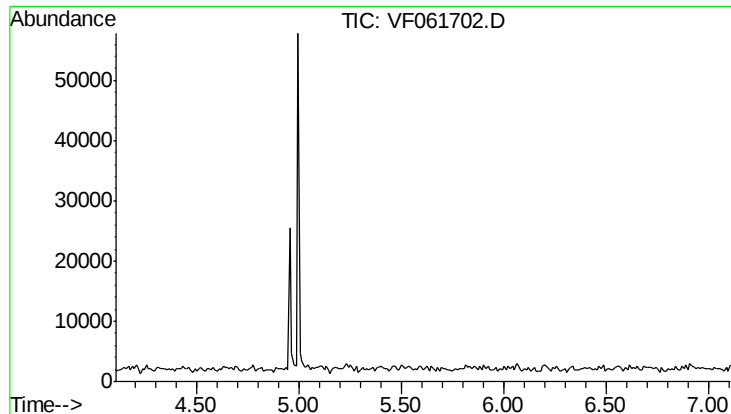

#34

1,4-Difluorobenzene

Concen: 0.000 ug/l

Expected RT: 5.61 min

Lab File: VF061702.D

Acq: 21 Feb 2019 17:08

Instrument :

MSVOA_F

ClientSampleId :

DRUM-1-2



Tot Ion: 114

Sig Exp Ratio

114 100

63 18.3

88 17.2

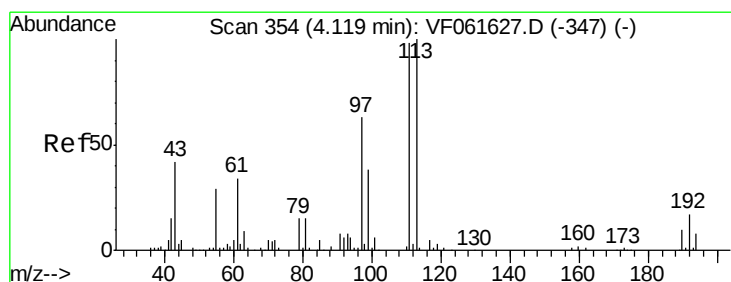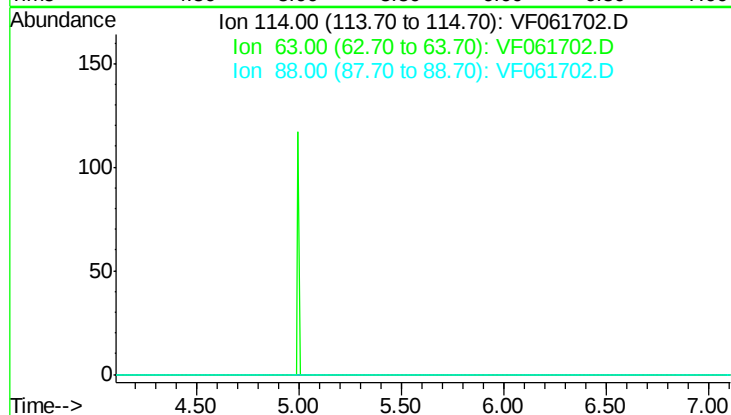

#35

Dibromofluoromethane

Concen: 0.000 ug/l

RT: 4.13 min Scan# 355

Delta R.T. 0.01 min

Lab File: VF061702.D

Acq: 21 Feb 2019 17:08




Tgt Ion: 113 Resp: 67


Ion Ratio Lower Upper

113 100

111 0.0 78.8 118.2#

192 0.0 13.4 20.0#

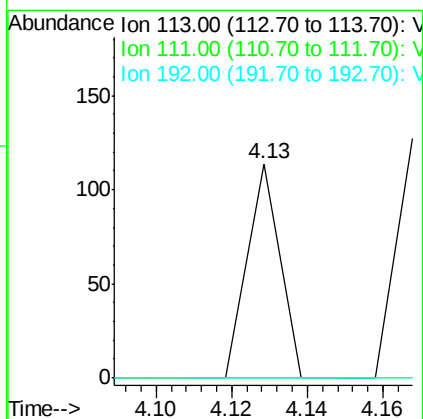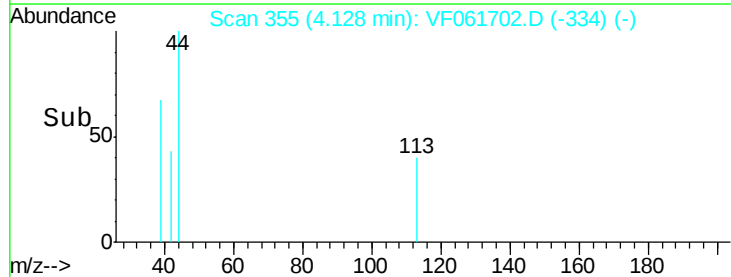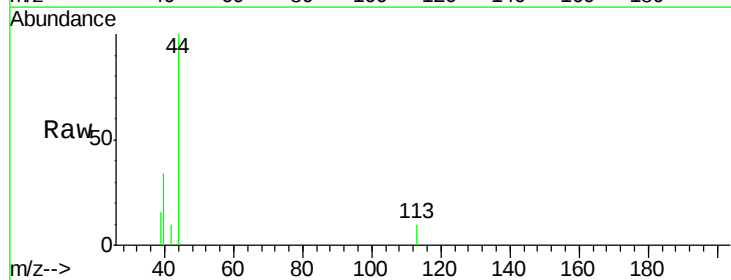


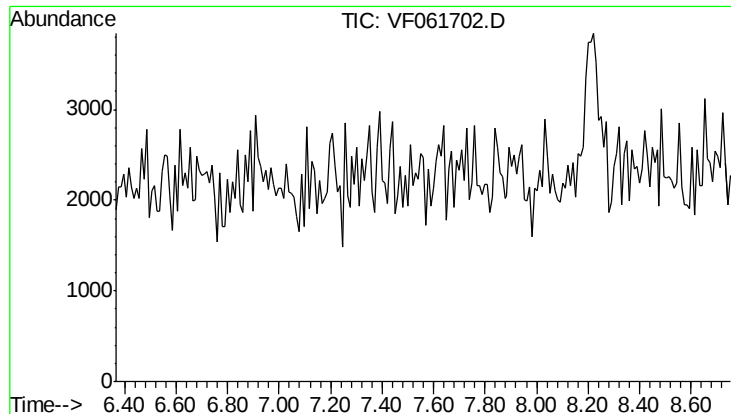


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 7.56 min

Lab File: VF061702.D
Acq: 21 Feb 2019 17:08




Instrument :
MSVOA_F
ClientSampleId :
DRUM-1-2


Tot Ion: 98
Sig Exp Ratio
98 100
100 69.3

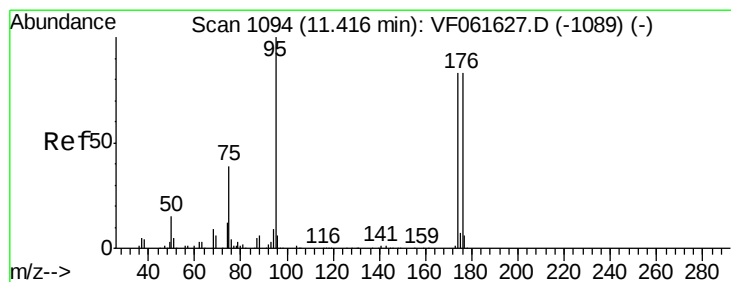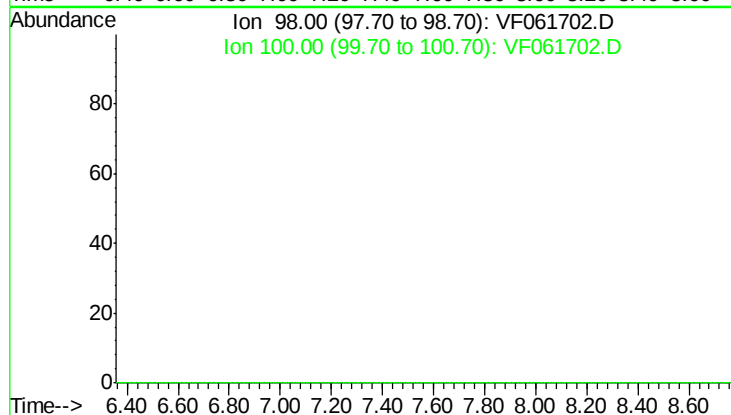

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 11.26 min Scan# 1078
Delta R.T. -0.16 min
Lab File: VF061702.D
Acq: 21 Feb 2019 17:08

Tgt Ion: 95 Resp: 60
Ion Ratio Lower Upper
95 100
174 0.0 0.0 165.8
176 0.0 0.0 167.0

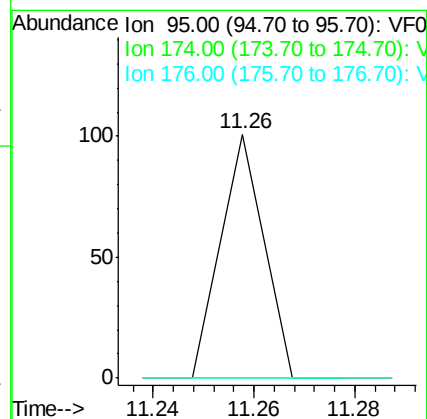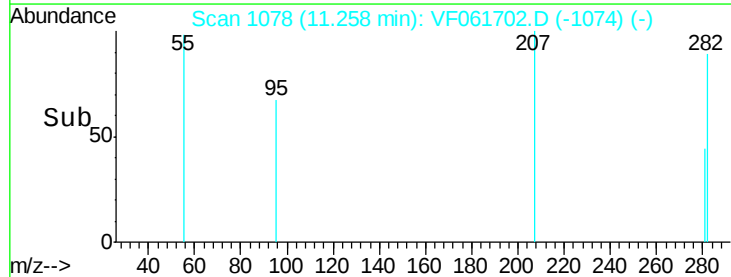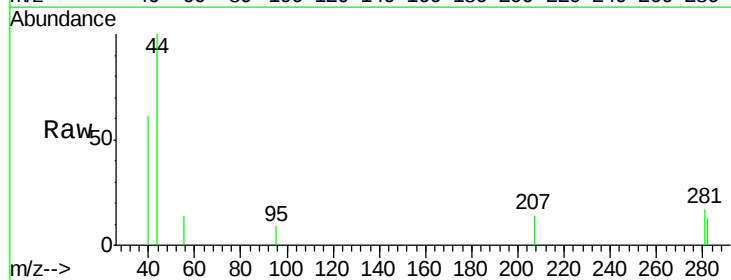


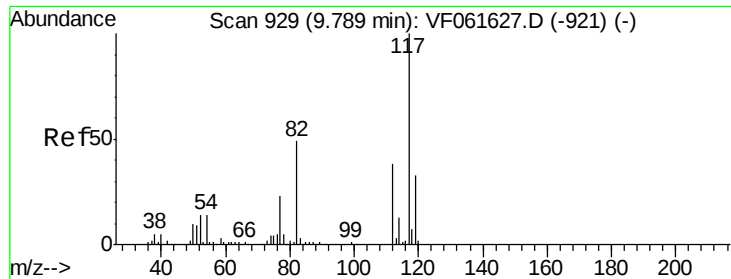

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.79 min Scan# 929
Delta R.T. -0.00 min
Lab File: VF061702.D
Acq: 21 Feb 2019 17:08

Instrument :
MSVOA_F
ClientSampleId :
DRUM-1-2




Tot Ion	Ratio	Lower	Upper
117	100		
82	0.0	39.3	58.9#
119	0.0	26.6	40.0#

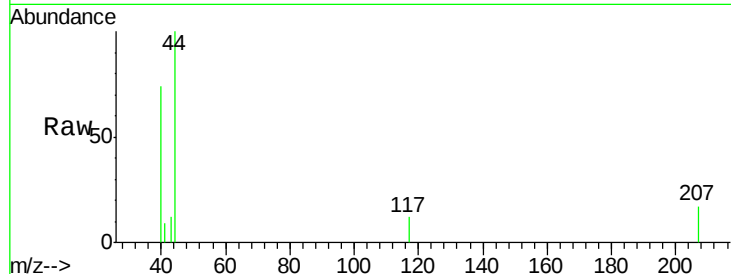

Abundance Ion 117.00 (116.70 to 117.70): V


Ion 82.00 (81.70 to 82.70): VF0

Ion 119.00 (118.70 to 119.70): V

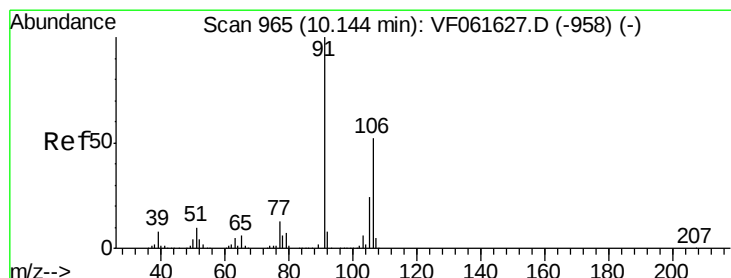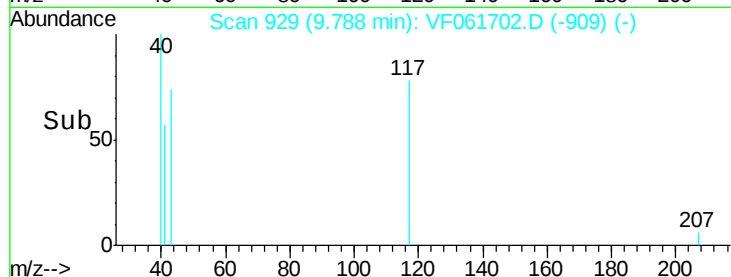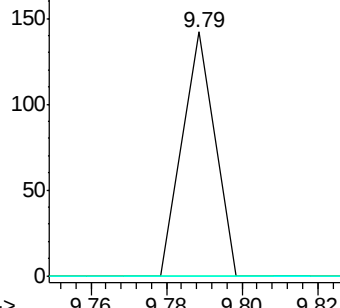



#68
m/p-Xylenes
Concen: 57.150 ug/l
RT: 9.98 min Scan# 948
Delta R.T. -0.17 min
Lab File: VF061702.D
Acq: 21 Feb 2019 17:08


Tgt Ion	Ratio	Lower	Upper
106	100		
91	0.0	153.0	229.6#

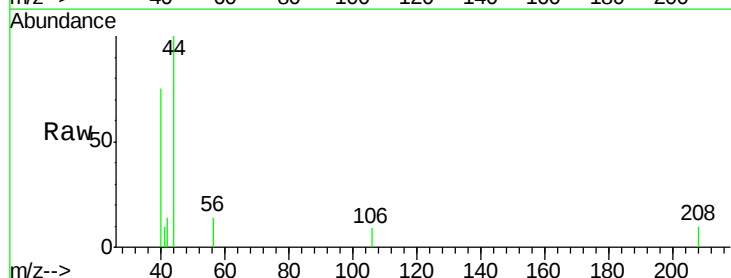

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VF0

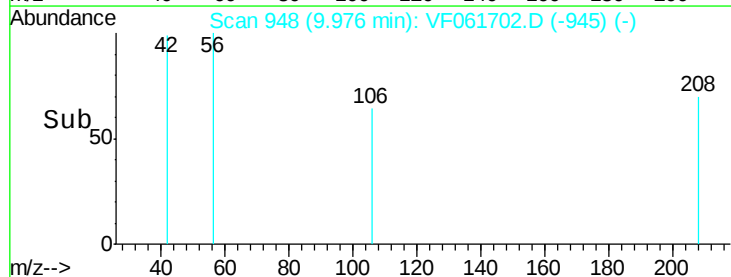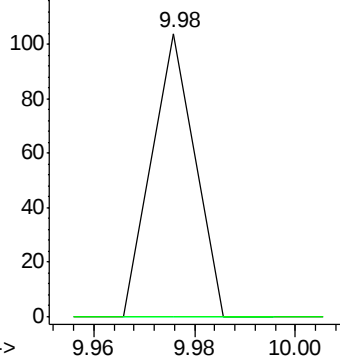

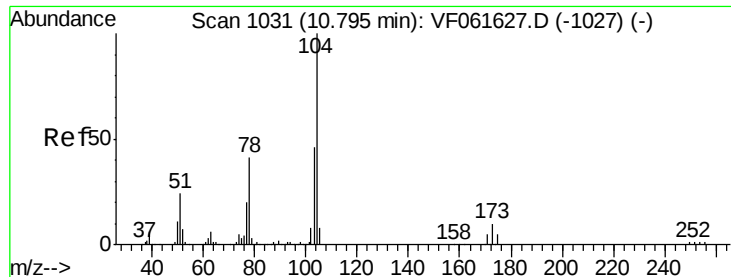

#70

Stvrene

Concen: 40.302 ug/l

RT: 10.79 min Scan# 1031

Delta R.T. -0.00 min

Lab File: VF061702.D

Acq: 21 Feb 2019 17:08

Instrument :

MSVOA_F

ClientSampleId :

DRUM-1-2


Tot Ion:104 Resp: 66

Ion Ratio Lower Upper

104 100

78 0.0 33.2 49.8#

103 0.0 37.2 55.8#

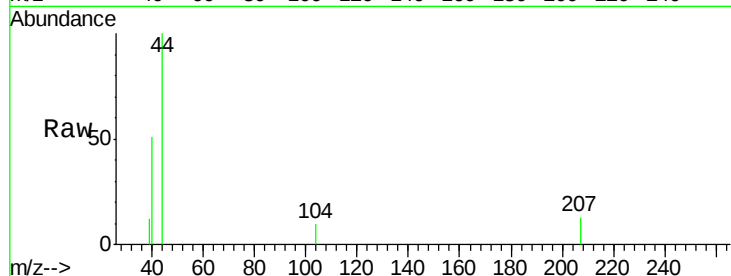

Abundance Ion 104.00 (103.70 to 104.70): V

Ion 78.00 (77.70 to 78.70): VF0

Ion 103.00 (102.70 to 103.70): V

10.79

10.82

10.76

10.78

10.80

10.82

10.84

10.86

10.88

10.90

10.92

10.94

10.96

10.98

11.00

11.02

11.04

11.06

11.08

11.10

11.12

11.14

11.16

11.18

11.20

11.22

11.24

11.26

11.28

11.30

11.32

11.34

11.36

11.38

11.40

11.42

11.44

11.46

11.48

11.50

11.52

11.54

11.56

11.58

11.60

11.62

11.64

11.66

11.68

11.70

11.72

11.74

11.76

11.78

11.80

11.82

11.84

11.86

11.88

11.90

11.92

11.94

11.96

11.98

12.00

12.02

12.04

12.06

12.08

12.10

12.12

12.14

12.16

12.18

12.20

12.22

12.24

12.26

12.28

12.30

12.32

12.34

12.36

12.38

12.40

12.42

12.44

12.46

12.48

12.50

12.52

12.54

12.56

12.58

12.60

12.62

12.64

12.66

12.68

12.70

12.72

12.74

12.76

12.78

12.80

12.82

12.84

12.86

12.88

12.90

12.92

12.94

12.96

12.98

13.00

13.02

13.04

13.06

13.08

13.10

13.12

13.14

13.16

13.18

13.20

13.22

13.24

13.26

13.28

13.30

13.32

13.34

13.36

13.38

13.40

13.42

13.44

13.46

13.48

13.50

13.52

13.54

13.56

13.58

13.60

13.62

13.64

13.66

13.68

13.70

13.72

13.74

13.76

13.78

13.80

13.82

13.84

13.86

13.88

13.90

13.92

13.94

13.96

13.98

14.00

14.02

14.04

14.06

14.08

14.10

14.12

14.14

14.16

14.18

14.20

14.22

14.24

14.26

14.28

14.30

14.32

14.34

14.36

14.38

14.40

14.42

14.44

14.46

14.48

14.50

14.52

14.54

14.56

14.58

14.60

14.62

14.64

14.66

14.68

14.70

14.72

14.74

14.76

14.78

14.80

14.82

14.84

14.86

14.88

14.90

14.92

14.94

14.96

14.98

15.00

15.02

15.04

15.06

15.08

15.10

15.12

15.14

15.16

15.18

15.20

15.22

15.24

15.26

15.28

15.30

15.32

15.34

15.36

15.38

15.40

15.42

15.44

15.46

15.48

15.50

15.52

15.54

15.56

15.58

15.60

15.62

15.64

15.66

15.68

15.70

15.72

15.74

15.76

15.78

15.80

15.82

15.84