

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF022519\
 Data File : VF061734.D
 Acq On : 25 Feb 2019 17:04
 Operator : VA/AP
 Sample : K1610-01
 Misc : 6.90g/5mL/MSVOA-F/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 WV-A

Quant Time: Feb 26 04:47:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 14 03:27:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-4.89
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-5.61
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-9.79
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.56

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	4.74	65	66	0.00	ug/l	-0.11
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF022519\
Data File : VF061734.D
Acq On : 25 Feb 2019 17:04
Operator : VA/AP
Sample : K1610-01
Misc : 6.90q/5mL/MSVOA-F/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
WV-A

Quant Time: Feb 26 04:47:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
Quant Title : SW846 8260
QLast Update : Thu Feb 14 03:27:56 2019
Response via : Initial Calibration

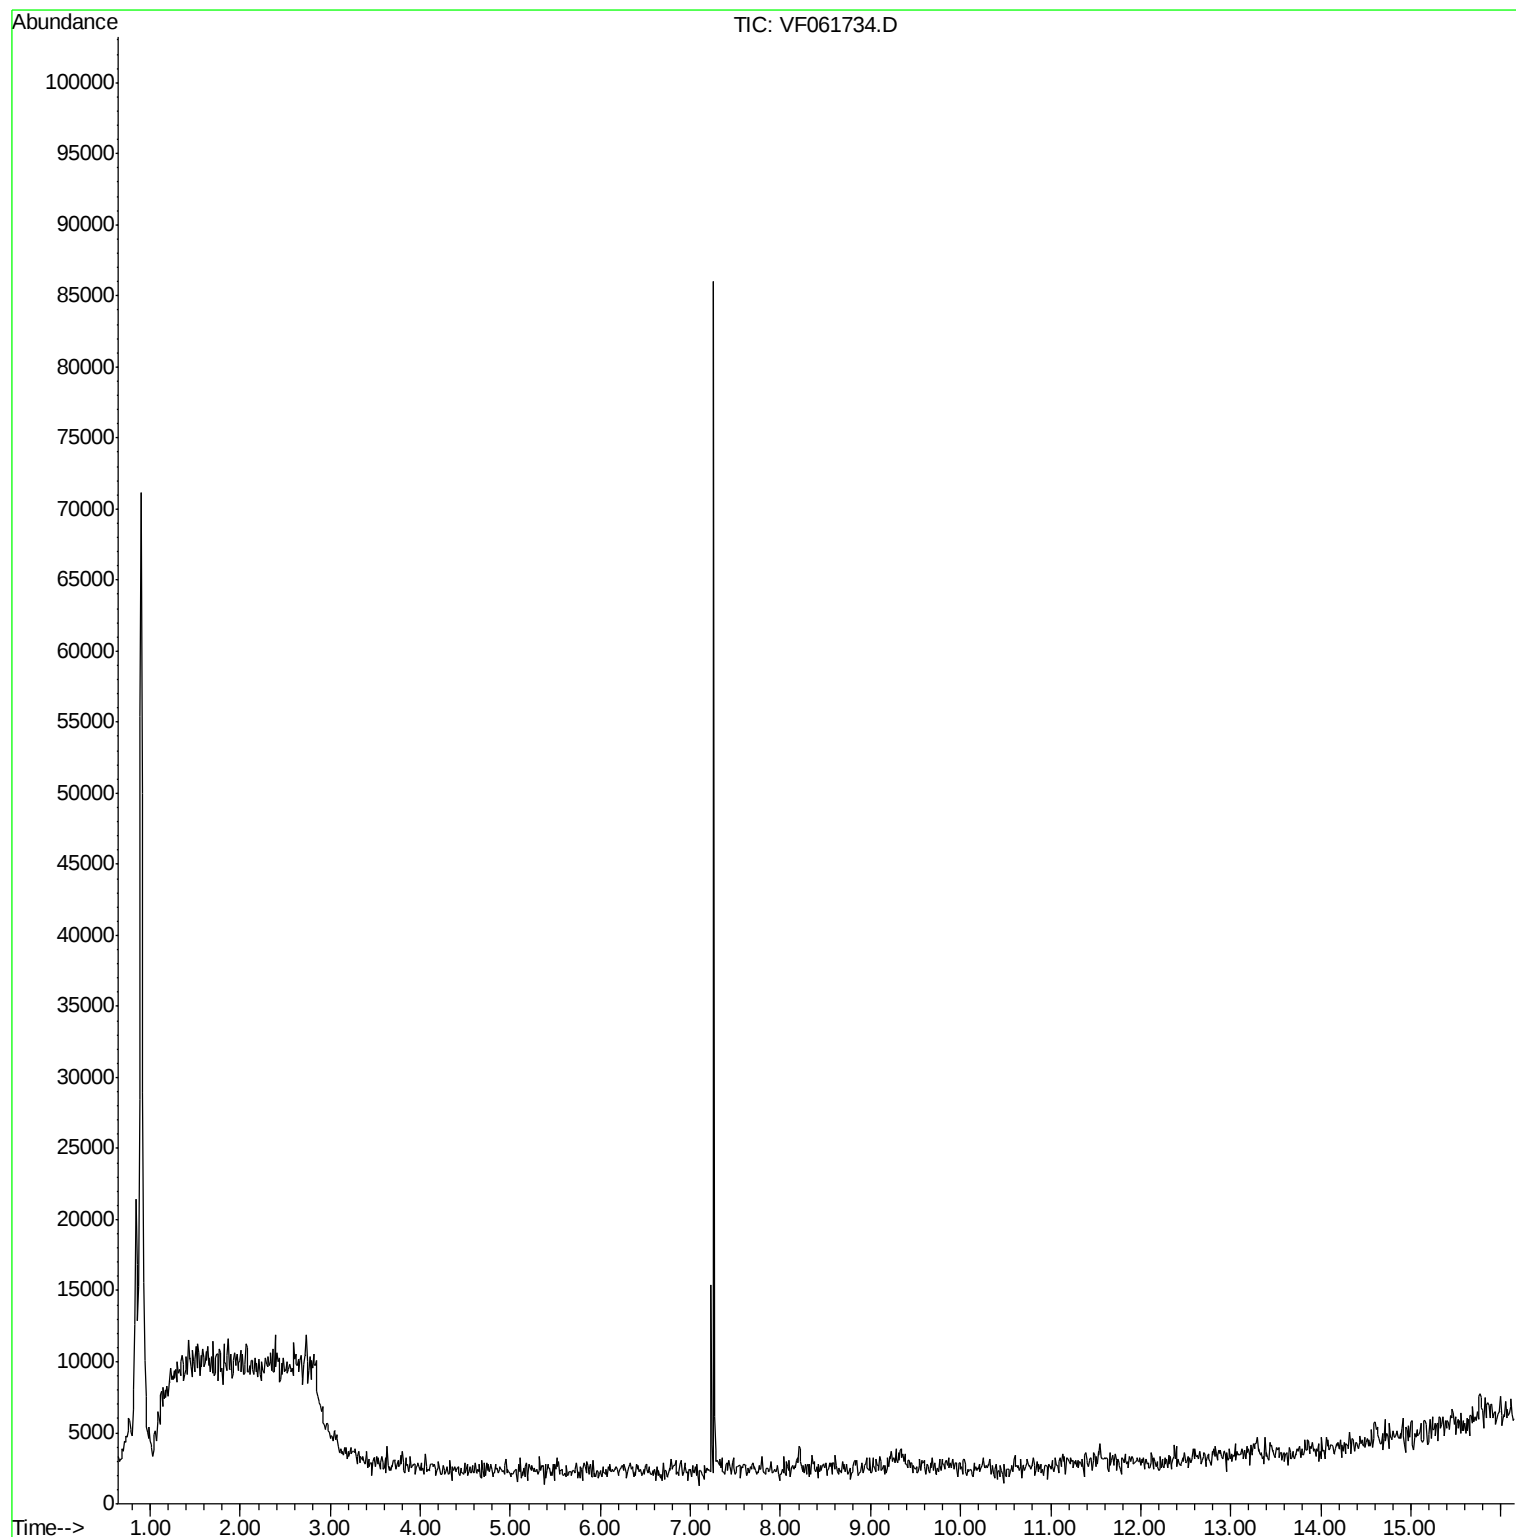

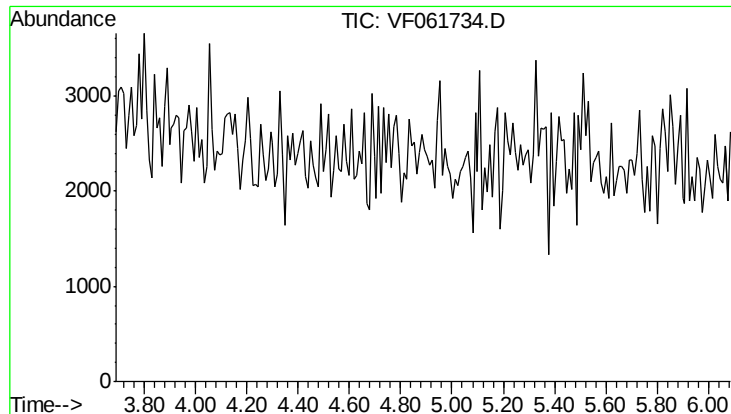

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 4.89 min

Lab File: VF061734.D

Acq: 25 Feb 2019 17:04

Tot Ion: 168

Sig Exp Ratio

168 100



99 43.6

Instrument :

MSVOA_F

ClientSampleId :

WV-A

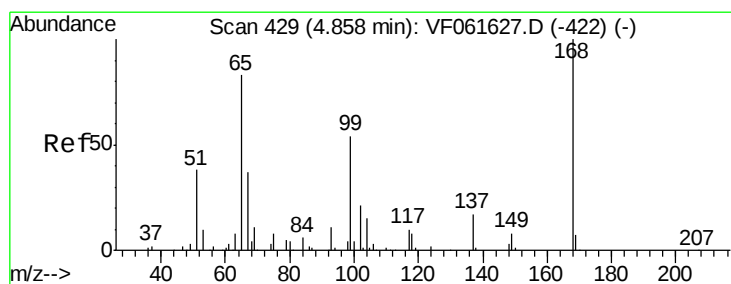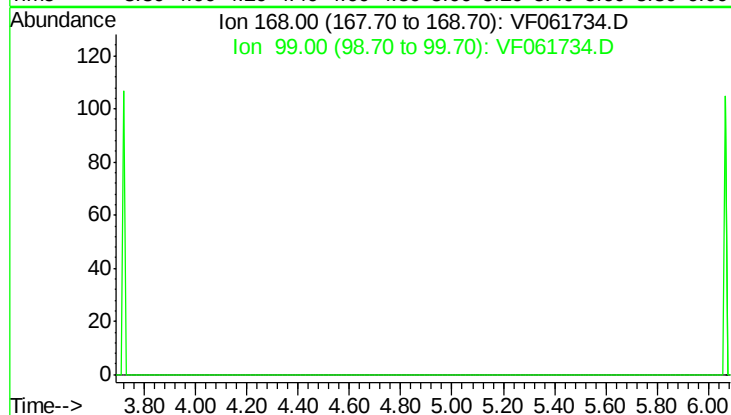

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

RT: 4.74 min Scan# 417

Delta R.T. -0.11 min

Lab File: VF061734.D




Acq: 25 Feb 2019 17:04


Tgt Ion: 65 Resp: 66

Ion Ratio Lower Upper

65 100

67 0.0 0.0 104.0

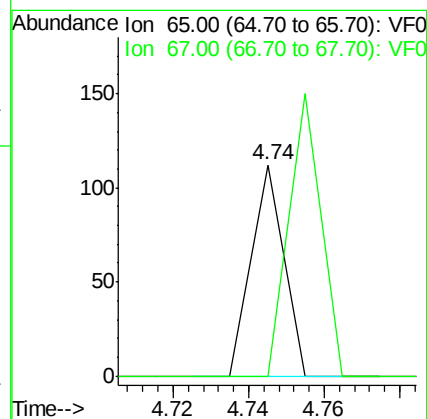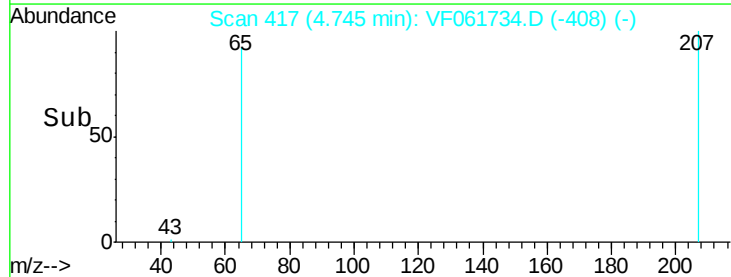
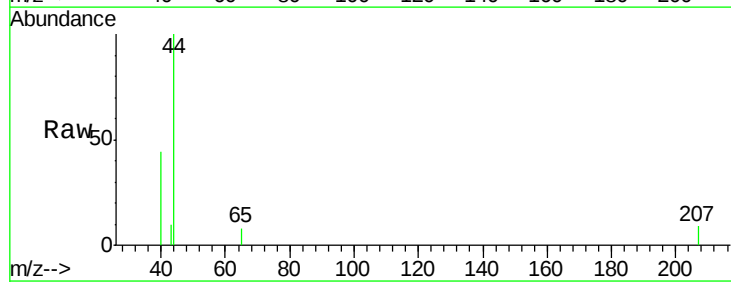


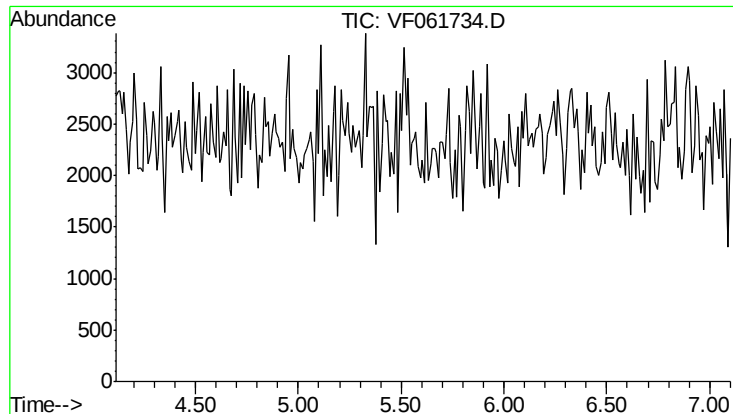

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 5.61 min
 Lab File: VF061734.D
 Acq: 25 Feb 2019 17:04


Instrument :
 MSVOA_F
 ClientSampleId :
 WV-A


Tot Ion	114
Sig	Exp Ratio
114	100
63	18.3
88	17.2

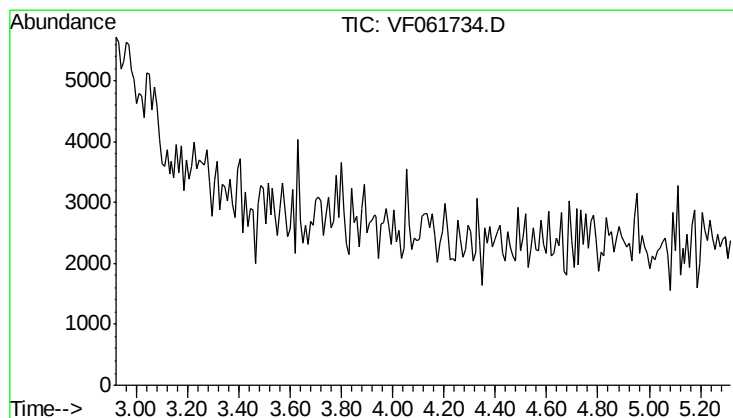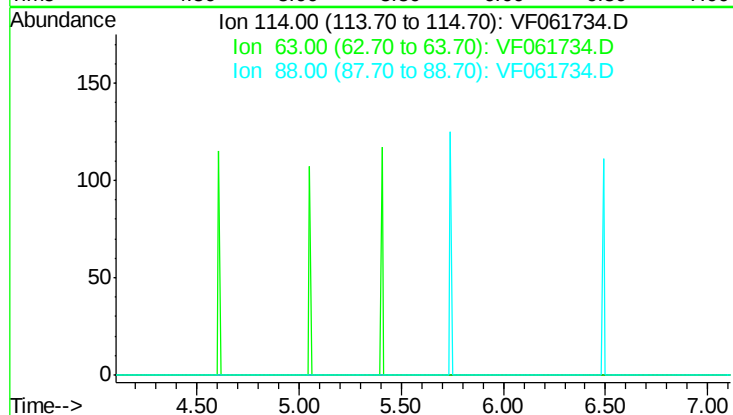

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 4.12 min
 Lab File: VF061734.D
 Acq: 25 Feb 2019 17:04

Tgt Ion	113
Sig	Exp Ratio
113	100
111	98.5
192	16.7


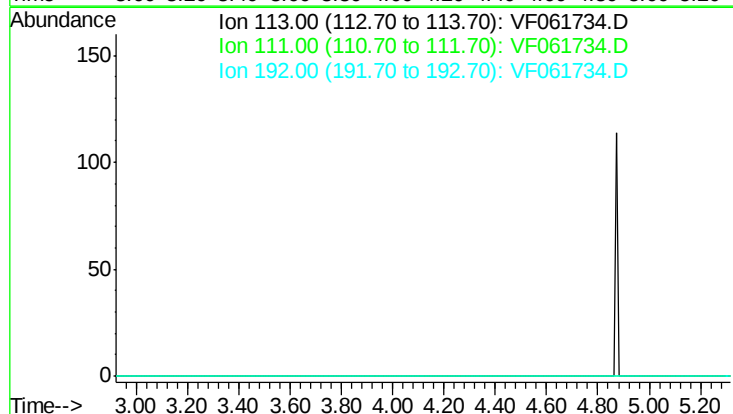


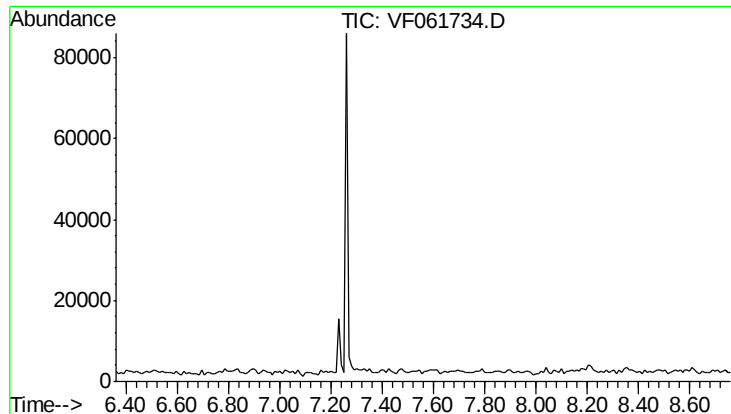

#50
 Toluene-d8
 Concen: 0.000 ug/l
 Expected RT: 7.56 min
 Lab File: VF061734.D
 Acq: 25 Feb 2019 17:04


Instrument :
 MSVOA_F
 ClientSampleId :
 WV-A


Tot Ion	98
Sig	Exp Ratio
98	100
100	69.3

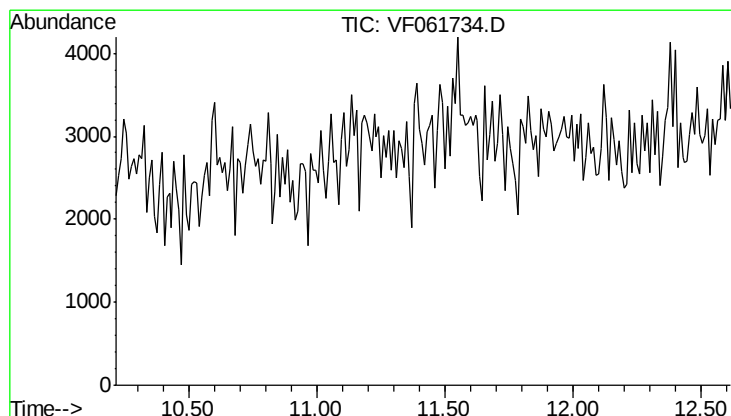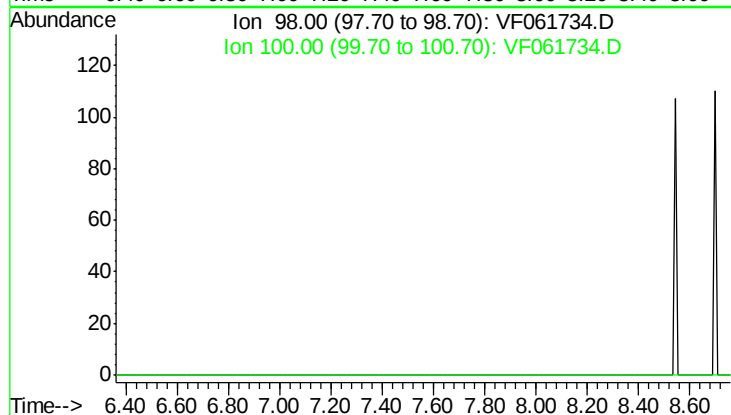

#62
 4-Bromofluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 11.42 min
 Lab File: VF061734.D
 Acq: 25 Feb 2019 17:04

Tgt Ion	95
Sig	Exp Ratio
95	100
174	82.9
176	83.5

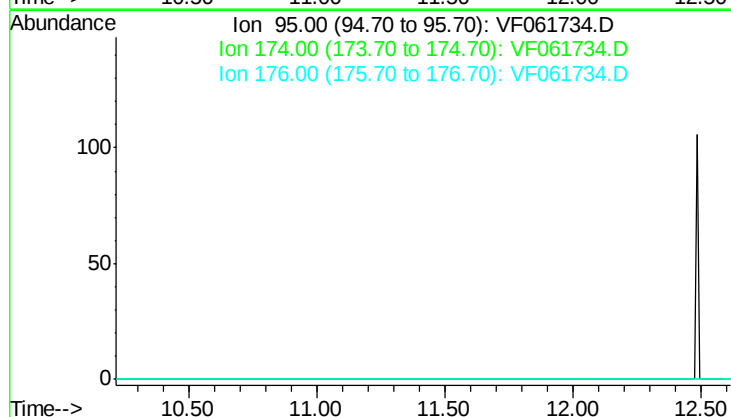


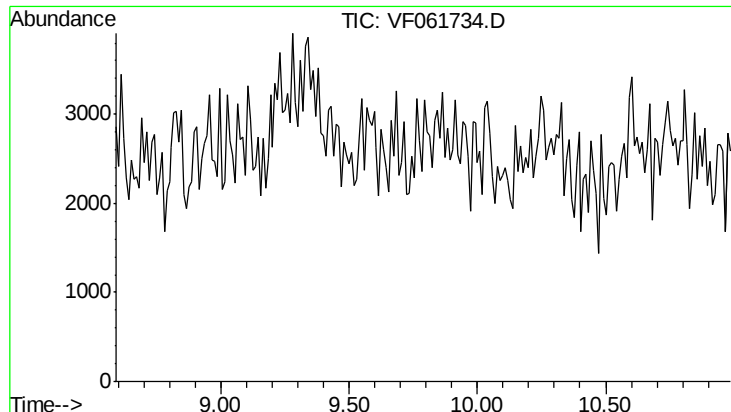


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 9.79 min

Lab File: VF061734.D
 Acq: 25 Feb 2019 17:04

Instrument :
 MSVOA_F
 ClientSampleId :
 WV-A

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 49.1
 119 33.3

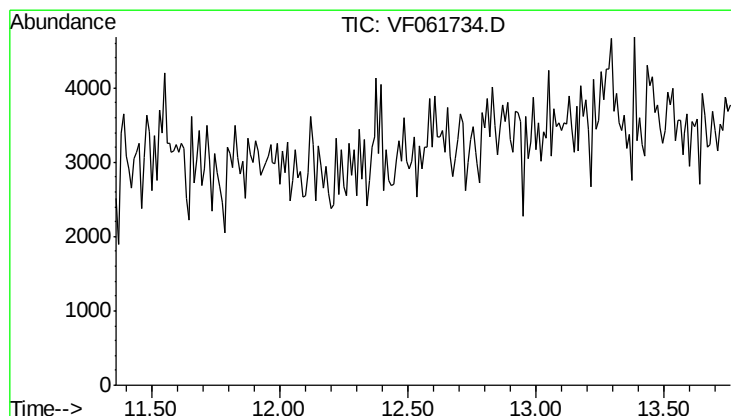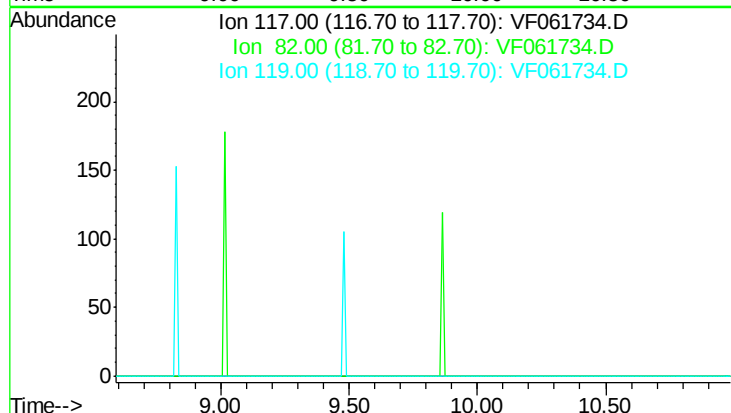

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 12.56 min

Lab File: VF061734.D
 Acq: 25 Feb 2019 17:04

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 48.5
 150 156.0

