


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF022519\
Data File : VF061722.D
Acq On : 25 Feb 2019 10:42
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F021319S.M
Title : SW846 8260
Last Update : Thu Feb 14 03:27:56 2019

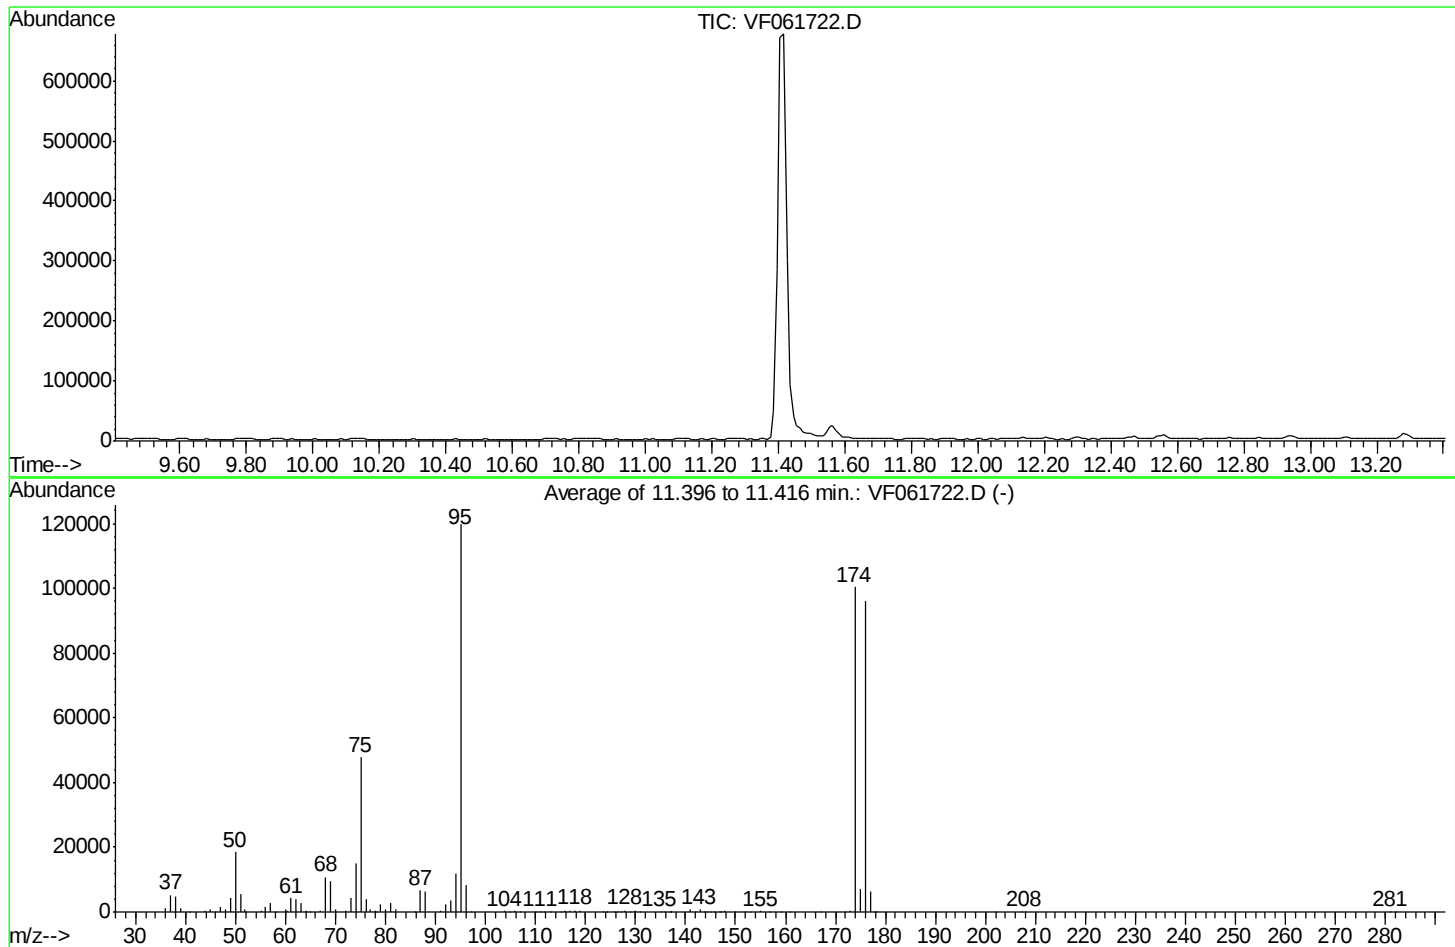

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1087

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	18559	PASS
75	95	30	60	39.9	47741	PASS
95	95	100	100	100.0	119768	PASS
96	95	5	9	6.9	8287	PASS
173	174	0.00	2	0.4	420	PASS
174	95	50	100	83.8	100354	PASS
175	174	5	9	7.3	7298	PASS
176	174	95	101	95.8	96096	PASS
177	176	5	9	6.8	6512	PASS