


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_F\DATA\VF022819\  
Data File : VF061784.D  
Acq On : 28 Feb 2019 10:09  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µ/5mL/MSVOA-F/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_F  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA\_F\METHODS\82F021319S.M  
Title : SW846 8260  
Last Update : Thu Feb 14 03:27:56 2019

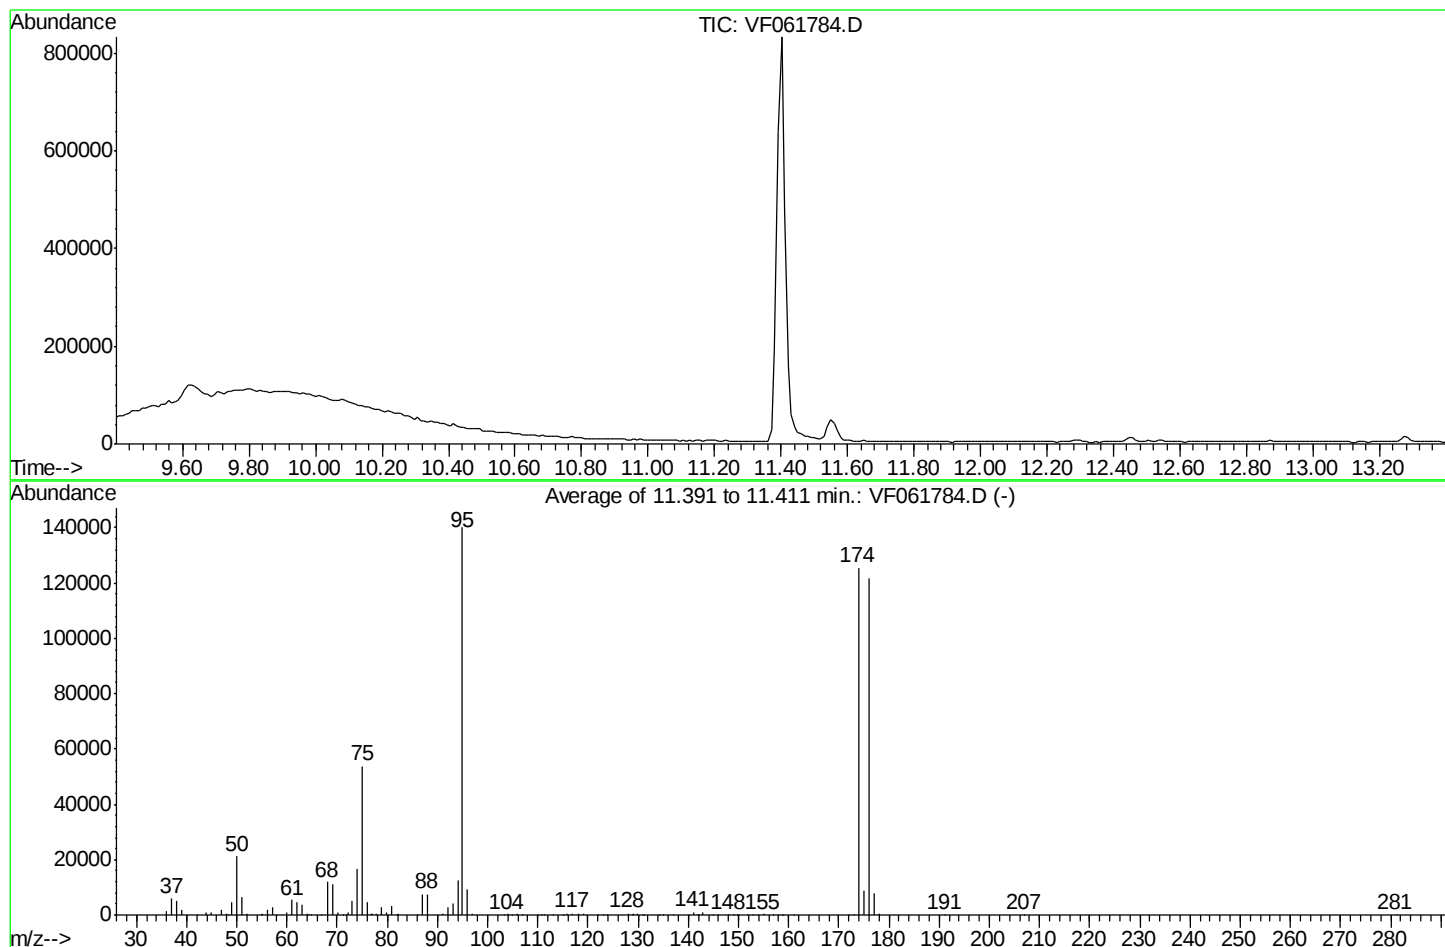

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1085

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.1      | 21208   | PASS             |
| 75          | 95           | 30           | 60           | 38.4      | 53861   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 140117  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 9399    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.1       | 173     | PASS             |
| 174         | 95           | 50           | 100          | 89.6      | 125565  | PASS             |
| 175         | 174          | 5            | 9            | 7.1       | 8902    | PASS             |
| 176         | 174          | 95           | 101          | 97.0      | 121789  | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 7968    | PASS             |