



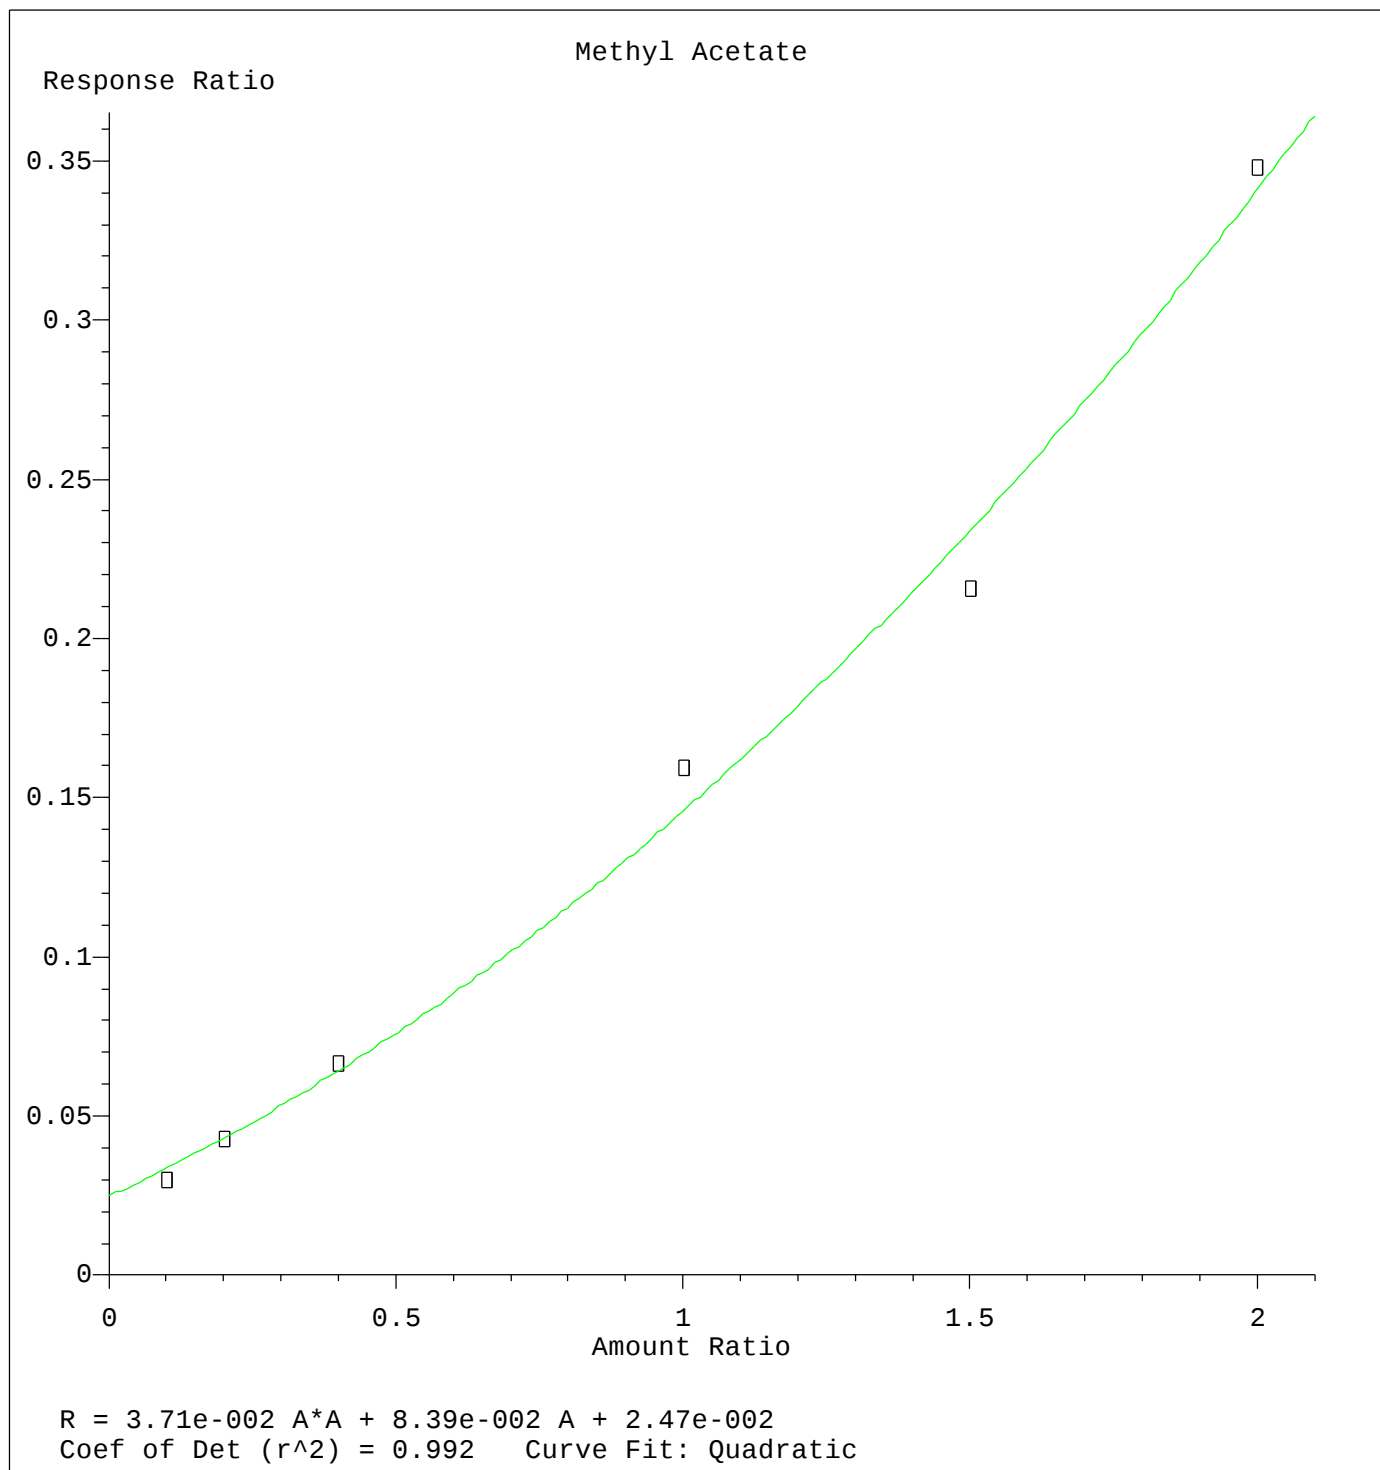


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
Calibration Table Last Updated: Tue Mar 05 04:50:44 2019

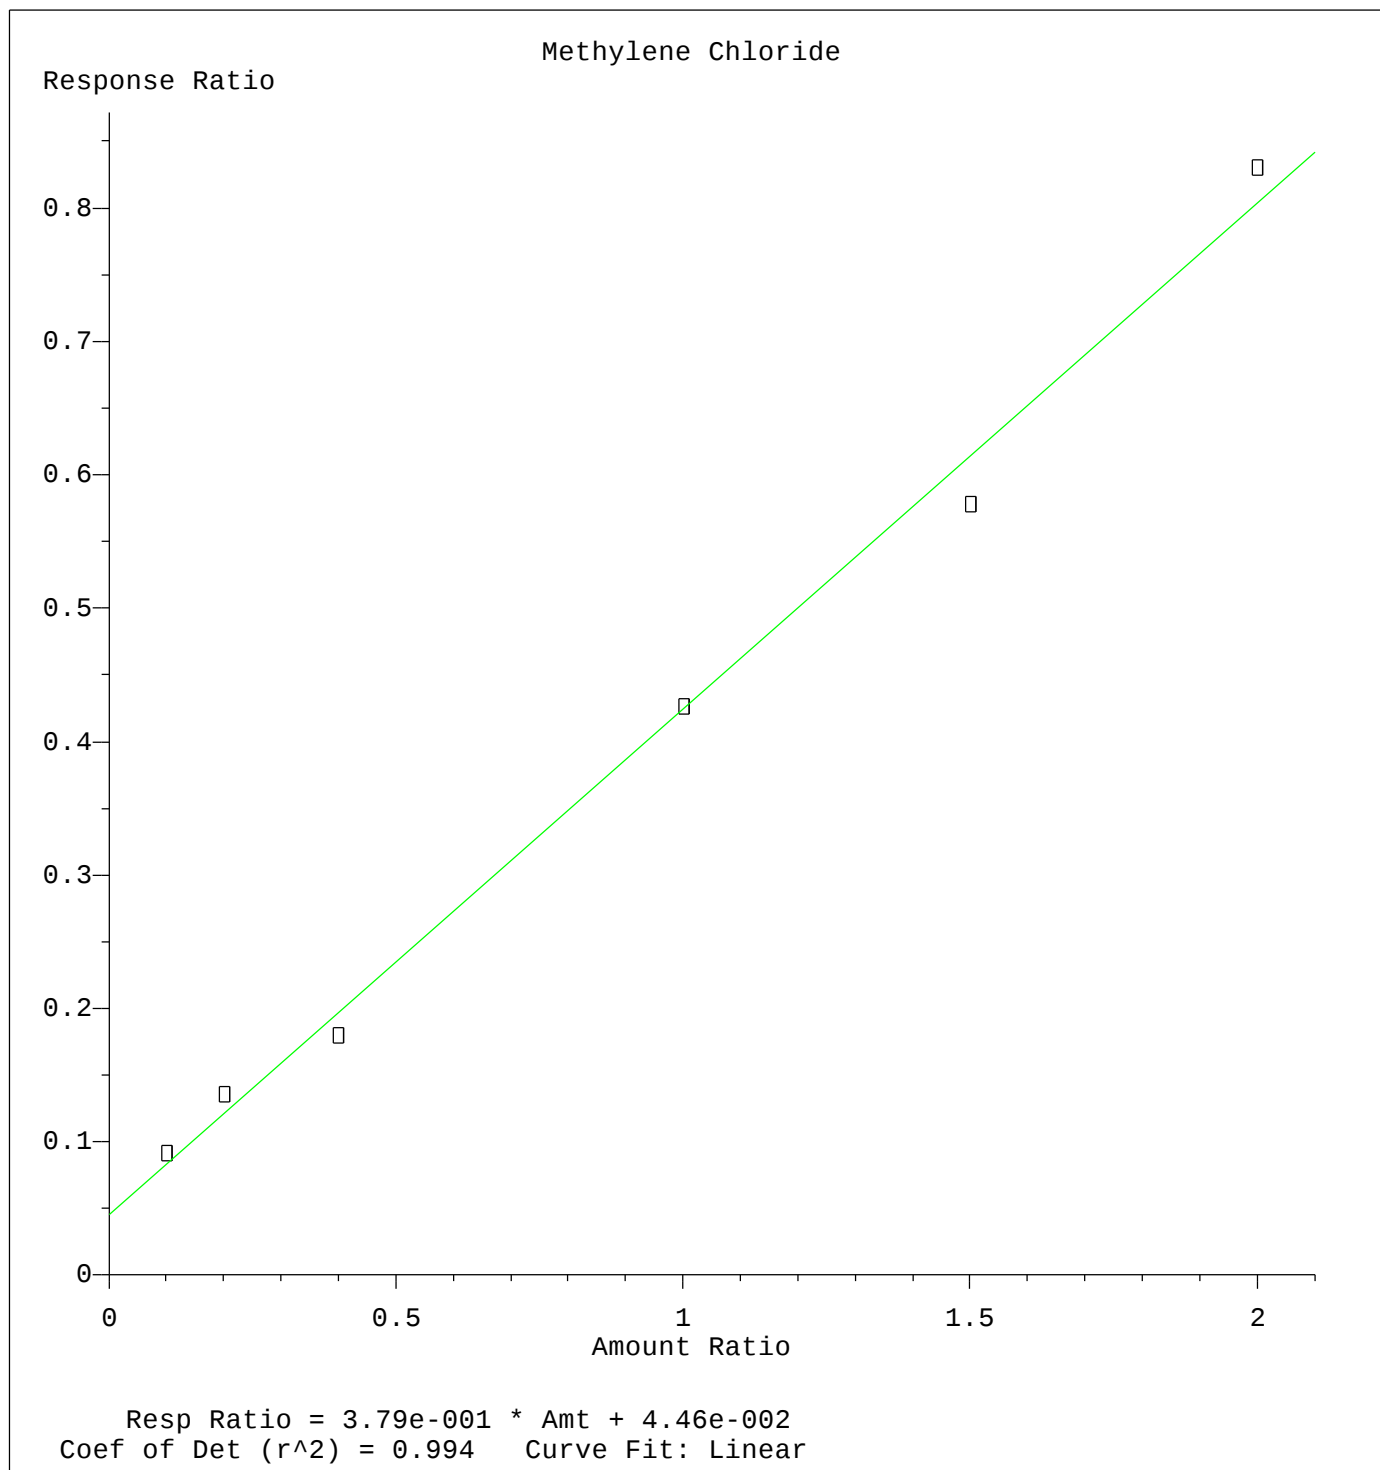

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
Calibration Table Last Updated: Tue Mar 05 04:50:44 2019

1,2-Dibromo-3-Chloropropane

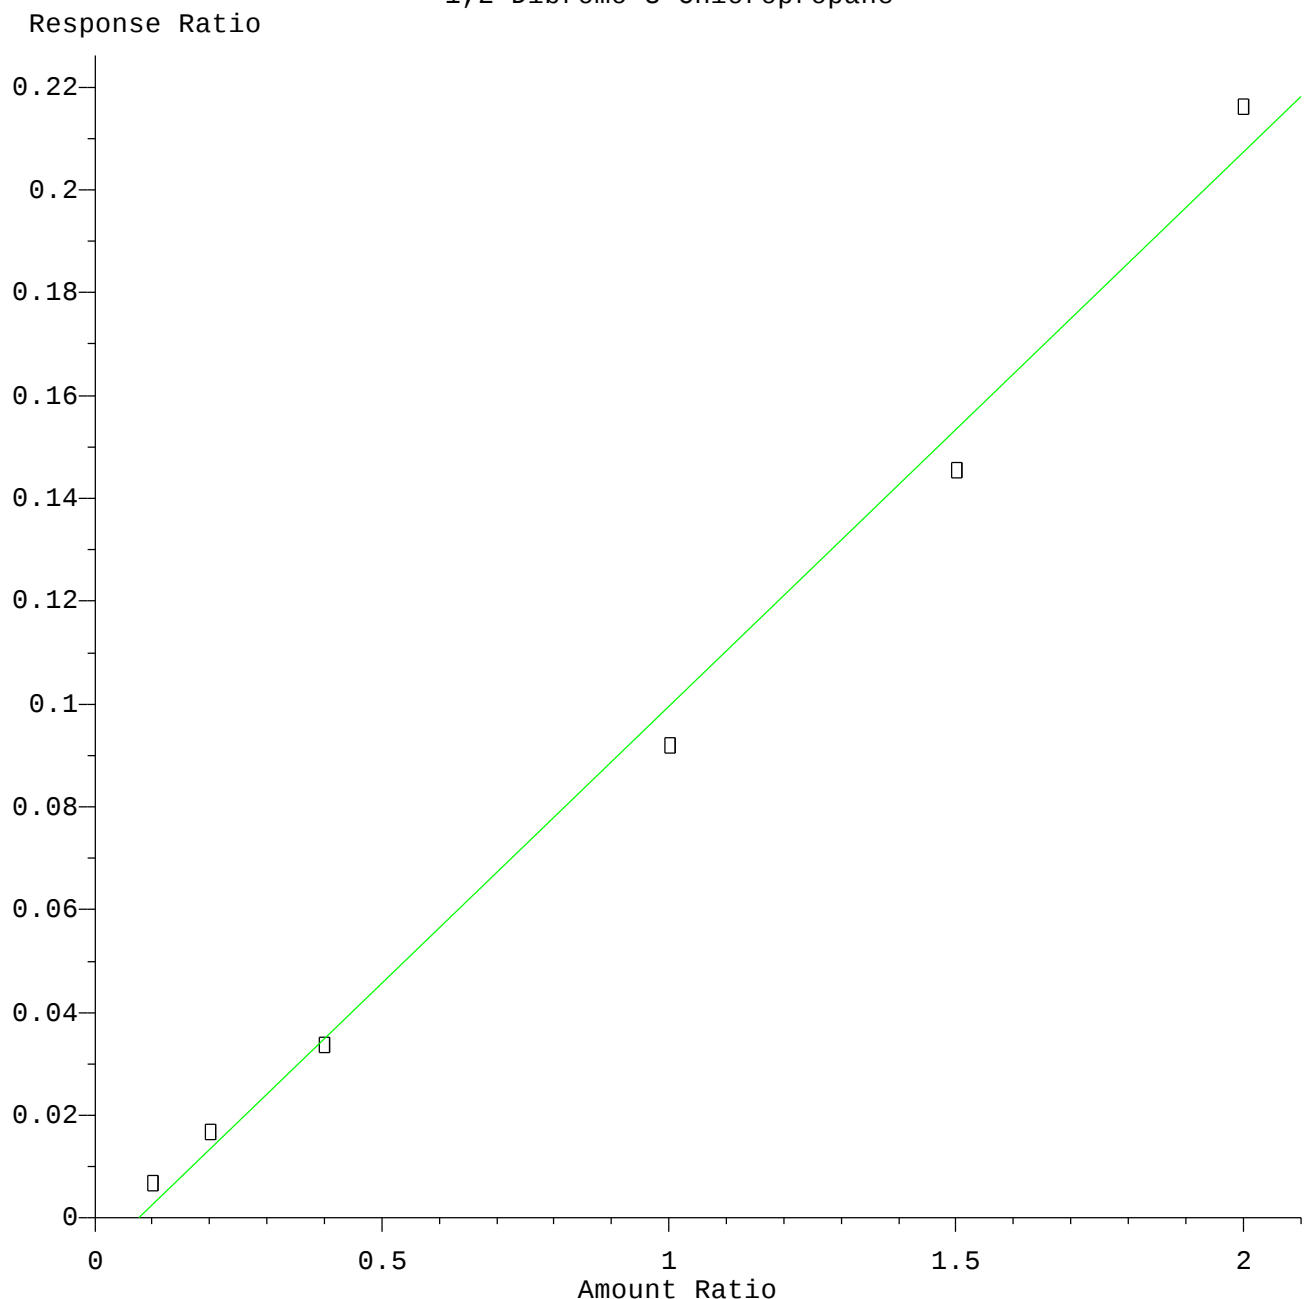

Resp Ratio = 1.07e-001 * Amt - 8.10e-003
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
Calibration Table Last Updated: Tue Mar 05 04:50:44 2019