

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF030419\
 Data File : VF061834.D
 Acq On : 4 Mar 2019 22:44
 Operator : VA/AP
 Sample : K1707-01
 Misc : 5.57g/5mL/MSVOA-F/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 S10

Quant Time: Mar 05 05:04:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 05 04:04:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-4.89
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-5.61
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-9.79
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.56

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		0.00	65	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
35) Dibromofluoromethane		0.00	113	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
50) Toluene-d8		0.00	98	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene		11.42	95	62	0.00	ug/l	0.00
Spiked Amount	50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF030419\
Data File : VF061834.D
Acq On : 4 Mar 2019 22:44
Operator : VA/AP
Sample : K1707-01
Misc : 5.57g/5mL/MSVOA-F/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
S10

Quant Time: Mar 05 05:04:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
Quant Title : SW846 8260
QLast Update : Tue Mar 05 04:04:51 2019
Response via : Initial Calibration

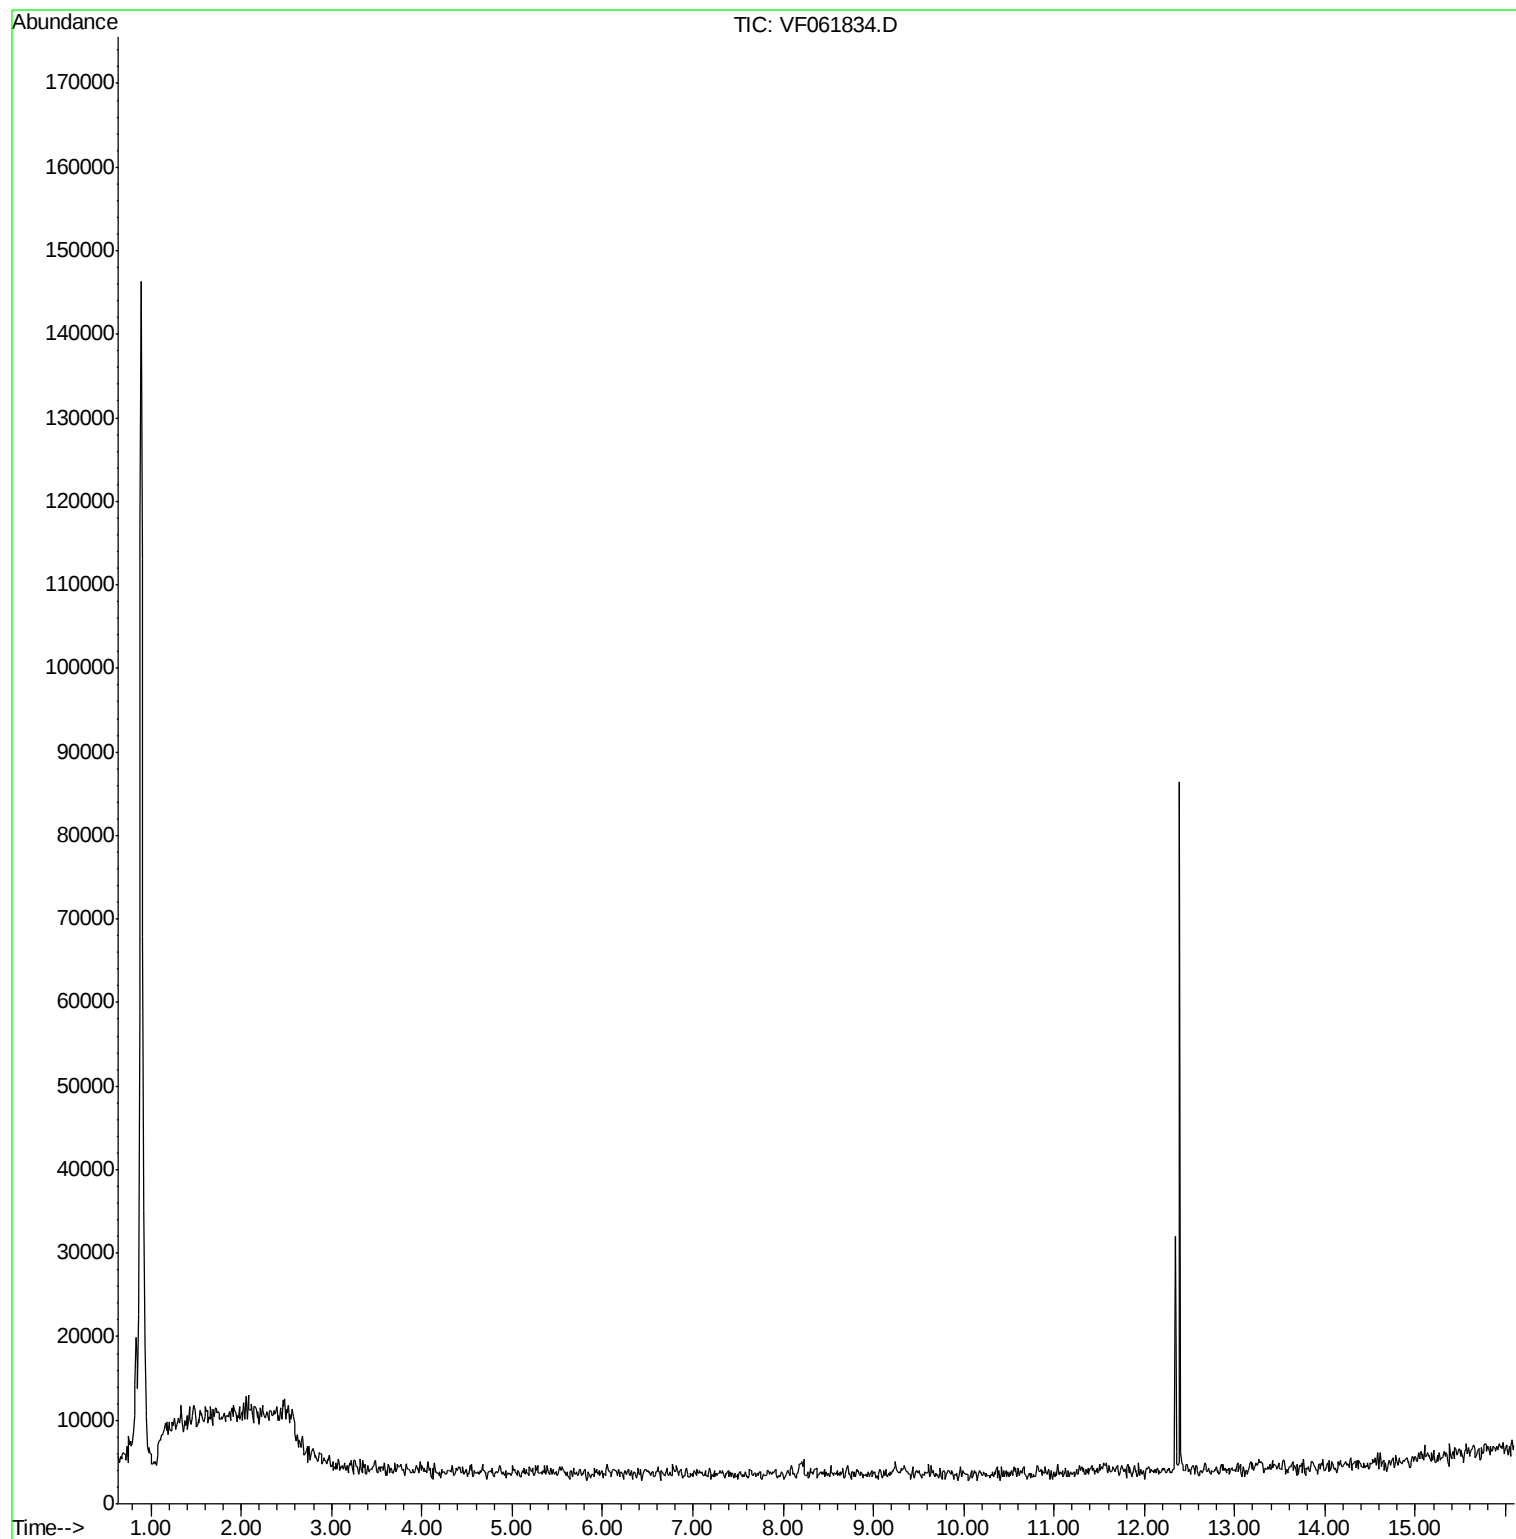

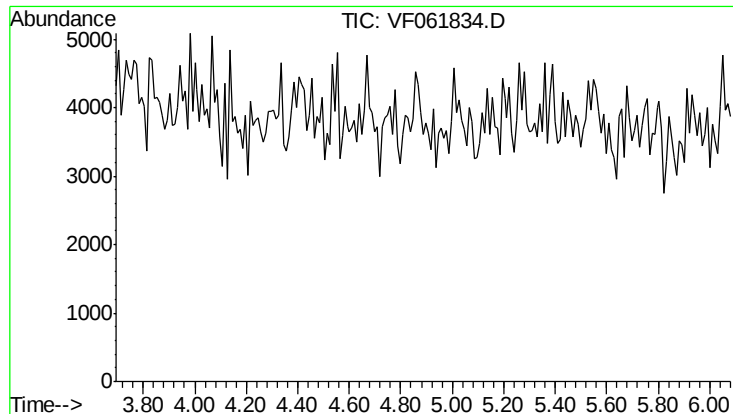

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 4.89 min

Lab File: VF061834.D

Acq: 4 Mar 2019 22:44

Tot Ion: 168

Sig Exp Ratio

168 100



99 43.6

Instrument :

MSVOA_F

ClientSampleId :

S10

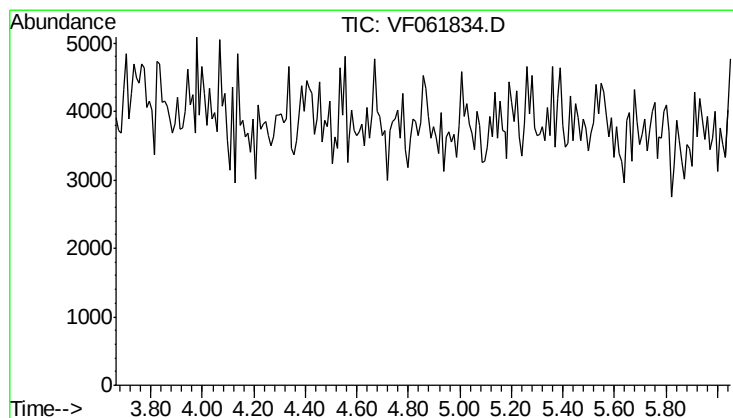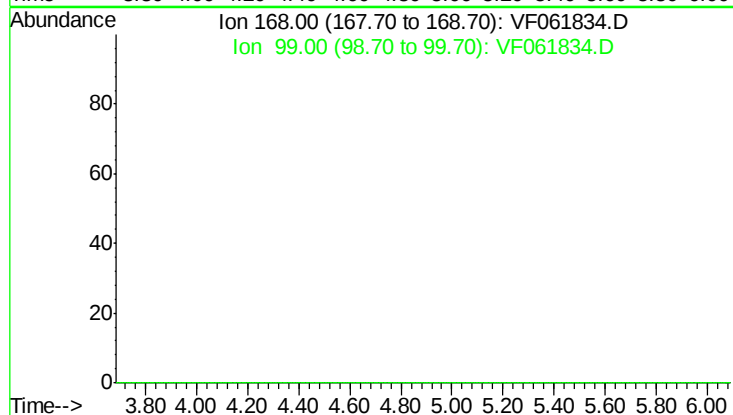

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 4.86 min

Lab File: VF061834.D


Acq: 4 Mar 2019 22:44


Tgt Ion: 65

Sig Exp Ratio

65 100

67 52.0


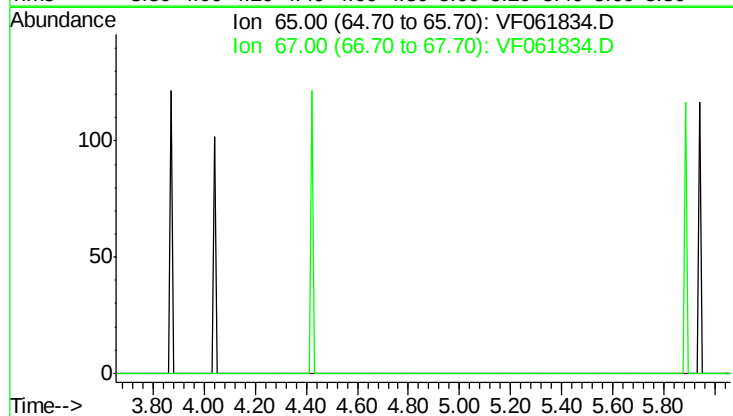


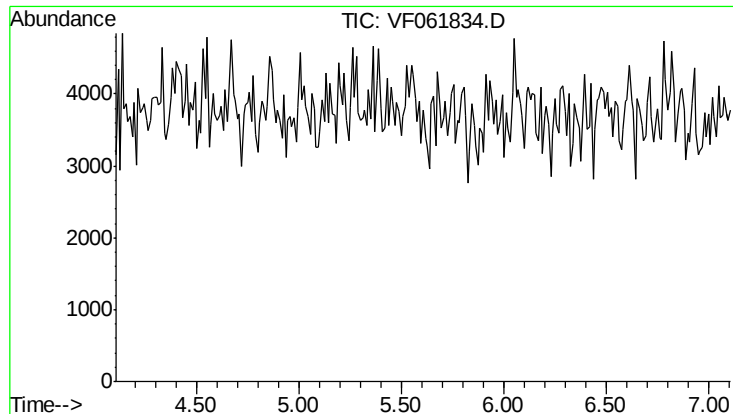

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 5.61 min
 Lab File: VF061834.D
 Acq: 4 Mar 2019 22:44


Instrument :
 MSVOA_F
 ClientSampleId :
 S10


Tot Ion: 114
 Sig Exp Ratio
 114 100
 63 18.3
 88 17.2

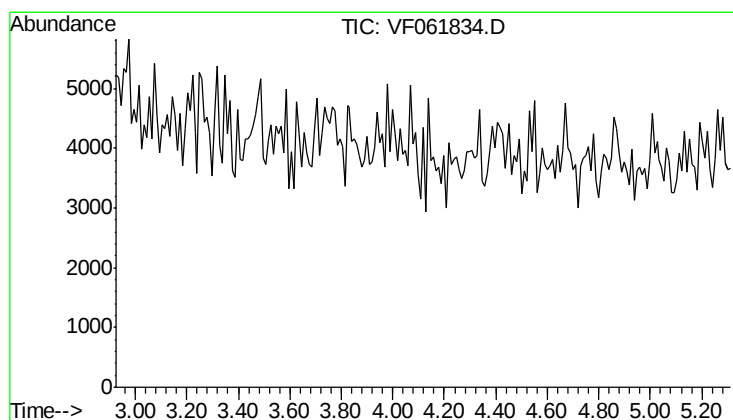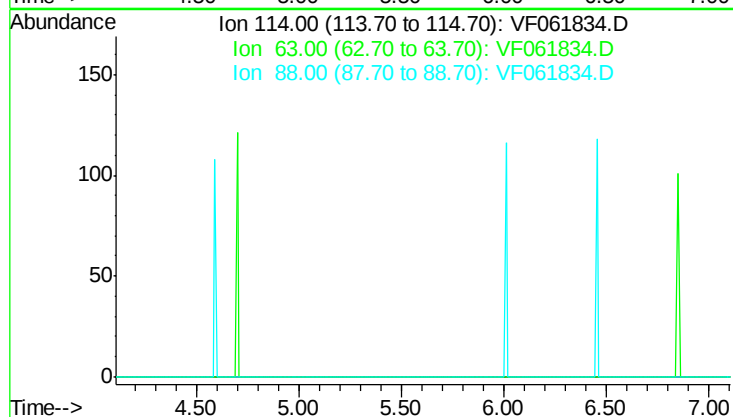

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 4.12 min
 Lab File: VF061834.D
 Acq: 4 Mar 2019 22:44

Tgt Ion: 113
 Sig Exp Ratio
 113 100
 111 98.5
 192 16.7


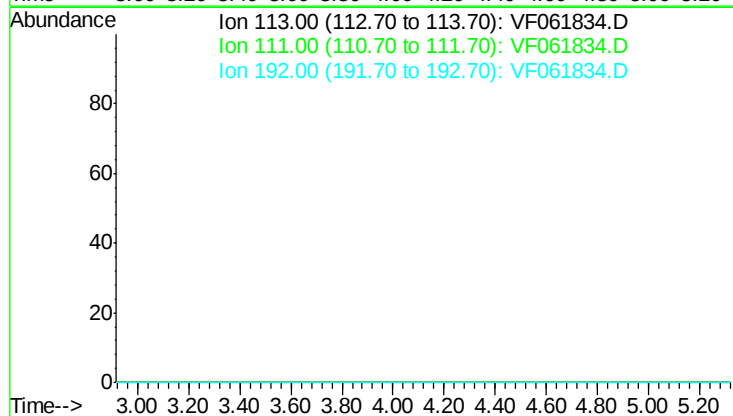


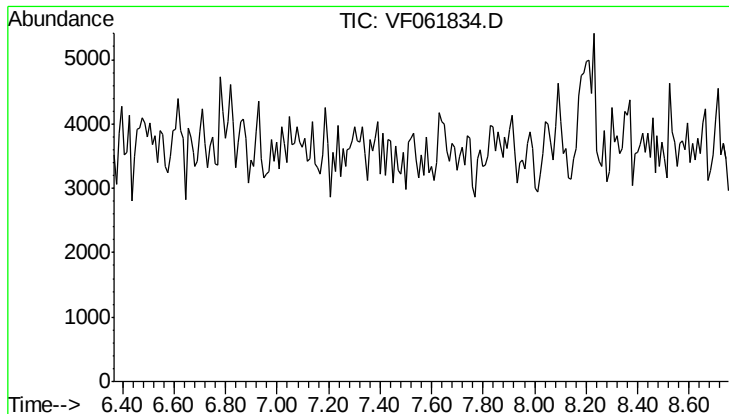

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 7.56 min
Lab File: VF061834.D
Acq: 4 Mar 2019 22:44




Instrument :
MSVOA_F
ClientSampleId :
S10


Tot Ion: 98
Sig Exp Ratio
98 100
100 69.3

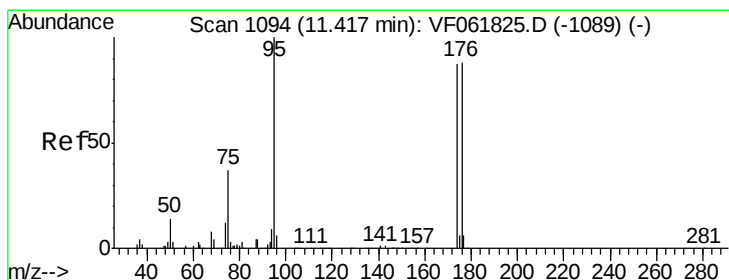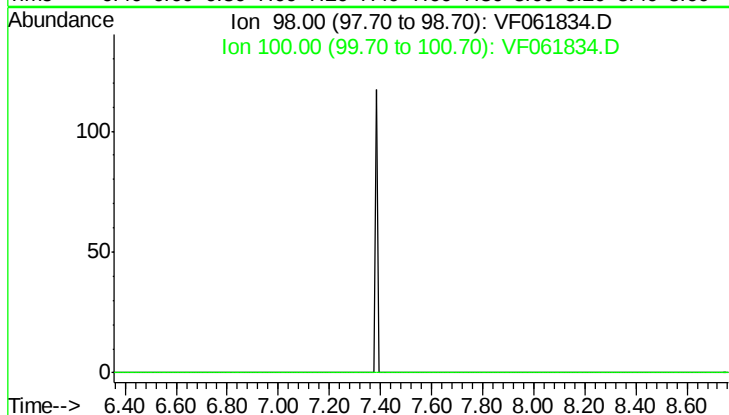

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 11.42 min Scan# 1094
Delta R.T. -0.00 min
Lab File: VF061834.D
Acq: 4 Mar 2019 22:44

Tgt Ion: 95 Resp: 62
Ion Ratio Lower Upper
95 100
174 0.0 0.0 165.8
176 0.0 0.0 167.0

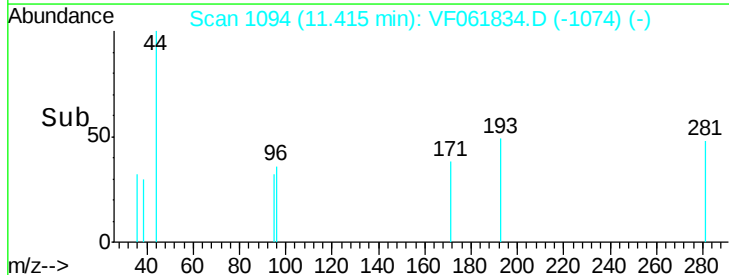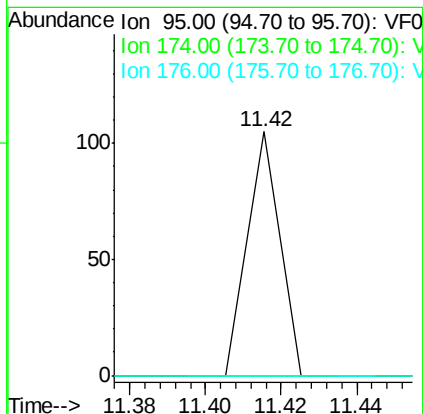
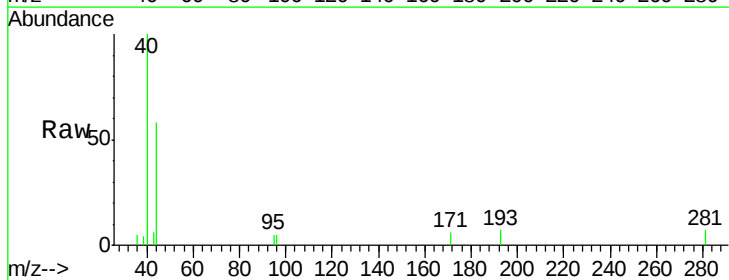


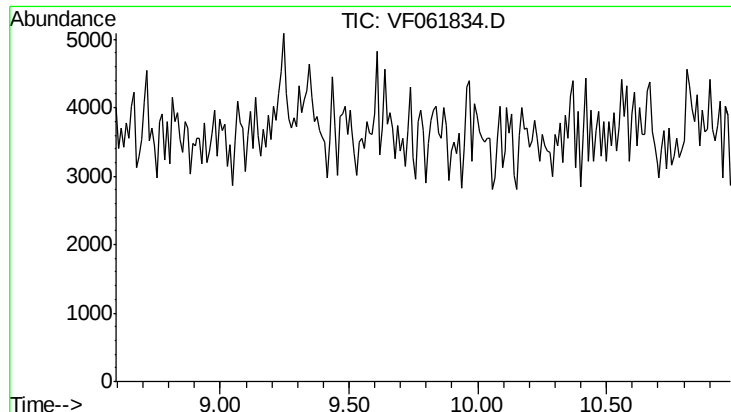

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 9.79 min
 Lab File: VF061834.D
 Acq: 4 Mar 2019 22:44

Instrument :
 MSVOA_F
 ClientSampleId :
 S10

Tot Ion	117
Sig	Exp Ratio
117	100
82	49.1
119	33.3

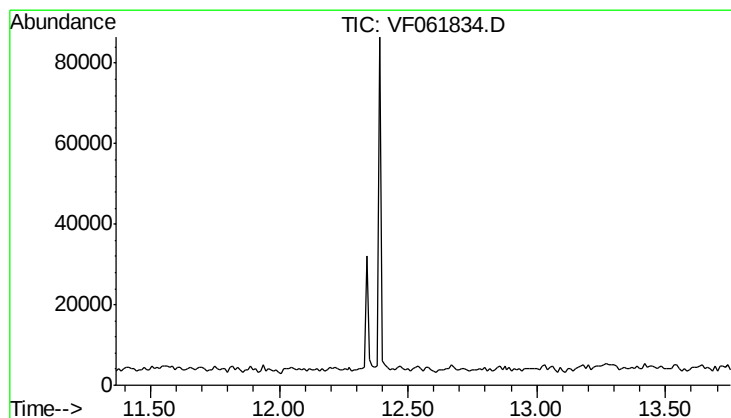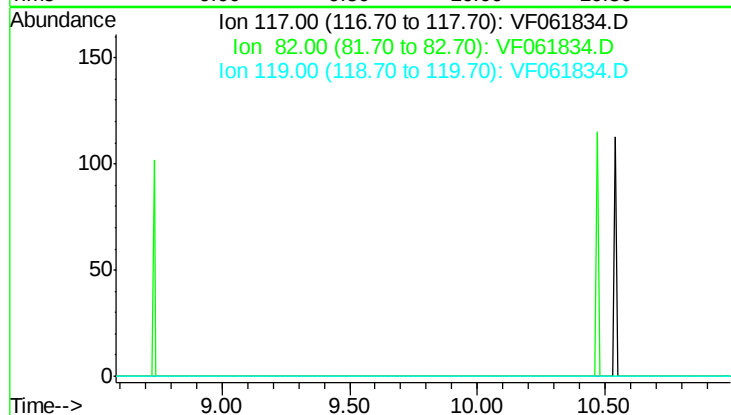

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 12.56 min
 Lab File: VF061834.D
 Acq: 4 Mar 2019 22:44

Tgt Ion	152
Sig	Exp Ratio
152	100
115	48.5
150	156.0

