


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF030419\
Data File : VF061821.D
Acq On : 4 Mar 2019 15:00
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
Title : SW846 8260
Last Update : Tue Mar 05 04:50:44 2019

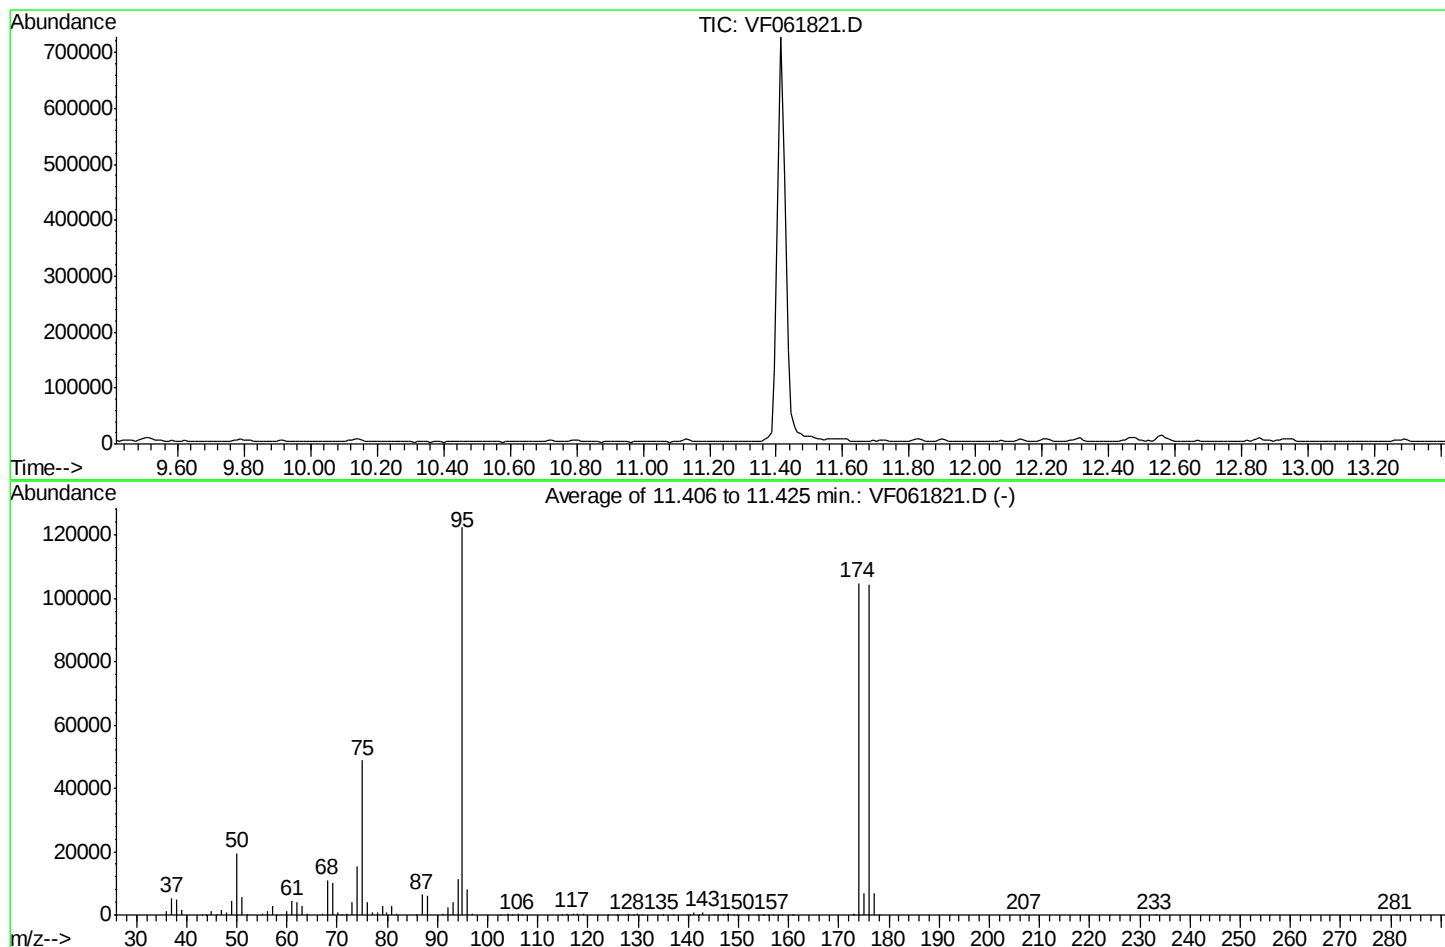

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	19439	PASS
75	95	30	60	39.9	48898	PASS
95	95	100	100	100.0	122458	PASS
96	95	5	9	6.6	8088	PASS
173	174	0.00	2	0.3	293	PASS
174	95	50	100	85.6	104858	PASS
175	174	5	9	6.8	7083	PASS
176	174	95	101	99.4	104216	PASS
177	176	5	9	6.7	6944	PASS