


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF030819\
 Data File : VF061860.D
 Acq On : 8 Mar 2019 12:52
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
 Title : SW846 8260
 Last Update : Tue Mar 05 04:50:44 2019

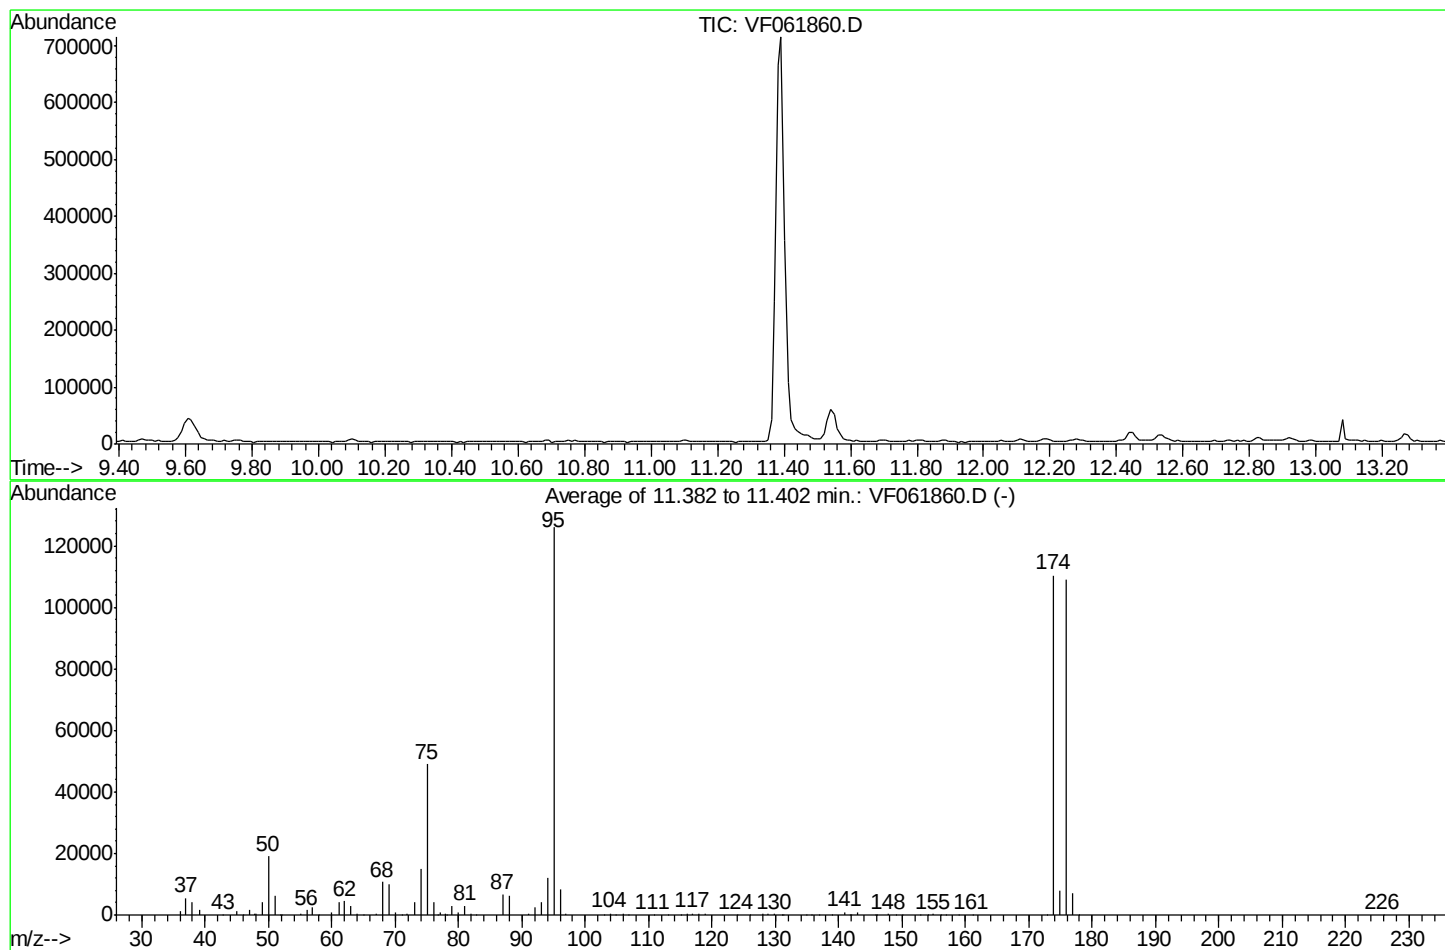

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1084

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	19143	PASS
75	95	30	60	38.9	49042	PASS
95	95	100	100	100.0	126032	PASS
96	95	5	9	6.8	8510	PASS
173	174	0.00	2	0.2	218	PASS
174	95	50	100	87.6	110376	PASS
175	174	5	9	7.1	7891	PASS
176	174	95	101	98.8	109013	PASS
177	176	5	9	6.4	7024	PASS