

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF031519\
 Data File : VF061969.D
 Acq On : 15 Mar 2019 19:05
 Operator : VA/AP
 Sample : K1928-12
 Misc : 6.68g/5mL/MSVOA-F/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 SI-2(5.5-6)

Quant Time: Mar 15 23:19:05 2019
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 05 04:50:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.88	168	244977	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.61	114	389662	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.79	117	329051	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.56	152	189208	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	4.86	65	93347	52.32	ug/l	0.00
Spiked Amount			Recovery	=	104.64%	
35) Dibromofluoromethane	4.13	113	123528	45.43	ug/l	0.00
Spiked Amount			Recovery	=	90.86%	
50) Toluene-d8	7.57	98	332714	41.16	ug/l	0.00
Spiked Amount			Recovery	=	82.32%	
62) 4-Bromofluorobenzene	11.42	95	139847	44.17	ug/l	0.00
Spiked Amount			Recovery	=	88.34%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	2.59	59	134	1.323	ug/l #	64
16) Acetone	2.25	43	4589	12.280	ug/l	93
18) Methyl Acetate	2.37	43	7780	4.075	ug/l	99
29) Tetrahydrofuran	4.12	42	1254	3.825	ug/l #	57
49) 1,4-Dioxane	6.29	88	62	5.627	ug/l #	1
51) 4-Methyl-2-Pentanone	8.28	43	2745	2.086	ug/l #	61
52) Toluene	7.64	92	22586	3.968	ug/l	99
67) Ethyl Benzene	9.92	91	15364	1.466	ug/l #	89
68) m/p-Xylenes	10.14	106	16613	4.139	ug/l	77
69) o-Xylene	10.72	106	6757	1.563	ug/l	78
84) 1,2,4-Trimethylbenzene	12.21	105	25349	2.473	ug/l	98
92) 1,2-Dibromo-3-Chloropropan	13.63	75	67	3.932	ug/l #	1
95) Naphthalene	14.47	128	11025	1.566	ug/l #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF031519\
Data File : VF061969.D
Acq On : 15 Mar 2019 19:05
Operator : VA/AP
Sample : K1928-12
Misc : 6.68g/5mL/MSVOA-F/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
SI-2(5.5-6)

Quant Time: Mar 15 23:19:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F030419S.M
Quant Title : SW846 8260
QLast Update : Tue Mar 05 04:50:44 2019
Response via : Initial Calibration

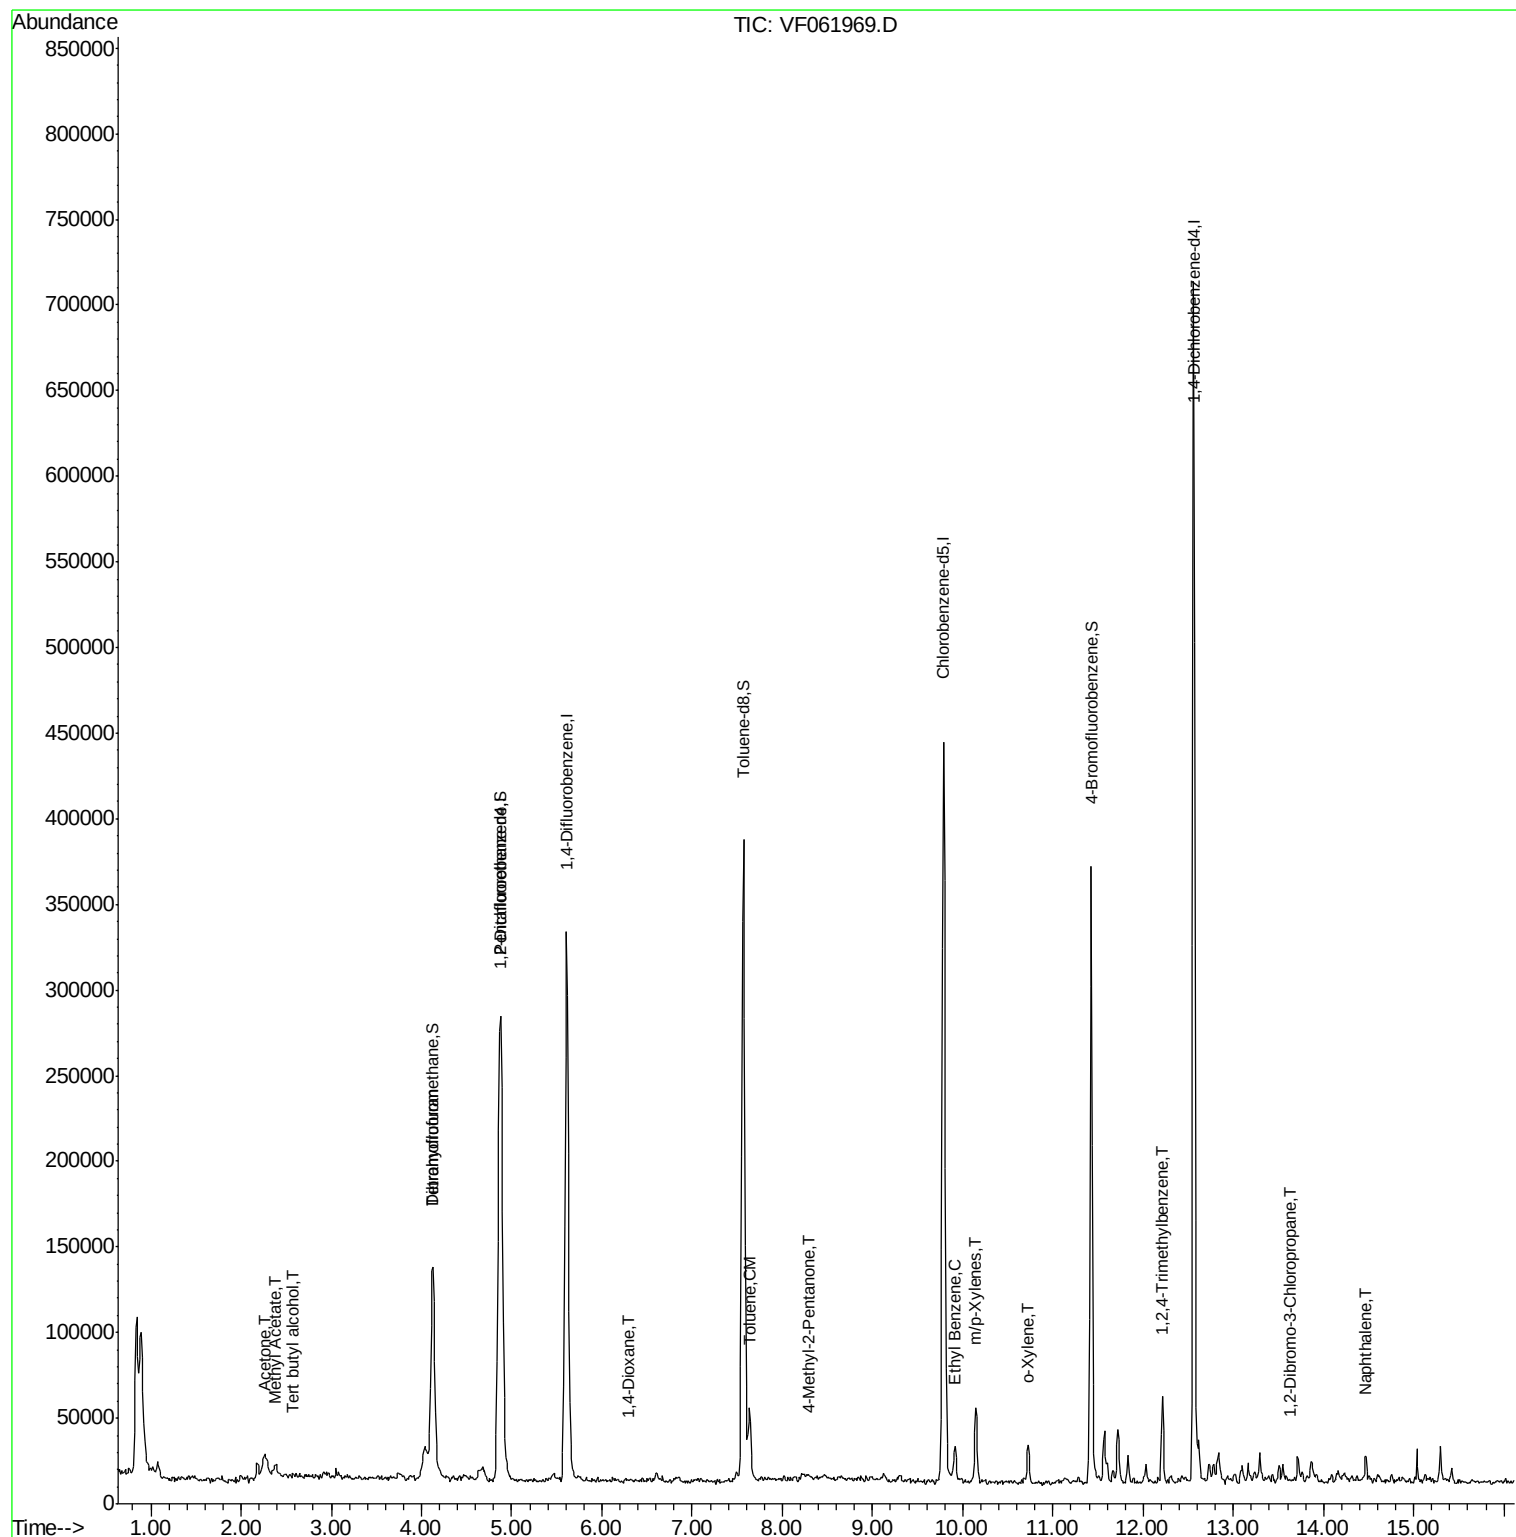

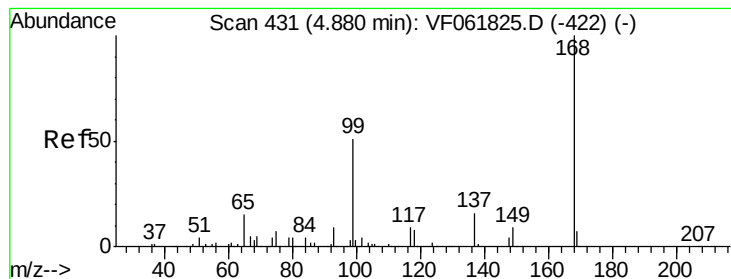

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.88 min Scan# 431

Delta R.T. -0.00 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :


SI-2(5.5-6)

Tot Ion:168 Resp: 244977

Ion Ratio Lower Upper

168 100

99 53.1 40.8 61.2



Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

4.88

80000

60000



40000

20000

0

Time-->

4.70 4.80 4.90 5.00 5.10



#11

Tert butyl alcohol

Concen: 1.323 ug/l

RT: 2.59 min Scan# 199

Delta R.T. 0.01 min

Lab File: VF061969.D


Acq: 15 Mar 2019 19:05

Tgt Ion: 59 Resp: 134

Ion Ratio Lower Upper

59 100

57 0.0 11.8 17.6#



Abundance Ion 59.00 (58.70 to 59.70): VF0

Ion 57.00 (56.70 to 57.70): VF0

2.59

150


100


50

0

Time-->

2.56 2.58 2.60 2.62



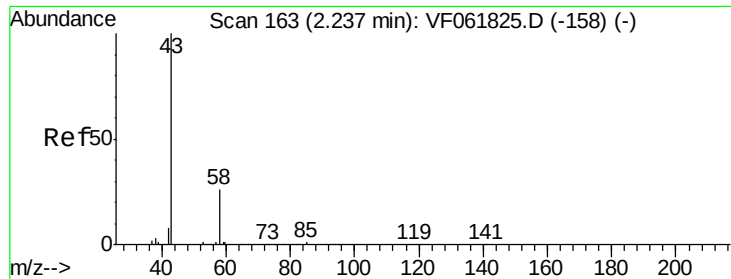

#16

Acetone

Concen: 12.280 ug/l

RT: 2.25 min Scan# 165

Delta R.T. 0.02 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :





SI-2(5.5-6)

Tot Ion: 43 Resp: 4589

Ion Ratio Lower Upper

43 100

58 21.9 20.3 30.5

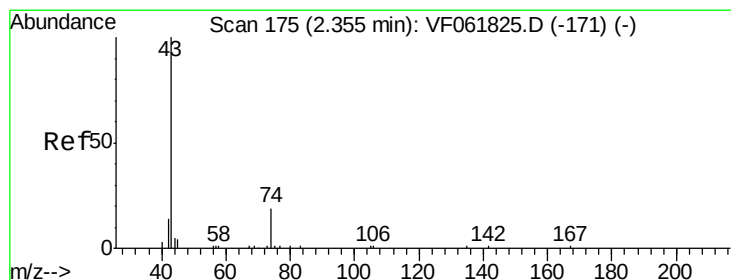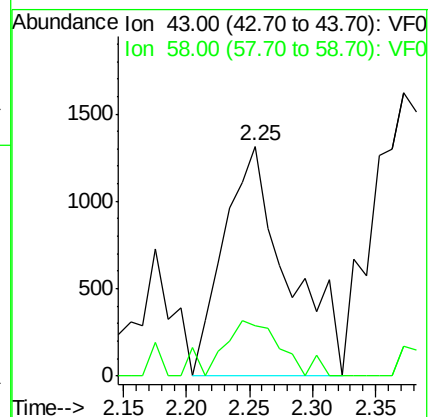

#18

Methyl Acetate

Concen: 4.075 ug/l

RT: 2.37 min Scan# 177

Delta R.T. 0.02 min

Lab File: VF061969.D




Acq: 15 Mar 2019 19:05


Tgt Ion: 43 Resp: 7780

Ion Ratio Lower Upper

43 100

74 16.9 13.2 19.8

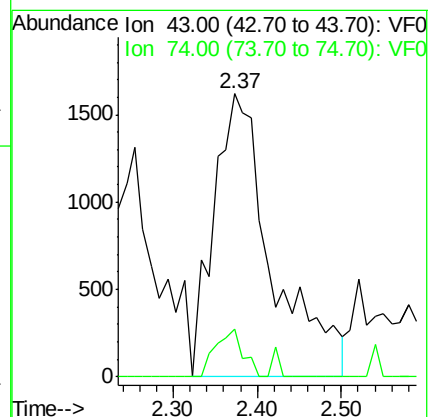

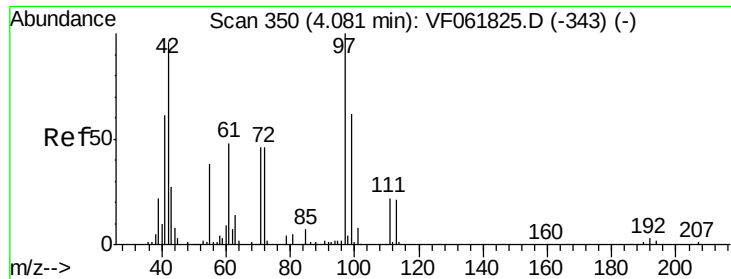

#29

Tetrahydrofuran

Concen: 3.825 ug/l

RT: 4.12 min Scan# 354

Delta R.T. 0.04 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :

SI-2(5.5-6)


Tot Ion: 42 Resp: 1254

Ion Ratio Lower Upper

42 100

72 0.0 34.4 51.6#




71 30.9 34.6 52.0#



Abundance Ion 42.00 (41.70 to 42.70): VF0

Ion 72.00 (71.70 to 72.70): VF0

Ion 71.00 (70.70 to 71.70): VF0

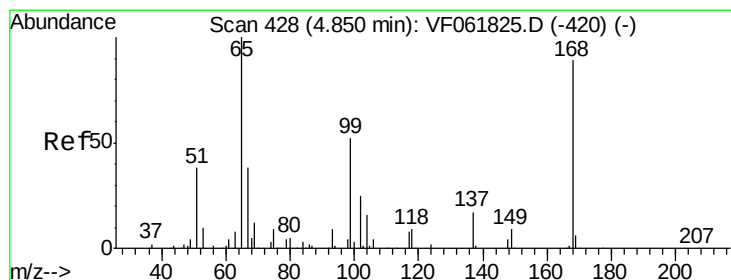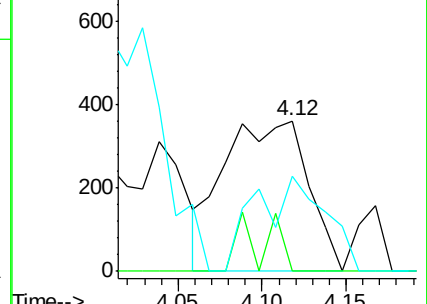

#33

1,2-Dichloroethane-d4

Concen: 52.324 ug/l

RT: 4.86 min Scan# 429

Delta R.T. 0.01 min

Lab File: VF061969.D


Acq: 15 Mar 2019 19:05

Tgt Ion: 65 Resp: 93347

Ion Ratio Lower Upper



65 100


67 53.3 0.0 108.6



Abundance Ion 65.00 (64.70 to 65.70): VF0

Ion 67.00 (66.70 to 67.70): VF0

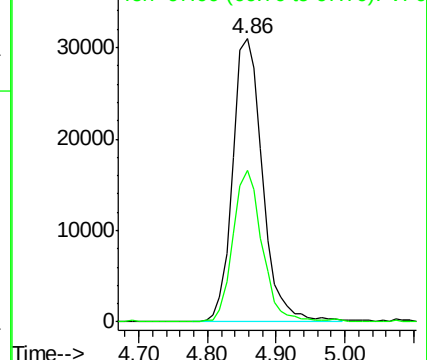



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.61 min Scan# 505

Delta R.T. -0.00 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :

SI-2(5.5-6)


Tot Ion:114 Resp: 389662

Ion Ratio Lower Upper

114 100

63 19.2 0.0 35.6




88 19.7 0.0 35.6

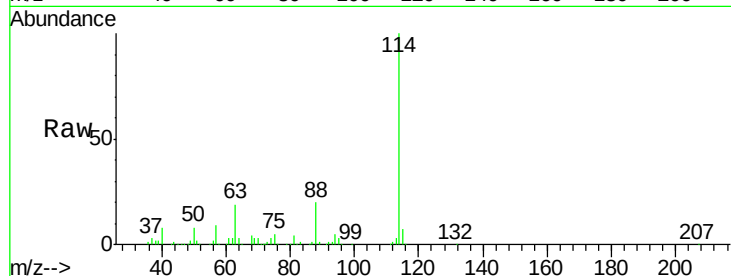

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

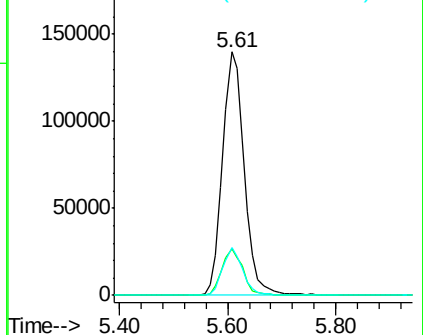

#35

Dibromofluoromethane

Concen: 45.426 ug/l

RT: 4.13 min Scan# 355

Delta R.T. 0.01 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05


Tgt Ion:113 Resp: 123528

Ion Ratio Lower Upper

113 100

111 103.9 77.6 116.4



192 17.3 15.9 23.9




Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V




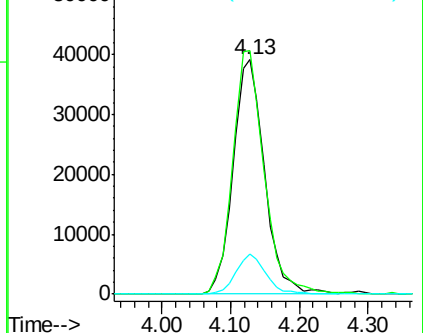


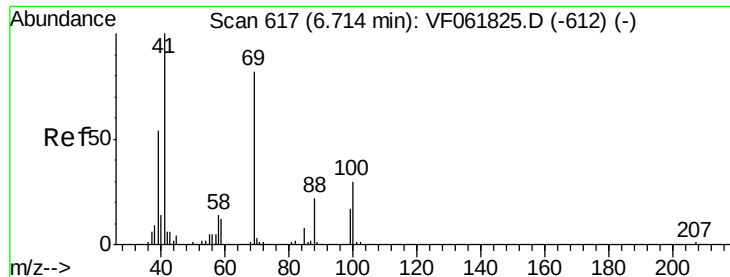

#49
1,4-Dioxane
Concen: 5.627 ug/l
RT: 6.29 min Scan# 574
Delta R.T. -0.43 min
Lab File: VF061969.D
Acq: 15 Mar 2019 19:05




Instrument :
MSVOA_F
ClientSampleId :
SI-2(5.5-6)


Tot Ion: 88 Resp: 62
Ion Ratio Lower Upper
88 100
43 269.5 28.4 42.6#
58 0.0 50.7 76.1#

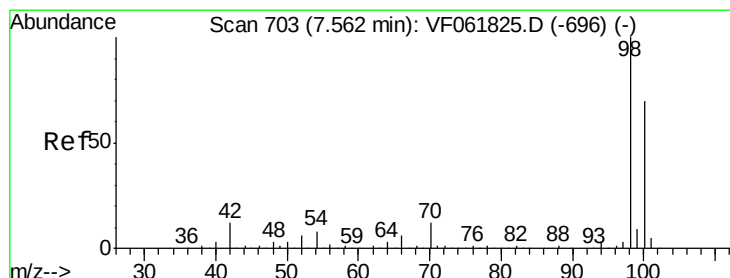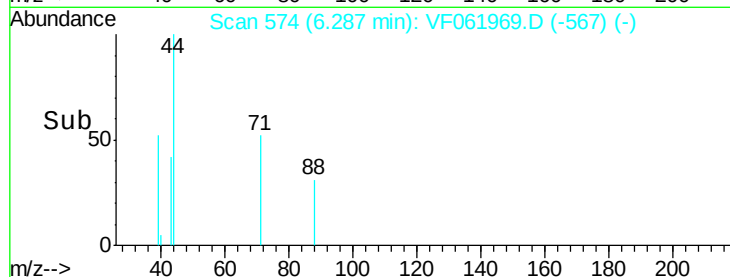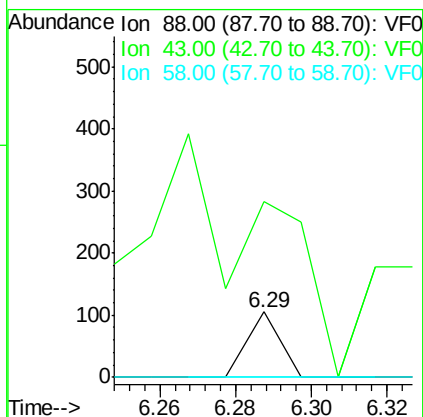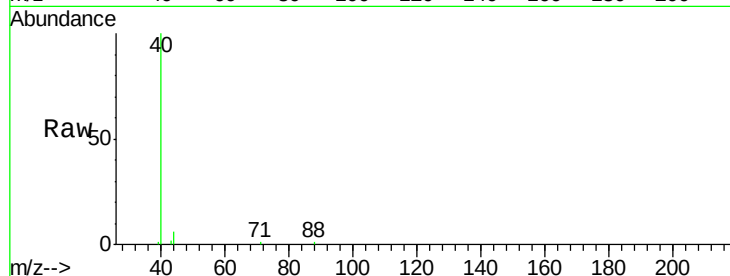

#50
Toluene-d8
Concen: 41.164 ug/l
RT: 7.57 min Scan# 704
Delta R.T. 0.01 min
Lab File: VF061969.D
Acq: 15 Mar 2019 19:05

Tgt Ion: 98 Resp: 332714
Ion Ratio Lower Upper
98 100
100 71.3 56.0 84.0

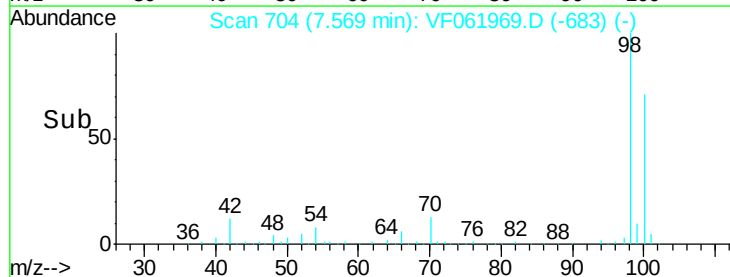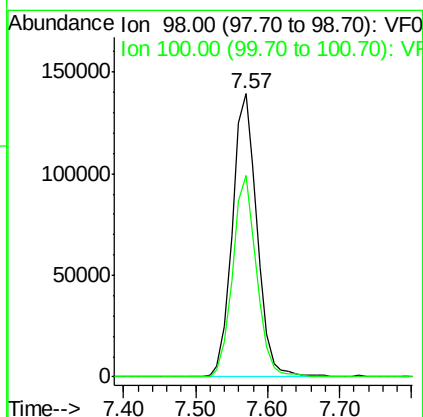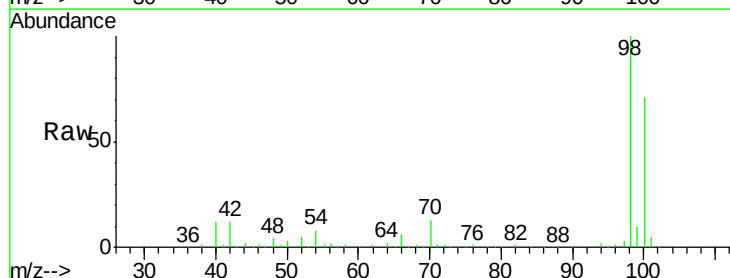

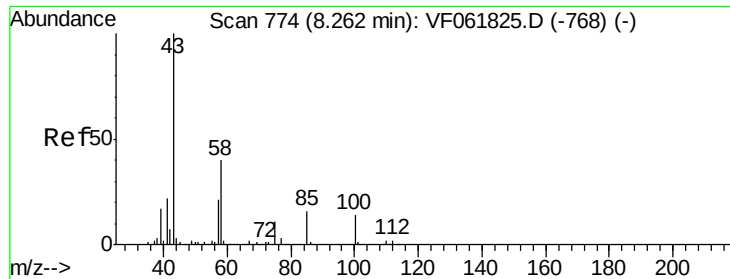

#51

4-Methyl-2-Pentanone

Concen: 2.086 ug/l

RT: 8.28 min Scan# 776

Delta R.T. 0.02 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :


SI-2(5.5-6)

Tot Ion: 43 Resp: 2745

Ion Ratio Lower Upper




43 100

58 16.0 31.8 47.8#

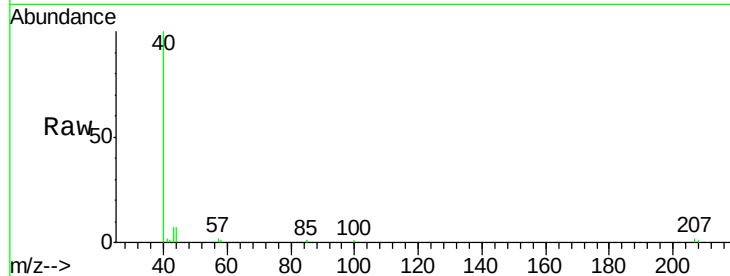

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0

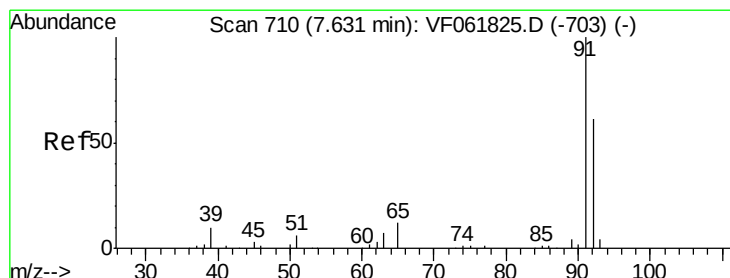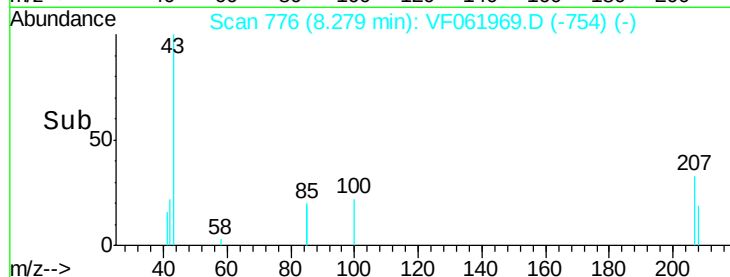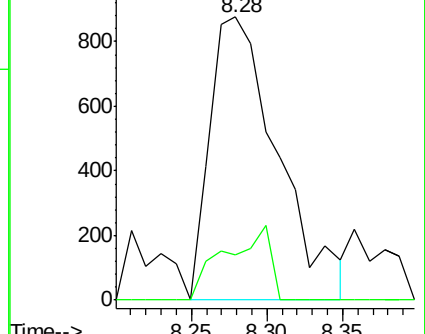

#52

Toluene

Concen: 3.968 ug/l

RT: 7.64 min Scan# 711

Delta R.T. 0.01 min

Lab File: VF061969.D


Acq: 15 Mar 2019 19:05

Tgt Ion: 92 Resp: 22586

Ion Ratio Lower Upper



92 100


91 166.5 132.0 198.0

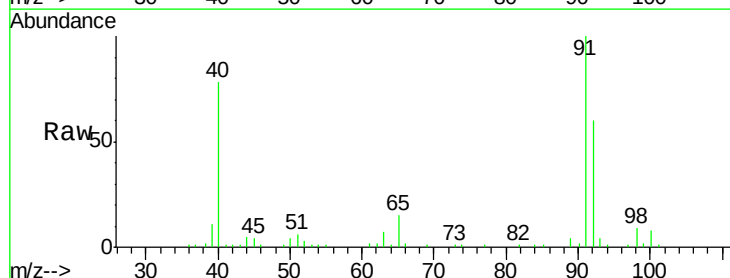

Abundance Ion 92.00 (91.70 to 92.70): VF0

Ion 91.00 (90.70 to 91.70): VF0

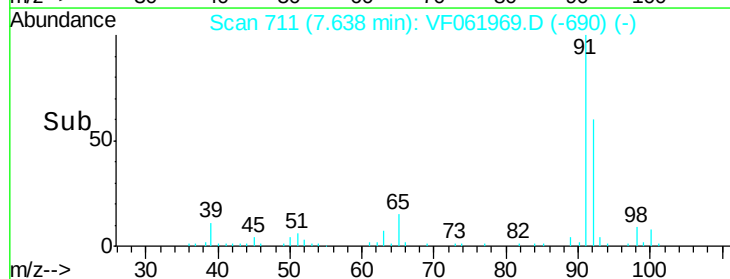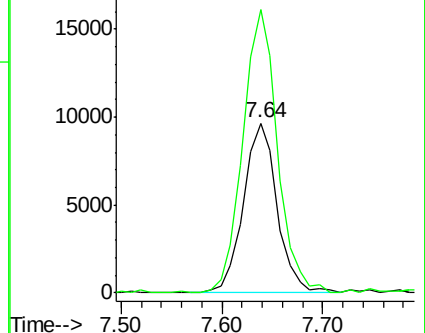

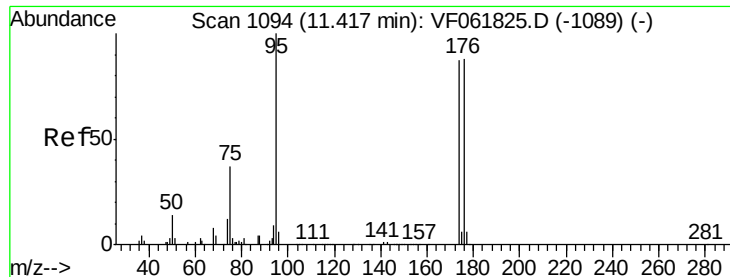

#62

4-Bromofluorobenzene

Concen: 44.169 ug/l

RT: 11.42 min Scan# 1095

Delta R.T. 0.01 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :

SI-2(5.5-6)


Tot Ion: 95 Resp: 139847

Ion Ratio Lower Upper

95 100

174 84.8 0.0 174.0




176 81.3 0.0 175.2

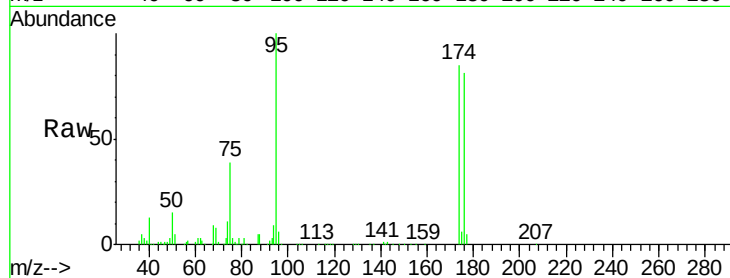

Abundance Ion 95.00 (94.70 to 95.70): VF0

Ion 174.00 (173.70 to 174.70): VF0

Ion 176.00 (175.70 to 176.70): VF0

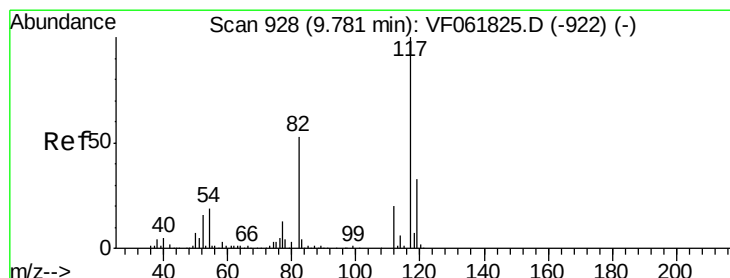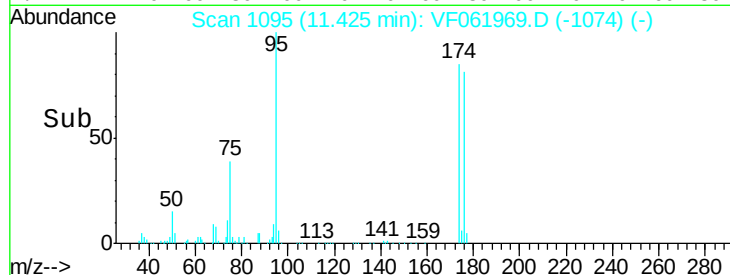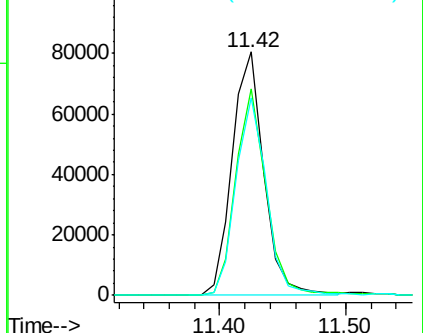

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.79 min Scan# 929

Delta R.T. 0.01 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05


Tgt Ion: 117 Resp: 329051

Ion Ratio Lower Upper

117 100

82 53.9 42.6 63.8



119 35.7 26.0 39.0

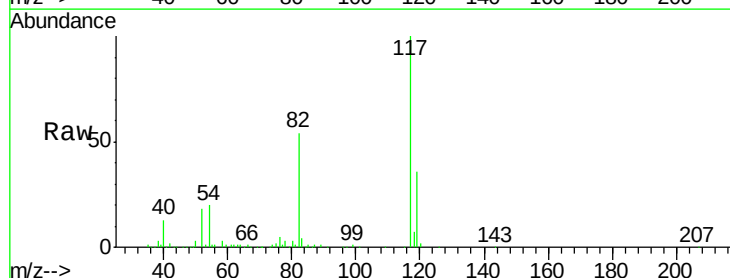


Abundance Ion 117.00 (116.70 to 117.70): VF0

Ion 82.00 (81.70 to 82.70): VF0

Ion 119.00 (118.70 to 119.70): VF0

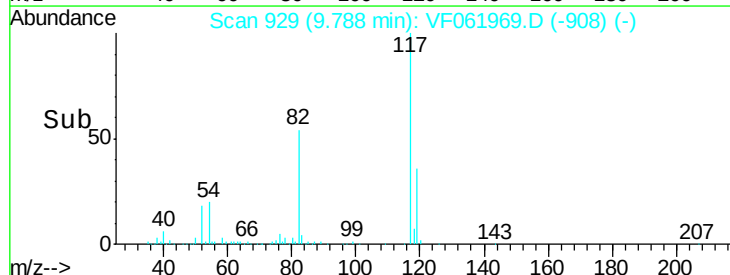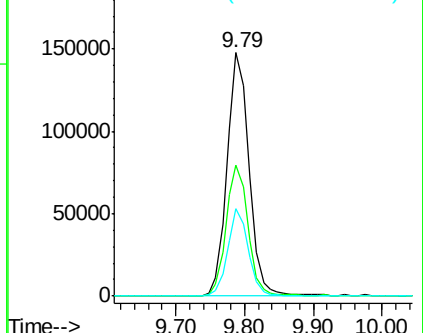

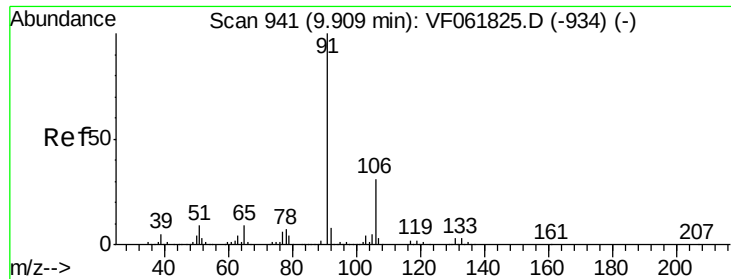

#67

Ethyl Benzene

Concen: 1.466 ug/l

RT: 9.92 min Scan# 942

Delta R.T. 0.01 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :





SI-2(5.5-6)

Tot Ion: 91 Resp: 15364

Ion Ratio Lower Upper

91 100

106 25.0 25.0 37.4#

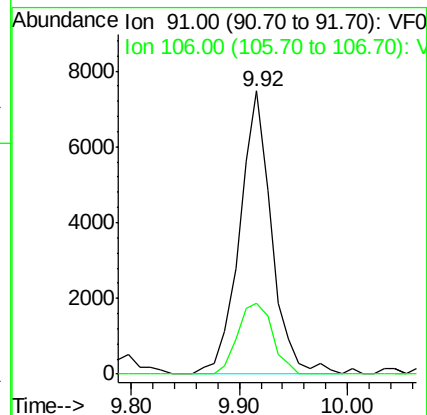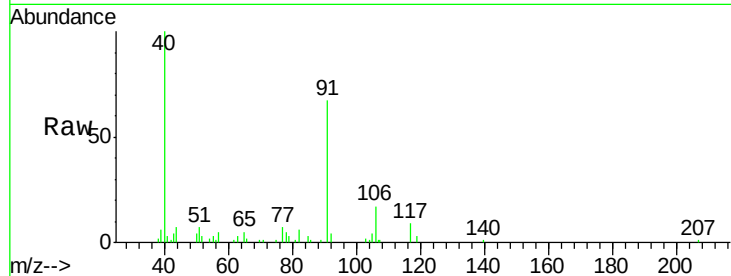

#68

m/p-Xylenes

Concen: 4.139 ug/l

RT: 10.14 min Scan# 965

Delta R.T. 0.01 min

Lab File: VF061969.D




Acq: 15 Mar 2019 19:05


Tgt Ion: 106 Resp: 16613

Ion Ratio Lower Upper

106 100

91 230.8 157.5 236.3


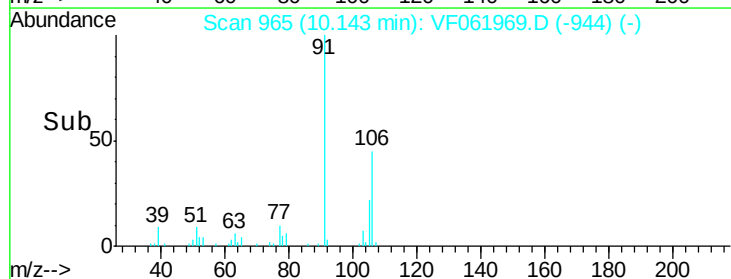
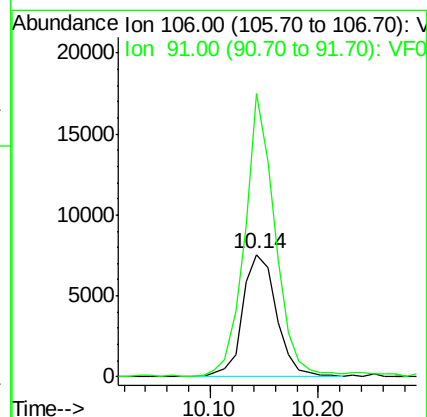



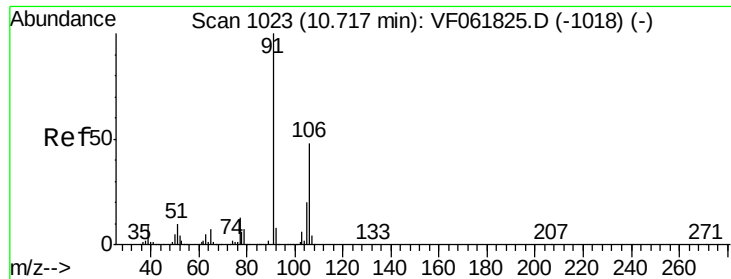

#69
o-Xylene
Concen: 1.563 ug/l
RT: 10.72 min Scan# 1024
Delta R.T. 0.01 min
Lab File: VF061969.D
Acq: 15 Mar 2019 19:05




Instrument :
MSVOA_F
ClientSampled :
SI-2(5.5-6)


Tot Ion:106 Resp: 6757
Ion Ratio Lower Upper
106 100
91 240.9 103.5 310.3

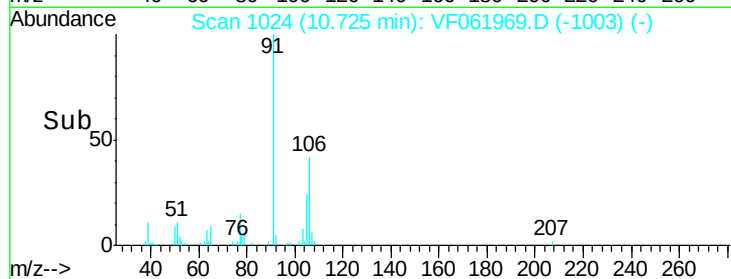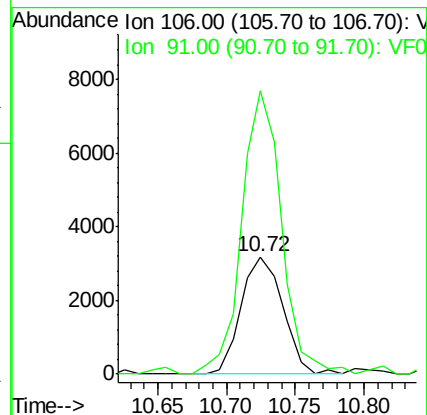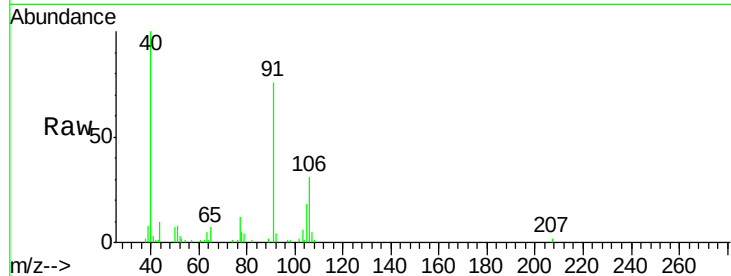

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.56 min Scan# 1210
Delta R.T. 0.01 min
Lab File: VF061969.D
Acq: 15 Mar 2019 19:05

Tgt Ion:152 Resp: 189208
Ion Ratio Lower Upper
152 100
115 54.3 27.7 83.1
150 153.2 0.0 304.2

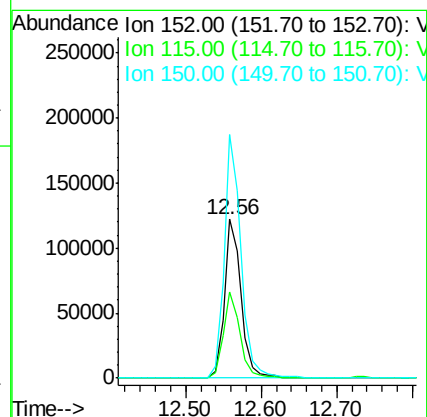



#84

1,2,4-Trimethylbenzene

Concen: 2.473 ug/l

RT: 12.21 min Scan# 1175

Delta R.T. 0.01 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :





SI-2(5.5-6)

Tot Ion:105 Resp: 25349

Ion Ratio Lower Upper

105 100

120 50.3 25.8 77.4

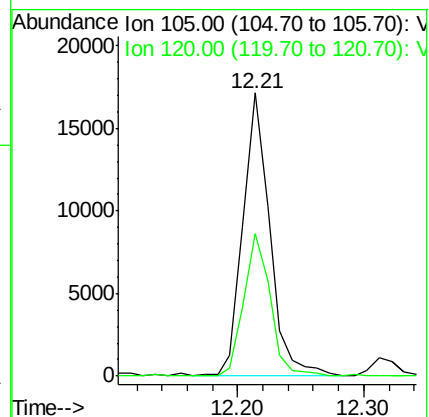

#92

1,2-Dibromo-3-Chloropropane

Concen: 3.932 ug/l

RT: 13.63 min Scan# 1319

Delta R.T. -0.01 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05




Tgt Ion: 75 Resp: 67


Ion Ratio Lower Upper

75 100

155 0.0 59.8 179.4#

157 0.0 81.2 243.4#

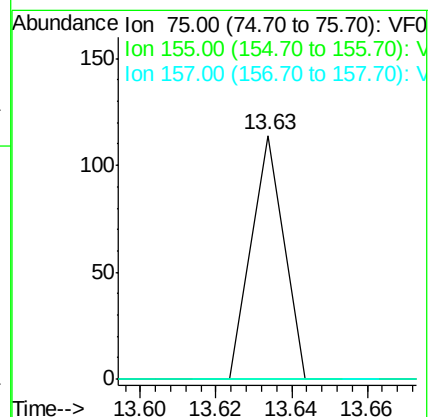

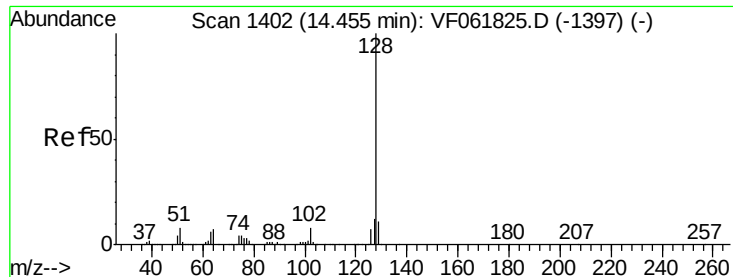

#95

Naphthalene

Concen: 1.566 ug/l

RT: 14.47 min Scan# 1404

Delta R.T. 0.02 min

Lab File: VF061969.D

Acq: 15 Mar 2019 19:05

Instrument :

MSVOA_F

ClientSampleId :

SI-2(5.5-6)


Tot Ion:128 Resp: 11025

Ion Ratio Lower Upper

128 100

127 16.2 9.3 13.9#

129 10.0 8.8 13.2

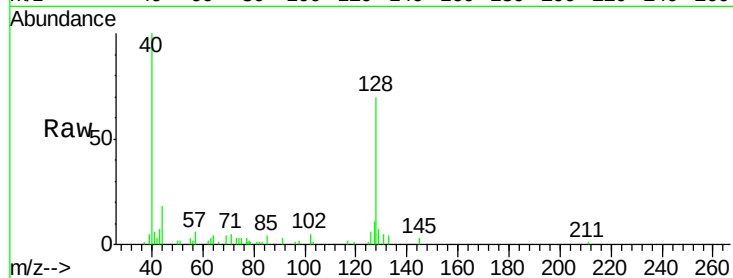

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

