


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF031619\
Data File : VF061971.D
Acq On : 16 Mar 2019 9:38
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F031619S.M
Title : SW846 8260
Last Update : Mon Mar 18 07:28:40 2019

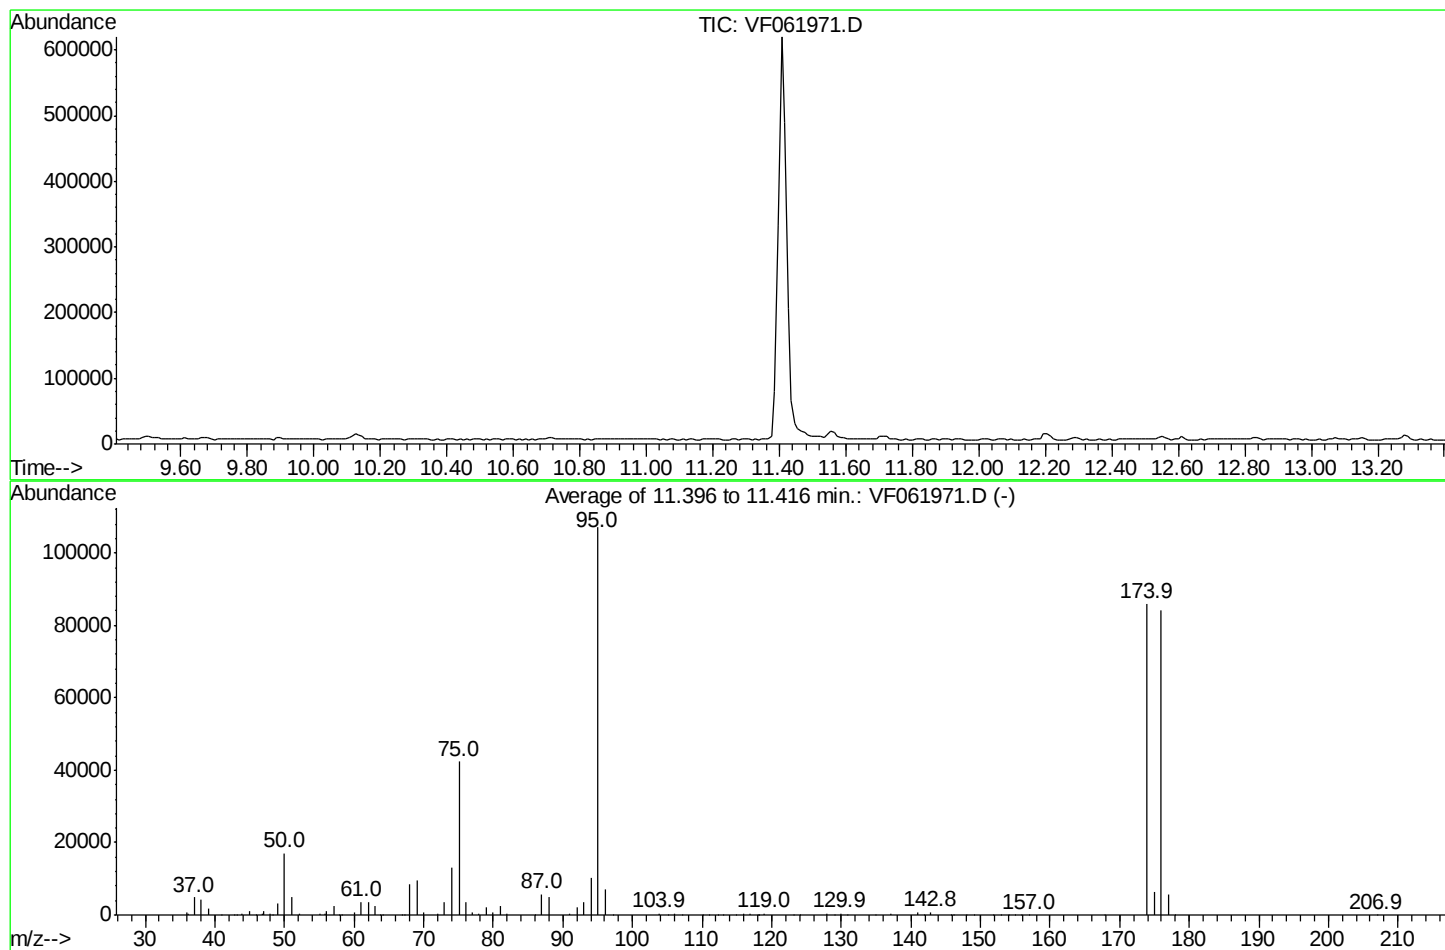

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1087

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	17045	PASS
75	95	30	60	39.6	42360	PASS
95	95	100	100	100.0	107098	PASS
96	95	5	9	6.5	6985	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.3	86048	PASS
175	174	5	9	7.4	6337	PASS
176	174	95	101	97.7	84090	PASS
177	176	5	9	6.7	5606	PASS