


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF031819\
 Data File : VF061988.D
 Acq On : 18 Mar 2019 9:42
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F031619S.M
 Title : SW846 8260
 Last Update : Mon Mar 18 07:28:40 2019

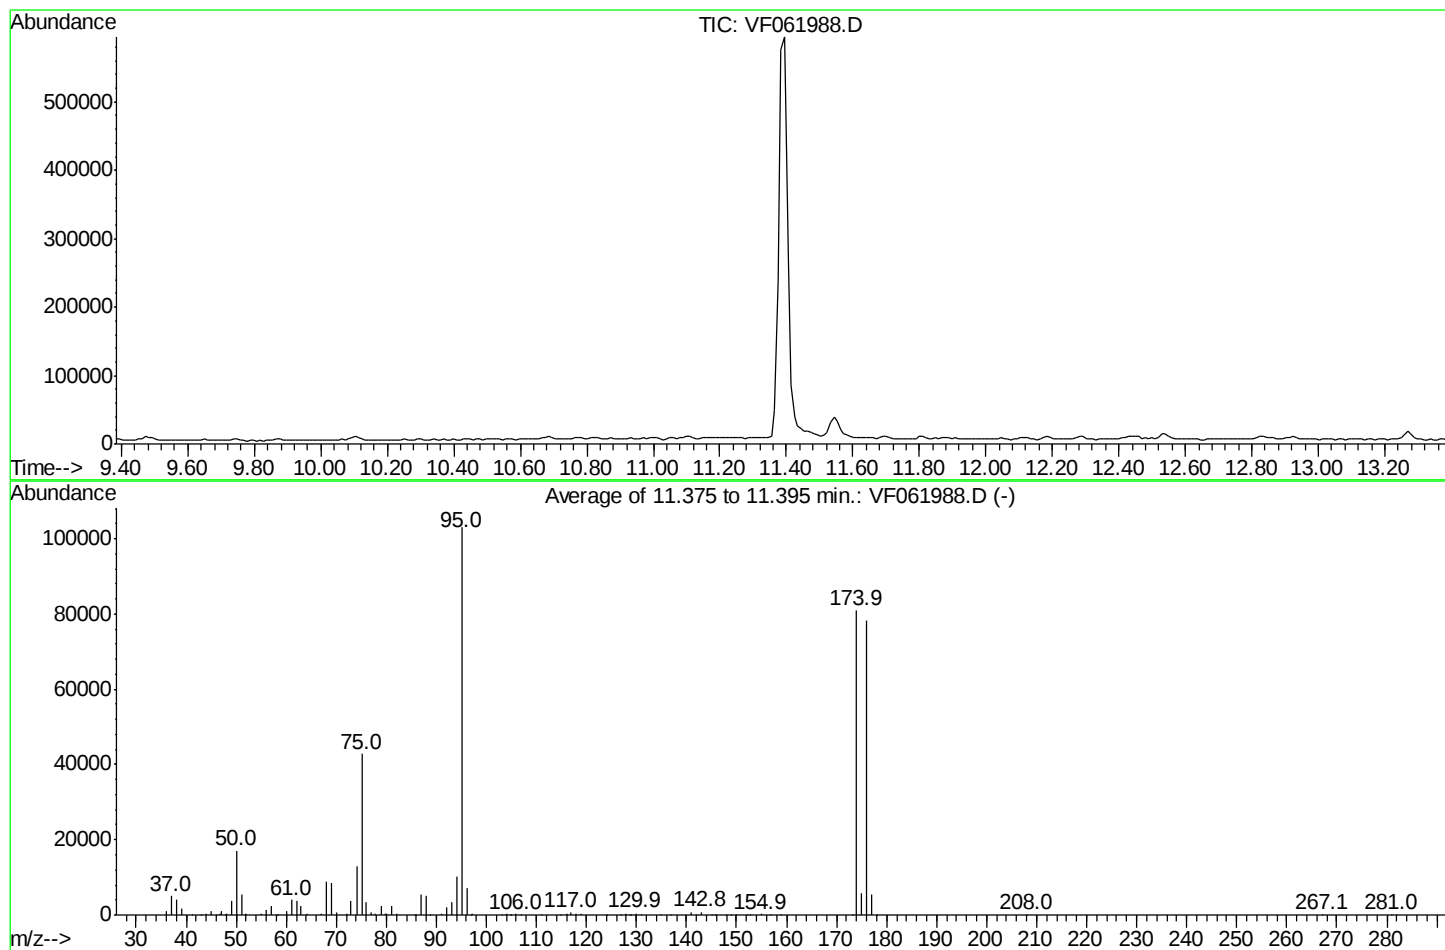

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	17110	PASS
75	95	30	60	41.6	42850	PASS
95	95	100	100	100.0	103029	PASS
96	95	5	9	7.0	7234	PASS
173	174	0.00	2	0.1	85	PASS
174	95	50	100	78.6	80949	PASS
175	174	5	9	7.2	5801	PASS
176	174	95	101	96.5	78096	PASS
177	176	5	9	6.8	5328	PASS