


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF032019\
Data File : VF062031.D
Acq On : 20 Mar 2019 9:54
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F031619S.M
Title : SW846 8260
Last Update : Fri Mar 22 03:22:44 2019

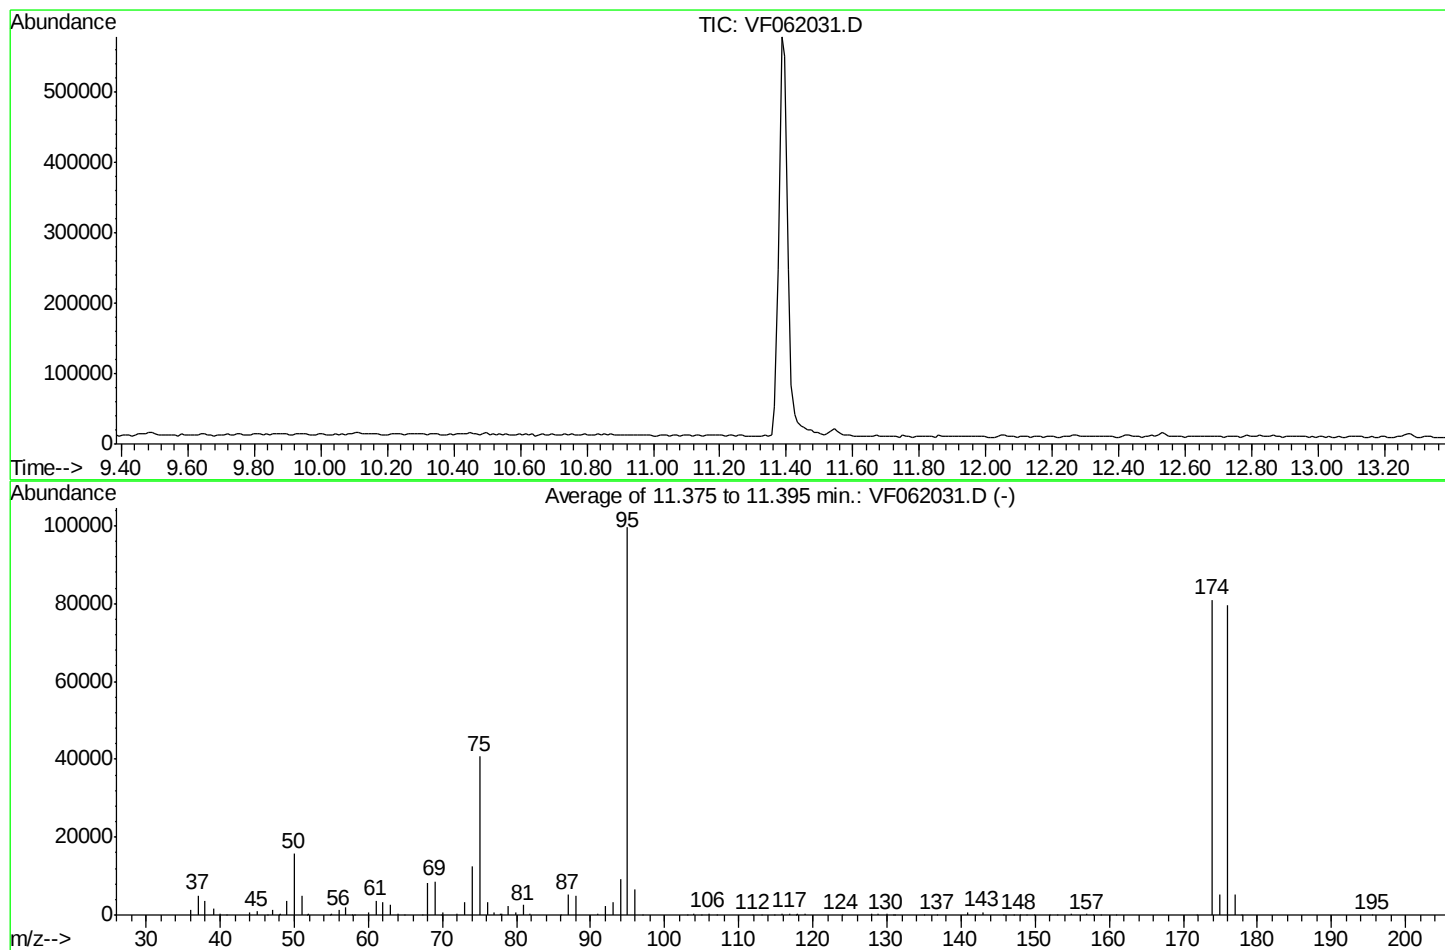

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1084

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	15672	PASS
75	95	30	60	40.9	40696	PASS
95	95	100	100	100.0	99581	PASS
96	95	5	9	6.6	6610	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.2	80909	PASS
175	174	5	9	6.6	5371	PASS
176	174	95	101	98.5	79674	PASS
177	176	5	9	6.7	5341	PASS