


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF032119\
 Data File : VF062053.D
 Acq On : 21 Mar 2019 9:59
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F031619S.M
 Title : SW846 8260
 Last Update : Fri Mar 22 03:22:44 2019

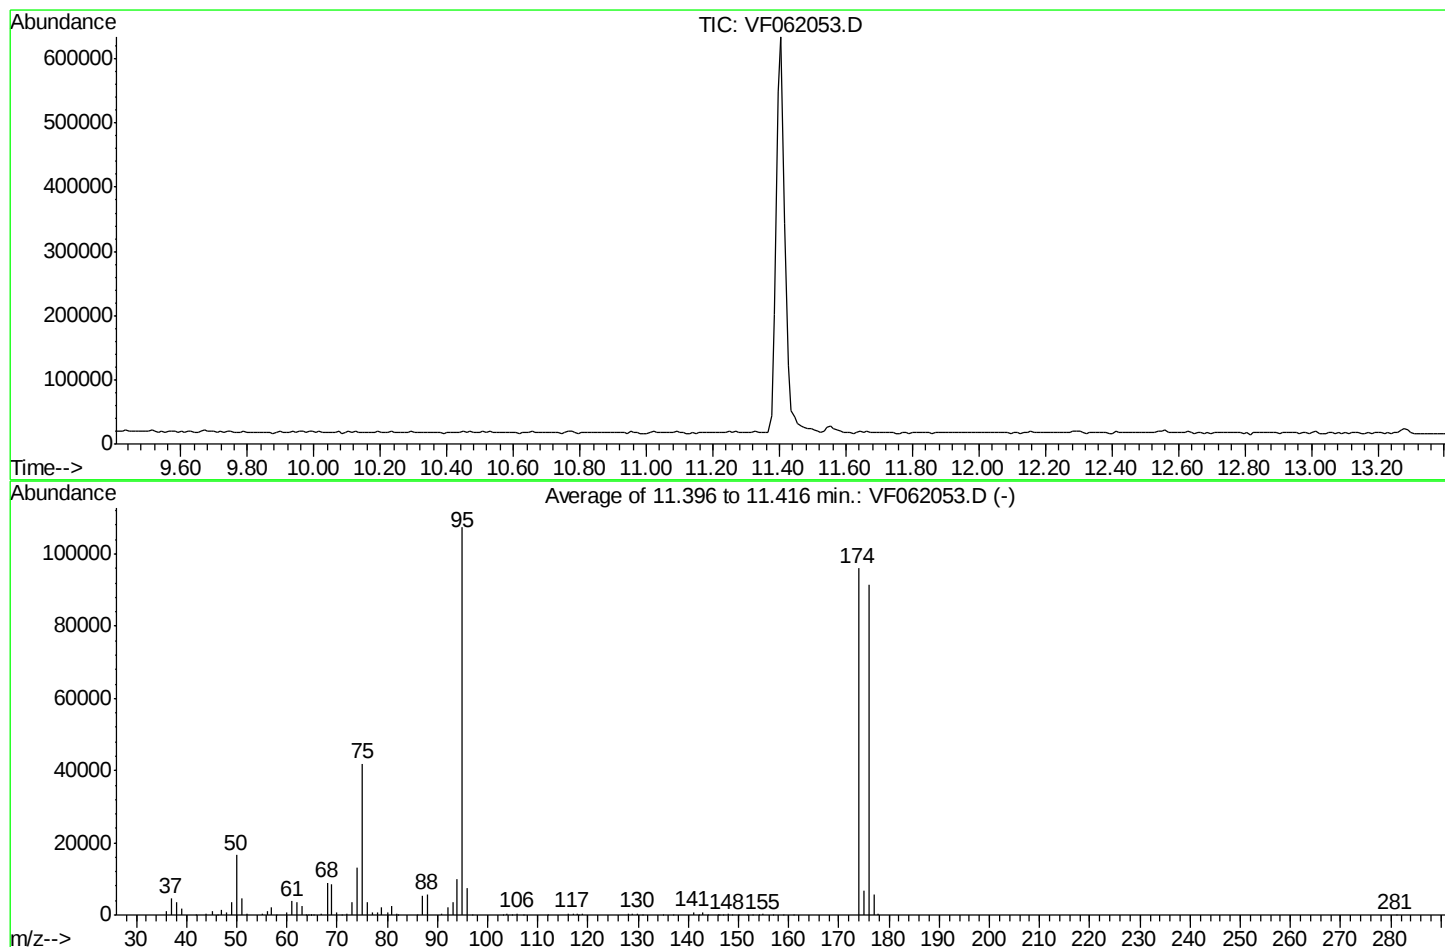

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	16637	PASS
75	95	30	60	39.0	41904	PASS
95	95	100	100	100.0	107397	PASS
96	95	5	9	7.0	7532	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.4	95997	PASS
175	174	5	9	7.0	6730	PASS
176	174	95	101	95.4	91538	PASS
177	176	5	9	6.2	5640	PASS