


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF032219\
Data File : VF062074.D
Acq On : 22 Mar 2019 9:29
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F032219S.M
Title : SW846 8260
Last Update : Sat Mar 23 01:16:37 2019

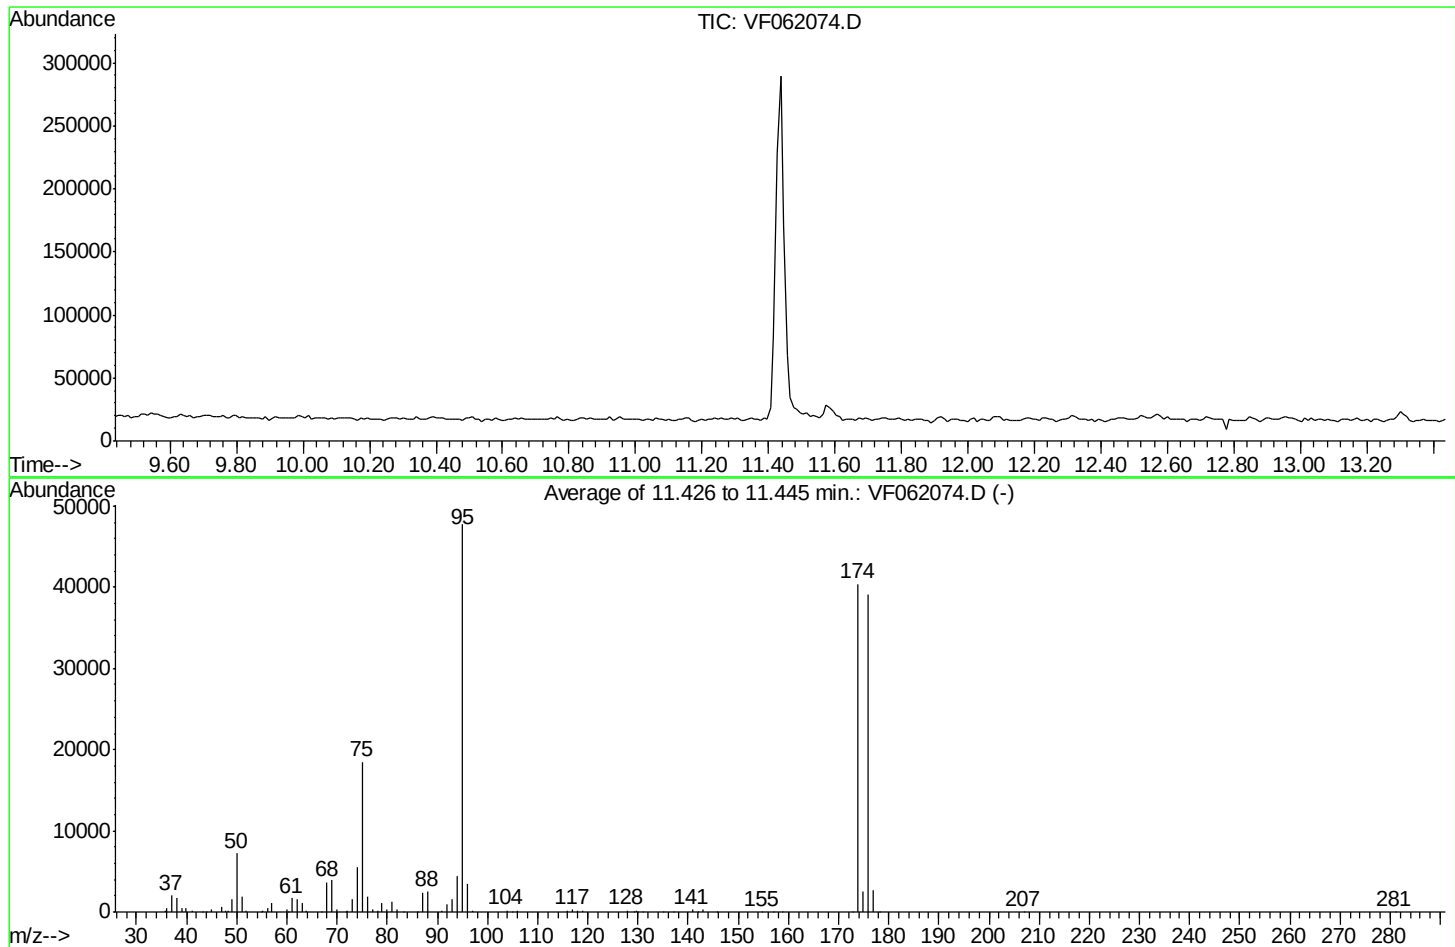

AutoFind: Scans 1095, 1096, 1097; Background Corrected with Scan 1090

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	7220	PASS
75	95	30	60	38.7	18472	PASS
95	95	100	100	100.0	47760	PASS
96	95	5	9	7.3	3499	PASS
173	174	0.00	2	0.1	48	PASS
174	95	50	100	84.7	40442	PASS
175	174	5	9	6.4	2603	PASS
176	174	95	101	96.7	39093	PASS
177	176	5	9	6.7	2615	PASS