


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_F\DATA\VF032219\
 Data File : VF062092.D
 Acq On : 22 Mar 2019 21:13
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F032219S.M
 Title : SW846 8260
 Last Update : Sat Mar 23 01:16:37 2019

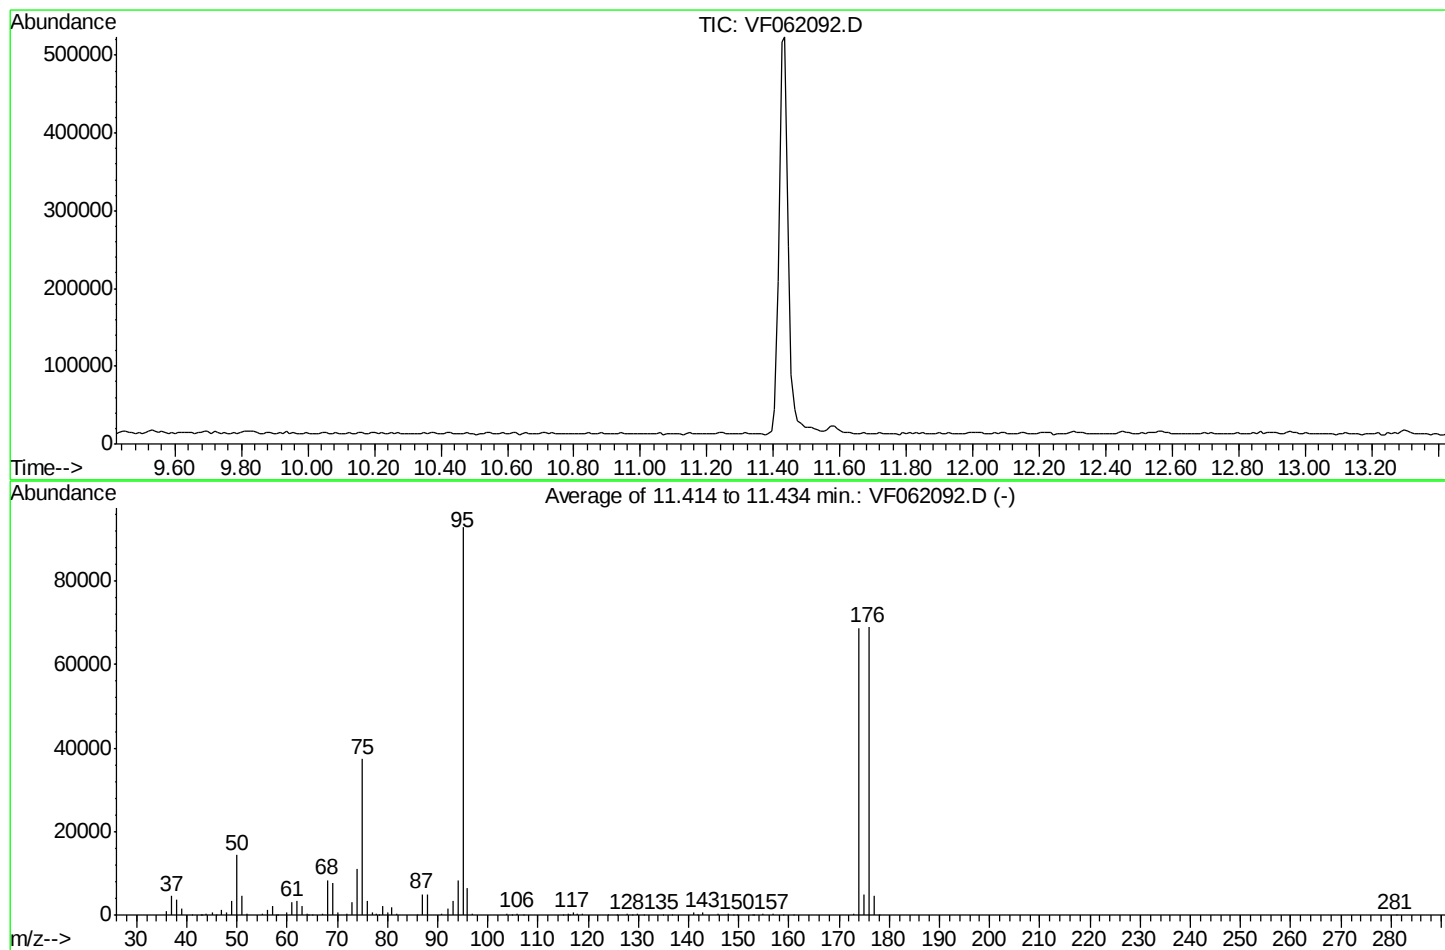

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1089

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	14326	PASS
75	95	30	60	40.2	37306	PASS
95	95	100	100	100.0	92856	PASS
96	95	5	9	6.9	6364	PASS
173	174	0.00	2	0.3	198	PASS
174	95	50	100	74.1	68800	PASS
175	174	5	9	7.3	5007	PASS
176	174	95	101	100.1	68845	PASS
177	176	5	9	6.8	4657	PASS