


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF032519\
Data File : VF062126.D
Acq On : 25 Mar 2019 12:11
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F032219S.M
Title : SW846 8260
Last Update : Sat Mar 23 01:16:37 2019

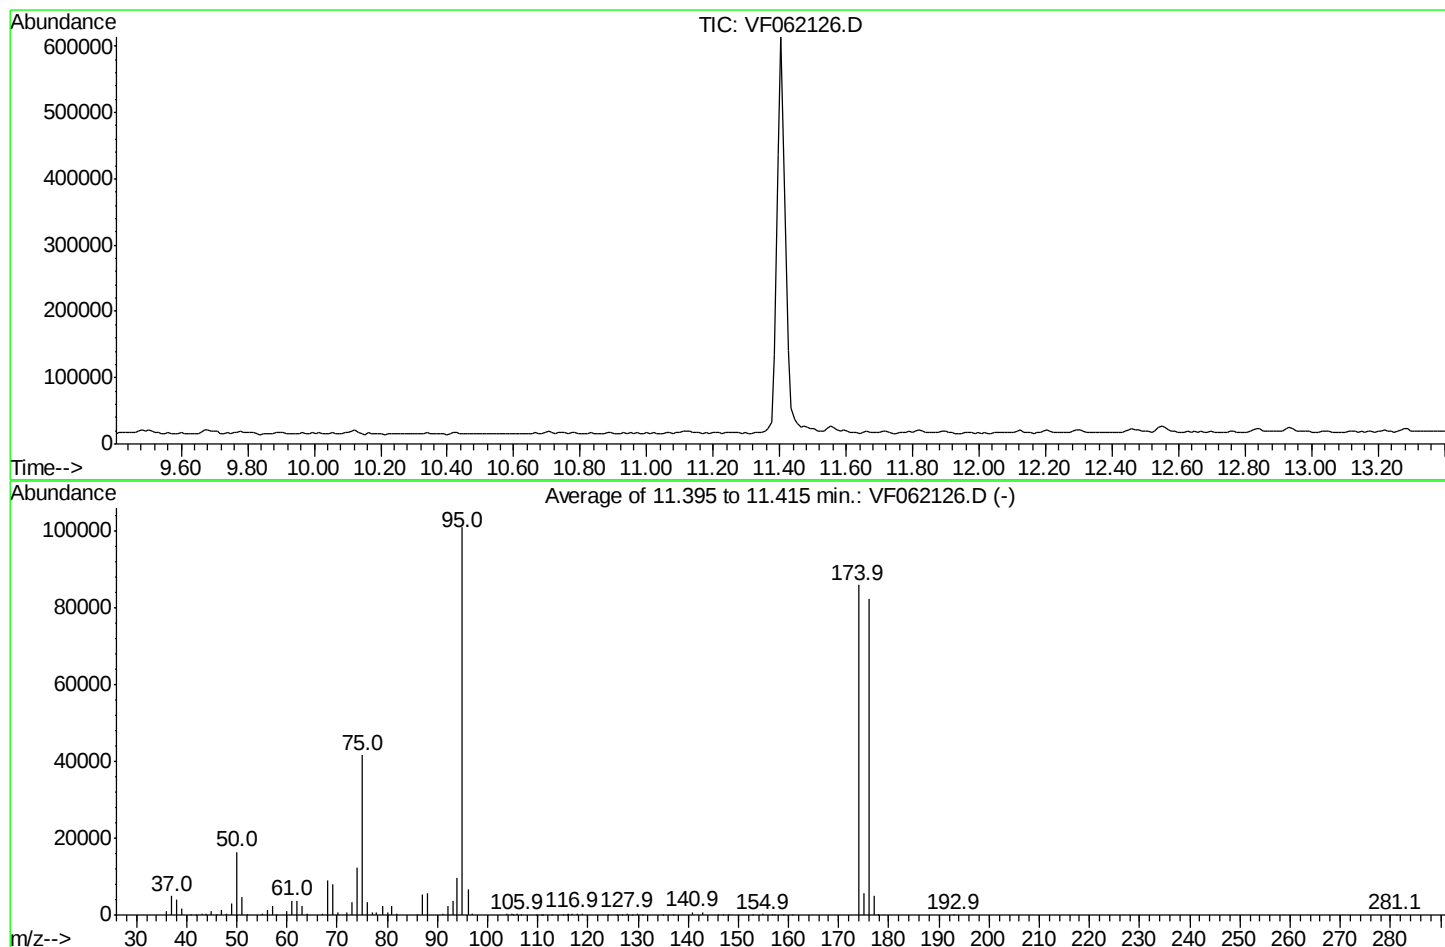

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	16461	PASS
75	95	30	60	41.1	41549	PASS
95	95	100	100	100.0	100973	PASS
96	95	5	9	6.6	6614	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.1	85904	PASS
175	174	5	9	6.7	5777	PASS
176	174	95	101	96.0	82482	PASS
177	176	5	9	6.0	4950	PASS