

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF032619\
 Data File : VF062156.D
 Acq On : 26 Mar 2019 20:04
 Operator : VA/AP
 Sample : K1693-13
 Misc : 6.78g/5mL/MSVOA-F/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 OR-01-032519-A

Quant Time: Mar 27 05:18:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F032219S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 23 01:16:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-4.91
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-5.63
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-9.81
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.57

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF032619\
Data File : VF062156.D
Acq On : 26 Mar 2019 20:04
Operator : VA/AP
Sample : K1693-13
Misc : 6.78g/5mL/MSVOA-F/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
OR-01-032519-A

Quant Time: Mar 27 05:18:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F032219S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 23 01:16:37 2019
Response via : Initial Calibration

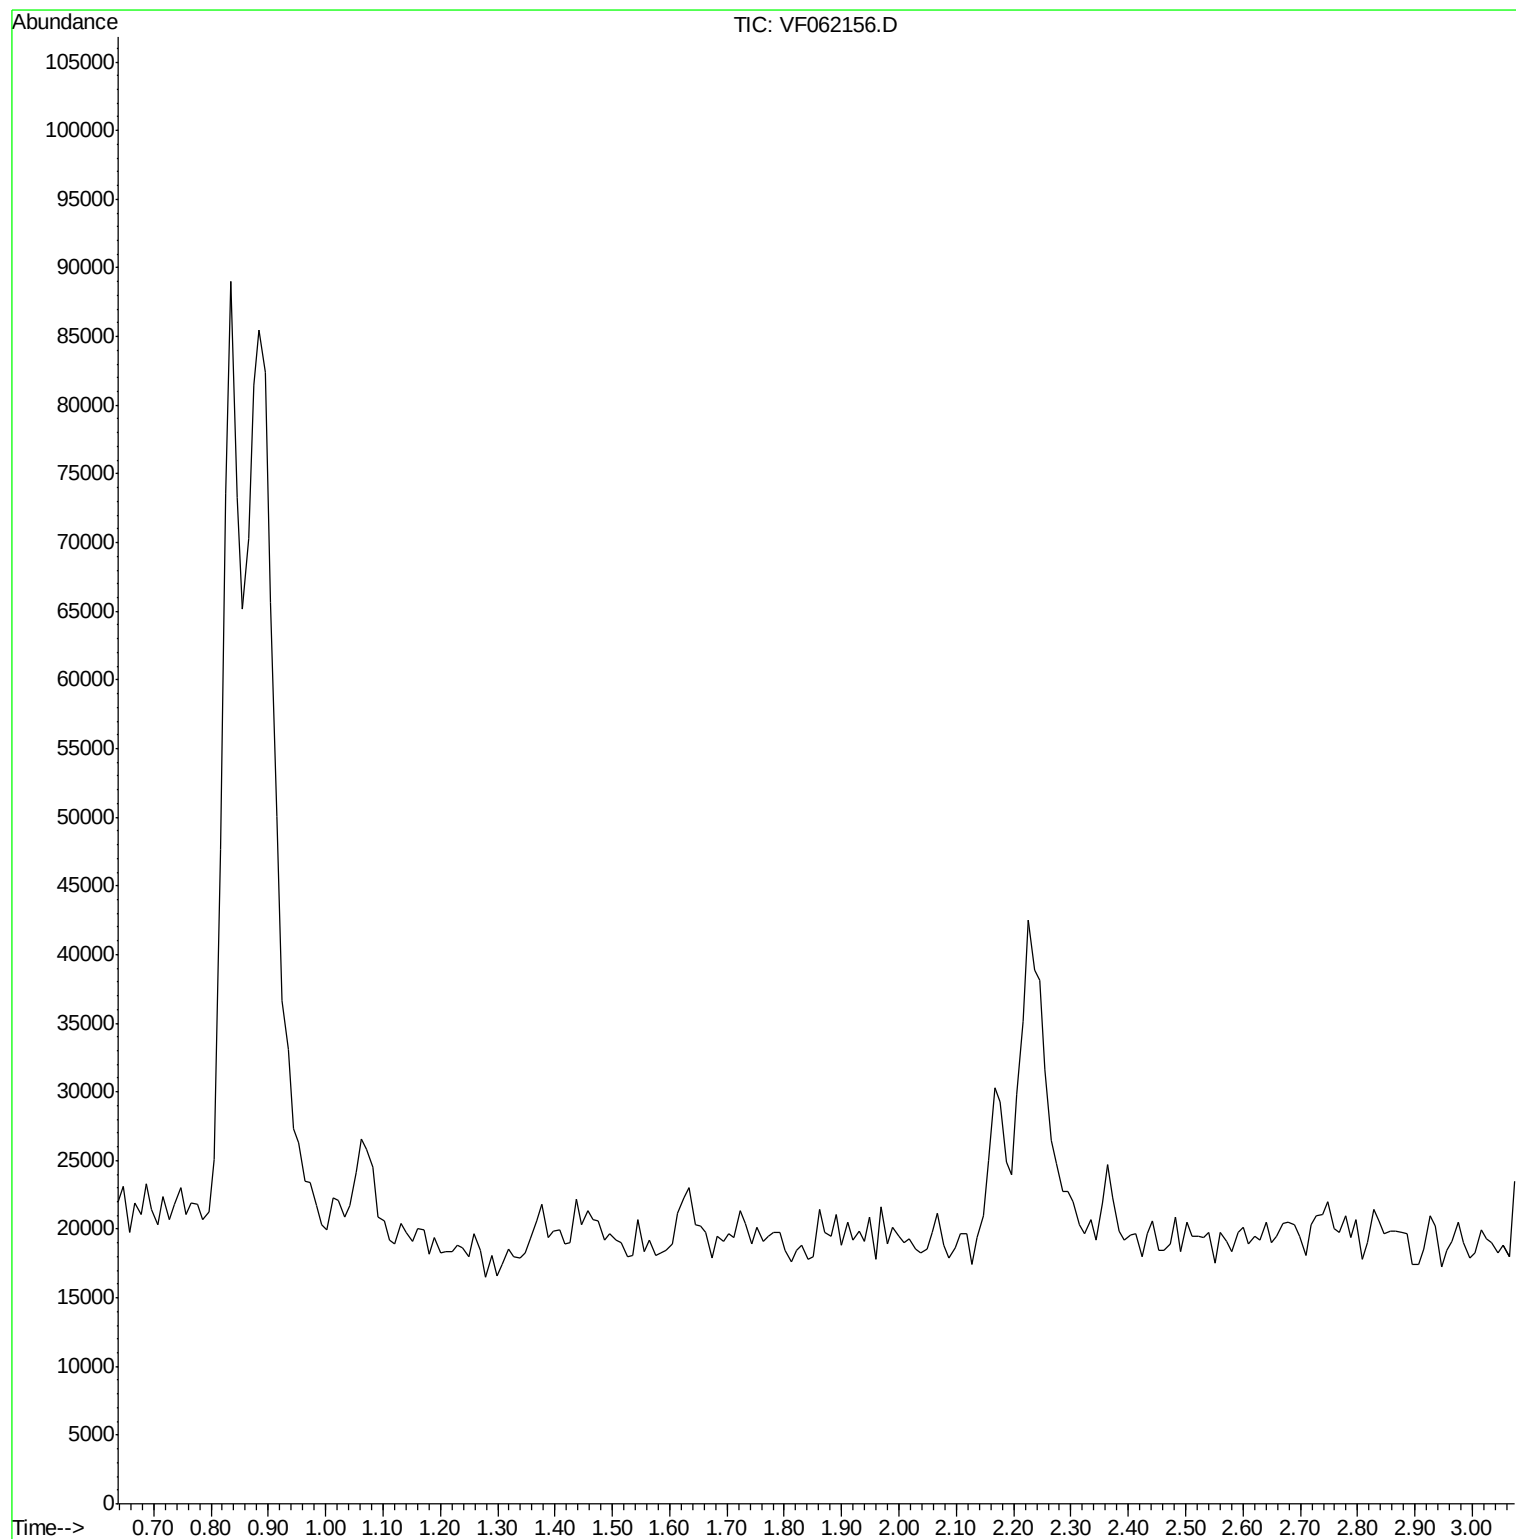


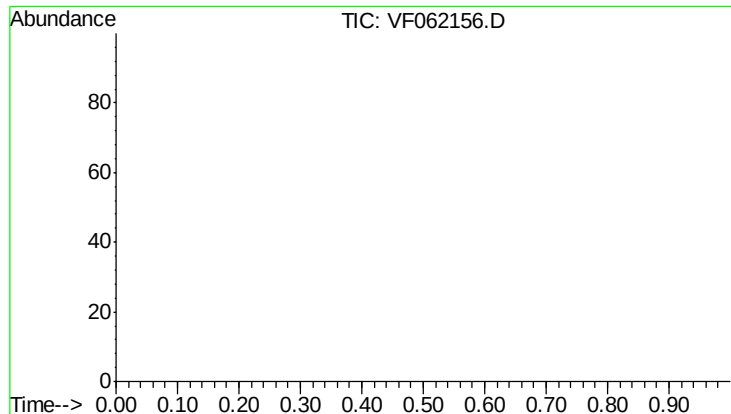


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 4.91 min

Lab File: VF062156.D
Acq: 26 Mar 2019 20:04

Instrument :
MSVOA_F
ClientSampleId :
OR-01-032519-A


Tot Ion: 168
Sig Exp Ratio
168 100
99 47.8

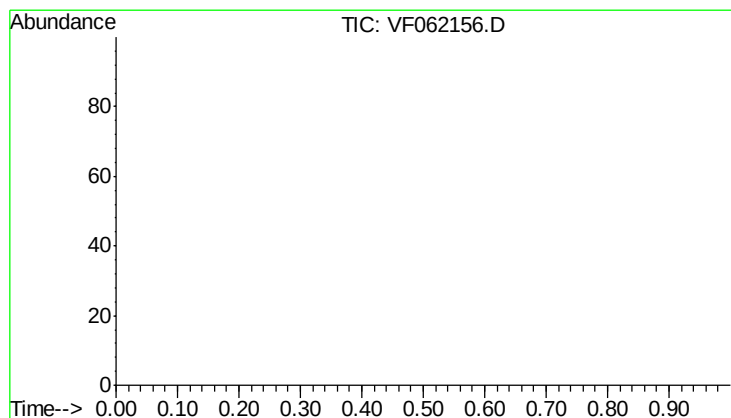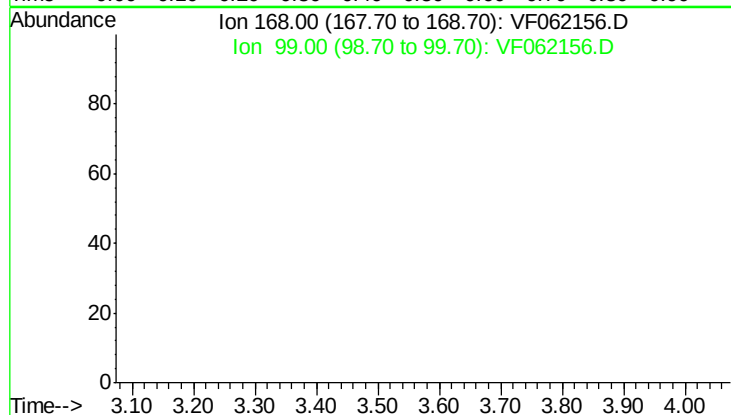


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 4.88 min

Lab File: VF062156.D
Acq: 26 Mar 2019 20:04

Tgt Ion: 65
Sig Exp Ratio
65 100
67 53.1


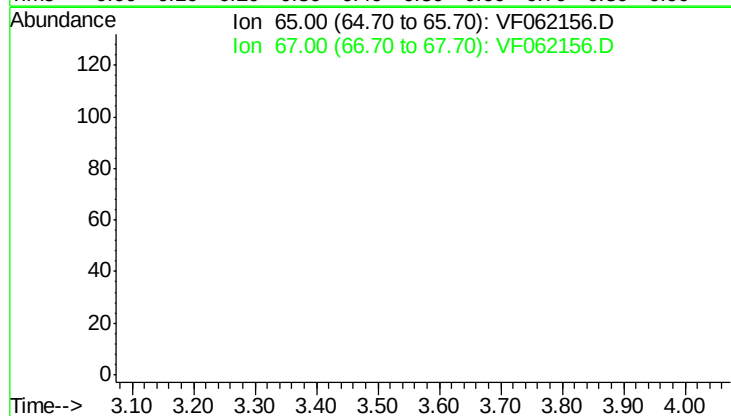


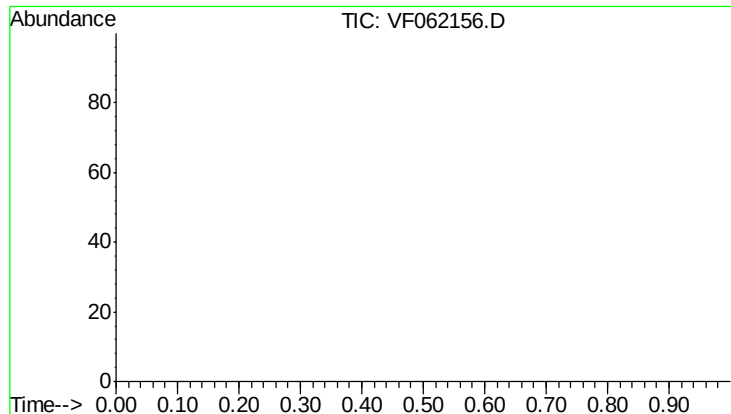

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 5.63 min
 Lab File: VF062156.D
 Acq: 26 Mar 2019 20:04


Instrument :
 MSVOA_F
 ClientSampleId :
 OR-01-032519-A


Tot Ion	114
Sig	Exp Ratio
114	100
63	18.9
88	18.2

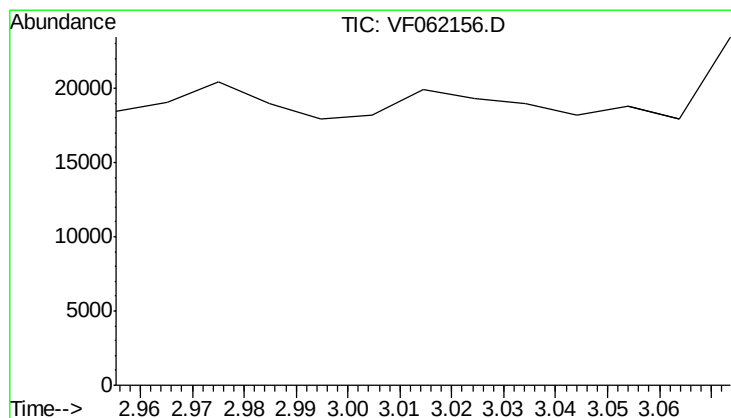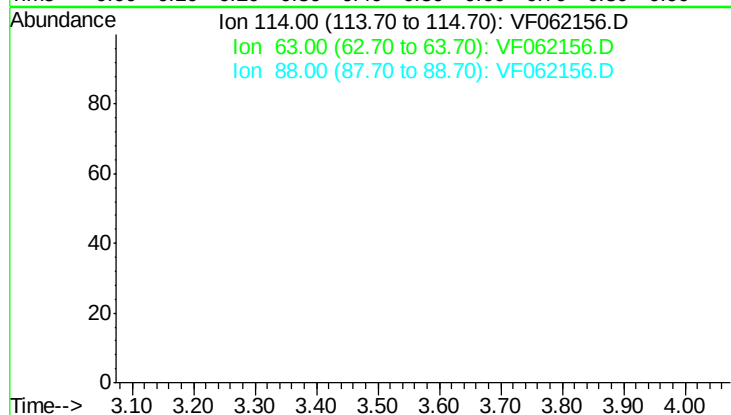

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 4.15 min
 Lab File: VF062156.D
 Acq: 26 Mar 2019 20:04

Tgt Ion	113
Sig	Exp Ratio
113	100
111	94.2
192	15.4

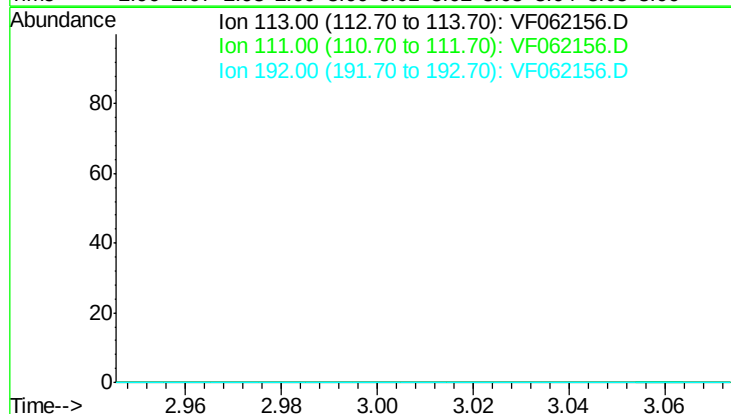


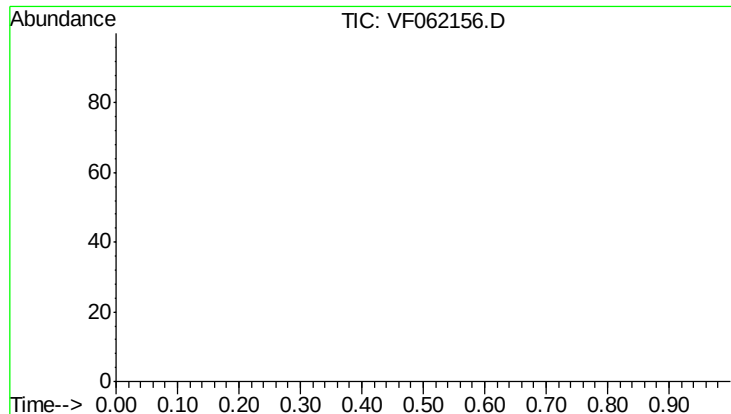


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 7.59 min

Lab File: VF062156.D
Acq: 26 Mar 2019 20:04

Instrument :
MSVOA_F
ClientSampleId :
OR-01-032519-A


Tot Ion	98
Sig	Exp Ratio
98	100
100	71.3

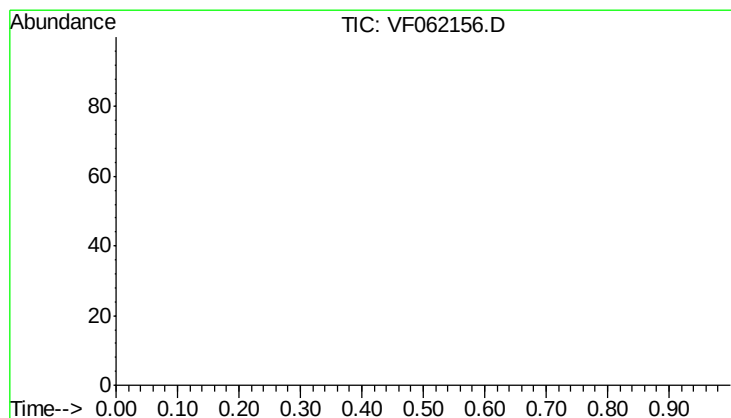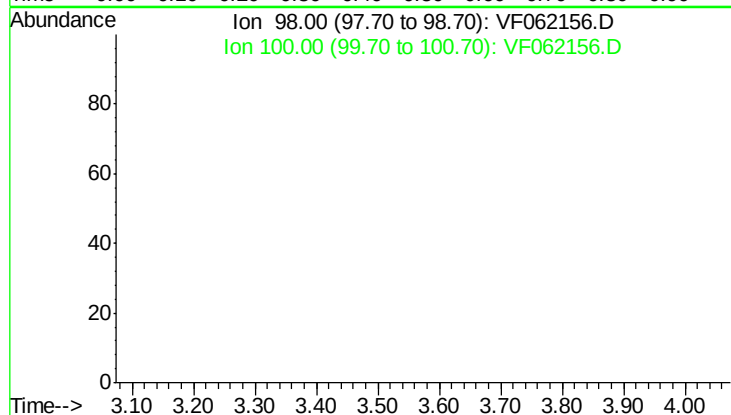


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 11.44 min

Lab File: VF062156.D
Acq: 26 Mar 2019 20:04

Tgt Ion	95
Sig	Exp Ratio
95	100
174	84.1
176	82.1


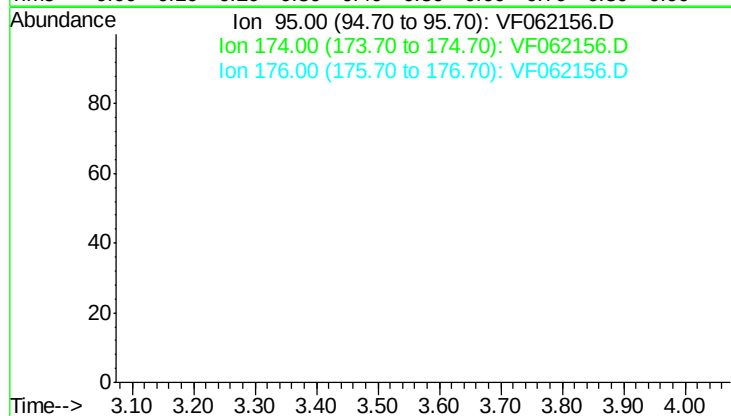


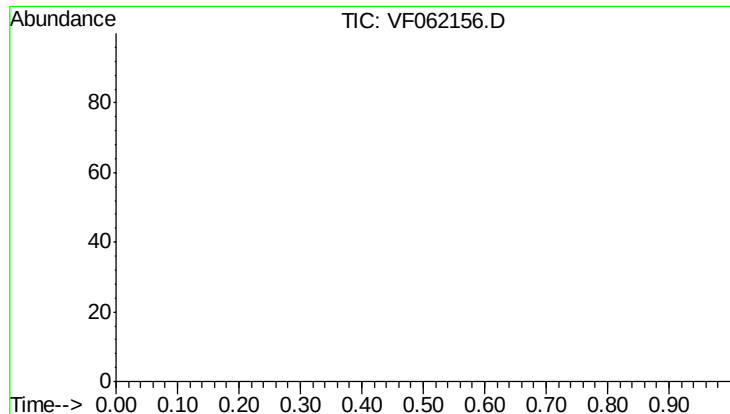

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 9.81 min
 Lab File: VF062156.D
 Acq: 26 Mar 2019 20:04

Instrument :
 MSVOA_F
 ClientSampleId :
 OR-01-032519-A

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 49.0
 119 31.8

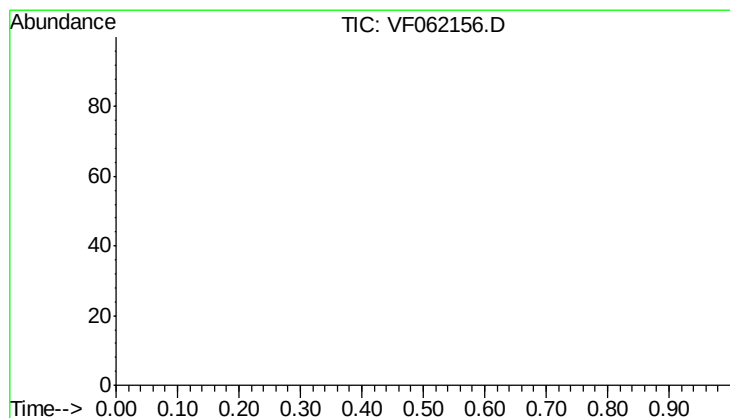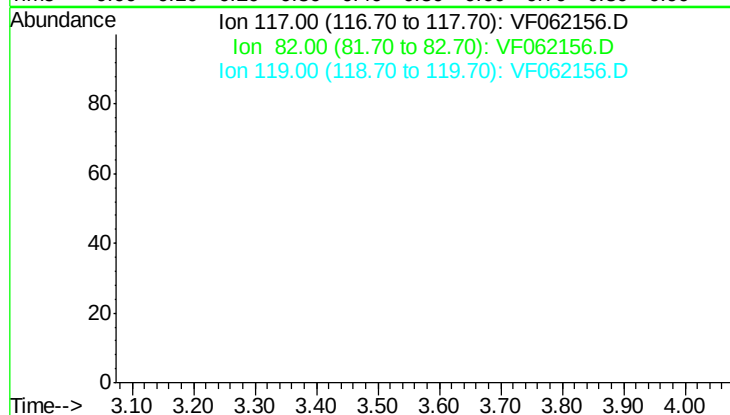

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 12.57 min
 Lab File: VF062156.D
 Acq: 26 Mar 2019 20:04

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 55.4
 150 156.6

