

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF032619\
 Data File : VF062154.D
 Acq On : 26 Mar 2019 19:07
 Operator : VA/AP
 Sample : K2086-01RE
 Misc : 6.05g/5mL/MSVOA-F/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 CS-11RE

Quant Time: Mar 27 05:18:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F032219S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 23 01:16:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-4.91
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-5.63
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-9.81
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.57

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF032619\
Data File : VF062154.D
Acq On : 26 Mar 2019 19:07
Operator : VA/AP
Sample : K2086-01RE
Misc : 6.05g/5mL/MSVOA-F/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
CS-11RE

Quant Time: Mar 27 05:18:16 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F032219S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 23 01:16:37 2019
Response via : Initial Calibration

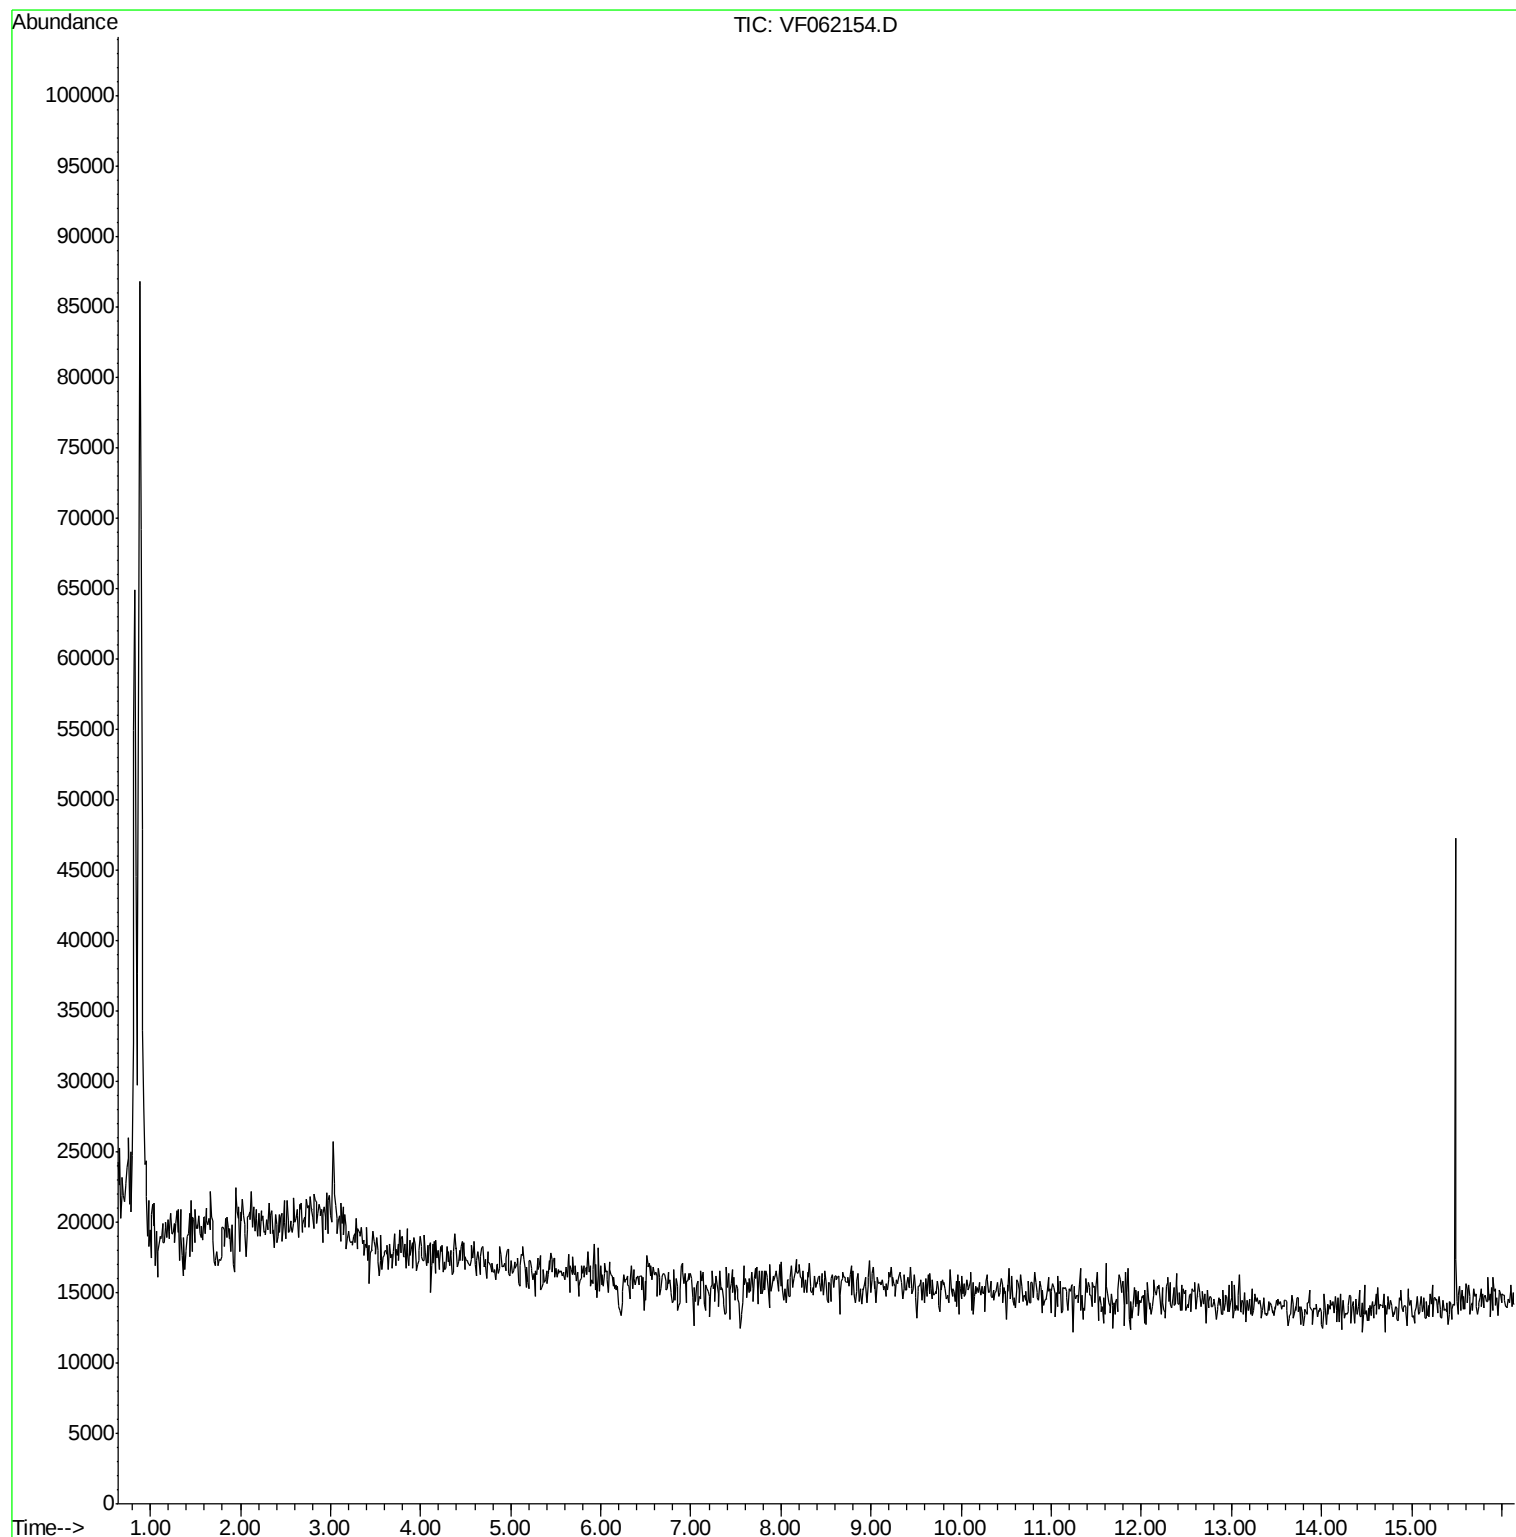

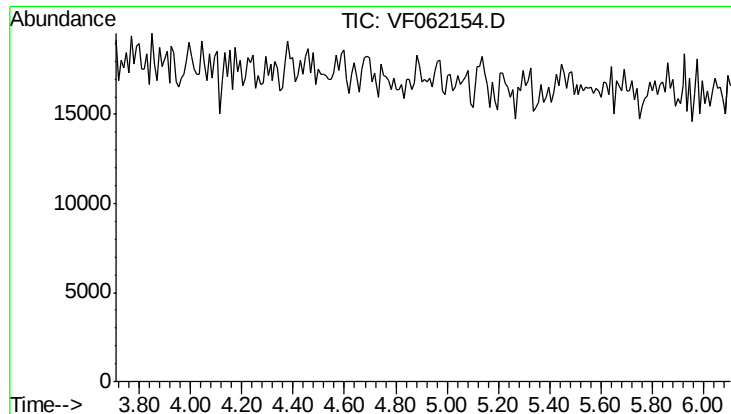

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 4.91 min

Lab File: VF062154.D

Acq: 26 Mar 2019 19:07

Tot Ion: 168

Sig Exp Ratio

168 100



99 47.8

Instrument :

MSVOA_F

ClientSampleId :

CS-11RE

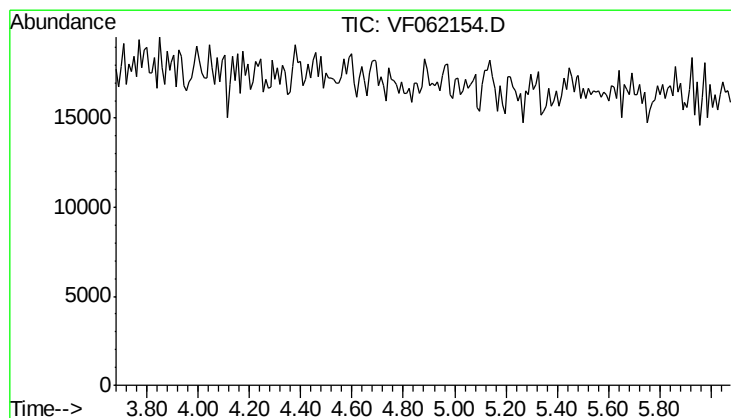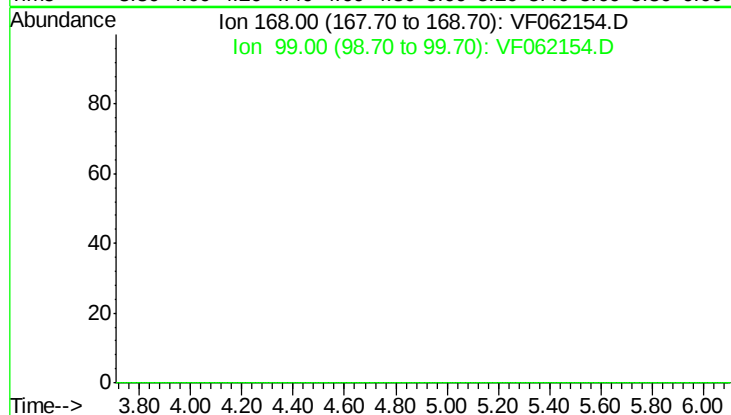

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 4.88 min

Lab File: VF062154.D


Acq: 26 Mar 2019 19:07


Tgt Ion: 65

Sig Exp Ratio

65 100

67 53.1

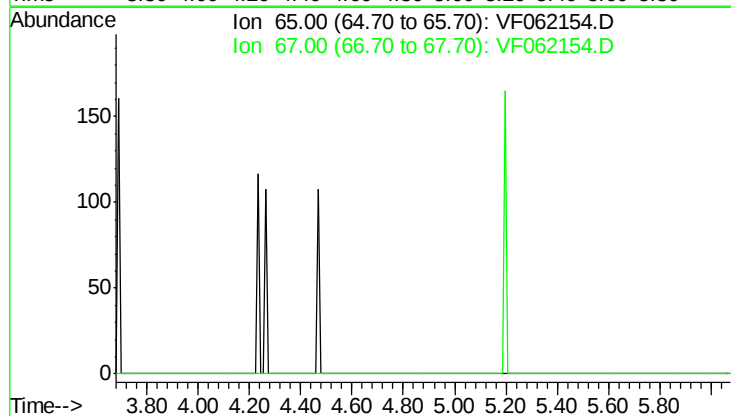


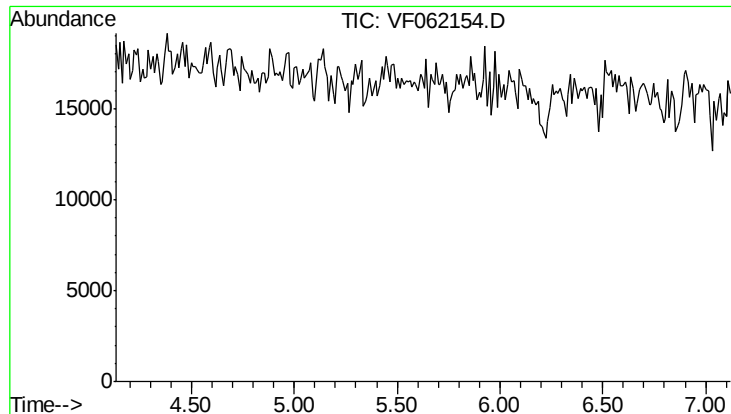


#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 5.63 min
 Lab File: VF062154.D
 Acq: 26 Mar 2019 19:07

Instrument :
 MSVOA_F
 ClientSampleId :
 CS-11RE

Tot Ion: 114


Sig	Exp Ratio
114	100
63	18.9
88	18.2

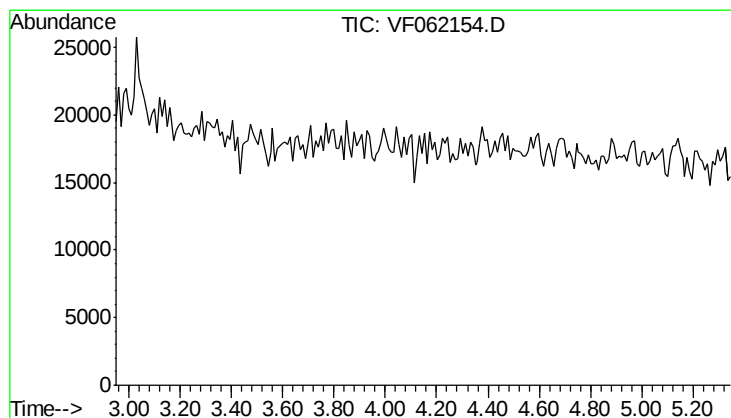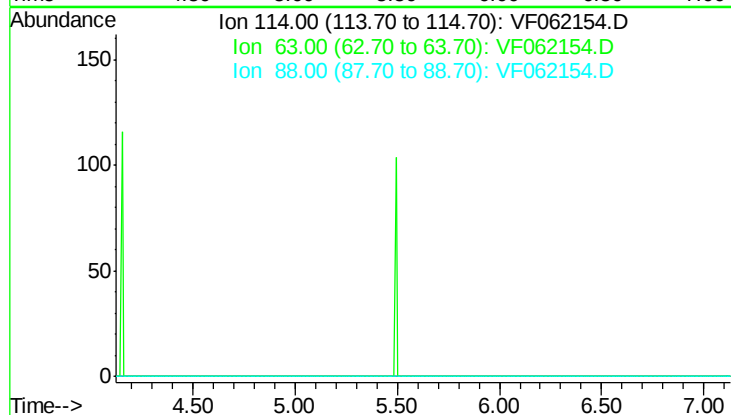


#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 4.15 min
 Lab File: VF062154.D
 Acq: 26 Mar 2019 19:07

Tgt Ion: 113

Sig	Exp Ratio
113	100
111	94.2
192	15.4

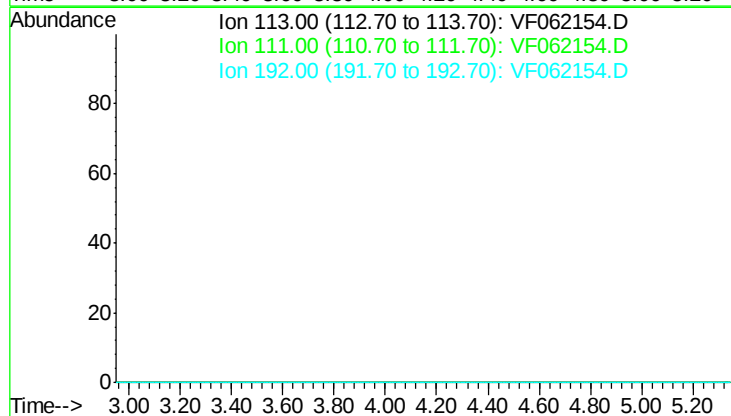


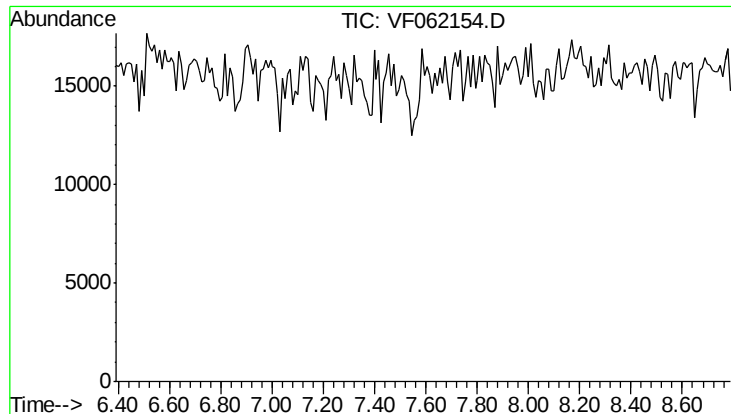


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 7.59 min

Lab File: VF062154.D
Acq: 26 Mar 2019 19:07

Instrument :
MSVOA_F
ClientSampleId :
CS-11RE


Tot Ion: 98
Sig Exp Ratio
98 100
100 71.3

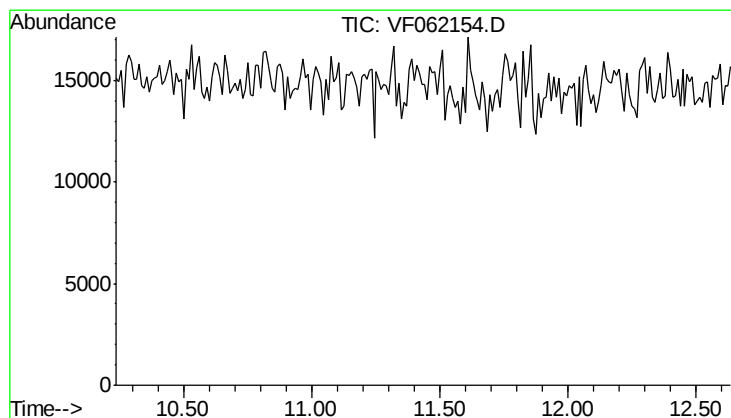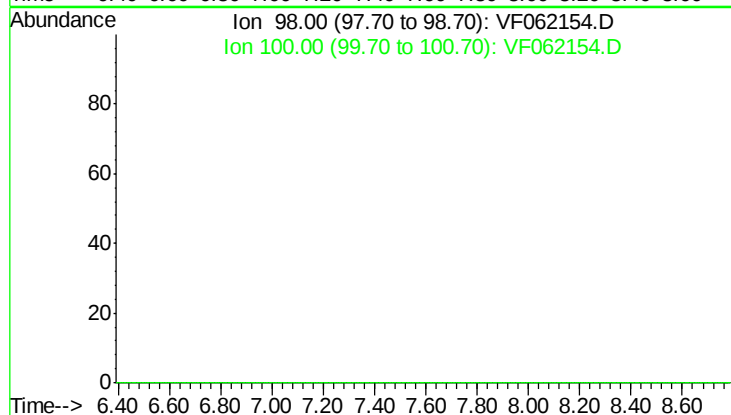


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 11.44 min

Lab File: VF062154.D
Acq: 26 Mar 2019 19:07

Tgt Ion: 95
Sig Exp Ratio
95 100
174 84.1
176 82.1


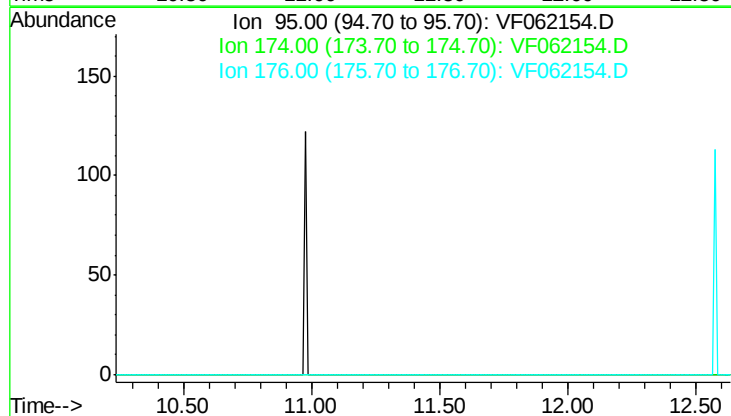


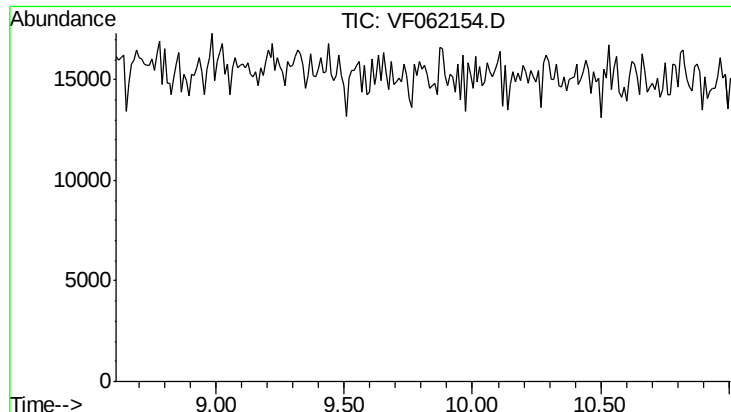

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 9.81 min
 Lab File: VF062154.D
 Acq: 26 Mar 2019 19:07

Instrument :
 MSVOA_F
 ClientSampleId :
 CS-11RE

Tot Ion	Sig	Exp Ratio
117	100	
82	49.0	
119	31.8	

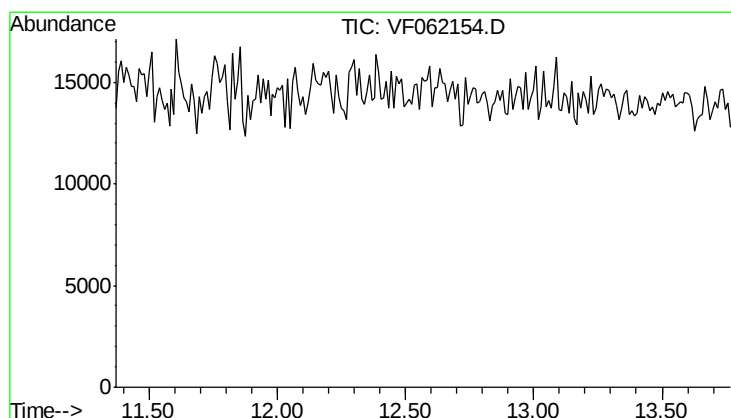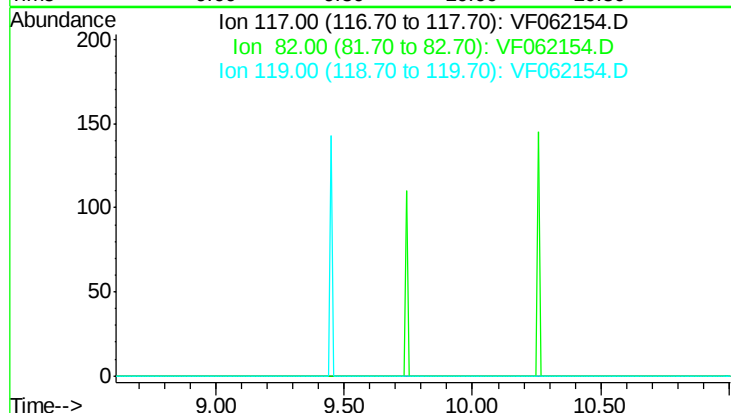

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 12.57 min
 Lab File: VF062154.D
 Acq: 26 Mar 2019 19:07

Tgt Ion	Sig	Exp Ratio
152	100	
115	55.4	
150	156.6	

